

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
 Data File : BG063096.D
 Acq On : 28 Sep 2024 6:20
 Operator : RC/JU
 Sample : P3927-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.681	96	101	104	rBV7	5699	11971	0.52%	0.059%
2	3.723	104	108	119	rVV2	77127	131572	5.73%	0.649%
3	3.834	125	127	131	rVB5	6774	5935	0.26%	0.029%
4	4.251	196	198	200	rVV2	6461	6570	0.29%	0.032%
5	4.287	202	204	206	rVB3	5241	4411	0.19%	0.022%
6	4.386	219	221	223	rBV3	5265	4318	0.19%	0.021%
7	4.533	245	246	250	rBV3	6390	6336	0.28%	0.031%
8	4.645	263	265	270	rVV4	4190	6732	0.29%	0.033%
9	4.698	270	274	276	rVB2	4682	4655	0.20%	0.023%
10	4.774	282	287	290	rBV3	5458	8695	0.38%	0.043%
11	4.827	290	296	297	rBV3	5670	8050	0.35%	0.040%
12	4.921	309	312	314	rBV3	3833	4925	0.21%	0.024%
13	5.021	326	329	332	rBV2	4041	5297	0.23%	0.026%
14	5.215	359	362	363	rBV	6020	5462	0.24%	0.027%
15	5.485	405	408	409	rBV3	7470	5614	0.24%	0.028%
16	5.532	412	416	419	rVB3	5525	7075	0.31%	0.035%
17	5.573	419	423	425	rBV3	3615	6728	0.29%	0.033%
18	5.626	430	432	437	rVB3	4123	4477	0.19%	0.022%
19	5.785	455	459	462	rBV2	4706	7392	0.32%	0.036%
20	6.049	499	504	505	rVV2	5405	4730	0.21%	0.023%
21	6.378	556	560	562	rBV3	4636	5420	0.24%	0.027%
22	7.019	663	669	680	rBV	132007	218254	9.51%	1.076%
23	7.183	690	697	705	rBV	75567	133990	5.84%	0.661%
24	7.383	724	731	741	rBV2	135308	243034	10.58%	1.198%
25	7.459	741	744	746	rBV2	5030	5232	0.23%	0.026%
26	7.630	769	773	775	rBV2	4722	6160	0.27%	0.030%
27	7.847	805	810	819	rBV	231371	401018	17.47%	1.977%
28	7.941	825	826	829	rBV2	3905	4069	0.18%	0.020%
29	8.288	882	885	890	rVB2	3449	5305	0.23%	0.026%
30	8.446	907	912	914	rBV3	3795	5911	0.26%	0.029%
31	8.493	917	920	922	rVB2	4821	4448	0.19%	0.022%
32	8.552	922	930	937	rBV2	178904	309015	13.46%	1.524%
33	8.740	958	962	964	rVB3	3549	4205	0.18%	0.021%
34	8.834	974	978	980	rBV2	5268	6867	0.30%	0.034%
35	8.999	999	1006	1016	rVB2	123137	219775	9.57%	1.084%
36	9.134	1027	1029	1033	rBV	4254	6757	0.29%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
 Data File : BG063096.D
 Acq On : 28 Sep 2024 6:20
 Operator : RC/JU
 Sample : P3927-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
 Title : SVOA CALIBRATION

37	9.175	1033	1036	1038	rVB2	4019	4457	0.19%	0.022%
38	9.193	1038	1039	1043	rBV2	7380	4813	0.21%	0.024%
39	9.480	1086	1088	1091	rVB2	4403	4239	0.18%	0.021%
40	9.516	1091	1094	1096	rVB2	3499	4233	0.18%	0.021%
41	9.551	1098	1100	1102	rBV3	5033	5754	0.25%	0.028%
42	9.721	1123	1129	1139	rVB3	113852	207094	9.02%	1.021%
43	10.133	1196	1199	1202	rVB2	4133	4735	0.21%	0.023%
44	10.262	1213	1221	1231	rBV3	201026	391912	17.07%	1.932%
45	10.638	1276	1285	1293	rVB	350676	625567	27.25%	3.085%
46	10.773	1301	1308	1315	rBV	174736	324443	14.13%	1.600%
47	11.184	1375	1378	1380	rBV4	4298	5760	0.25%	0.028%
48	11.237	1385	1387	1389	rBV2	5229	5003	0.22%	0.025%
49	11.455	1419	1424	1427	rBV2	3901	5095	0.22%	0.025%
50	12.218	1551	1554	1555	rBV	5051	4335	0.19%	0.021%
51	12.236	1555	1557	1561	rVB4	5513	6261	0.27%	0.031%
52	12.265	1561	1562	1568	rVB2	3739	5362	0.23%	0.026%
53	13.358	1747	1748	1751	rBV	4384	4345	0.19%	0.021%
54	13.482	1767	1769	1773	rBV2	3506	4872	0.21%	0.024%
55	13.723	1808	1810	1815	rVB2	4272	5860	0.26%	0.029%
56	13.787	1818	1821	1823	rVV	3721	4765	0.21%	0.023%
57	13.887	1832	1838	1846	rBV	466041	685136	29.84%	3.378%
58	14.081	1869	1871	1876	rVB2	3895	5035	0.22%	0.025%
59	14.175	1876	1887	1894	rBV	508336	835676	36.40%	4.121%
60	14.392	1921	1924	1927	rBV	4139	5013	0.22%	0.025%
61	14.486	1933	1940	1947	rBV	727630	1152230	50.18%	5.682%
62	14.616	1957	1962	1964	rBV3	4751	6996	0.30%	0.034%
63	14.692	1970	1975	1986	rBV2	126792	250742	10.92%	1.236%
64	14.821	1995	1997	2001	rVB3	3283	4218	0.18%	0.021%
65	15.086	2040	2042	2044	rVB3	5682	5057	0.22%	0.025%
66	15.115	2044	2047	2054	rBV3	9358	20690	0.90%	0.102%
67	15.479	2102	2109	2116	rBV	803919	1180273	51.40%	5.820%
68	15.603	2125	2130	2135	rBV	145393	228563	9.95%	1.127%
69	15.720	2147	2150	2151	rBV	4863	4246	0.18%	0.021%
70	15.844	2165	2171	2178	rVB	304401	418316	18.22%	2.063%
71	16.173	2223	2227	2230	rBV4	7581	11128	0.48%	0.055%
72	16.408	2262	2267	2272	rVB2	48745	73495	3.20%	0.362%
73	16.555	2290	2292	2296	rVB2	4022	4192	0.18%	0.021%
74	16.660	2309	2310	2314	rVB3	4955	5627	0.25%	0.028%
75	16.831	2336	2339	2340	rBV	5124	4631	0.20%	0.023%
76	16.848	2340	2342	2345	rVB2	5714	4549	0.20%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
 Data File : BG063096.D
 Acq On : 28 Sep 2024 6:20
 Operator : RC/JU
 Sample : P3927-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
 Title : SVOA CALIBRATION

77	16.895	2345	2350	2357	rBV4	35696	68428	2.98%	0.337%
78	17.019	2369	2371	2375	rVB4	6398	7148	0.31%	0.035%
79	17.054	2375	2377	2381	rVV3	4366	5394	0.23%	0.027%
80	17.236	2401	2408	2415	rBV	1155396	1735660	75.59%	8.558%
81	17.336	2419	2425	2434	rVB	957160	1453371	63.30%	7.166%
82	17.424	2436	2440	2442	rBV4	8671	13873	0.60%	0.068%
83	17.559	2461	2463	2466	rBV2	6592	6087	0.27%	0.030%
84	17.853	2510	2513	2519	rBV4	33114	45612	1.99%	0.225%
85	18.129	2556	2560	2567	rVV4	53021	83851	3.65%	0.413%
86	18.417	2607	2609	2610	rBV2	6773	4420	0.19%	0.022%
87	18.435	2610	2612	2614	rVV3	9258	7904	0.34%	0.039%
88	18.582	2633	2637	2640	rBV6	5754	7103	0.31%	0.035%
89	18.717	2658	2660	2661	rBV	5511	4302	0.19%	0.021%
90	18.822	2677	2678	2681	rBV3	4654	4905	0.21%	0.024%
91	18.864	2683	2685	2688	rVB4	6814	6605	0.29%	0.033%
92	19.157	2733	2735	2738	rBV2	4617	5411	0.24%	0.027%
93	19.193	2738	2741	2744	rBV4	16256	23552	1.03%	0.116%
94	19.269	2752	2754	2758	rVB4	11980	9533	0.42%	0.047%
95	19.627	2809	2815	2822	rBV	1349948	1949594	84.91%	9.613%
96	20.074	2889	2891	2894	rBV4	10850	10104	0.44%	0.050%
97	21.155	3071	3075	3080	rBV5	56721	80342	3.50%	0.396%
98	21.484	3125	3131	3140	rBV	1339019	2152089	93.73%	10.612%
99	24.316	3604	3613	3624	rBV	756501	1933758	84.22%	9.535%
100	24.528	3640	3649	3658	rVB2	878940	2296077	100.00%	11.322%


Sum of corrected areas: 20280246

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
Data File : BG063096.D
Acq On : 28 Sep 2024 6:20
Operator : RC/JU
Sample : P3927-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

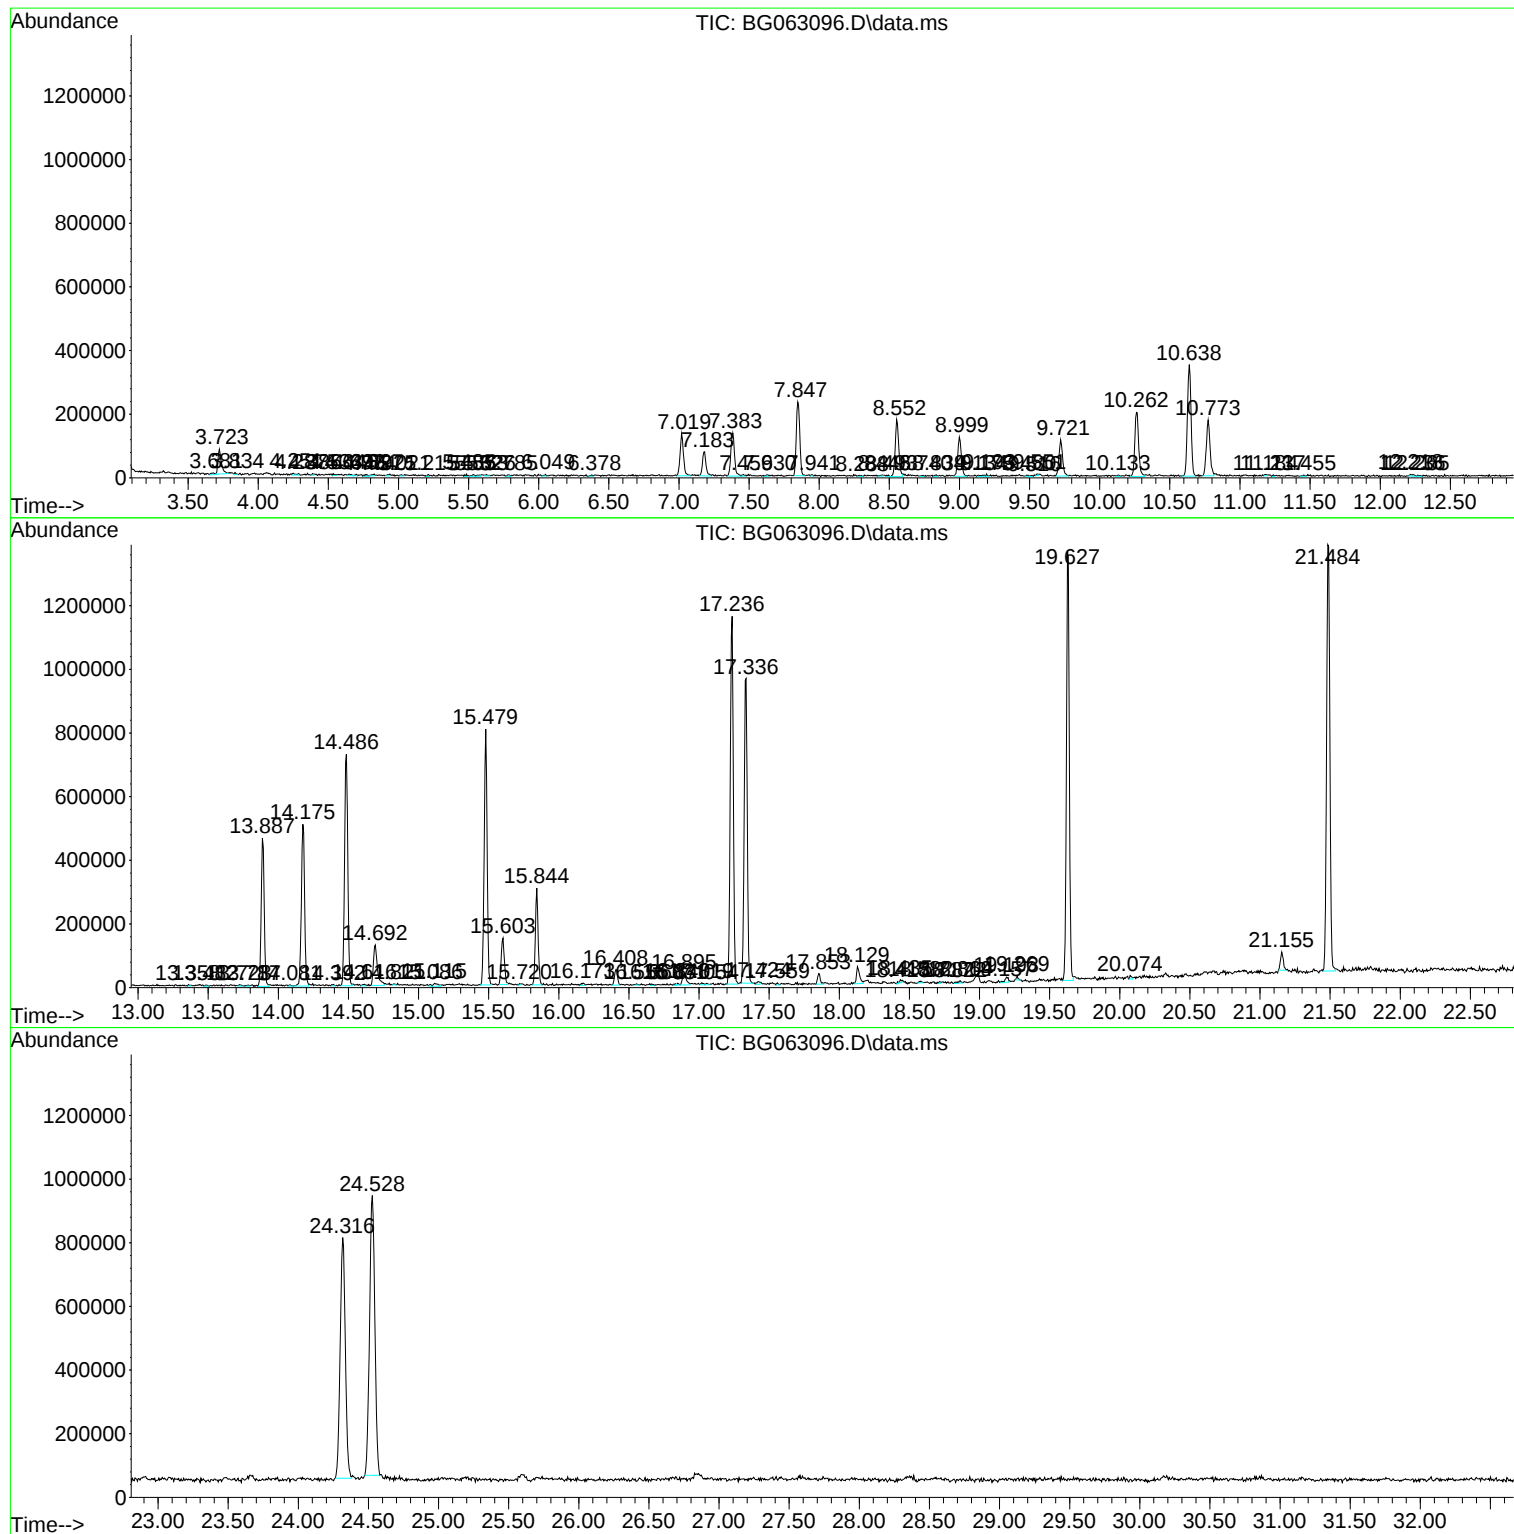

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
Data File : BG063096.D
Acq On : 28 Sep 2024 6:20
Operator : RC/JU
Sample : P3927-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC84










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.844	7.26 ng/ul	418316	Acenaphthene-d10	14.486

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	95
3			Benzophenone	182	C13H10O	000119-61-9	95
4			Benzophenone	182	C13H10O	000119-61-9	87
5			Benzophenone	182	C13H10O	000119-61-9	80

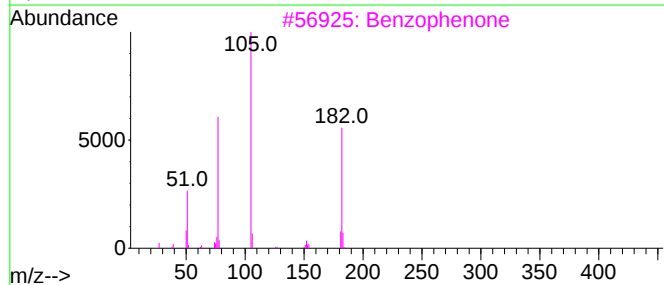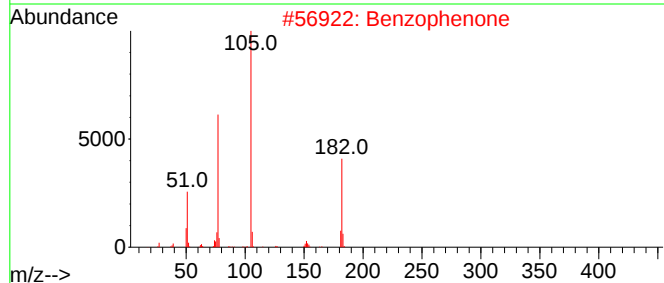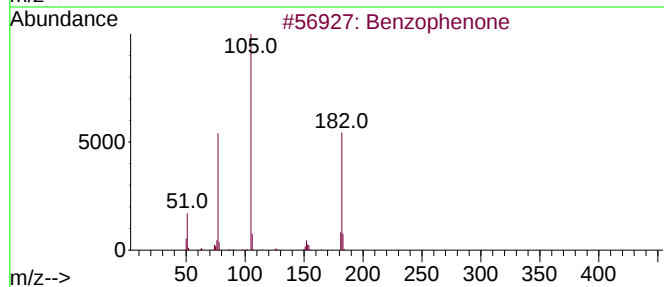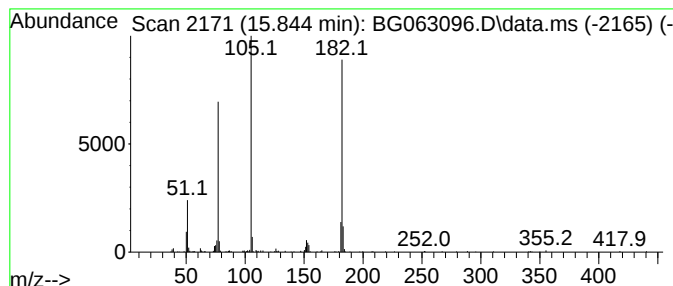

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
Data File : BG063096.D
Acq On : 28 Sep 2024 6:20
Operator : RC/JU
Sample : P3927-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.844	7.3	ng/u1	418316	3	14.486	1152230	20.0