

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059234.D
 Acq On : 28 Sep 2023 14:57
 Operator : MA/JU
 Sample : 04480-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020576

Quant Time: Sep 29 00:42:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 04:33:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.232	152	43174	20.000	ng/ul	0.00
20) Naphthalene-d8	11.075	136	205512	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.865	164	130348	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.615	188	291094	20.000	ng/ul	0.00
79) Chrysene-d12	21.916	240	272137	20.000	ng/ul	0.00
88) Perylene-d12	25.400	264	337725	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.531	96	6731	5.884	ng/uL	0.00
4) Pyridine-d5	3.966	84	60651	18.171	ng/ul	0.00
7) Phenol-d5	7.356	99	42671	9.874	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.550	67	141521	51.262	ng/ul	0.00
11) 2-Chlorophenol-d4	7.750	132	120237	41.389	ng/ul	0.00
15) 4-Methylphenol-d8	8.925	113	73753	22.078	ng/ul	0.00
21) Nitrobenzene-d5	9.430	128	80638	55.604	ng/ul	0.00
24) 2-Nitrophenol-d4	10.147	143	78608	55.215	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.676	165	137054	46.863	ng/ul	0.00
31) 4-Chloroaniline-d4	11.222	131	145750	30.802	ng/ul	0.00
46) Dimethylphthalate-d6	14.266	166	505540	53.643	ng/ul	0.00
49) Acenaphthylene-d8	14.571	160	603234	50.996	ng/ul	0.00
54) 4-Nitrophenol-d4	15.059	143	14491	8.805	ng/ul	0.00
60) Fluorene-d10	15.858	176	466415	51.999	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.964	200	72406	48.391	ng/ul	0.00
73) Anthracene-d10	17.715	188	700130	52.785	ng/ul	0.00
81) Pyrene-d10	19.994	212	870576	57.125	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.165	264	899268	55.410	ng/ul	0.00
Target Compounds						
43) 1,1'-Biphenyl	13.702	154	21366	2.030	ng/ul#	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059234.D
Acq On : 28 Sep 2023 14:57
Operator : MA/JU
Sample : 04480-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD020576

Quant Time: Sep 29 00:42:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 28 04:33:25 2023
Response via : Initial Calibration

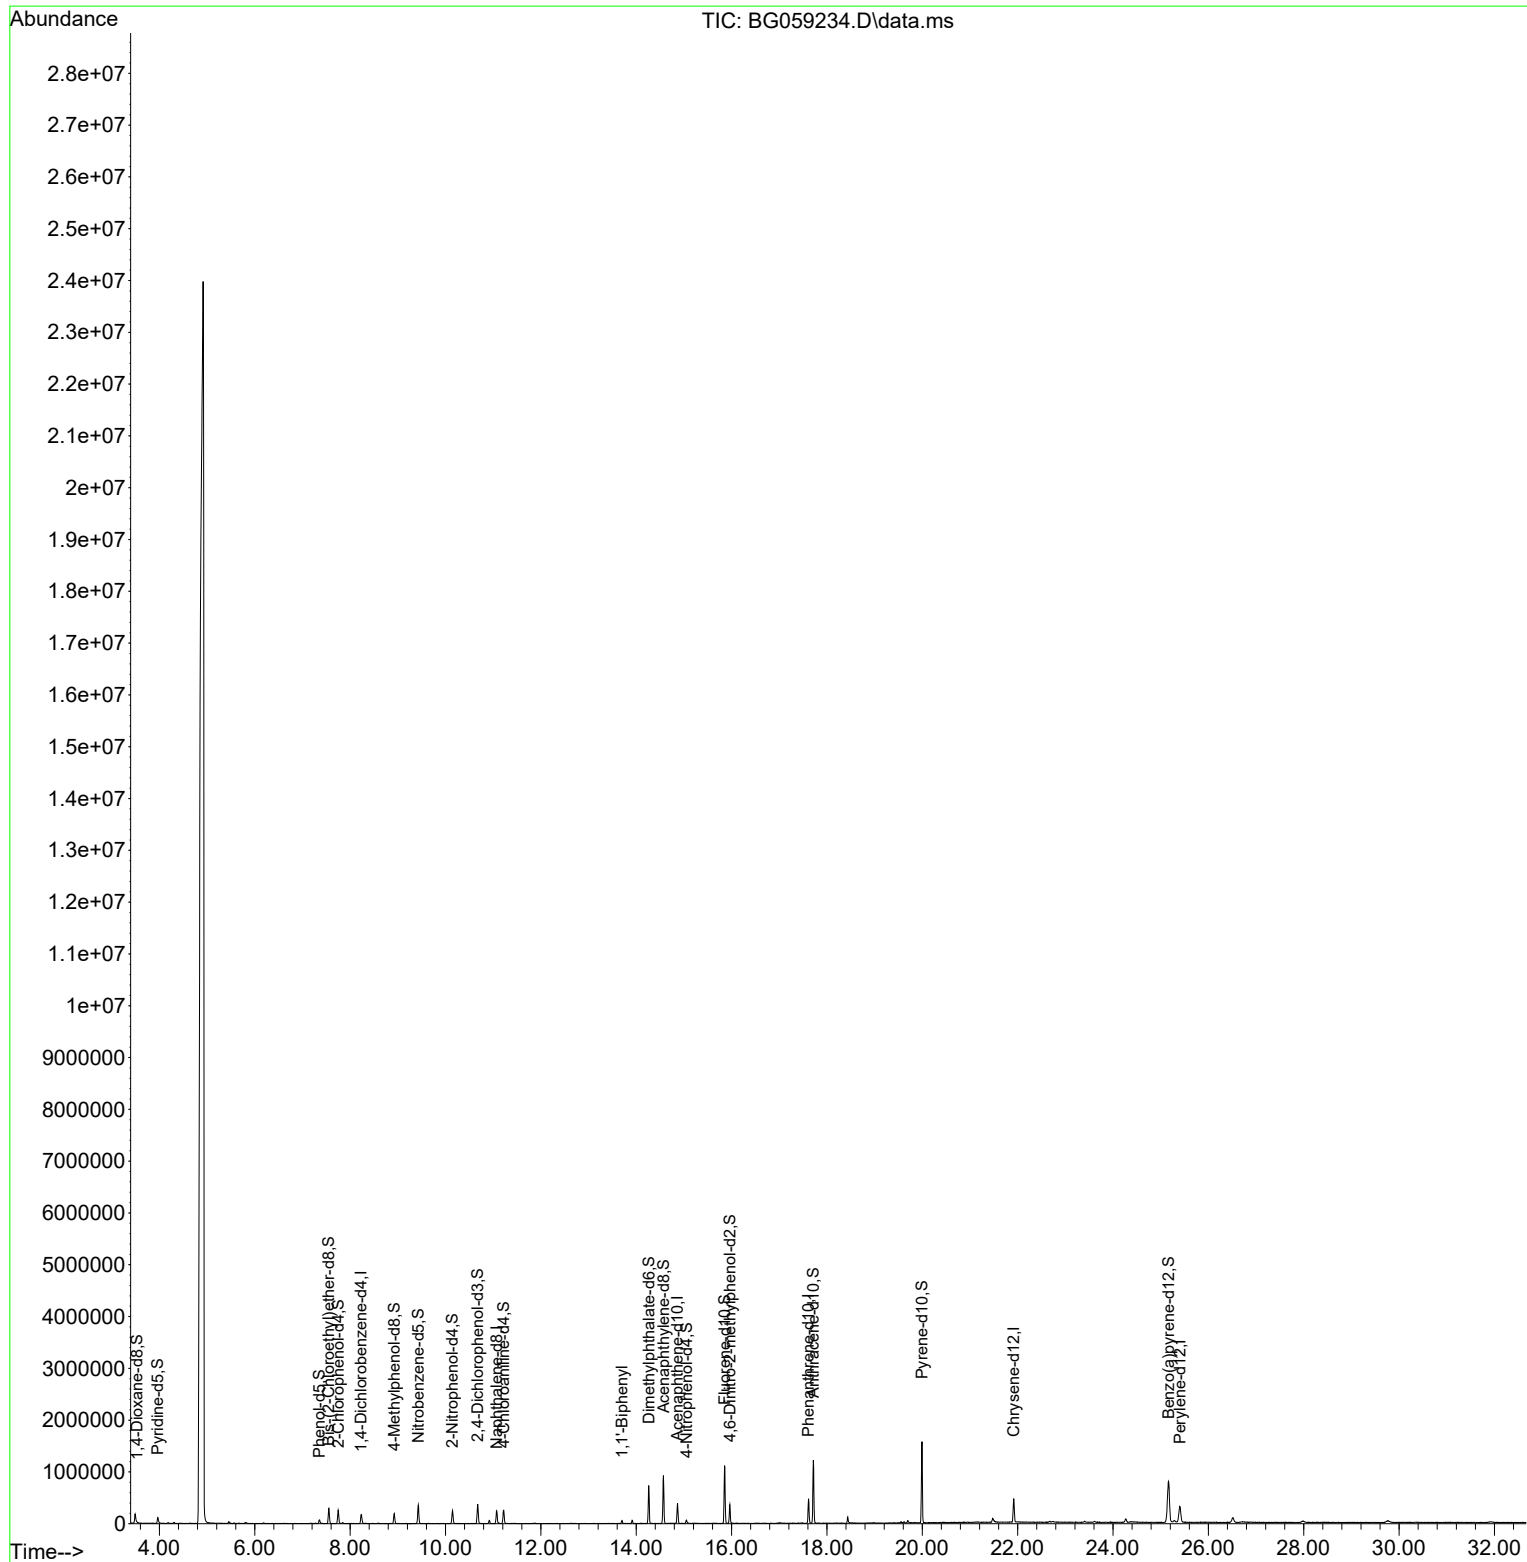

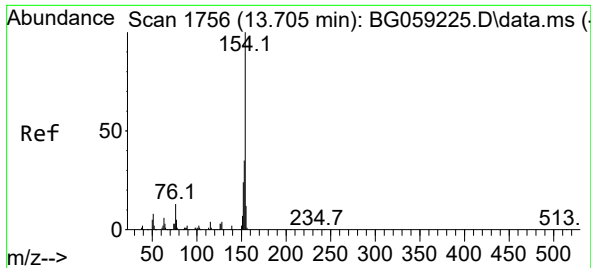

#43
 1,1'-Biphenyl
 Concen: 2.030 ng/ul
 RT: 13.702 min Scan# 11
 Delta R.T. -0.005 min
 Lab File: BG059234.D
 Acq: 28 Sep 2023 14:57

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020576

Tgt Ion	Ratio	Lower	Upper
154	100		
153	35.6	29.2	43.8
76	22.1	10.1	15.1#

