

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059226.D
 Acq On : 28 Sep 2023 9:31
 Operator : MA/JU
 Sample : PB155814BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK814

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.531	19	24	33	rVB4	18707	36171	1.86%	0.200%
2	3.595	33	35	37	rBV3	3184	3035	0.16%	0.017%
3	3.642	40	43	46	rBV2	3219	3399	0.17%	0.019%
4	3.960	93	97	110	rBV	246552	440233	22.66%	2.432%
5	4.524	188	193	198	rVB6	4211	8766	0.45%	0.048%
6	5.053	281	283	286	rVB2	2460	2703	0.14%	0.015%
7	5.564	369	370	374	rVB3	3883	3349	0.17%	0.019%
8	5.611	374	378	381	rBV3	2422	3819	0.20%	0.021%
9	5.705	393	394	401	rVB4	2996	4790	0.25%	0.026%
10	5.763	401	404	407	rBV2	2392	3577	0.18%	0.020%
11	5.869	419	422	424	rBV2	2223	2812	0.14%	0.016%
12	7.132	634	637	642	rBV2	2701	3966	0.20%	0.022%
13	7.356	668	675	690	rVB	269333	468187	24.10%	2.587%
14	7.555	702	709	718	rBV	226811	380100	19.57%	2.100%
15	7.749	735	742	752	rBV	252067	438025	22.55%	2.420%
16	7.896	765	767	776	rVB3	2454	3316	0.17%	0.018%
17	8.120	803	805	810	rVB3	2817	3827	0.20%	0.021%
18	8.161	810	812	815	rBV	2457	2664	0.14%	0.015%
19	8.231	818	824	831	rVV2	157263	268174	13.81%	1.482%
20	8.296	833	835	838	rBV2	2254	2995	0.15%	0.017%
21	8.537	871	876	879	rBV2	2092	3425	0.18%	0.019%
22	8.924	934	942	949	rBV2	324438	558740	28.76%	3.087%
23	9.195	986	988	991	rBV2	2467	2916	0.15%	0.016%
24	9.430	1019	1028	1036	rBV	268833	474124	24.41%	2.620%
25	9.500	1039	1040	1045	rVB	2624	3059	0.16%	0.017%
26	10.147	1139	1150	1158	rBV2	201912	368967	18.99%	2.039%
27	10.675	1229	1240	1252	rBV2	299336	547204	28.17%	3.023%
28	11.075	1301	1308	1318	rVB	254995	440815	22.69%	2.436%
29	11.222	1325	1333	1344	rBV2	339741	635548	32.72%	3.511%
30	11.316	1346	1349	1353	rVB2	2676	4580	0.24%	0.025%
31	11.715	1412	1417	1420	rBV	1934	4127	0.21%	0.023%
32	12.644	1569	1575	1577	rBV2	5693	8621	0.44%	0.048%
33	13.178	1662	1666	1669	rBV	2136	3454	0.18%	0.019%
34	13.701	1750	1755	1758	rBV3	6195	10073	0.52%	0.056%
35	13.936	1792	1795	1798	rBV3	2554	2633	0.14%	0.015%
36	14.265	1844	1851	1859	rBV	655989	934857	48.13%	5.165%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059226.D
 Acq On : 28 Sep 2023 9:31
 Operator : MA/JU
 Sample : PB155814BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK814

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

37	14.571	1897	1903	1911	rBV2	730842	1119339	57.62%	6.184%
38	14.870	1947	1954	1961	rVB2	396025	629581	32.41%	3.478%
39	15.058	1977	1986	1998	rBV	287625	485109	24.97%	2.680%
40	15.858	2114	2122	2131	rBV	921090	1374919	70.78%	7.597%
41	15.963	2134	2140	2149	rBV	301058	437261	22.51%	2.416%
42	16.093	2158	2162	2164	rBV2	4779	4944	0.25%	0.027%
43	16.433	2216	2220	2221	rVB2	2590	2799	0.14%	0.015%
44	16.639	2251	2255	2257	rBV	1883	2973	0.15%	0.016%
45	17.197	2346	2350	2352	rBV	2317	2916	0.15%	0.016%
46	17.620	2413	2422	2430	rBV	512728	772924	39.79%	4.270%
47	17.720	2430	2439	2446	rVV	1027319	1547568	79.67%	8.550%
48	17.796	2450	2452	2456	rVB2	2879	3066	0.16%	0.017%
49	17.838	2456	2459	2461	rBV	3485	3566	0.18%	0.020%
50	18.120	2506	2507	2510	rBV	2605	2613	0.13%	0.014%
51	18.537	2574	2578	2580	rBV2	2754	3290	0.17%	0.018%
52	18.566	2580	2583	2586	rVB3	2303	2861	0.15%	0.016%
53	18.830	2625	2628	2629	rVB2	3827	2812	0.14%	0.016%
54	19.001	2654	2657	2658	rBV	3141	2591	0.13%	0.014%
55	19.283	2703	2705	2708	rBV3	3031	2617	0.13%	0.014%
56	19.312	2708	2710	2712	rBV4	3146	2561	0.13%	0.014%
57	19.383	2717	2722	2723	rBV5	3029	5477	0.28%	0.030%
58	19.553	2748	2751	2755	rVB2	14877	19275	0.99%	0.106%
59	19.618	2760	2762	2768	rVB5	12132	20775	1.07%	0.115%
60	19.847	2799	2801	2803	rVB3	8245	7277	0.37%	0.040%
61	19.994	2819	2826	2835	rVB	1331124	1852815	95.38%	10.237%
62	20.105	2842	2845	2850	rVB6	5107	7436	0.38%	0.041%
63	20.264	2870	2872	2875	rBV2	5370	4707	0.24%	0.026%
64	20.434	2900	2901	2904	rVB3	3996	2920	0.15%	0.016%
65	20.875	2974	2976	2979	rVB3	7431	7549	0.39%	0.042%
66	21.040	3002	3004	3006	rBV3	6526	6084	0.31%	0.034%
67	21.921	3147	3154	3161	rBV	492125	837969	43.14%	4.630%
68	25.164	3695	3706	3721	rBV2	664935	1942553	100.00%	10.733%
69	25.405	3738	3747	3758	rVB2	314168	891098	45.87%	4.923%




Sum of corrected areas: 18099296

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059226.D
Acq On : 28 Sep 2023 9:31
Operator : MA/JU
Sample : PB155814BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK814

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

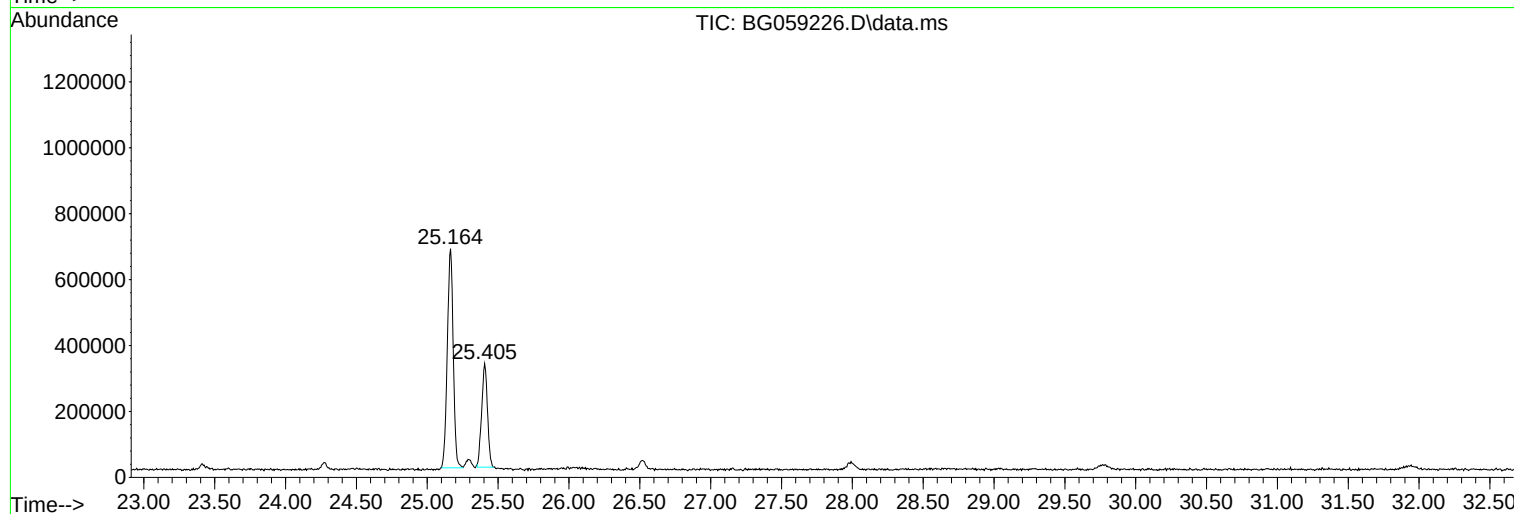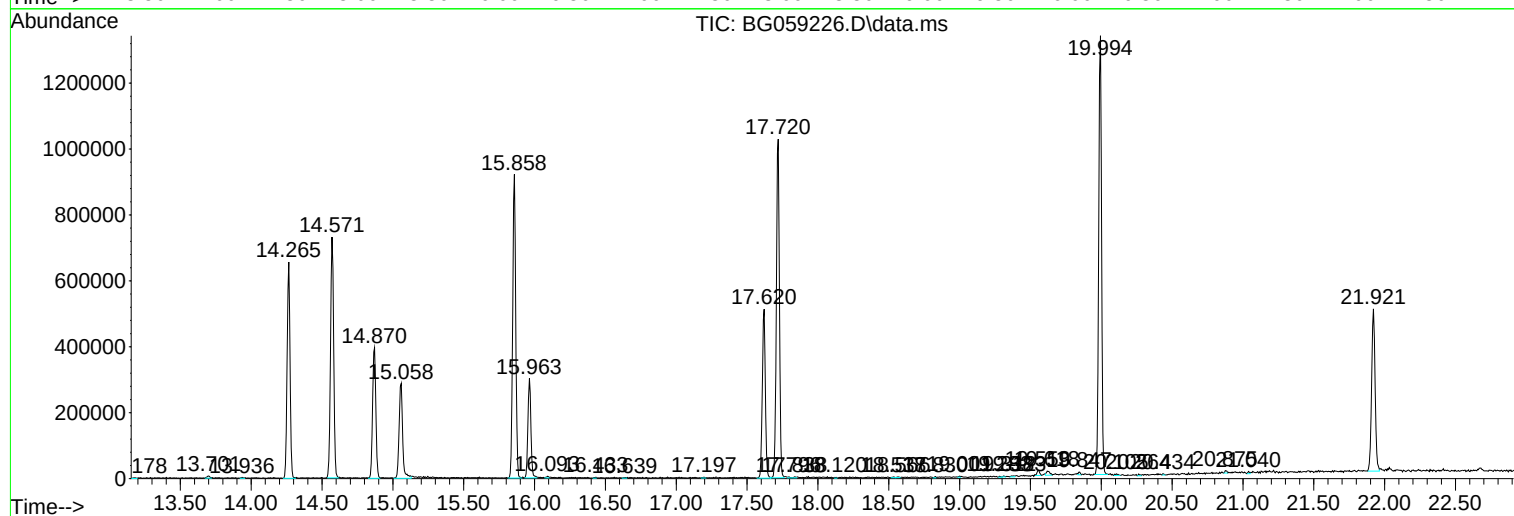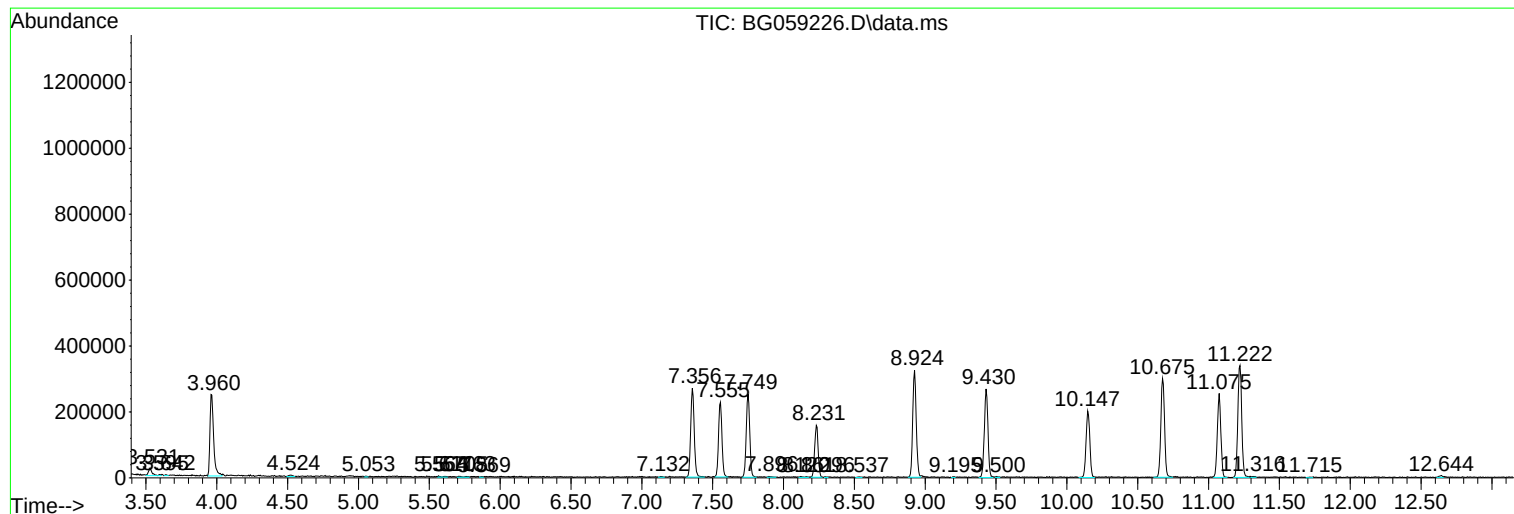

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059226.D
Acq On : 28 Sep 2023 9:31
Operator : MA/JU
Sample : PB155814BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK814

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059226.D
Acq On : 28 Sep 2023 9:31
Operator : MA/JU
Sample : PB155814BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK814

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc