

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059230.D
 Acq On : 28 Sep 2023 12:14
 Operator : MA/JU
 Sample : PB155856BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK856

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.466	11	13	17	rBV4	3435	4877	0.32%	0.031%
2	3.531	19	24	28	rVV3	17088	24932	1.66%	0.159%
3	3.719	54	56	59	rVB3	4220	3775	0.25%	0.024%
4	3.960	93	97	110	rBV	215710	379716	25.24%	2.418%
5	4.048	110	112	118	rVB5	3786	4412	0.29%	0.028%
6	4.301	153	155	158	rVB2	2550	2161	0.14%	0.014%
7	4.383	168	169	174	rVB4	2335	2976	0.20%	0.019%
8	4.612	207	208	213	rBV2	2874	3073	0.20%	0.020%
9	4.647	213	214	218	rBV3	2088	2721	0.18%	0.017%
10	4.865	249	251	253	rBV2	2224	2234	0.15%	0.014%
11	5.041	278	281	283	rBV3	3551	2356	0.16%	0.015%
12	5.482	354	356	361	rBV3	2218	2989	0.20%	0.019%
13	5.881	420	424	425	rVB2	2418	2209	0.15%	0.014%
14	5.981	438	441	443	rBV3	2868	2619	0.17%	0.017%
15	6.909	596	599	602	rBV2	2951	3801	0.25%	0.024%
16	7.027	617	619	620	rBV2	3445	2192	0.15%	0.014%
17	7.068	622	626	629	rVB	3860	4726	0.31%	0.030%
18	7.356	667	675	684	rBV	232658	400668	26.63%	2.551%
19	7.503	698	700	702	rBV	2544	2540	0.17%	0.016%
20	7.550	702	708	717	rVB	190323	326427	21.70%	2.079%
21	7.750	735	742	750	rBV	224882	372666	24.77%	2.373%
22	7.955	776	777	780	rBV	1647	2104	0.14%	0.013%
23	8.090	797	800	803	rBV	2177	2548	0.17%	0.016%
24	8.149	808	810	812	rBV	2269	2348	0.16%	0.015%
25	8.231	818	824	833	rVB2	151412	258035	17.15%	1.643%
26	8.519	872	873	877	rVB	2980	2365	0.16%	0.015%
27	8.925	933	942	951	rBV2	277593	492827	32.76%	3.138%
28	9.371	1014	1018	1019	rBV	2261	2634	0.18%	0.017%
29	9.430	1021	1028	1035	rVV	225344	399780	26.57%	2.546%
30	9.571	1050	1052	1055	rVB	2465	2935	0.20%	0.019%
31	9.612	1055	1059	1060	rBV	3346	2878	0.19%	0.018%
32	9.747	1080	1082	1086	rBV2	1564	2278	0.15%	0.015%
33	9.953	1114	1117	1123	rVB	2567	5436	0.36%	0.035%
34	10.147	1143	1150	1157	rBV2	182957	311157	20.68%	1.981%
35	10.247	1162	1167	1168	rBV2	2257	2245	0.15%	0.014%
36	10.306	1176	1177	1180	rBV	2662	2383	0.16%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059230.D
 Acq On : 28 Sep 2023 12:14
 Operator : MA/JU
 Sample : PB155856BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK856

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

37	10.676	1232	1240	1248	rBV	270258	473555	31.48%	3.015%
38	11.075	1300	1308	1315	rBV	243535	434901	28.91%	2.769%
39	11.163	1321	1323	1325	rVB	2838	2266	0.15%	0.014%
40	11.216	1325	1332	1340	rBV	291987	546412	36.32%	3.479%
41	11.357	1354	1356	1360	rVB2	2334	2509	0.17%	0.016%
42	11.604	1395	1398	1400	rBV	2431	2814	0.19%	0.018%
43	11.633	1400	1403	1407	rVB	2345	3893	0.26%	0.025%
44	11.745	1421	1422	1427	rBV	2810	3051	0.20%	0.019%
45	12.203	1498	1500	1502	rBV	2529	2557	0.17%	0.016%
46	12.250	1506	1508	1511	rVV	2658	2578	0.17%	0.016%
47	12.626	1569	1572	1574	rBV2	3908	5266	0.35%	0.034%
48	12.697	1581	1584	1587	rVB2	2124	2760	0.18%	0.018%
49	12.820	1603	1605	1608	rBV	2200	2270	0.15%	0.014%
50	12.855	1608	1611	1613	rBV3	2263	2343	0.16%	0.015%
51	12.979	1630	1632	1634	rBV3	2763	2107	0.14%	0.013%
52	13.184	1664	1667	1671	rVB	1963	2378	0.16%	0.015%
53	13.572	1732	1733	1736	rVB	2681	2164	0.14%	0.014%
54	13.696	1749	1754	1759	rBV2	11095	15011	1.00%	0.096%
55	13.825	1775	1776	1780	rBV2	2088	2873	0.19%	0.018%
56	14.260	1843	1850	1856	rBV	527199	762453	50.68%	4.855%
57	14.348	1862	1865	1866	rBV	2301	2140	0.14%	0.014%
58	14.571	1895	1903	1913	rBV	605369	960387	63.83%	6.115%
59	14.865	1947	1953	1961	rVB	413311	629951	41.87%	4.011%
60	15.053	1976	1985	1994	rBV2	226495	383973	25.52%	2.445%
61	15.229	2013	2015	2018	rVB	2656	2488	0.17%	0.016%
62	15.364	2037	2038	2043	rBV2	1911	2724	0.18%	0.017%
63	15.511	2061	2063	2068	rBV	1917	3098	0.21%	0.020%
64	15.611	2078	2080	2082	rVB	2813	2348	0.16%	0.015%
65	15.852	2114	2121	2130	rVV	744785	1150965	76.50%	7.329%
66	15.964	2133	2140	2149	rBV	230195	354093	23.54%	2.255%
67	16.058	2153	2156	2158	rBV	3298	3841	0.26%	0.024%
68	16.087	2158	2161	2166	rVB4	4651	7495	0.50%	0.048%
69	16.134	2167	2169	2172	rVB	2405	2590	0.17%	0.016%
70	16.169	2172	2175	2176	rBV	2196	2593	0.17%	0.017%
71	16.316	2196	2200	2201	rBV2	1868	2392	0.16%	0.015%
72	16.504	2229	2232	2236	rVB2	1770	2117	0.14%	0.013%
73	16.651	2255	2257	2260	rVB	3438	2789	0.19%	0.018%
74	16.680	2260	2262	2265	rBV	2096	2536	0.17%	0.016%
75	17.156	2342	2343	2348	rVB	2794	3196	0.21%	0.020%
76	17.221	2352	2354	2357	rBV	2106	2185	0.15%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059230.D
 Acq On : 28 Sep 2023 12:14
 Operator : MA/JU
 Sample : PB155856BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK856

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

77	17.615	2414	2421	2429	rBV	533139	777789	51.70%	4.953%
78	17.714	2431	2438	2445	rBV2	833821	1263316	83.97%	8.044%
79	18.132	2505	2509	2513	rBV	2258	4275	0.28%	0.027%
80	18.326	2538	2542	2546	rVB2	2979	4618	0.31%	0.029%
81	18.455	2562	2564	2567	rVB2	3119	2379	0.16%	0.015%
82	18.525	2574	2576	2583	rBV3	3312	6401	0.43%	0.041%
83	18.831	2626	2628	2630	rVB2	4111	2502	0.17%	0.016%
84	18.913	2640	2642	2646	rBV3	3349	3993	0.27%	0.025%
85	18.954	2646	2649	2650	rVB2	3057	2822	0.19%	0.018%
86	18.984	2650	2654	2655	rBV2	2547	3021	0.20%	0.019%
87	19.154	2681	2683	2685	rBV	2538	2466	0.16%	0.016%
88	19.401	2724	2725	2728	rBV2	3003	2771	0.18%	0.018%
89	19.554	2746	2751	2755	rBV4	13049	17216	1.14%	0.110%
90	19.836	2797	2799	2803	rVB4	6941	7789	0.52%	0.050%
91	19.988	2819	2825	2834	rVB	1096057	1501321	99.79%	9.560%
92	20.047	2834	2835	2837	rBV2	5225	4399	0.29%	0.028%
93	20.159	2852	2854	2855	rBV2	5080	3823	0.25%	0.024%
94	20.423	2897	2899	2901	rBV3	4734	4073	0.27%	0.026%
95	20.447	2901	2903	2904	rBV2	4827	3649	0.24%	0.023%
96	21.463	3074	3076	3077	rVB2	8540	4631	0.31%	0.029%
97	21.915	3147	3153	3169	rVB	474643	833431	55.40%	5.307%
98	25.153	3694	3704	3719	rVB2	515939	1504488	100.00%	9.580%
99	25.400	3737	3746	3759	rVB2	296073	888742	59.07%	5.659%
100	32.585	4967	4969	4973	rBV5	8608	10670	0.71%	0.068%




Sum of corrected areas: 15704670

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059230.D
Acq On : 28 Sep 2023 12:14
Operator : MA/JU
Sample : PB155856BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK856

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

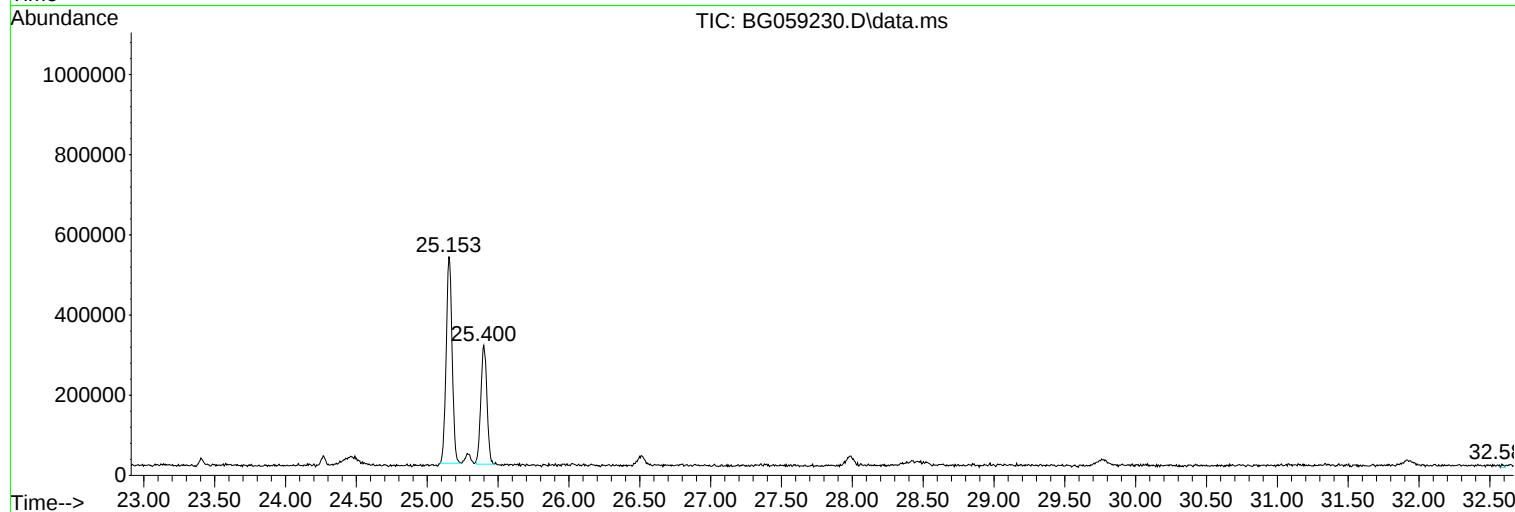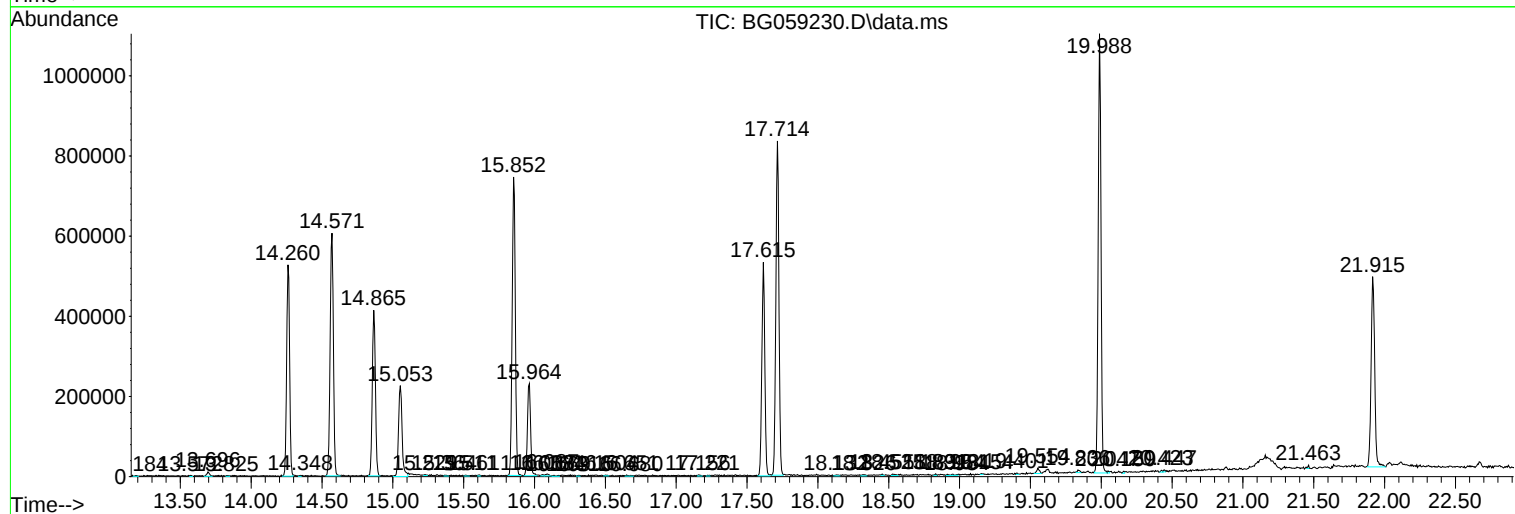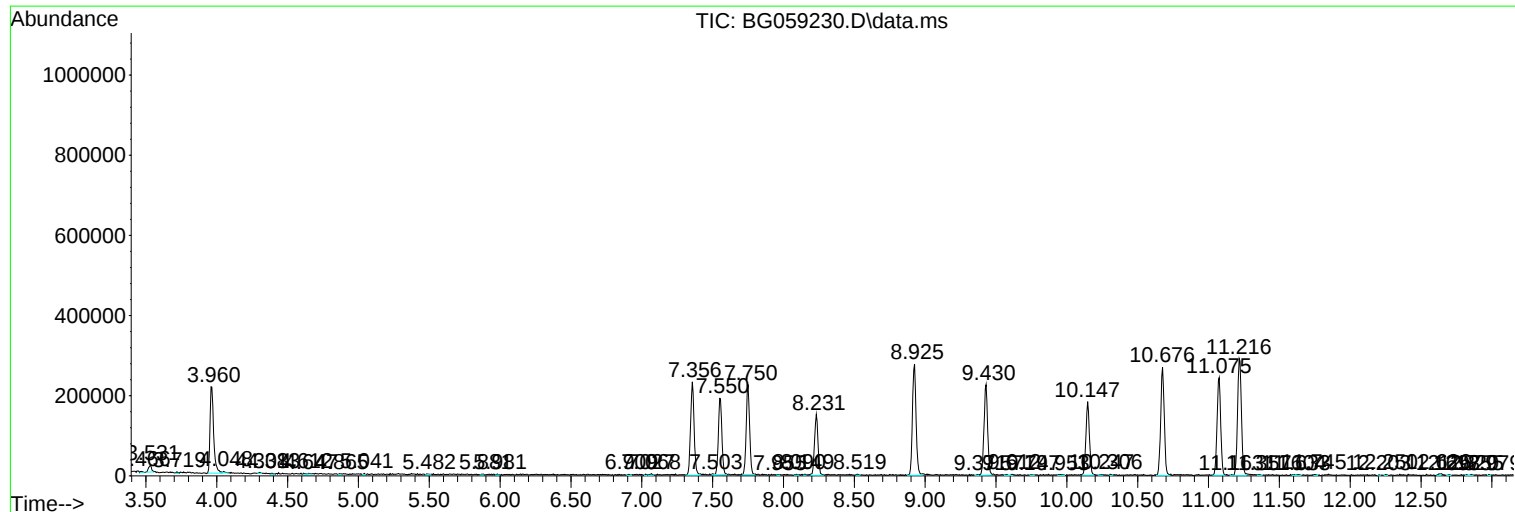

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059230.D
Acq On : 28 Sep 2023 12:14
Operator : MA/JU
Sample : PB155856BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK856

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059230.D
Acq On : 28 Sep 2023 12:14
Operator : MA/JU
Sample : PB155856BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK856

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc