

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059231.D
 Acq On : 28 Sep 2023 12:54
 Operator : MA/JU
 Sample : PB155590TB 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLEB590

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059231.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.529	20	24	30	rBV3	14750	25306	1.65%	0.154%
2	3.963	93	98	107	rBV	231311	386904	25.29%	2.354%
3	4.281	151	152	154	rBV2	2903	2410	0.16%	0.015%
4	4.986	269	272	275	rBV3	1907	2496	0.16%	0.015%
5	5.015	275	277	279	rBV	2416	2542	0.17%	0.015%
6	5.315	325	328	330	rBV	2251	2578	0.17%	0.016%
7	5.473	353	355	361	rVB3	2003	3164	0.21%	0.019%
8	5.520	361	363	366	rBV2	2283	3093	0.20%	0.019%
9	5.849	418	419	424	rBV3	2779	3749	0.25%	0.023%
10	5.996	441	444	447	rVB3	2014	2191	0.14%	0.013%
11	6.378	507	509	513	rBV2	2106	2641	0.17%	0.016%
12	6.443	518	520	525	rVB2	2237	2769	0.18%	0.017%
13	6.766	571	575	576	rVB	2250	2400	0.16%	0.015%
14	6.801	576	581	582	rBV3	2815	4514	0.30%	0.027%
15	6.860	588	591	593	rBV	2428	3176	0.21%	0.019%
16	6.936	599	604	607	rBV4	2450	4085	0.27%	0.025%
17	7.354	665	675	684	rBV	236025	415978	27.19%	2.531%
18	7.553	702	709	717	rBV	208165	339792	22.21%	2.068%
19	7.747	736	742	749	rBV	221397	376767	24.63%	2.293%
20	8.088	796	800	801	rBV2	2004	2838	0.19%	0.017%
21	8.229	817	824	834	rBV	164563	278663	18.22%	1.696%
22	8.922	935	942	954	rBV2	283767	493879	32.28%	3.005%
23	9.428	1021	1028	1036	rBV	237465	414953	27.12%	2.525%
24	9.616	1056	1060	1062	rVB	2646	3403	0.22%	0.021%
25	9.633	1062	1063	1067	rBV	2832	3031	0.20%	0.018%
26	9.780	1084	1088	1091	rBV	2408	3893	0.25%	0.024%
27	10.150	1142	1151	1159	rBV	180539	323362	21.14%	1.968%
28	10.397	1190	1193	1196	rVB	1860	2156	0.14%	0.013%
29	10.515	1209	1213	1218	rBV2	1998	4142	0.27%	0.025%
30	10.673	1233	1240	1249	rBV	278987	488810	31.95%	2.975%
31	11.073	1301	1308	1316	rVB	273451	484713	31.68%	2.950%
32	11.161	1321	1323	1325	rVB2	3457	2614	0.17%	0.016%
33	11.220	1325	1333	1343	rBV	302724	555244	36.29%	3.379%
34	11.760	1422	1425	1428	rBV	1930	2800	0.18%	0.017%
35	12.177	1493	1496	1498	rBV	1994	2186	0.14%	0.013%
36	12.283	1511	1514	1517	rBV2	2196	2688	0.18%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059231.D
 Acq On : 28 Sep 2023 12:54
 Operator : MA/JU
 Sample : PB155590TB 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLEB590

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

37	12.354	1524	1526	1529	rBV2	2447	2159	0.14%	0.013%
38	12.641	1570	1575	1579	rBV2	5617	9269	0.61%	0.056%
39	12.923	1621	1623	1626	rBV	2951	2325	0.15%	0.014%
40	13.194	1664	1669	1670	rBV	2001	2412	0.16%	0.015%

41	13.623	1741	1742	1745	rVB	2725	2257	0.15%	0.014%
42	13.699	1750	1755	1759	rBV	7647	10424	0.68%	0.063%
43	13.969	1798	1801	1804	rVB	2708	2631	0.17%	0.016%
44	14.069	1816	1818	1819	rBV	2544	2356	0.15%	0.014%
45	14.263	1845	1851	1859	rVB	563077	786405	51.40%	4.785%

46	14.381	1868	1871	1872	rVB	2856	2273	0.15%	0.014%
47	14.569	1895	1903	1910	rBV2	631147	992423	64.87%	6.039%
48	14.868	1947	1954	1961	rBV	453388	688782	45.02%	4.191%
49	14.945	1963	1967	1969	rBV	2952	2518	0.16%	0.015%
50	15.056	1978	1986	1992	rBV	234023	388687	25.41%	2.365%

51	15.403	2044	2045	2047	rBV	2929	2555	0.17%	0.016%
52	15.614	2077	2081	2085	rVB2	2875	2826	0.18%	0.017%
53	15.650	2085	2087	2090	rBV	2953	3055	0.20%	0.019%
54	15.791	2108	2111	2113	rBV	2638	2652	0.17%	0.016%
55	15.855	2115	2122	2130	rVV	822377	1202098	78.58%	7.315%

56	15.961	2134	2140	2152	rVV	254638	373419	24.41%	2.272%
57	16.061	2154	2157	2159	rBV	1714	2197	0.14%	0.013%
58	16.096	2159	2163	2169	rVB2	3240	6506	0.43%	0.040%
59	16.302	2195	2198	2199	rBV2	2658	2634	0.17%	0.016%
60	16.366	2207	2209	2211	rBV	2717	2325	0.15%	0.014%

61	16.419	2215	2218	2221	rVB	2054	3228	0.21%	0.020%
62	16.566	2240	2243	2245	rBV	1849	2174	0.14%	0.013%
63	16.737	2270	2272	2274	rBV2	2834	2357	0.15%	0.014%
64	17.025	2318	2321	2324	rBV	2102	2446	0.16%	0.015%
65	17.119	2333	2337	2338	rBV2	2574	2411	0.16%	0.015%

66	17.395	2381	2384	2387	rBV2	2616	2808	0.18%	0.017%
67	17.518	2401	2405	2407	rVB	3113	3568	0.23%	0.022%
68	17.612	2413	2421	2432	rBV	550288	844434	55.20%	5.139%
69	17.718	2432	2439	2451	rVV	874984	1330845	86.99%	8.099%
70	17.959	2477	2480	2481	rBV	1943	2266	0.15%	0.014%

71	17.994	2484	2486	2492	rVV2	2647	4865	0.32%	0.030%
72	18.047	2492	2495	2496	rVB	3238	2707	0.18%	0.016%
73	18.370	2548	2550	2552	rBV2	2841	2368	0.15%	0.014%
74	18.441	2558	2562	2565	rBV2	3112	4431	0.29%	0.027%
75	18.499	2568	2572	2574	rBV2	2056	3118	0.20%	0.019%

76	18.605	2588	2590	2592	rBV2	3130	2166	0.14%	0.013%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059231.D
 Acq On : 28 Sep 2023 12:54
 Operator : MA/JU
 Sample : PB155590TB 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLEB590

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

77	18.640	2595	2596	2600	rVB2	2465	2197	0.14%	0.013%
78	18.899	2638	2640	2642	rBV3	2914	2310	0.15%	0.014%
79	19.275	2702	2704	2709	rVB	1838	2857	0.19%	0.017%
80	19.322	2709	2712	2714	rBV3	4371	4626	0.30%	0.028%
81	19.381	2720	2722	2723	rBV	3215	2973	0.19%	0.018%
82	19.504	2742	2743	2746	rBV3	3102	3292	0.22%	0.020%
83	19.557	2748	2752	2756	rVB6	13691	18967	1.24%	0.115%
84	19.621	2758	2763	2768	rVB6	11602	23396	1.53%	0.142%
85	19.710	2776	2778	2781	rBV3	3543	3265	0.21%	0.020%
86	19.839	2797	2800	2805	rBV7	8119	11451	0.75%	0.070%
87	19.992	2820	2826	2833	rBV	1101109	1529831	100.00%	9.309%
88	20.168	2854	2856	2857	rBV	5079	2719	0.18%	0.017%
89	20.227	2864	2866	2867	rBV2	3359	2665	0.17%	0.016%
90	20.332	2882	2884	2885	rBV	3591	3744	0.24%	0.023%
91	20.362	2887	2889	2890	rBV2	3984	2793	0.18%	0.017%
92	20.462	2904	2906	2907	rBV2	5146	2853	0.19%	0.017%
93	21.919	3147	3154	3162	rBV	509467	858981	56.15%	5.227%
94	22.177	3196	3198	3199	rBV	7032	5030	0.33%	0.031%
95	25.156	3694	3705	3718	rBV2	540331	1529385	99.97%	9.307%
96	25.280	3724	3726	3733	rVB5	26267	51581	3.37%	0.314%
97	25.397	3737	3746	3756	rVB2	319889	937319	61.27%	5.704%
98	26.519	3929	3937	3939	rBV7	20542	51256	3.35%	0.312%
99	27.929	4175	4177	4178	rBV2	8225	5769	0.38%	0.035%
100	28.247	4229	4231	4234	rBV3	6798	6580	0.43%	0.040%




Sum of corrected areas: 16433150

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059231.D
Acq On : 28 Sep 2023 12:54
Operator : MA/JU
Sample : PB155590TB 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLEB590

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

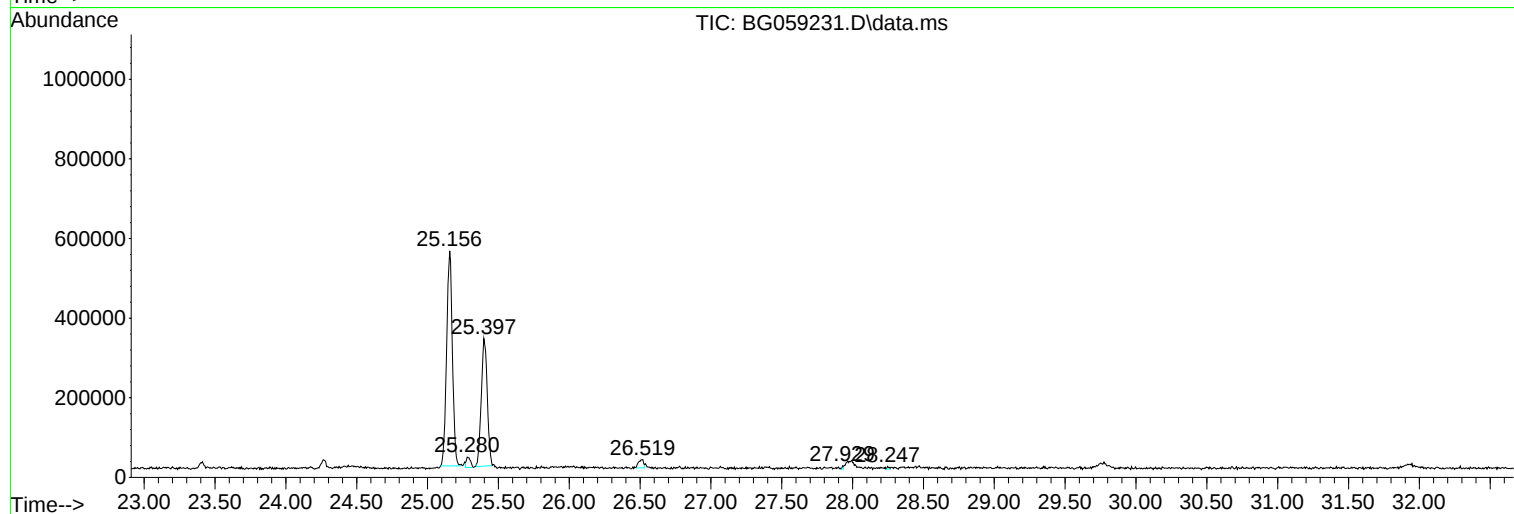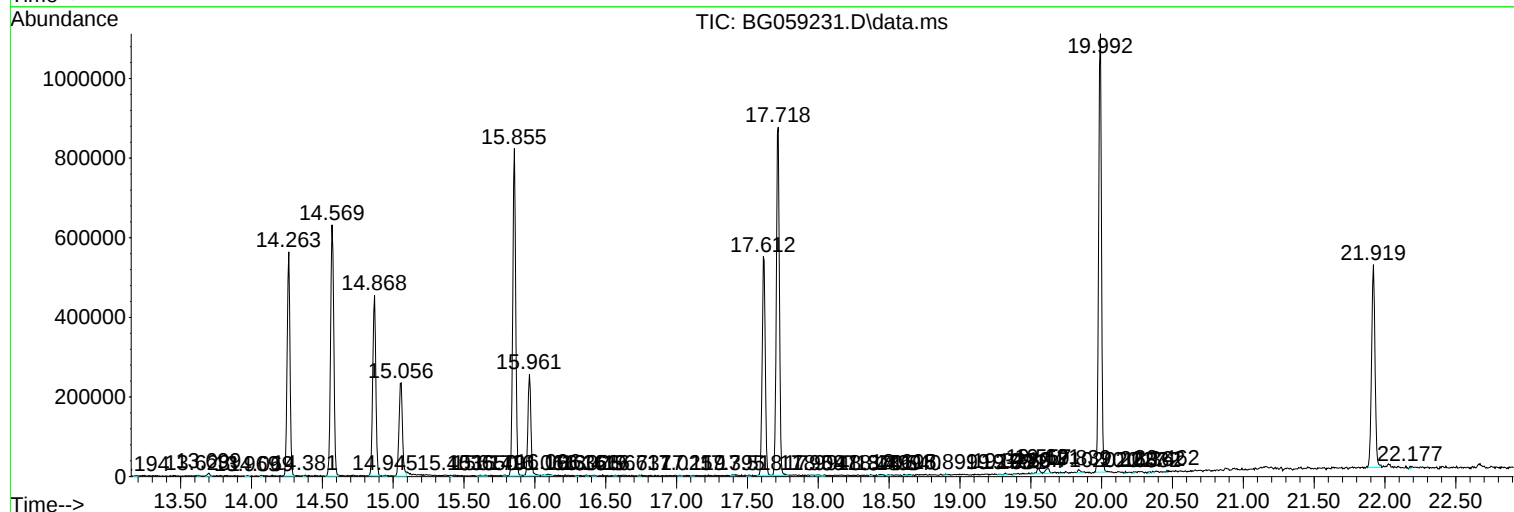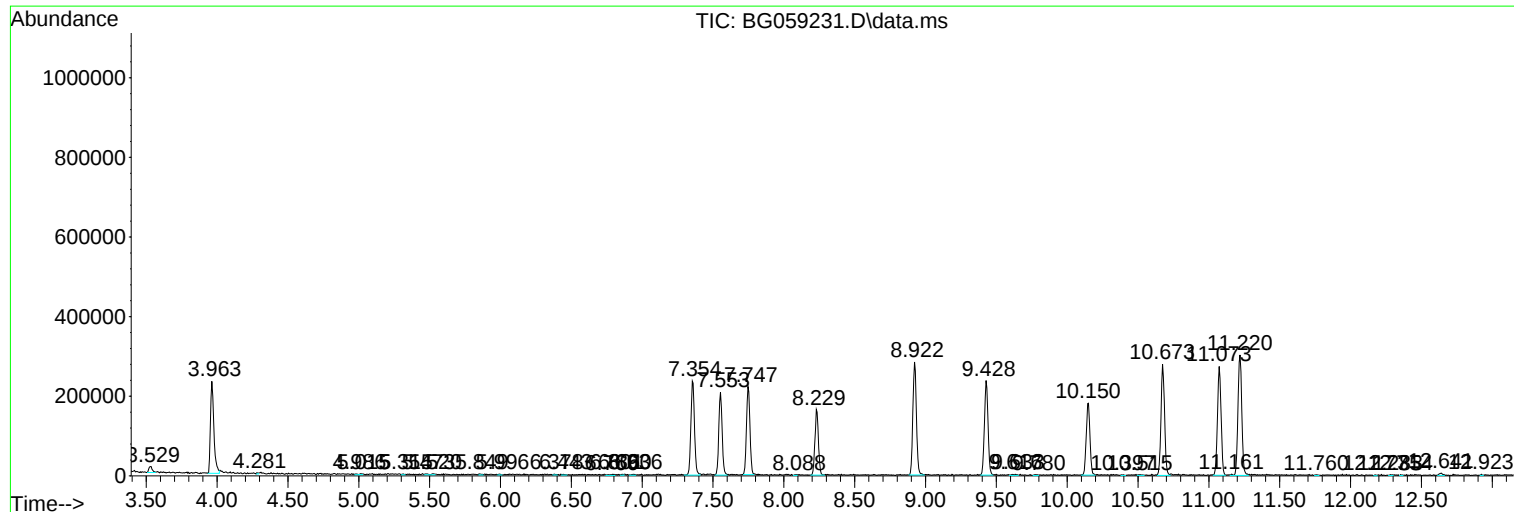

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059231.D
Acq On : 28 Sep 2023 12:54
Operator : MA/JU
Sample : PB155590TB 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLEB590

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059231.D
Acq On : 28 Sep 2023 12:54
Operator : MA/JU
Sample : PB155590TB 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLEB590

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc