

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059235.D
 Acq On : 28 Sep 2023 18:21
 Operator : MA/JU
 Sample : PB155817BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK817

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059239.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.461	11	12	15	rBV3	4142	3134	0.18%	0.018%
2	3.526	20	23	27	rVB2	14260	21765	1.22%	0.126%
3	3.961	93	97	109	rBV	236923	414238	23.14%	2.401%
4	4.260	146	148	153	rBV3	2157	3964	0.22%	0.023%
5	4.301	153	155	159	rVB3	3913	3647	0.20%	0.021%
6	4.713	223	225	227	rVB	4190	2796	0.16%	0.016%
7	5.929	431	432	435	rBV	3739	2789	0.16%	0.016%
8	6.052	450	453	456	rBV2	1696	2505	0.14%	0.015%
9	6.869	590	592	596	rVB2	2244	3039	0.17%	0.018%
10	6.916	596	600	601	rBV	2962	3239	0.18%	0.019%
11	7.057	621	624	626	rBV3	1519	2411	0.13%	0.014%
12	7.139	637	638	640	rBV	3072	2441	0.14%	0.014%
13	7.357	668	675	685	rBV	260466	438595	24.50%	2.542%
14	7.551	702	708	718	rVB	216243	349981	19.55%	2.029%
15	7.662	726	727	731	rBV2	2006	2420	0.14%	0.014%
16	7.750	735	742	750	rVV	235553	410909	22.96%	2.382%
17	8.044	791	792	799	rBV2	1917	2360	0.13%	0.014%
18	8.232	817	824	831	rBV	176105	305699	17.08%	1.772%
19	8.878	931	934	935	rBV	2867	2526	0.14%	0.015%
20	8.920	935	941	952	rVV	305244	530754	29.65%	3.076%
21	9.425	1020	1027	1037	rVB	244076	437742	24.46%	2.537%
22	9.901	1105	1108	1111	rBV	2413	3646	0.20%	0.021%
23	10.148	1143	1150	1157	rBV	194029	341000	19.05%	1.977%
24	10.324	1178	1180	1183	rVB2	2908	2556	0.14%	0.015%
25	10.430	1195	1198	1199	rBV2	2932	2478	0.14%	0.014%
26	10.676	1233	1240	1249	rVB2	274429	506595	28.30%	2.936%
27	10.735	1249	1250	1253	rBV	2753	2682	0.15%	0.016%
28	11.076	1300	1308	1316	rVB	264653	471988	26.37%	2.736%
29	11.217	1325	1332	1345	rBV	313632	578446	32.32%	3.353%
30	11.505	1380	1381	1387	rVB	2260	3631	0.20%	0.021%
31	11.757	1423	1424	1430	rVB	2257	2620	0.15%	0.015%
32	11.981	1460	1462	1466	rBV	1903	2962	0.17%	0.017%
33	12.039	1471	1472	1476	rVB	3029	3142	0.18%	0.018%
34	12.462	1541	1544	1546	rBV	2872	3220	0.18%	0.019%
35	12.633	1570	1573	1578	rVB2	4973	7582	0.42%	0.044%
36	13.103	1652	1653	1656	rBV	2209	2401	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059235.D
 Acq On : 28 Sep 2023 18:21
 Operator : MA/JU
 Sample : PB155817BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK817

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

37	13.309	1684	1688	1690	rVB	1859	2324	0.13%	0.013%
38	13.373	1698	1699	1705	rVB2	3089	3900	0.22%	0.023%
39	13.514	1718	1723	1726	rBV2	2203	4250	0.24%	0.025%
40	13.696	1748	1754	1759	rVB4	11996	20283	1.13%	0.118%
41	13.896	1785	1788	1793	rVB	1726	2845	0.16%	0.016%
42	14.178	1832	1836	1839	rBV	1606	2515	0.14%	0.015%
43	14.260	1844	1850	1857	rBV	581480	816439	45.61%	4.732%
44	14.390	1870	1872	1876	rBV	2026	3205	0.18%	0.019%
45	14.572	1895	1903	1909	rBV2	642004	1021962	57.10%	5.924%
46	14.683	1918	1922	1924	rBV	2515	2757	0.15%	0.016%
47	14.866	1946	1953	1963	rVB	440323	670124	37.44%	3.884%
48	15.054	1978	1985	1996	rBV	252642	427344	23.88%	2.477%
49	15.676	2088	2091	2093	rBV	2831	2593	0.14%	0.015%
50	15.712	2095	2097	2100	rVB	2239	2619	0.15%	0.015%
51	15.853	2114	2121	2128	rBV	853622	1239696	69.26%	7.186%
52	15.900	2128	2129	2134	rVV2	3603	4626	0.26%	0.027%
53	15.958	2134	2139	2149	rVV2	244172	368816	20.61%	2.138%
54	16.029	2149	2151	2154	rVB3	3086	3521	0.20%	0.020%
55	16.088	2155	2161	2165	rVB3	4572	6873	0.38%	0.040%
56	16.846	2288	2290	2293	rVB2	3368	3552	0.20%	0.021%
57	17.286	2362	2365	2367	rVB	3383	3752	0.21%	0.022%
58	17.310	2367	2369	2372	rBV2	3542	3343	0.19%	0.019%
59	17.433	2388	2390	2395	rVB2	2117	3451	0.19%	0.020%
60	17.615	2414	2421	2429	rBV	546049	813044	45.43%	4.713%
61	17.715	2431	2438	2447	rVV2	979814	1436507	80.26%	8.326%
62	17.980	2481	2483	2485	rBV	2775	2802	0.16%	0.016%
63	18.079	2497	2500	2504	rVB2	3092	3668	0.20%	0.021%
64	18.232	2522	2526	2529	rVB2	3494	4457	0.25%	0.026%
65	18.726	2608	2610	2611	rBV2	2925	2659	0.15%	0.015%
66	18.767	2614	2617	2619	rBV2	2260	2906	0.16%	0.017%
67	18.925	2643	2644	2648	rBV4	3113	4707	0.26%	0.027%
68	19.090	2670	2672	2675	rBV3	3034	3557	0.20%	0.021%
69	19.319	2709	2711	2716	rBV4	2514	4260	0.24%	0.025%
70	19.384	2720	2722	2724	rBV	3407	2584	0.14%	0.015%
71	19.548	2747	2750	2755	rVB5	14323	23409	1.31%	0.136%
72	19.619	2757	2762	2766	rBV3	12212	20843	1.16%	0.121%
73	19.783	2788	2790	2793	rBV3	3496	4308	0.24%	0.025%
74	19.989	2818	2825	2833	rBV	1208460	1686178	94.21%	9.774%
75	20.083	2839	2841	2842	rBV	4021	2799	0.16%	0.016%
76	20.341	2883	2885	2886	rBV	4122	2471	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059235.D
Acq On : 28 Sep 2023 18:21
Operator : MA/JU
Sample : PB155817BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK817

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Title : SVOA CALIBRATION

77	20.847	2969	2971	2974	rBV4	5239	7639	0.43%	0.044%
78	21.916	3146	3153	3160	rBV2	525557	888378	49.63%	5.149%
79	24.260	3549	3552	3561	rVB4	31081	63356	3.54%	0.367%
80	25.153	3693	3704	3718	rBV2	592076	1789849	100.00%	10.374%
81	25.400	3735	3746	3756	rVB	328623	979329	54.72%	5.676%




Sum of corrected areas: 17252403

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059235.D
Acq On : 28 Sep 2023 18:21
Operator : MA/JU
Sample : PB155817BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK817

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

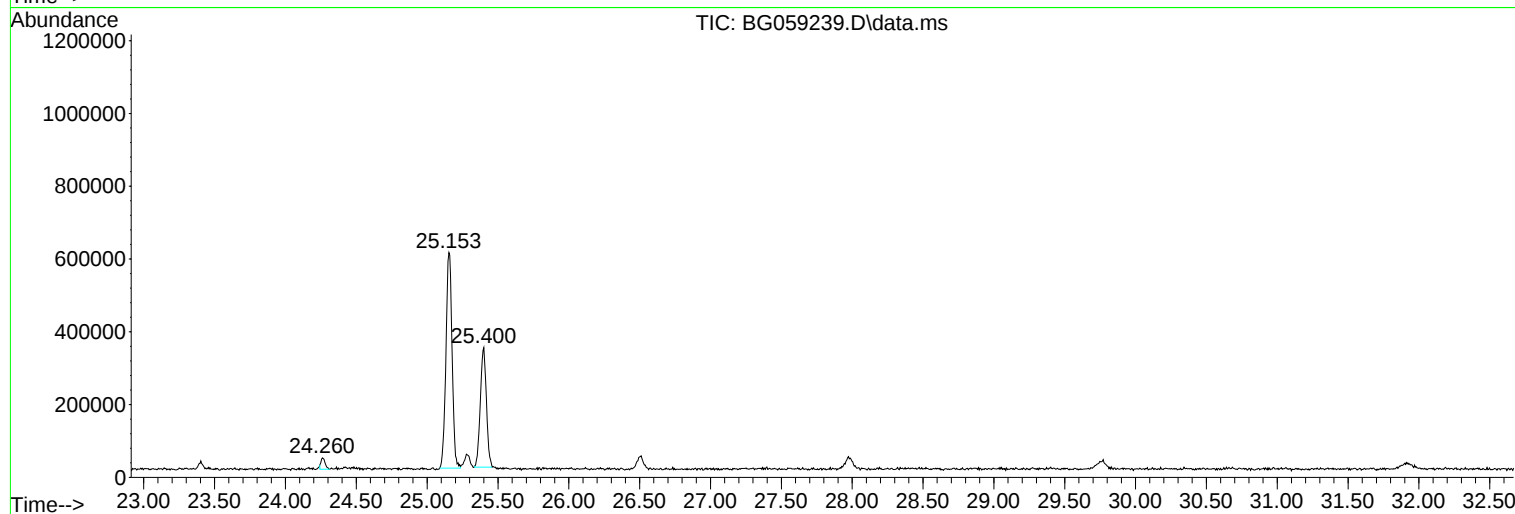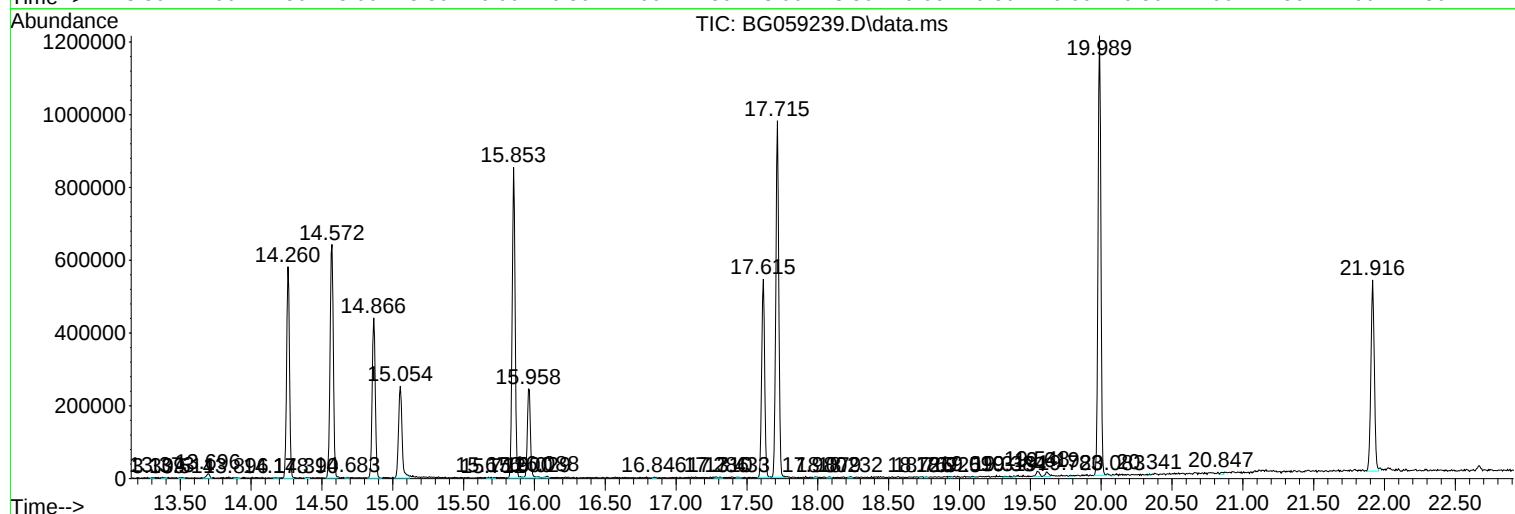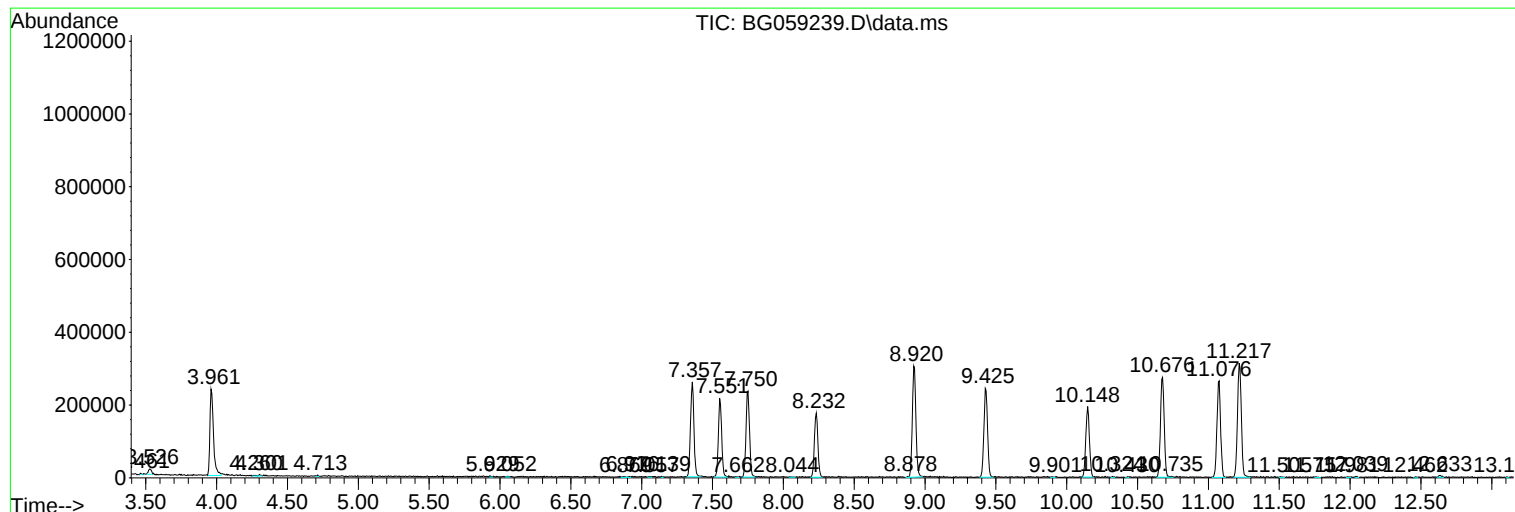

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059235.D
Acq On : 28 Sep 2023 18:21
Operator : MA/JU
Sample : PB155817BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK817

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059235.D
Acq On : 28 Sep 2023 18:21
Operator : MA/JU
Sample : PB155817BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK817

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------