

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059236.D
 Acq On : 28 Sep 2023 19:02
 Operator : MA/JU
 Sample : PB155820BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK820

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059240.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.531	19	24	29	rVB2	18503	30756	1.80%	0.183%
2	3.572	29	31	32	rBV2	3424	2796	0.16%	0.017%
3	3.619	37	39	43	rBV3	2837	3387	0.20%	0.020%
4	3.966	93	98	110	rBV	241916	418306	24.47%	2.496%
5	4.248	142	146	148	rVB3	4235	3134	0.18%	0.019%
6	4.301	154	155	159	rVB4	5396	4466	0.26%	0.027%
7	4.406	172	173	177	rBV3	2975	3447	0.20%	0.021%
8	4.959	265	267	269	rBV2	2102	2518	0.15%	0.015%
9	5.047	279	282	284	rVB3	2793	2716	0.16%	0.016%
10	5.111	291	293	296	rVB2	2721	2256	0.13%	0.013%
11	5.329	326	330	333	rVB3	2513	2816	0.16%	0.017%
12	6.028	446	449	451	rBV	2537	2365	0.14%	0.014%
13	6.187	475	476	479	rBV2	2705	3049	0.18%	0.018%
14	6.986	608	612	613	rBV2	3164	3782	0.22%	0.023%
15	7.356	668	675	685	rBV	251518	437271	25.58%	2.609%
16	7.556	702	709	720	rVB	209031	349083	20.42%	2.083%
17	7.750	733	742	749	rBV	234925	406305	23.77%	2.424%
18	7.943	773	775	778	rVB	3613	3526	0.21%	0.021%
19	8.126	803	806	809	rBV2	2133	2623	0.15%	0.016%
20	8.155	809	811	815	rVV2	2110	3032	0.18%	0.018%
21	8.231	817	824	830	rVV	163721	272971	15.97%	1.629%
22	8.696	900	903	906	rBV	2482	2541	0.15%	0.015%
23	8.766	912	915	917	rBV	2191	2249	0.13%	0.013%
24	8.925	932	942	951	rBV	298100	529014	30.95%	3.156%
25	9.001	953	955	960	rVB4	2588	4211	0.25%	0.025%
26	9.072	966	967	971	rVB2	2703	2601	0.15%	0.016%
27	9.430	1020	1028	1038	rBV	241940	425465	24.89%	2.538%
28	9.500	1038	1040	1043	rVB2	3141	3226	0.19%	0.019%
29	9.559	1047	1050	1052	rBV	2151	2288	0.13%	0.014%
30	10.147	1143	1150	1157	rBV2	191174	341961	20.00%	2.040%
31	10.211	1159	1161	1166	rVB2	3080	4266	0.25%	0.025%
32	10.587	1224	1225	1228	rBV	2172	2235	0.13%	0.013%
33	10.676	1233	1240	1250	rVV	290586	506491	29.63%	3.022%
34	10.858	1268	1271	1273	rBV	2388	2873	0.17%	0.017%
35	11.075	1300	1308	1317	rBV	252086	446200	26.10%	2.662%
36	11.216	1324	1332	1343	rBV	306052	571121	33.41%	3.407%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059236.D
 Acq On : 28 Sep 2023 19:02
 Operator : MA/JU
 Sample : PB155820BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK820

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

37	11.915	1449	1451	1454	rVB	2804	2309	0.14%	0.014%
38	12.327	1518	1521	1524	rBV	2484	2615	0.15%	0.016%
39	12.515	1550	1553	1556	rBV2	1894	2609	0.15%	0.016%
40	12.626	1570	1572	1579	rVB3	4785	8317	0.49%	0.050%

41	12.932	1619	1624	1627	rVB3	2501	4029	0.24%	0.024%
42	13.149	1658	1661	1665	rBV3	2323	3357	0.20%	0.020%
43	13.696	1750	1754	1758	rBV2	2952	4211	0.25%	0.025%
44	14.260	1844	1850	1857	rBV	565646	810378	47.40%	4.835%
45	14.571	1896	1903	1910	rBV	657424	1023153	59.85%	6.104%

46	14.677	1918	1921	1927	rVB2	2589	4404	0.26%	0.026%
47	14.724	1927	1929	1932	rBV	2864	2777	0.16%	0.017%
48	14.865	1947	1953	1961	rBV	382483	606374	35.47%	3.618%
49	15.053	1978	1985	1995	rBV	260855	427758	25.02%	2.552%
50	15.399	2041	2044	2045	rVB	2747	2257	0.13%	0.013%

51	15.493	2056	2060	2063	rBV	2579	3940	0.23%	0.024%
52	15.852	2115	2121	2131	rVB	836612	1250358	73.14%	7.460%
53	15.916	2131	2132	2134	rBV	3693	2426	0.14%	0.014%
54	15.958	2134	2139	2149	rBV	246368	377383	22.08%	2.251%
55	16.087	2157	2161	2166	rVB4	4945	8432	0.49%	0.050%

56	16.140	2169	2170	2173	rVB	3180	2873	0.17%	0.017%
57	16.198	2177	2180	2182	rBV2	3039	4603	0.27%	0.027%
58	16.475	2225	2227	2231	rVB2	2113	2439	0.14%	0.015%
59	16.616	2249	2251	2253	rBV2	2394	2570	0.15%	0.015%
60	16.768	2274	2277	2280	rVB2	3460	4032	0.24%	0.024%

61	16.815	2284	2285	2288	rVB2	2905	2388	0.14%	0.014%
62	16.892	2295	2298	2300	rVB2	2893	3070	0.18%	0.018%
63	17.356	2374	2377	2381	rVB3	2055	2559	0.15%	0.015%
64	17.397	2381	2384	2385	rBV	2736	3549	0.21%	0.021%
65	17.614	2414	2421	2430	rBV	488310	738784	43.22%	4.408%

66	17.714	2431	2438	2451	rVB2	938260	1409366	82.44%	8.408%
67	17.867	2463	2464	2467	rVB	2726	2338	0.14%	0.014%
68	18.049	2493	2495	2500	rBV2	3013	4308	0.25%	0.026%
69	18.196	2515	2520	2521	rVB3	2151	2402	0.14%	0.014%
70	18.220	2521	2524	2526	rBV2	2613	2730	0.16%	0.016%

71	18.284	2534	2535	2540	rVB2	2140	2709	0.16%	0.016%
72	18.372	2547	2550	2551	rBV	3018	2709	0.16%	0.016%
73	18.443	2558	2562	2563	rBV2	5096	4838	0.28%	0.029%
74	18.472	2565	2567	2570	rVB3	2770	2748	0.16%	0.016%
75	18.625	2591	2593	2594	rBV	3664	2438	0.14%	0.015%

76	18.801	2622	2623	2625	rBV2	3694	2346	0.14%	0.014%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059236.D
 Acq On : 28 Sep 2023 19:02
 Operator : MA/JU
 Sample : PB155820BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK820

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

77	19.124	2675	2678	2679	rBV2	2146	2456	0.14%	0.015%
78	19.336	2711	2714	2717	rBV2	2755	2751	0.16%	0.016%
79	19.465	2734	2736	2737	rBV	4418	2534	0.15%	0.015%
80	19.483	2737	2739	2740	rBV	3292	2588	0.15%	0.015%
81	19.500	2740	2742	2745	rVV	3707	3840	0.22%	0.023%
82	19.530	2745	2747	2748	rVV2	3087	2994	0.18%	0.018%
83	19.553	2748	2751	2756	rVV3	14142	21784	1.27%	0.130%
84	19.624	2759	2763	2768	rVB2	12272	20370	1.19%	0.122%
85	19.871	2803	2805	2807	rBV3	3175	3521	0.21%	0.021%
86	19.988	2818	2825	2833	rBV	1166255	1662375	97.24%	9.918%
87	20.047	2833	2835	2838	rVB2	6290	4923	0.29%	0.029%
88	20.258	2870	2871	2876	rBV3	3687	4617	0.27%	0.028%
89	20.370	2888	2890	2891	rBV	4002	2314	0.14%	0.014%
90	20.535	2915	2918	2921	rBV4	6424	9239	0.54%	0.055%
91	21.915	3146	3153	3165	rBV	467223	817127	47.80%	4.875%
92	22.820	3306	3307	3308	rBV	7579	3372	0.20%	0.020%
93	23.273	3379	3384	3385	rBV4	17644	23162	1.35%	0.138%
94	25.153	3694	3704	3717	rVB3	578544	1709514	100.00%	10.199%
95	25.399	3736	3746	3758	rVB2	299900	901927	52.76%	5.381%



Sum of corrected areas: 16761641

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059236.D
Acq On : 28 Sep 2023 19:02
Operator : MA/JU
Sample : PB155820BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK820

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

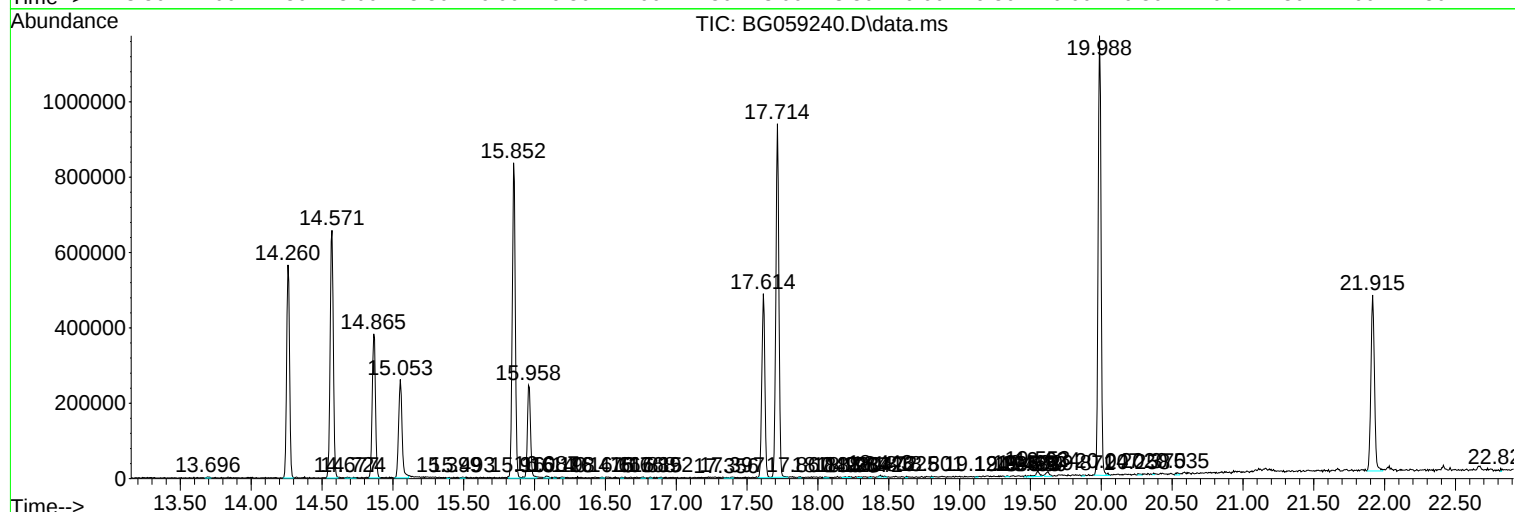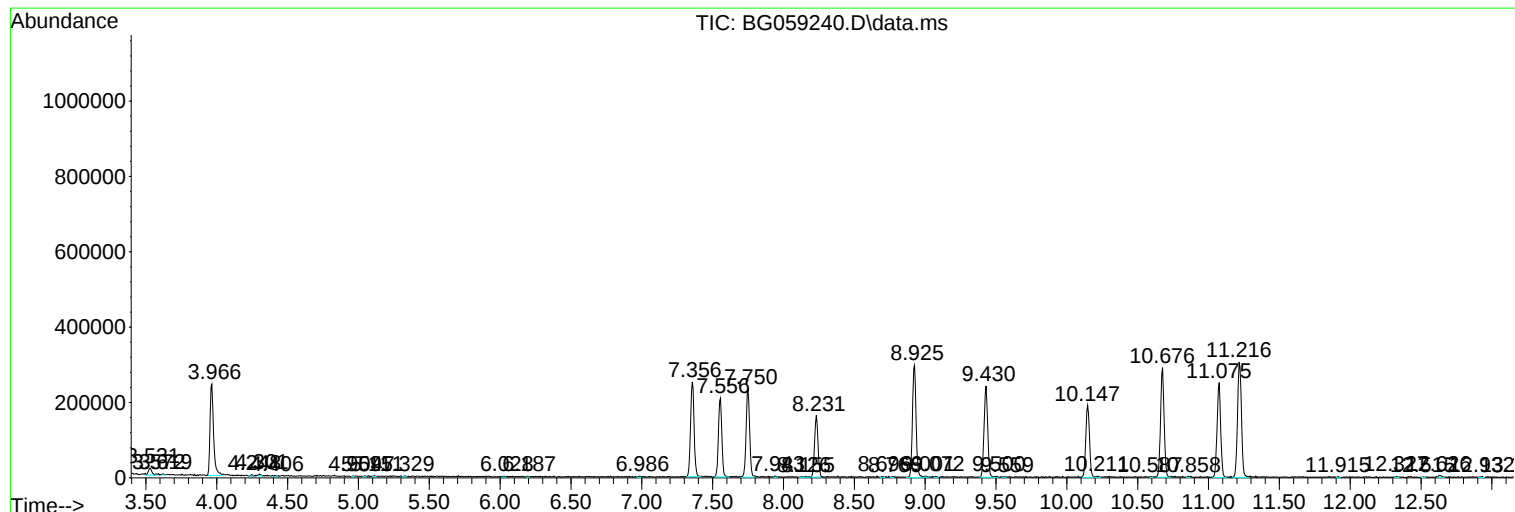

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059236.D
Acq On : 28 Sep 2023 19:02
Operator : MA/JU
Sample : PB155820BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK820

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059236.D
Acq On : 28 Sep 2023 19:02
Operator : MA/JU
Sample : PB155820BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK820

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc