

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059241.D
 Acq On : 29 Sep 2023 5:52
 Operator : MA/JU
 Sample : PB155826BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK826

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059255.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.531	19	24	28	rBV4	16171	24487	1.50%	0.156%
2	3.960	92	97	107	rBV	221474	370910	22.77%	2.365%
3	4.325	157	159	164	rVB4	3379	3738	0.23%	0.024%
4	4.753	230	232	234	rBV	2952	2494	0.15%	0.016%
5	4.865	247	251	252	rBV	3044	3155	0.19%	0.020%
6	5.300	324	325	329	rVB2	2537	2451	0.15%	0.016%
7	5.412	342	344	347	rVB2	2650	2375	0.15%	0.015%
8	5.964	435	438	441	rVB2	3073	3645	0.22%	0.023%
9	5.999	441	444	447	rBV3	2798	2906	0.18%	0.019%
10	6.587	540	544	546	rBV	2570	3617	0.22%	0.023%
11	6.916	598	600	604	rVB3	2259	2392	0.15%	0.015%
12	6.992	611	613	615	rBV2	3226	2451	0.15%	0.016%
13	7.356	668	675	686	rVB	251543	424741	26.07%	2.708%
14	7.550	701	708	717	rBV	204636	337705	20.73%	2.153%
15	7.627	720	721	724	rBV2	2605	2511	0.15%	0.016%
16	7.744	735	741	753	rVB	221805	391867	24.05%	2.498%
17	8.144	806	809	810	rBV	3052	2912	0.18%	0.019%
18	8.161	810	812	816	rVB3	2380	2986	0.18%	0.019%
19	8.232	816	824	832	rBV	150012	261939	16.08%	1.670%
20	8.543	871	877	878	rBV	2514	2455	0.15%	0.016%
21	8.584	881	884	888	rBV	2139	2420	0.15%	0.015%
22	8.708	902	905	908	rVB2	2292	2573	0.16%	0.016%
23	8.925	933	942	954	rBV	295823	510517	31.34%	3.255%
24	9.189	984	987	990	rVB2	2718	2648	0.16%	0.017%
25	9.430	1020	1028	1034	rBV	231185	406546	24.95%	2.592%
26	9.783	1086	1088	1091	rVB3	2960	2440	0.15%	0.016%
27	10.147	1143	1150	1159	rBV	184643	329830	20.24%	2.103%
28	10.482	1203	1207	1210	rVB2	2425	3549	0.22%	0.023%
29	10.517	1210	1213	1215	rBV2	2930	3190	0.20%	0.020%
30	10.676	1233	1240	1249	rBV	282222	504805	30.98%	3.219%
31	10.770	1255	1256	1260	rVB2	2533	2369	0.15%	0.015%
32	10.888	1274	1276	1280	rBV	1703	2561	0.16%	0.016%
33	10.952	1285	1287	1291	rVB2	2208	3204	0.20%	0.020%
34	10.993	1291	1294	1296	rBV2	2742	3259	0.20%	0.021%
35	11.076	1296	1308	1314	rBV	214821	385986	23.69%	2.461%
36	11.217	1323	1332	1344	rBV	290926	547394	33.60%	3.490%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059241.D
 Acq On : 29 Sep 2023 5:52
 Operator : MA/JU
 Sample : PB155826BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK826

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

37	11.311	1344	1348	1349	rBV	2346	2836	0.17%	0.018%
38	12.198	1496	1499	1504	rVB	1680	2519	0.15%	0.016%
39	12.638	1569	1574	1581	rVB3	5039	9657	0.59%	0.062%
40	13.249	1674	1678	1680	rVB3	3042	2987	0.18%	0.019%
41	13.625	1739	1742	1744	rBV	1980	2692	0.17%	0.017%
42	13.690	1748	1753	1761	rBV5	8564	16849	1.03%	0.107%
43	13.825	1773	1776	1780	rVB3	1692	2627	0.16%	0.017%
44	13.954	1795	1798	1800	rBV	2112	2349	0.14%	0.015%
45	14.260	1843	1850	1858	rVB	566882	776566	47.67%	4.951%
46	14.325	1858	1861	1866	rVB	2583	3740	0.23%	0.024%
47	14.566	1896	1902	1910	rBV	594571	940852	57.75%	5.999%
48	14.789	1938	1940	1942	rBV	2762	2605	0.16%	0.017%
49	14.865	1946	1953	1960	rVV	365522	553341	33.96%	3.528%
50	14.918	1960	1962	1969	rVB	2098	3072	0.19%	0.020%
51	15.053	1975	1985	1993	rBV2	249076	394325	24.20%	2.514%
52	15.153	2001	2002	2007	rVV5	2706	2545	0.16%	0.016%
53	15.212	2010	2012	2017	rBV3	1594	2386	0.15%	0.015%
54	15.852	2114	2121	2129	rBV	764594	1170519	71.85%	7.463%
55	15.958	2133	2139	2150	rVB	206479	325236	19.96%	2.074%
56	16.029	2150	2151	2156	rBV2	2958	3163	0.19%	0.020%
57	16.093	2161	2162	2166	rVB2	5367	3678	0.23%	0.023%
58	16.134	2166	2169	2172	rBV2	2424	3196	0.20%	0.020%
59	16.252	2187	2189	2193	rVB3	2442	2933	0.18%	0.019%
60	16.287	2193	2195	2198	rBV	2179	2892	0.18%	0.018%
61	16.804	2281	2283	2286	rVB2	2861	2927	0.18%	0.019%
62	16.851	2286	2291	2294	rBV	3758	4417	0.27%	0.028%
63	16.886	2294	2297	2299	rBV	2171	2817	0.17%	0.018%
64	17.080	2327	2330	2331	rBV	2451	2381	0.15%	0.015%
65	17.245	2355	2358	2360	rBV2	2204	2351	0.14%	0.015%
66	17.286	2362	2365	2366	rVB	2514	2439	0.15%	0.016%
67	17.615	2415	2421	2428	rBV	458273	668980	41.06%	4.265%
68	17.715	2431	2438	2446	rBV	925999	1351429	82.95%	8.616%
69	17.885	2464	2467	2470	rVB2	1797	2493	0.15%	0.016%
70	17.979	2480	2483	2484	rBV	2424	2763	0.17%	0.018%
71	18.091	2499	2502	2505	rVB	2059	2637	0.16%	0.017%
72	18.120	2505	2507	2510	rBV	2133	3012	0.18%	0.019%
73	18.338	2539	2544	2545	rBV3	1559	2372	0.15%	0.015%
74	18.543	2576	2579	2580	rBV2	3091	2456	0.15%	0.016%
75	18.631	2593	2594	2598	rVB	4015	3436	0.21%	0.022%
76	18.819	2624	2626	2630	rBV3	2358	3534	0.22%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
 Data File : BG059241.D
 Acq On : 29 Sep 2023 5:52
 Operator : MA/JU
 Sample : PB155826BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK826

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

77	19.060	2661	2667	2668	rBV3	2952	4066	0.25%	0.026%
78	19.143	2679	2681	2684	rBV3	2999	3705	0.23%	0.024%
79	19.260	2698	2701	2702	rBV3	2963	2775	0.17%	0.018%
80	19.554	2746	2751	2755	rBV4	12469	18807	1.15%	0.120%
81	19.618	2758	2762	2770	rVB3	11745	22289	1.37%	0.142%
82	19.671	2770	2771	2776	rBV2	3273	4304	0.26%	0.027%
83	19.742	2782	2783	2785	rVB2	3679	2588	0.16%	0.017%
84	19.771	2785	2788	2790	rBV4	2964	3260	0.20%	0.021%
85	19.806	2790	2794	2796	rBV4	2791	4989	0.31%	0.032%
86	19.836	2798	2799	2801	rVB2	5106	2474	0.15%	0.016%
87	19.924	2811	2814	2815	rBV2	3236	3670	0.23%	0.023%
88	19.989	2819	2825	2831	rBV	1134269	1580206	96.99%	10.075%
89	20.153	2851	2853	2854	rBV2	5331	3114	0.19%	0.020%
90	20.218	2862	2864	2867	rVB3	3875	3362	0.21%	0.021%
91	20.359	2886	2888	2890	rBV2	4107	2448	0.15%	0.016%
92	20.811	2963	2965	2966	rBV2	4422	3396	0.21%	0.022%
93	21.916	3146	3153	3164	rVB	431196	719619	44.17%	4.588%
94	22.274	3212	3214	3215	rBV	6327	3288	0.20%	0.021%
95	22.292	3215	3217	3218	rBV2	5390	2589	0.16%	0.017%
96	22.662	3278	3280	3285	rVB5	9803	9603	0.59%	0.061%
97	25.153	3694	3704	3718	rVB2	555934	1629204	100.00%	10.387%
98	25.400	3736	3746	3756	rVB2	263291	785901	48.24%	5.011%
99	26.710	3967	3969	3971	rBV3	6419	6288	0.39%	0.040%
100	29.519	4445	4447	4448	rVB2	6330	3410	0.21%	0.022%




Sum of corrected areas: 15684392

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059241.D
Acq On : 29 Sep 2023 5:52
Operator : MA/JU
Sample : PB155826BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK826

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

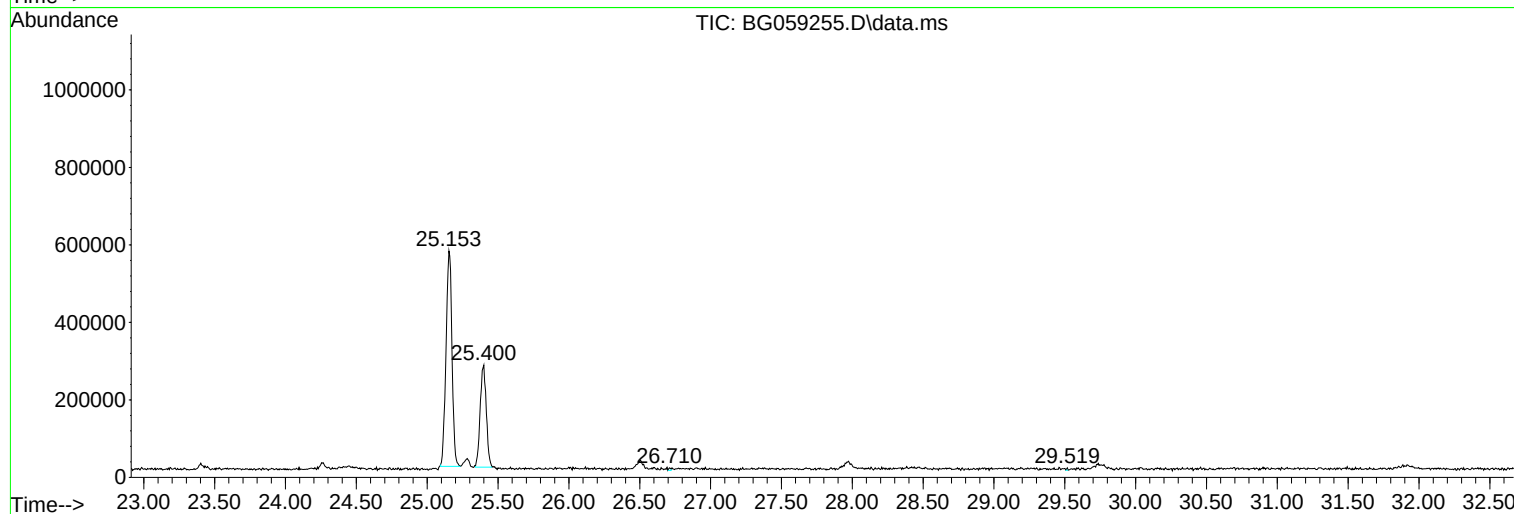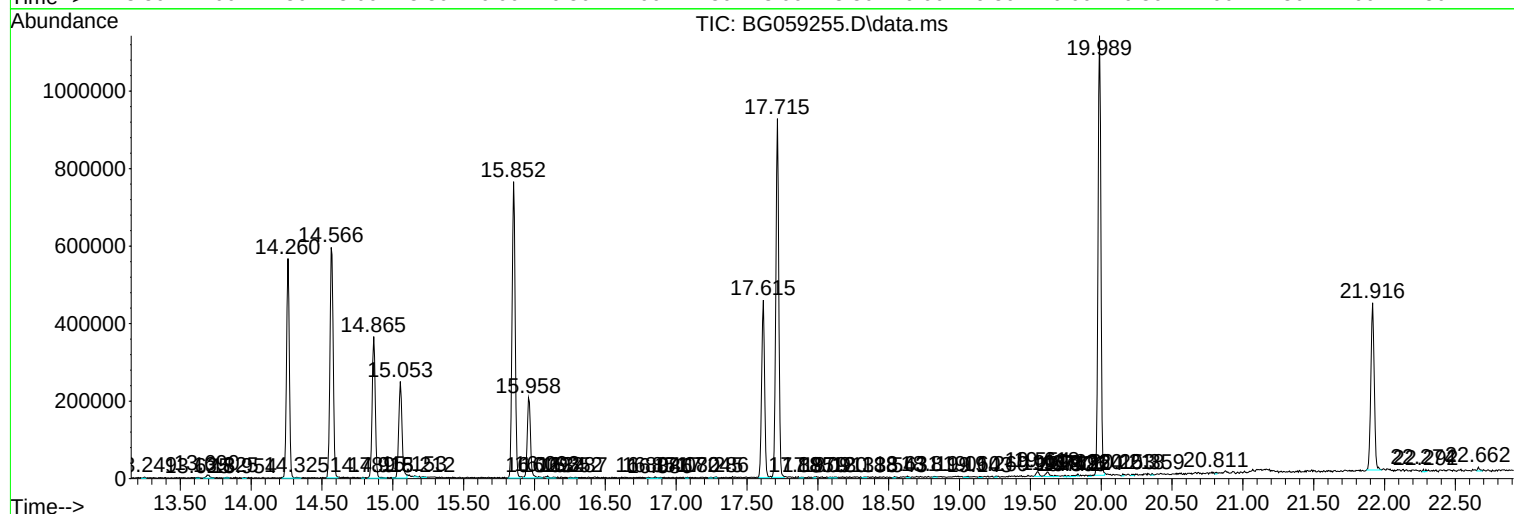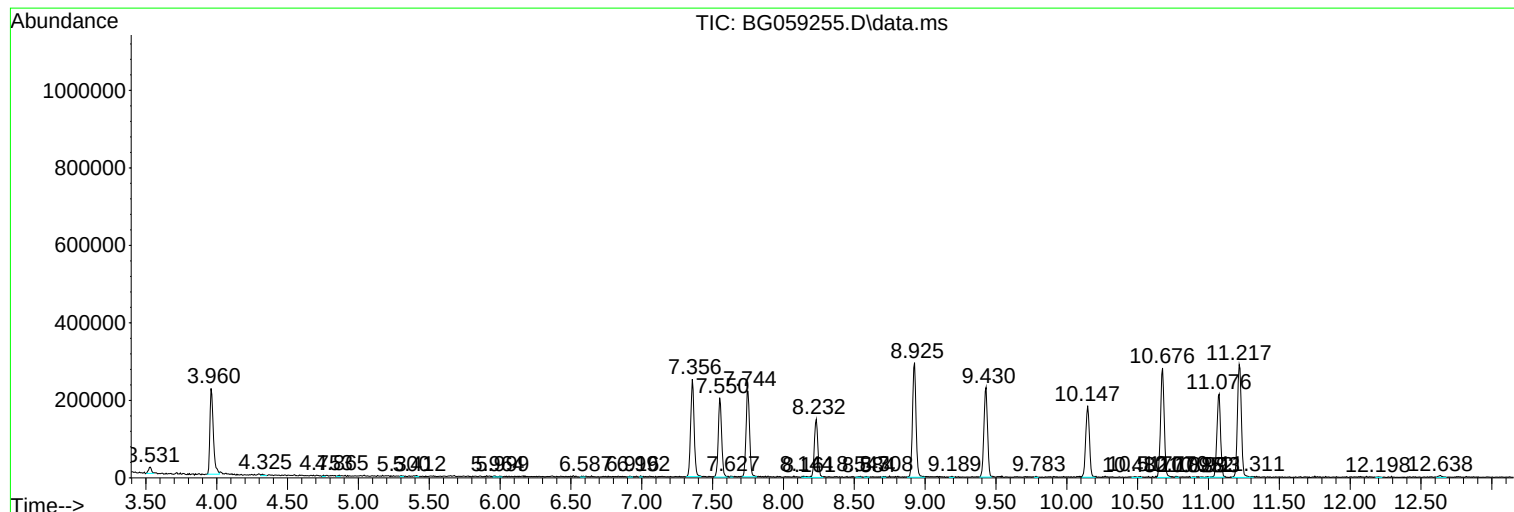

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059241.D
Acq On : 29 Sep 2023 5:52
Operator : MA/JU
Sample : PB155826BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK826

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092823\
Data File : BG059241.D
Acq On : 29 Sep 2023 5:52
Operator : MA/JU
Sample : PB155826BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK826

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc