

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG093019\
 Data File : BG042946.D
 Acq On : 30 Sep 2019 17:01
 Operator : JU
 Sample : K5083-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 20190706-RR-COMP-6

Quant Time: Oct 01 07:42:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 25 15:35:52 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	68700	20.00	ng	0.00
21) Naphthalene-d8	10.88	136	254227	20.00	ng	0.00
39) Acenaphthene-d10	14.69	164	175349	20.00	ng	0.00
64) Phenanthrene-d10	17.43	188	421868	20.00	ng	0.00
76) Chrysene-d12	21.70	240	475521	20.00	ng	-0.01
87) Perylene-d12	24.92	264	546311	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	433931	112.72	ng	0.00
7) Phenol-d6	7.24	99	633426	114.26	ng	0.00
23) Nitrobenzene-d5	9.23	82	401011	76.67	ng	0.00
42) 2,4,6-Tribromophenol	16.18	330	338488	112.26	ng	0.00
45) 2-Fluorobiphenyl	13.32	172	943290	77.99	ng	0.00
79) Terphenyl-d14	20.04	244	1700192	76.19	ng	0.00
Target Compounds						
10) Phenol	7.27	94	18921	3.720	ng	96
50) Dimethylphthalate	14.14	163	104567	7.959	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG093019\
Data File : BG042946.D
Acq On : 30 Sep 2019 17:01
Operator : JU
Sample : K5083-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20190706-RR-COMP-6

Quant Time: Oct 01 07:42:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 25 15:35:52 2019
Response via : Initial Calibration

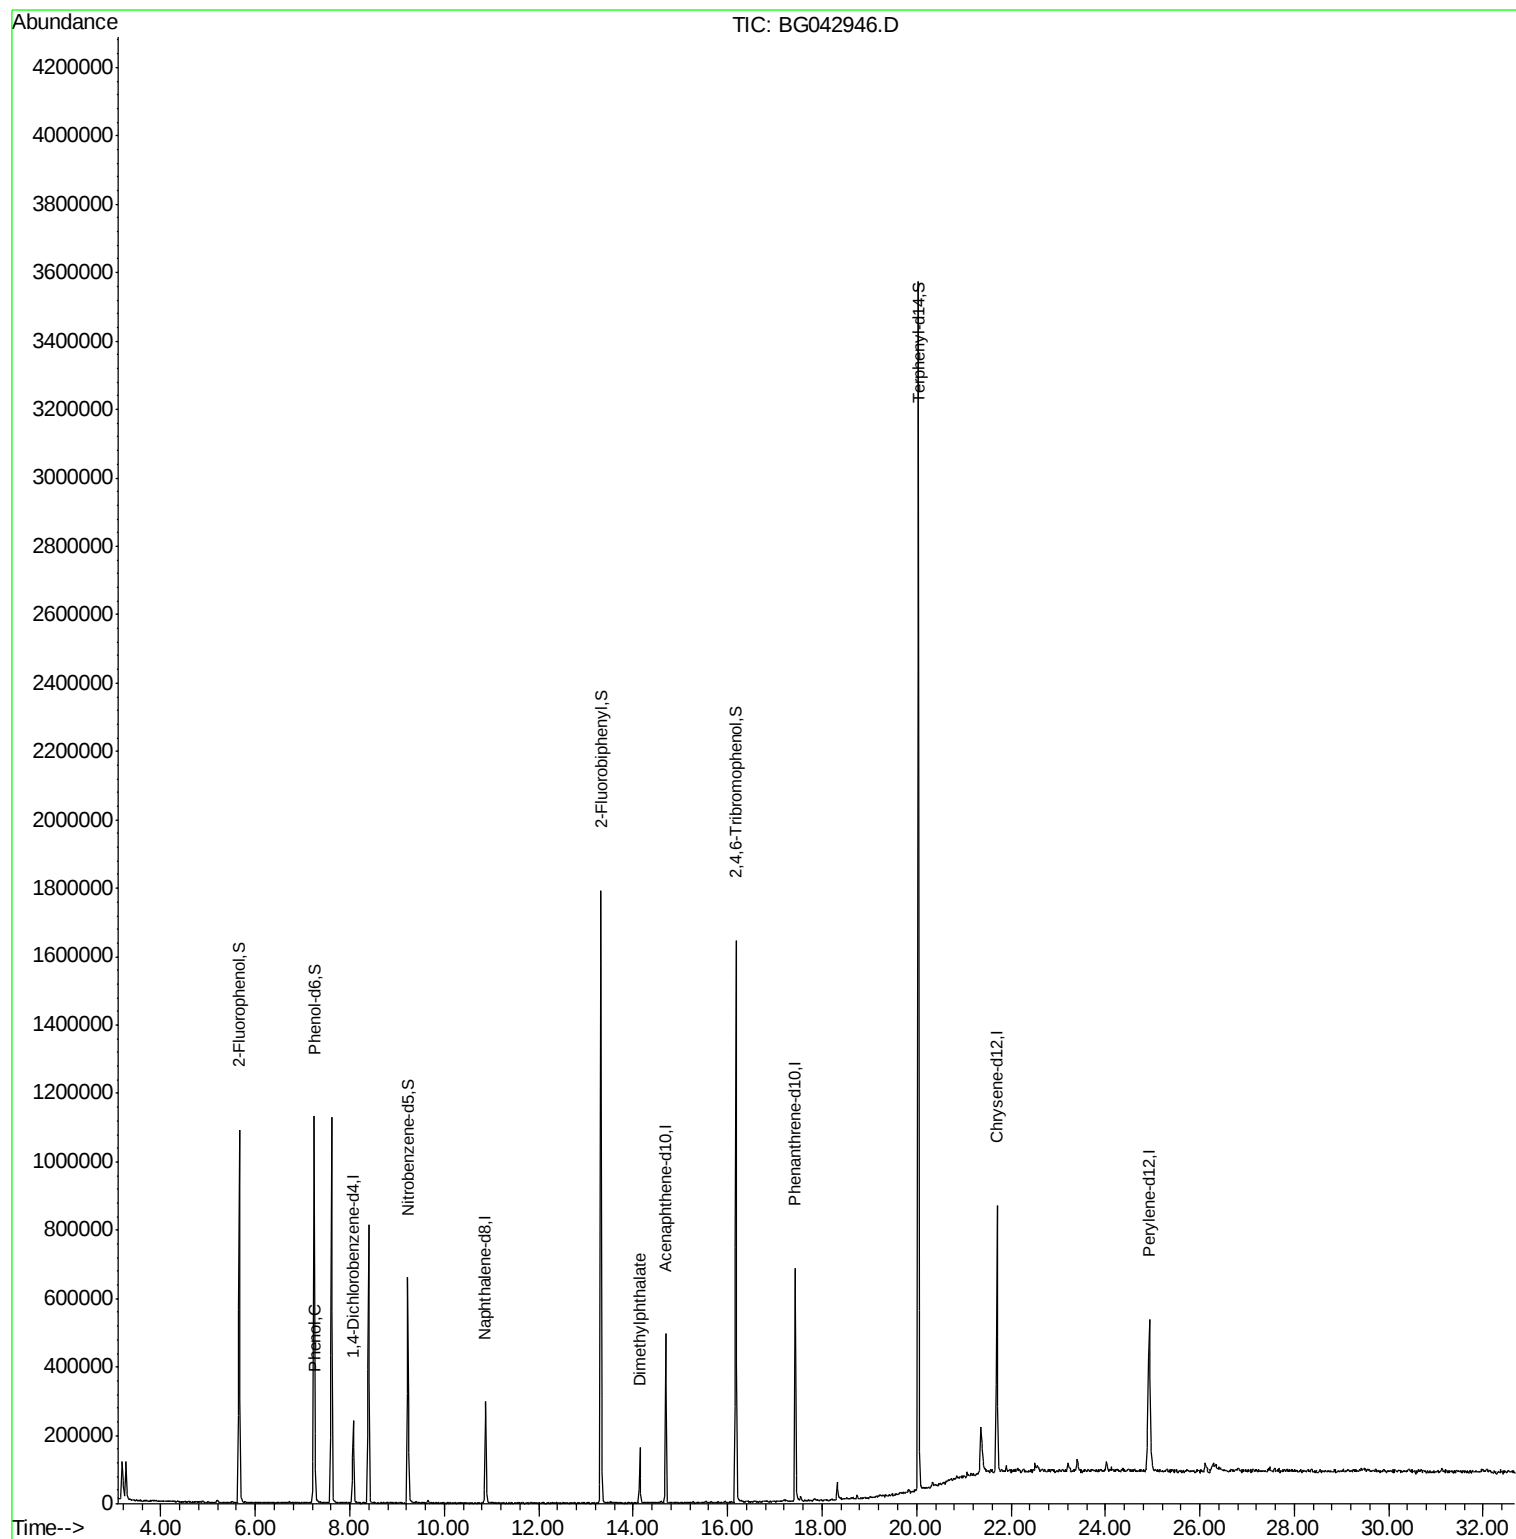

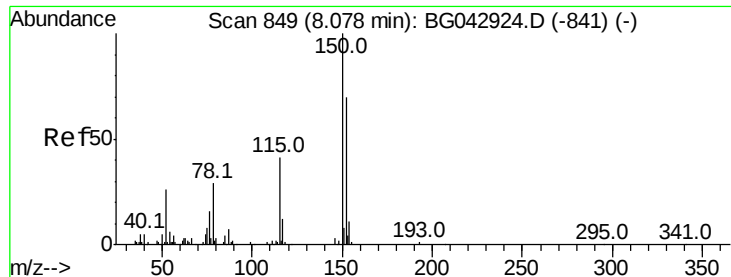


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.07 min Scan# 848
 Delta R.T. -0.01 min
 Lab File: BG042946.D
 Acq: 30 Sep 2019 17:01

Instrument :
 BNA_G
 ClientSampleId :
 20190706-RR-COMP-6

Tot Ion	Ratio	Lower	Upper
152	100		
150	150.6	115.0	172.4
115	58.5	47.0	70.6



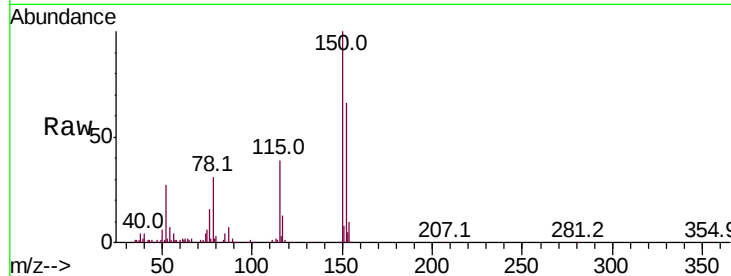


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

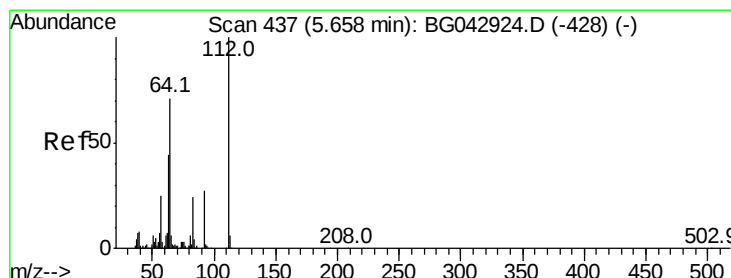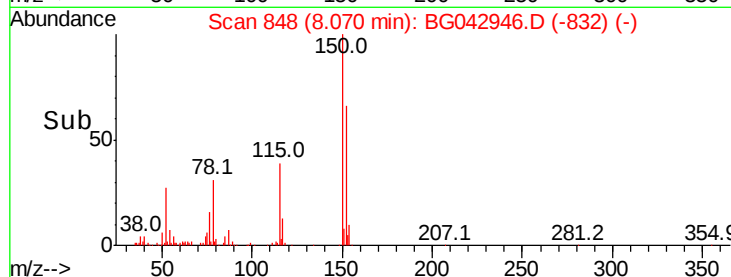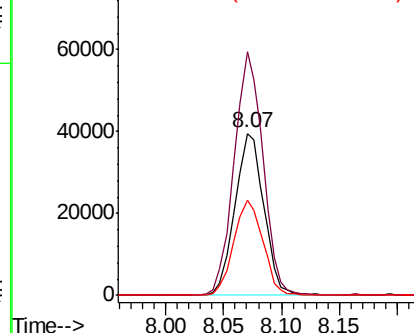

#5

2-Fluorophenol
 Concen: 112.722 ng
 RT: 5.66 min Scan# 437
 Delta R.T. -0.00 min
 Lab File: BG042946.D
 Acq: 30 Sep 2019 17:01

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.8	56.6	84.8
63	41.2	35.1	52.7


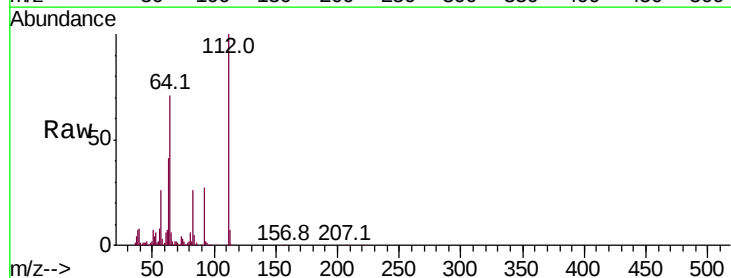



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

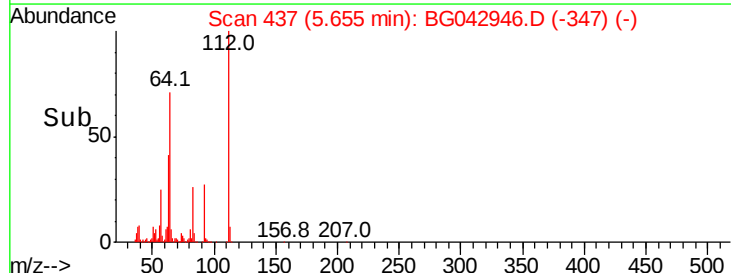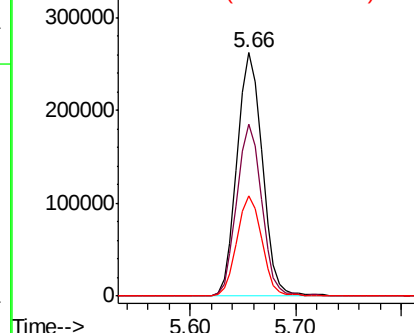

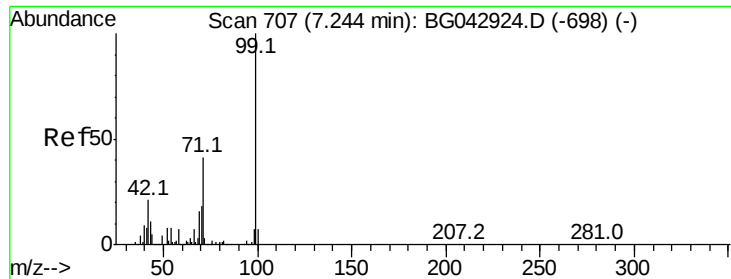

#7

Phenol-d6

Concen: 114.263 ng

RT: 7.24 min Scan# 707

Delta R.T. -0.00 min

Lab File: BG042946.D

Acq: 30 Sep 2019 17:01

Instrument :

BNA_G

ClientSampleId :

20190706-RR-COMP-6


Tot Ion: 99 Resp: 633426

Ion Ratio Lower Upper




99 100

42 21.8 17.2 25.8

71 43.8 33.1 49.7

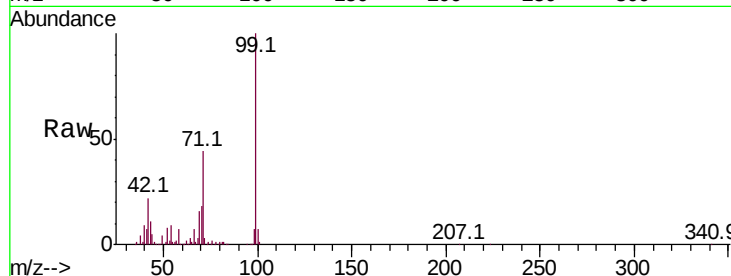

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

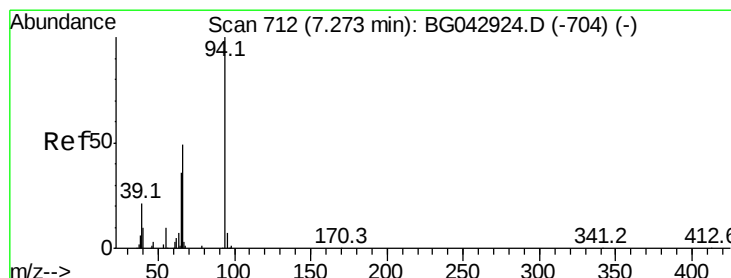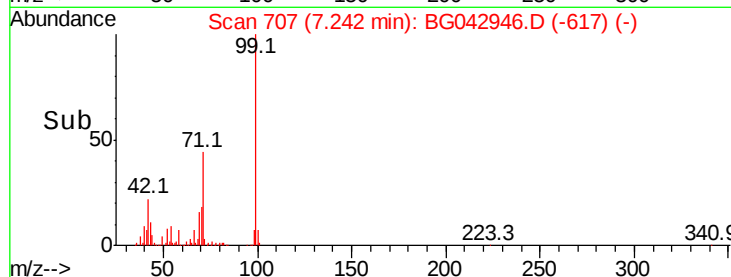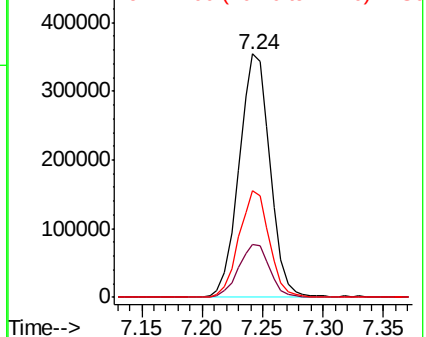

#10

Phenol

Concen: 3.720 ng

RT: 7.27 min Scan# 712

Delta R.T. -0.00 min

Lab File: BG042946.D

Acq: 30 Sep 2019 17:01


Tgt Ion: 94 Resp: 18921

Ion Ratio Lower Upper



94 100


65 40.8 16.6 56.6

66 54.2 32.4 72.4

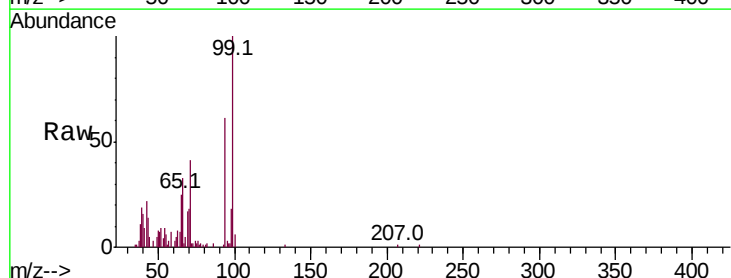

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC



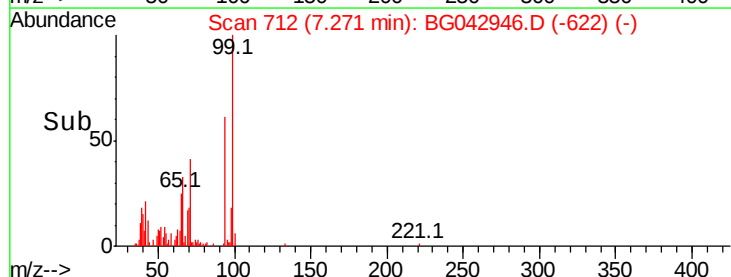
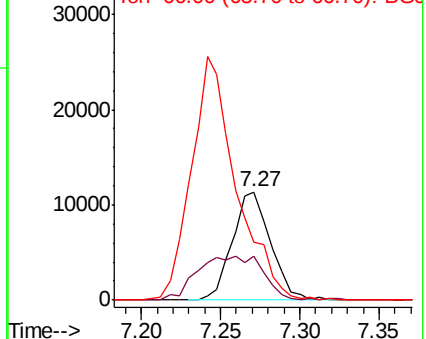


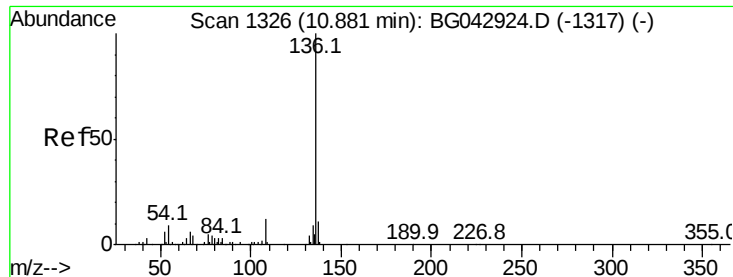

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.88 min Scan# 1326
Delta R.T. -0.00 min
Lab File: BG042946.D
Acq: 30 Sep 2019 17:01




Instrument :
BNA_G
ClientSampleId :
20190706-RR-COMP-6


Tot Ion:136	Resp:	254227
Ion Ratio	Lower	Upper
136	100	
137	10.8	8.5 12.7
54	9.7	7.4 11.2
68	4.5	3.6 5.4

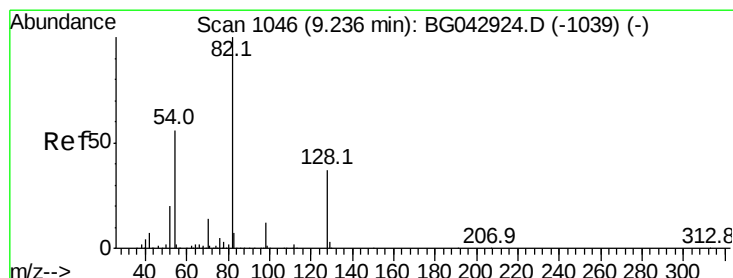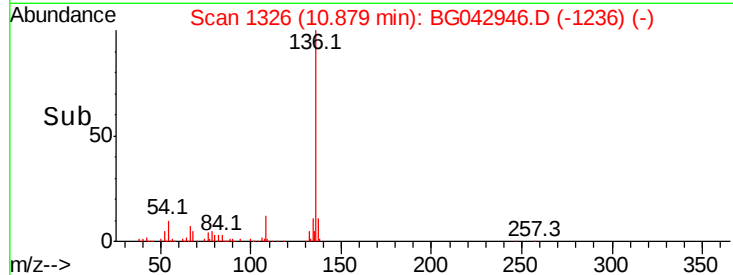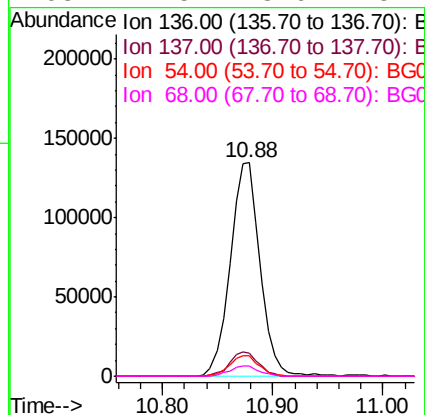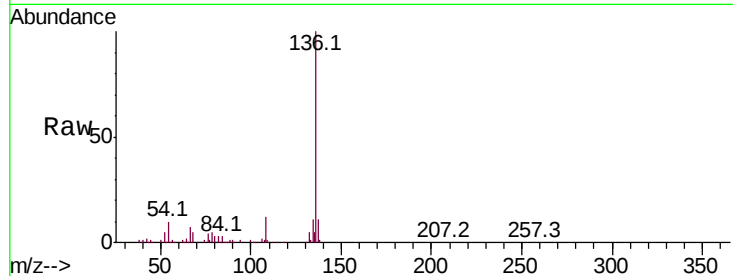

#23
Nitrobenzene-d5
Concen: 76.669 ng
RT: 9.23 min Scan# 1045
Delta R.T. -0.01 min
Lab File: BG042946.D
Acq: 30 Sep 2019 17:01

Tgt Ion: 82	Resp:	401011
Ion Ratio	Lower	Upper
82	100	
128	36.8	29.5 44.3
54	56.9	44.6 67.0

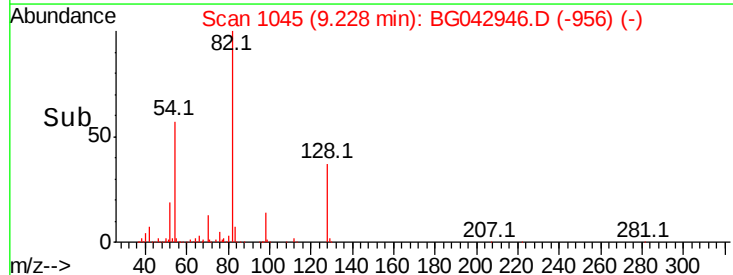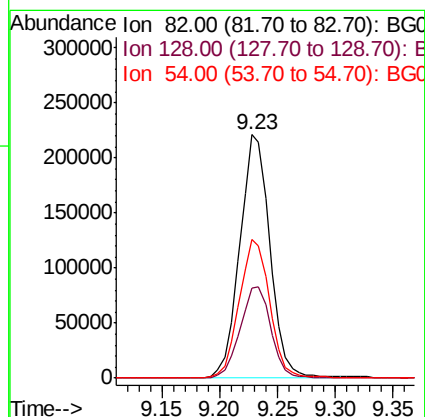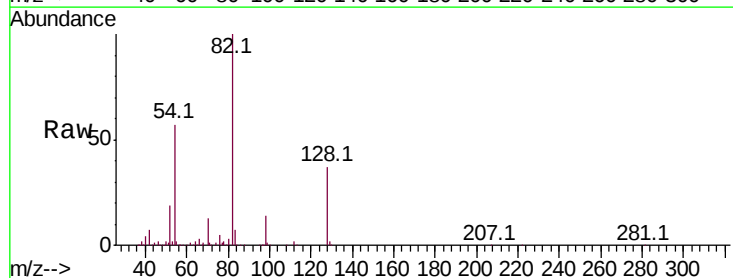

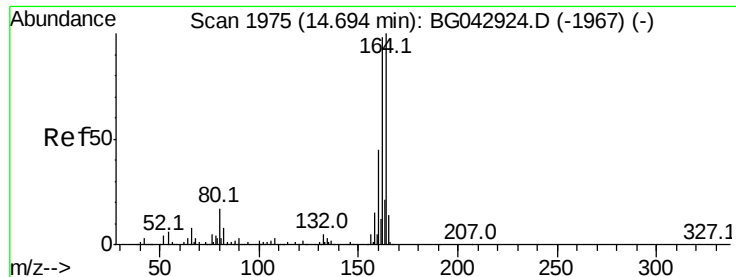

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.69 min Scan# 1974

Delta R.T. -0.01 min

Lab File: BG042946.D

Acq: 30 Sep 2019 17:01

Instrument :

BNA_G

ClientSampleId :

20190706-RR-COMP-6


Tot Ion:164 Resp: 175349

Ion Ratio Lower Upper

164 100

162 99.9 78.5 117.7




160 43.8 35.9 53.9

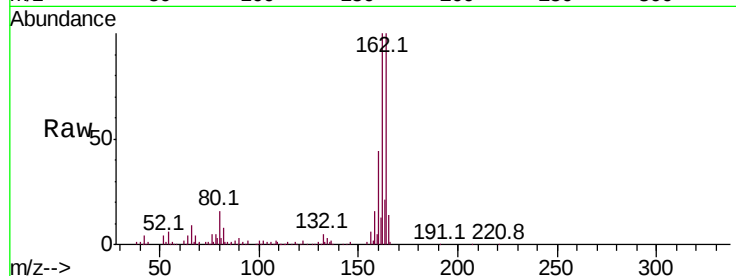

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

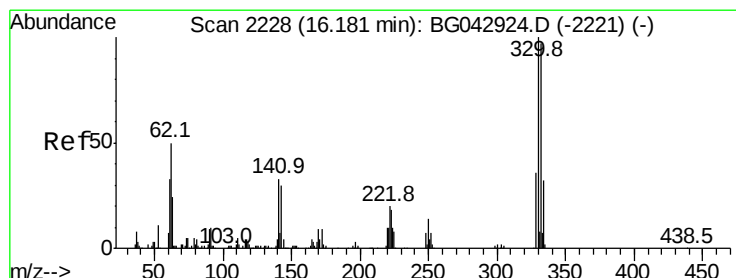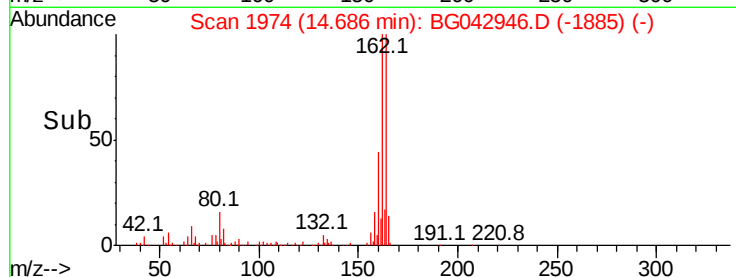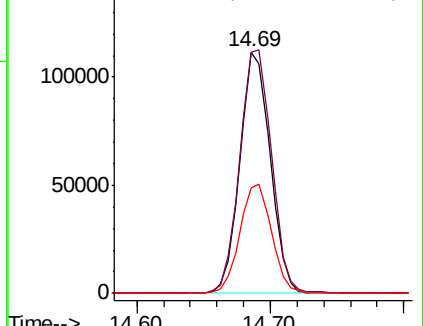

#42

2,4,6-Tribromophenol

Concen: 112.259 ng

RT: 16.18 min Scan# 2228

Delta R.T. -0.00 min

Lab File: BG042946.D

Acq: 30 Sep 2019 17:01


Tgt Ion:330 Resp: 338488

Ion Ratio Lower Upper

330 100

332 96.2 78.2 117.2



141 31.9 26.0 39.0

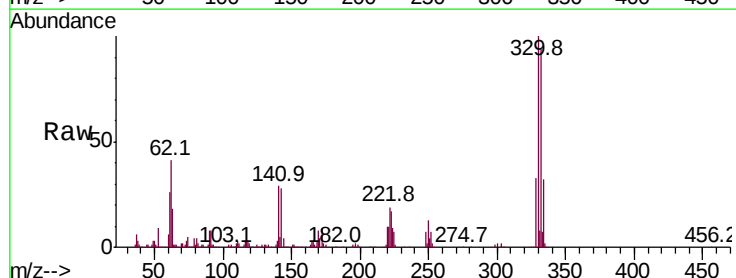


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



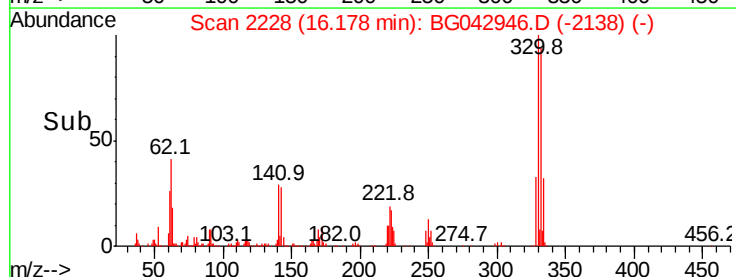
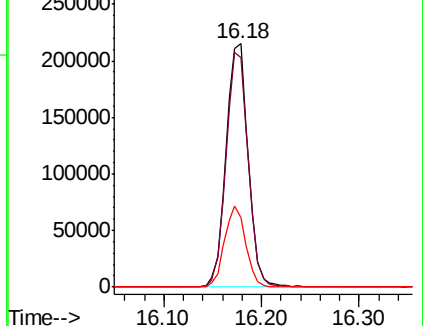


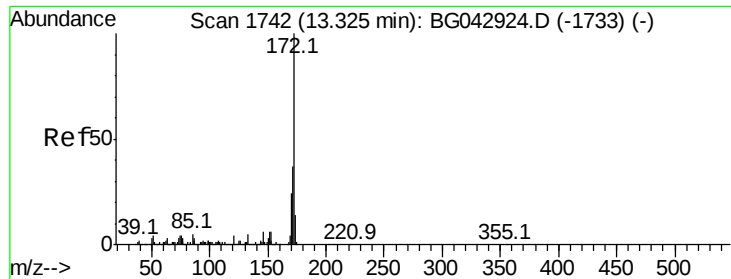

#45
 2-Fluorobiphenyl
 Concen: 77.987 ng
 RT: 13.32 min Scan# 1741
 Delta R.T. -0.01 min
 Lab File: BG042946.D
 Acq: 30 Sep 2019 17:01




Instrument :
 BNA_G
 ClientSampleId :
 20190706-RR-COMP-6


Tot Ion	Ratio	Lower	Upper
172	100		
171	35.7	29.6	44.4
170	24.2	19.6	29.4

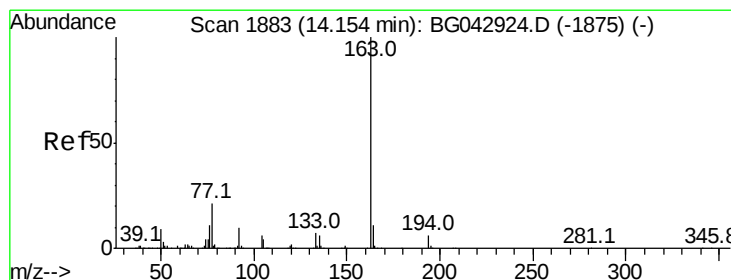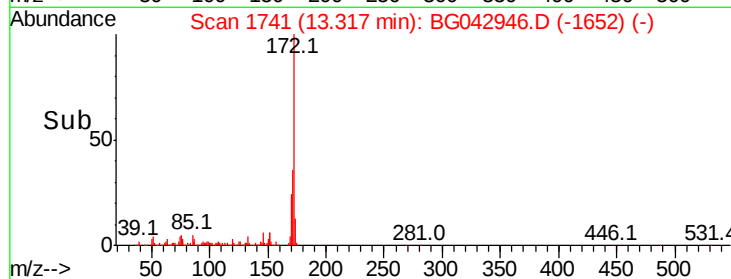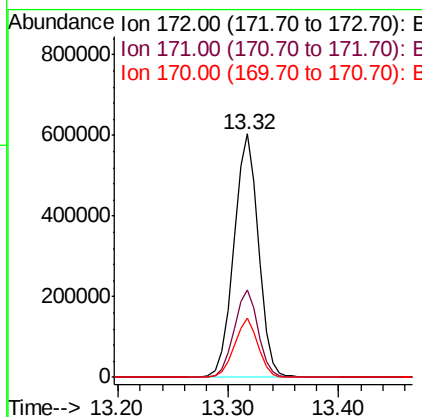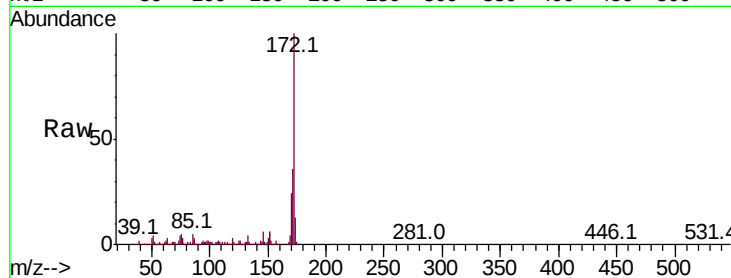

#50
 Dimethylphthalate
 Concen: 7.959 ng
 RT: 14.14 min Scan# 1881
 Delta R.T. -0.01 min
 Lab File: BG042946.D
 Acq: 30 Sep 2019 17:01

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.9	4.4	6.6
164	10.9	8.6	12.8

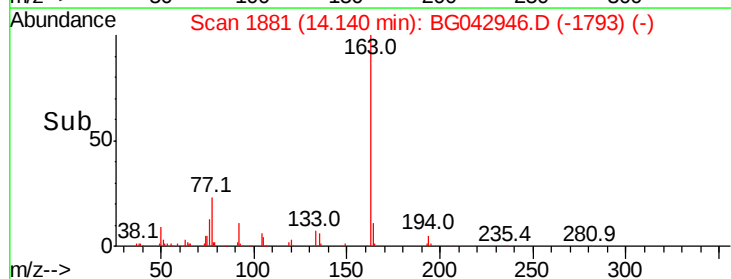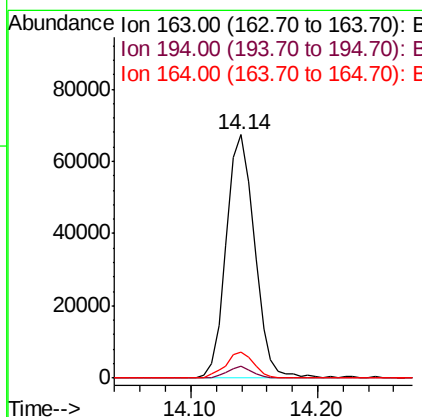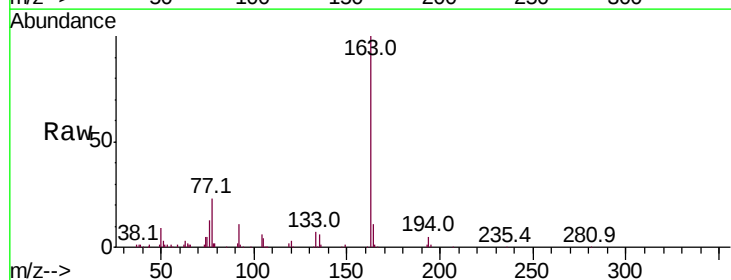

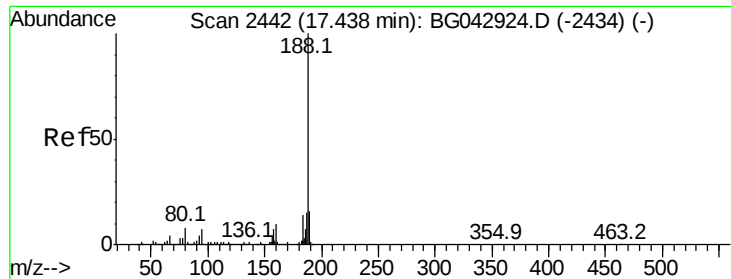

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.43 min Scan# 2441

Delta R.T. -0.01 min

Lab File: BG042946.D

Acq: 30 Sep 2019 17:01

Instrument :

BNA_G

ClientSampleId :

20190706-RR-COMP-6


Tot Ion:188 Resp: 421868

Ion Ratio Lower Upper

188 100

94 6.5 5.7 8.5




80 7.7 6.5 9.7

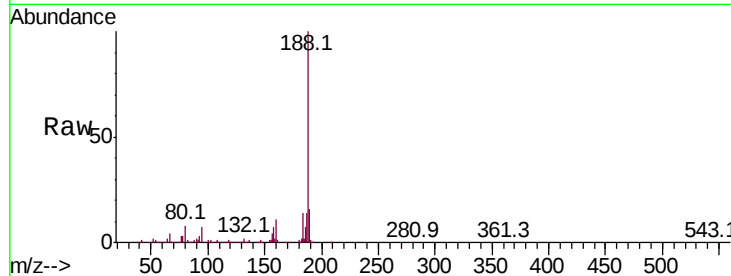

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

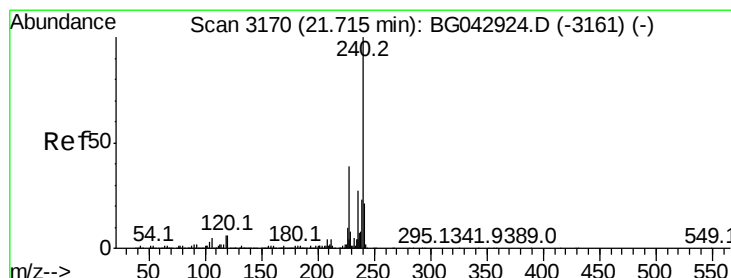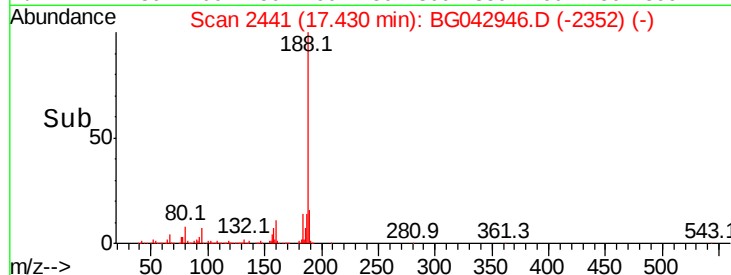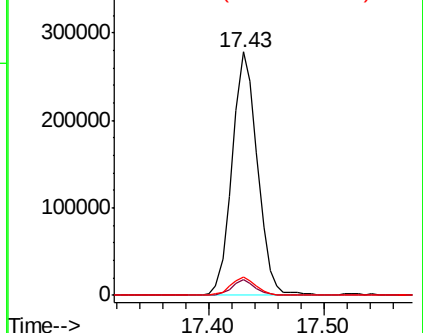

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.70 min Scan# 3168

Delta R.T. -0.01 min

Lab File: BG042946.D

Acq: 30 Sep 2019 17:01


Tgt Ion:240 Resp: 475521

Ion Ratio Lower Upper

240 100

120 5.3 4.8 7.2



236 26.1 21.4 32.0

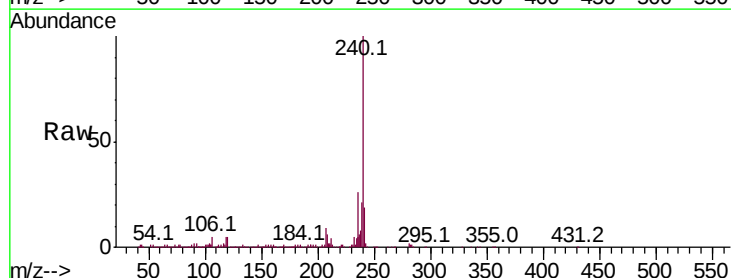


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

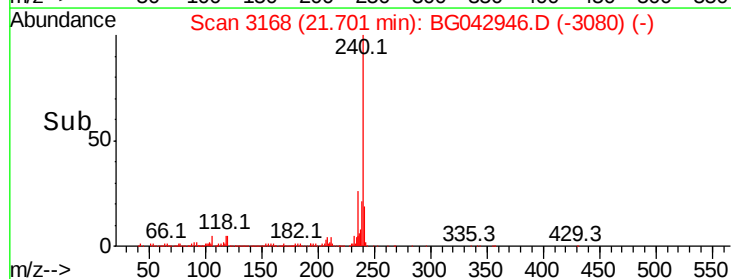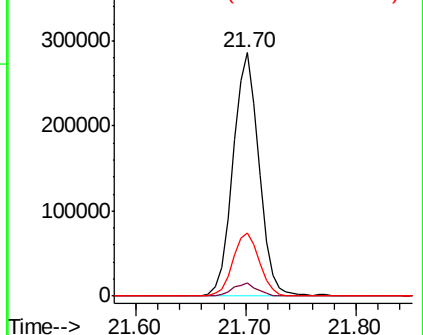

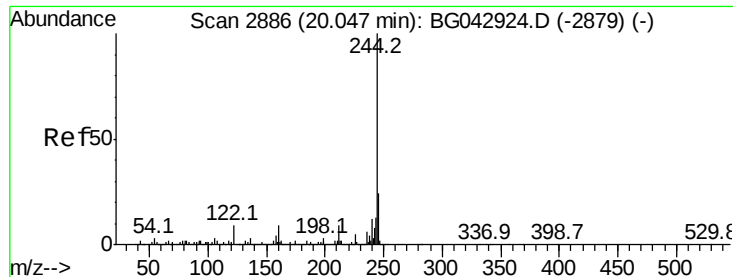

#79

Terphenyl-d14

Concen: 76.188 ng

RT: 20.04 min Scan# 2885

Delta R.T. -0.01 min

Lab File: BG042946.D

Acq: 30 Sep 2019 17:01

Instrument :

BNA_G

ClientSampleId :

20190706-RR-COMP-6


Tot Ion:244 Resp: 1700192

Ion Ratio Lower Upper

244 100

212 8.1 7.4 11.0




122 7.6 7.0 10.4

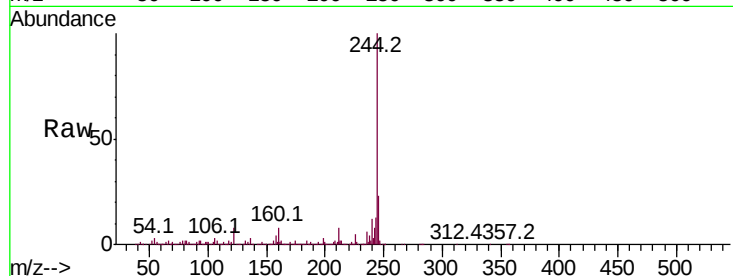

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

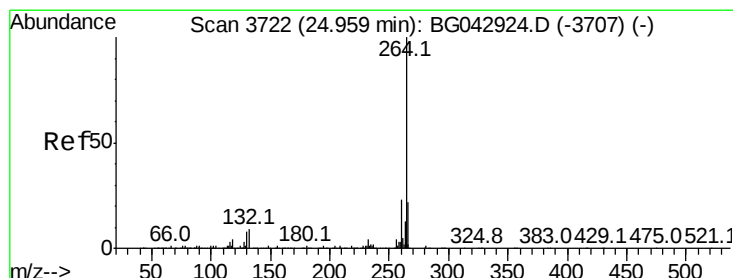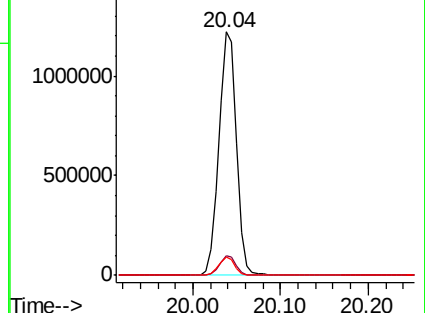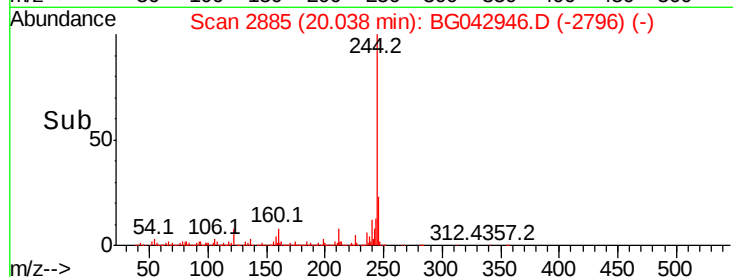

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.92 min Scan# 3716

Delta R.T. -0.04 min

Lab File: BG042946.D

Acq: 30 Sep 2019 17:01


Tgt Ion:264 Resp: 546311

Ion Ratio Lower Upper

264 100

260 21.7 18.7 28.1

265 21.5 17.7 26.5

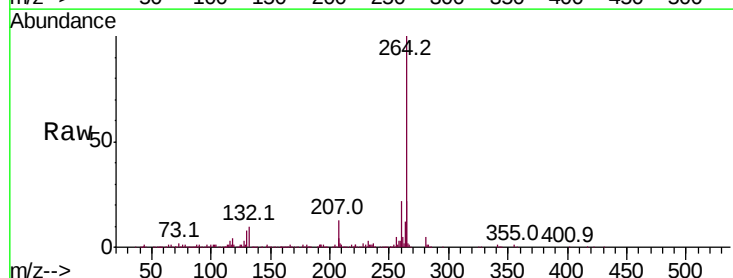

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

