


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG093019\
 Data File : BG042938.D
 Acq On : 30 Sep 2019 11:32
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 25 15:35:52 2019

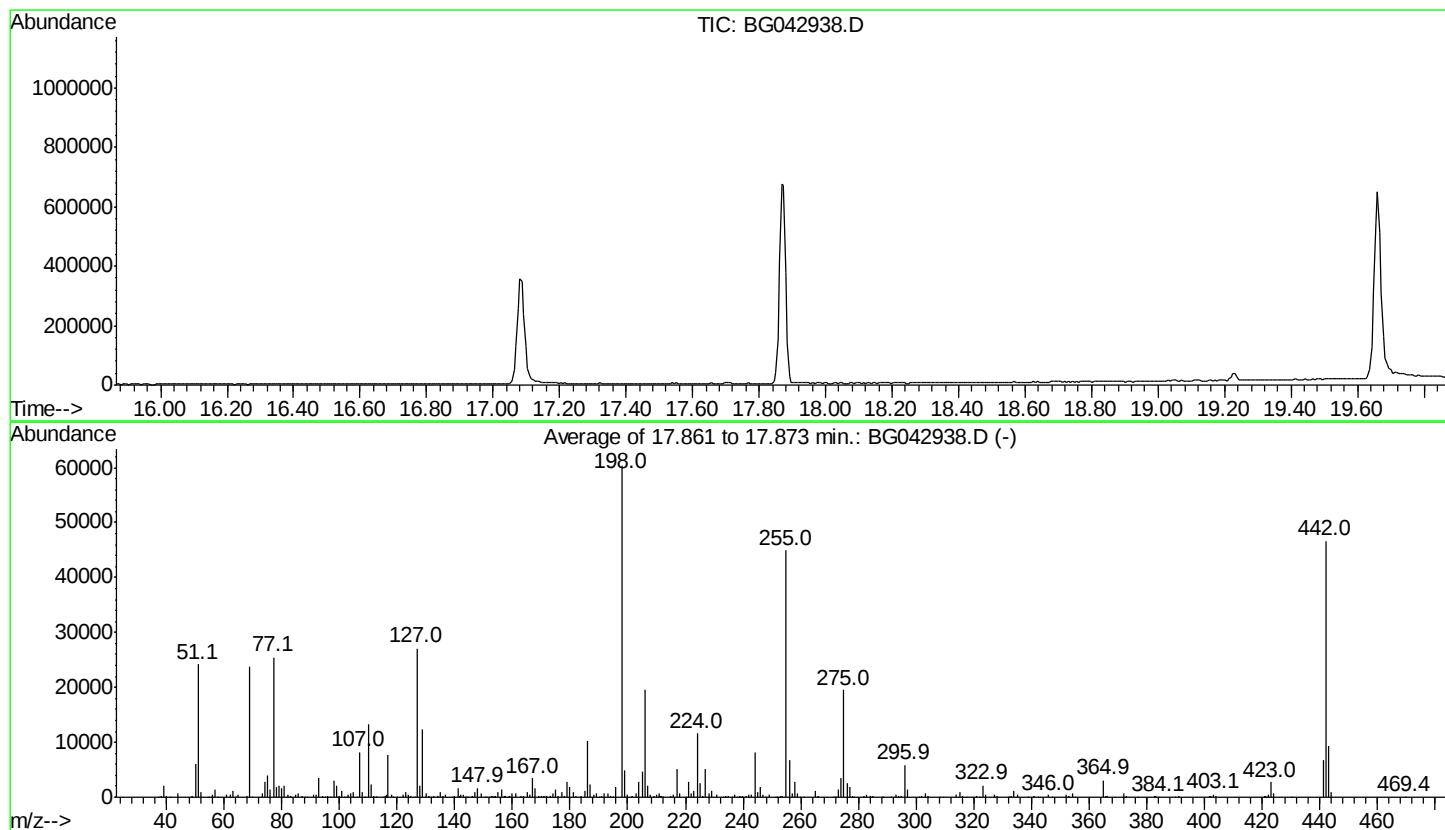

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	24157	PASS
68	69	0.00	2	0.8	188	PASS
69	198	0.00	100	39.3	23730	PASS
70	69	0.00	2	0.2	52	PASS
127	198	10	80	44.8	27042	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60373	PASS
199	198	5	9	7.9	4796	PASS
275	198	10	60	32.3	19511	PASS
365	198	1	100	5.0	3034	PASS
441	198	0.01	100	11.3	6808	PASS
442	198	50	100	77.3	46661	PASS
443	442	15	24	19.8	9230	PASS