

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG100118\
 Data File : BG037092.D
 Acq On : 2 Oct 2018 1:26
 Operator : JU/SJ
 Sample : PB113379BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB113379BL

Quant Time: Oct 02 05:34:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 24 10:41:23 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	42081	20.00	ng	0.00
21) Naphthalene-d8	10.84	136	174269	20.00	ng	-0.01
38) Acenaphthene-d10	14.66	164	108737	20.00	ng	-0.01
63) Phenanthrene-d10	17.41	188	288064	20.00	ng	0.00
75) Chrysene-d12	21.67	240	320719	20.00	ng	-0.02
86) Perylene-d12	24.88	264	304687	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	326801	148.94	ng	0.00
7) Phenol-d6	7.20	99	436241	128.50	ng	-0.01
23) Nitrobenzene-d5	9.20	82	293574	90.21	ng	-0.01
41) 2,4,6-Tribromophenol	16.16	330	158335	121.71	ng	-0.01
44) 2-Fluorobiphenyl	13.29	172	640030	87.67	ng	-0.01
78) Terphenyl-d14	20.02	244	1193988	97.89	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.20	70	36402	12.889	ng	# 70
50) 2,6-Dinitrotoluene	14.66	165	13406	7.020	ng	# 21
56) 2,4-Dinitrotoluene	14.66	165	13406	5.031	ng	# 19
66) 4-Bromophenyl-phenylether	16.16	248	11181	3.412	ng	# 1
76) Benzidine	20.02	184	19885	2.051	ng	# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG100118\
Data File : BG037092.D
Acq On : 2 Oct 2018 1:26
Operator : JU/SJ
Sample : PB113379BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB113379BL

Quant Time: Oct 02 05:34:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

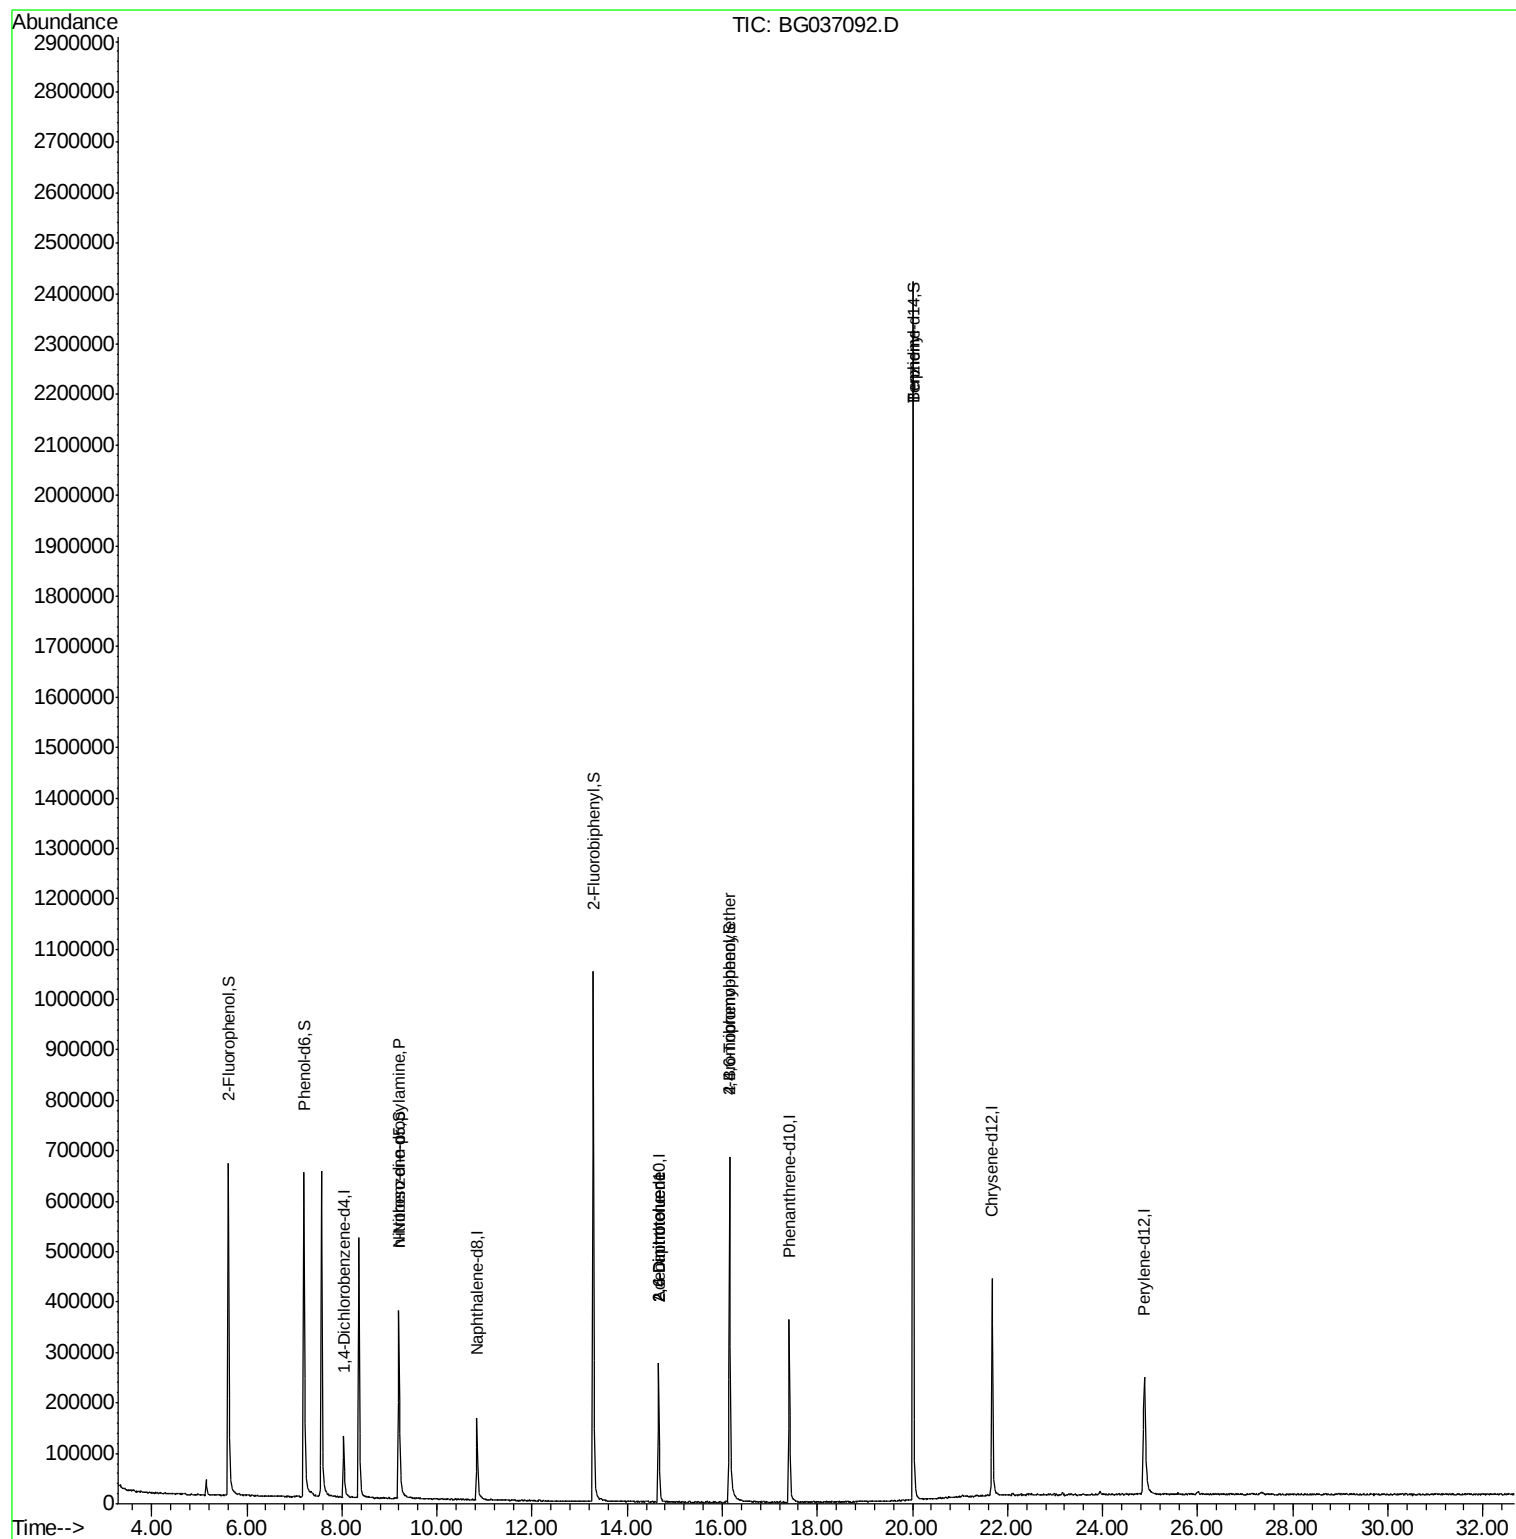

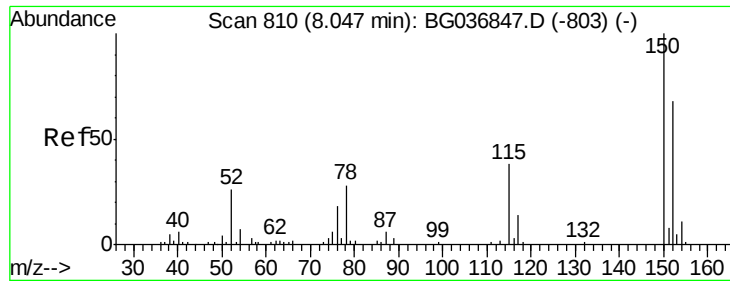

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.04 min Scan# 809

Delta R.T. -0.01 min

Lab File: BG037092.D

Acq: 2 Oct 2018 1:26

Instrument :

BNA_G

ClientSampleId :

PB113379BL


Tgt Ion:152 Resp: 42081

Ion Ratio Lower Upper

152 100

150 154.1 119.5 179.3




115 60.6 44.5 66.7

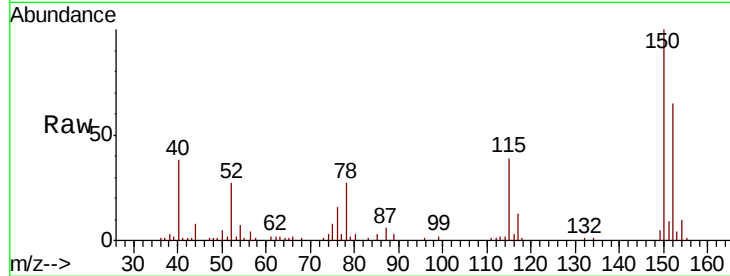

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

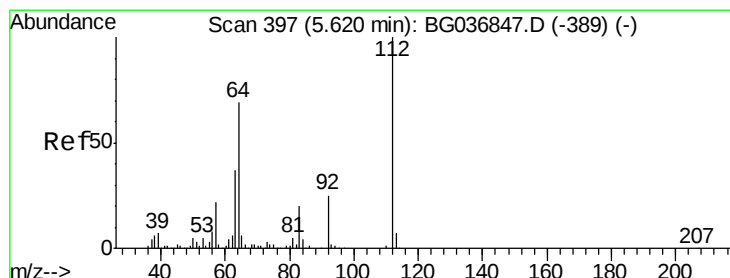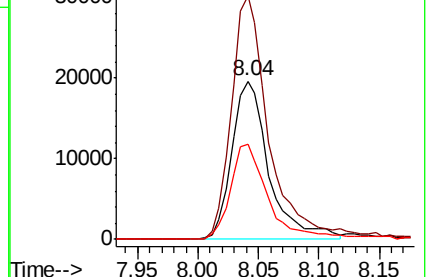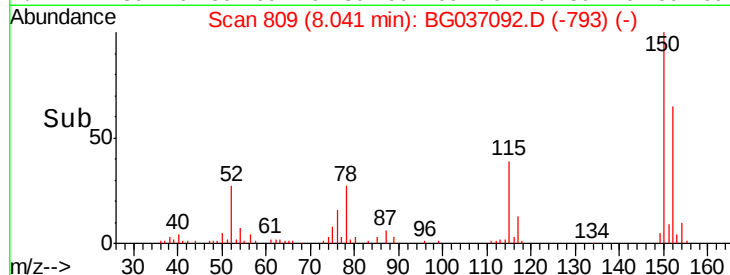

#5

2-Fluorophenol

Concen: 148.935 ng

RT: 5.61 min Scan# 396

Delta R.T. -0.01 min

Lab File: BG037092.D

Acq: 2 Oct 2018 1:26


Tgt Ion:112 Resp: 326801

Ion Ratio Lower Upper

112 100

64 68.9 57.2 85.8



63 35.0 30.8 46.2

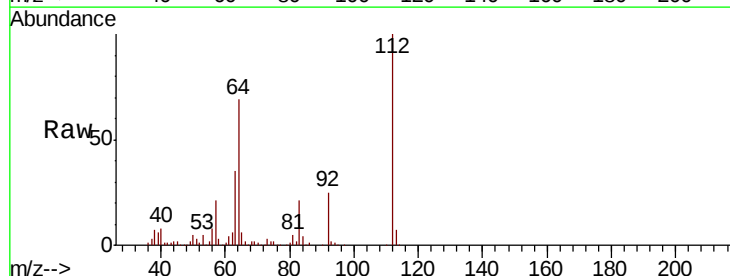


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

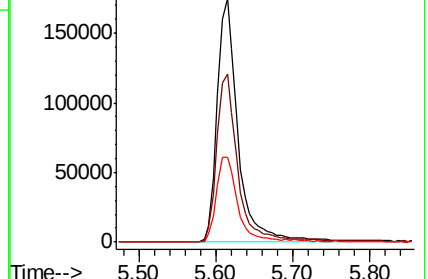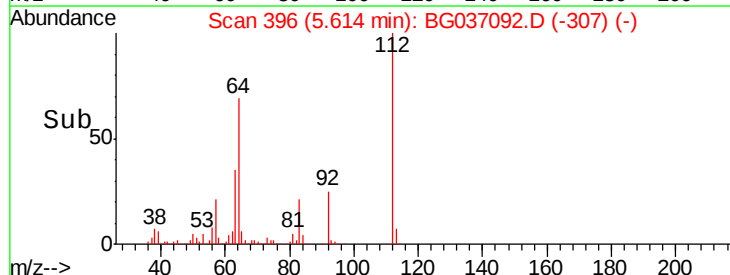

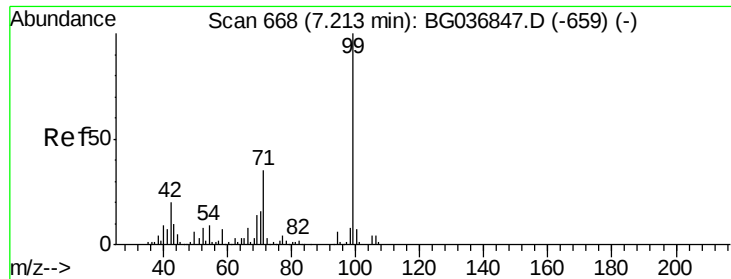

#7

Phenol-d6

Concen: 128.500 ng

RT: 7.20 min Scan# 666

Delta R.T. -0.01 min

Lab File: BG037092.D

Acq: 2 Oct 2018 1:26

Instrument :

BNA_G

ClientSampleId :

PB113379BL





Tgt Ion: 99 Resp: 436241

Ion Ratio Lower Upper

99 100

42 20.3 16.5 24.7

71 34.5 29.4 44.2

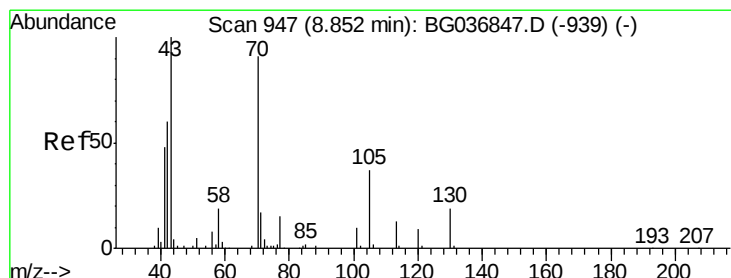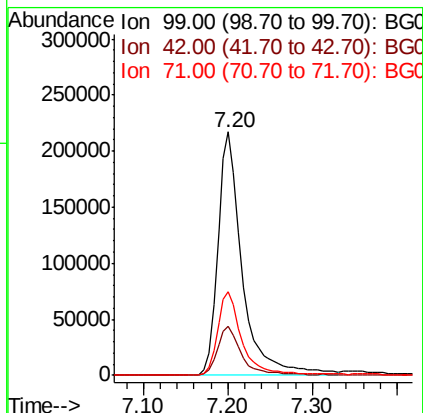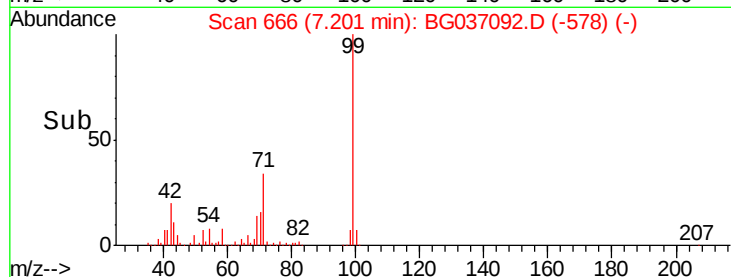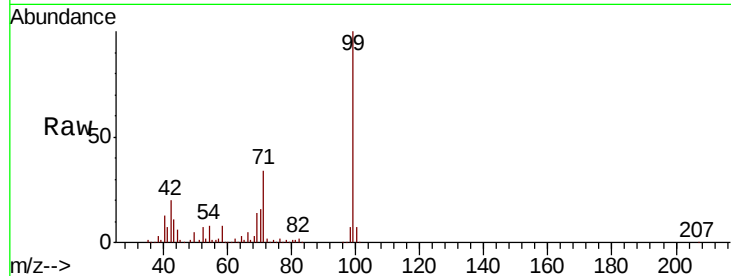

#19

n-Nitroso-di-n-propylamine

Concen: 12.889 ng

RT: 9.20 min Scan# 1006

Delta R.T. 0.35 min

Lab File: BG037092.D

Acq: 2 Oct 2018 1:26

Tgt Ion: 70 Resp: 36402




Ion Ratio Lower Upper


70 100

42 47.6 56.2 84.4#

101 0.0 7.8 11.6#

130 2.1 16.2 24.2#

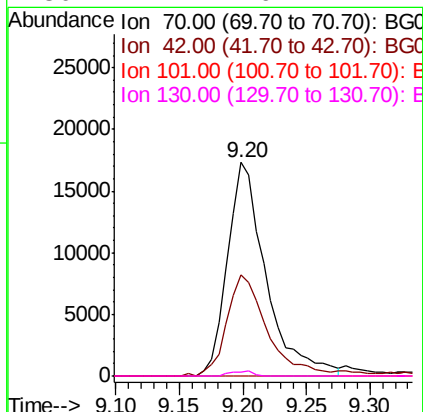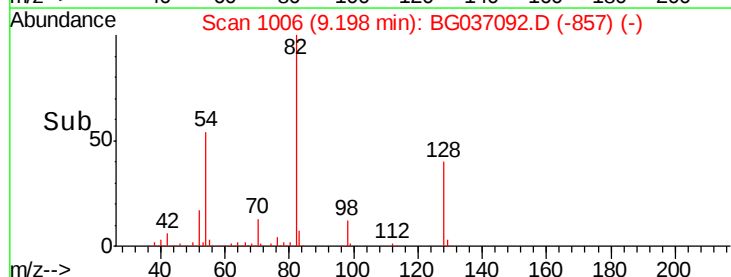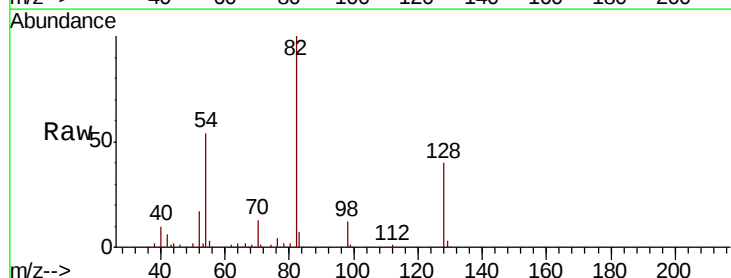


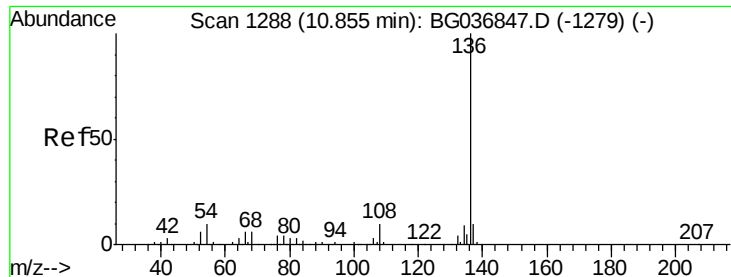




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.84 min Scan# 1286
Delta R.T. -0.01 min
Lab File: BG037092.D
Acq: 2 Oct 2018 1:26

Instrument :
BNA_G
ClientSampleId :
PB113379BL

Tgt Ion:	136	Resp:	174269
Ion	Ratio	Lower	Upper
136	100		
137	10.5	8.8	13.2
54	10.5	9.2	13.8
68	7.0	5.8	8.6

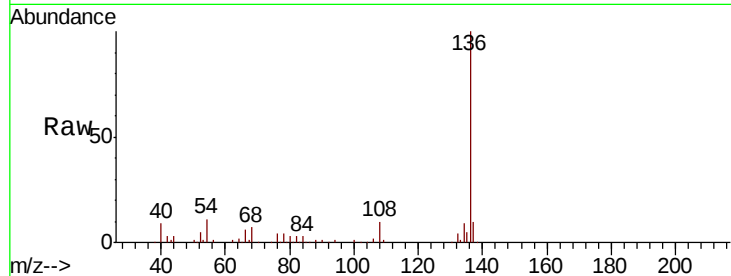


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

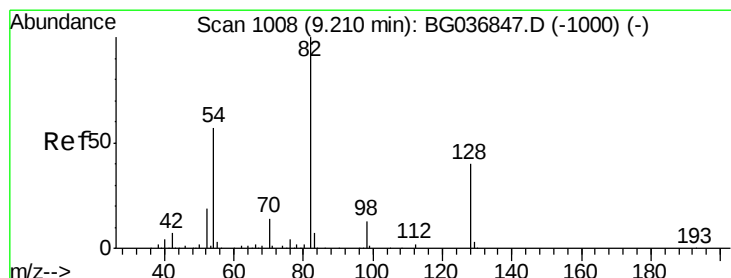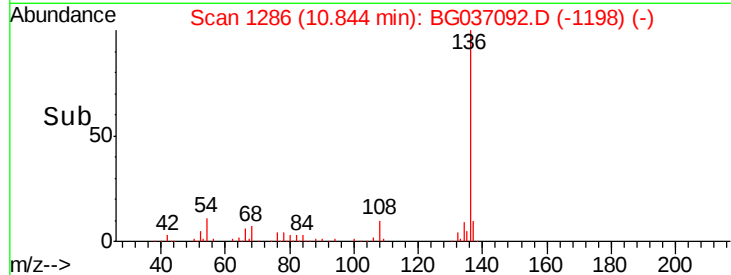
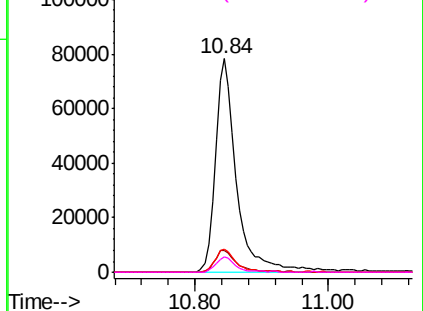



#23
Nitrobenzene-d5
Concen: 90.212 ng
RT: 9.20 min Scan# 1006
Delta R.T. -0.01 min
Lab File: BG037092.D
Acq: 2 Oct 2018 1:26

Tgt Ion:	82	Resp:	293574
Ion	Ratio	Lower	Upper
82	100		
128	39.9	33.3	49.9
54	53.8	45.1	67.7

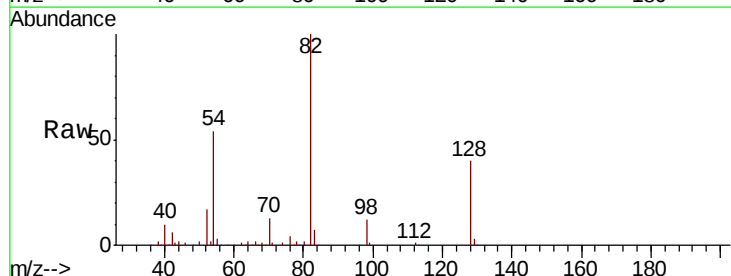

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

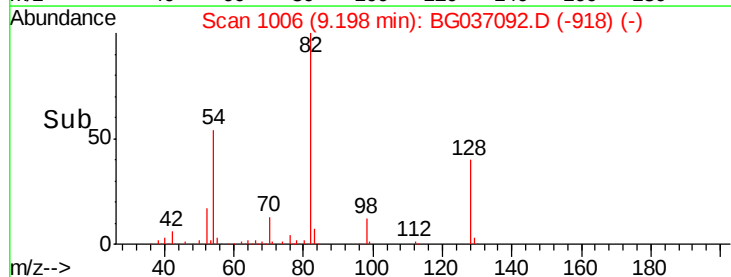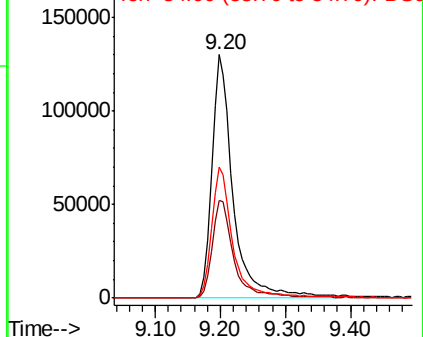

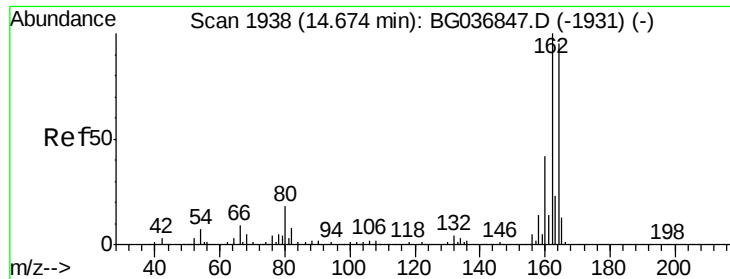

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.66 min Scan# 1936

Delta R.T. -0.01 min

Lab File: BG037092.D

Acq: 2 Oct 2018 1:26

Instrument :

BNA_G

ClientSampleId :

PB113379BL


Tgt Ion:164 Resp: 108737

Ion Ratio Lower Upper

164 100

162 105.7 80.7 121.1




160 46.5 35.3 52.9

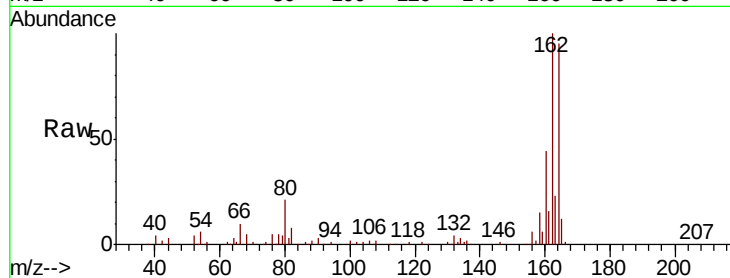

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

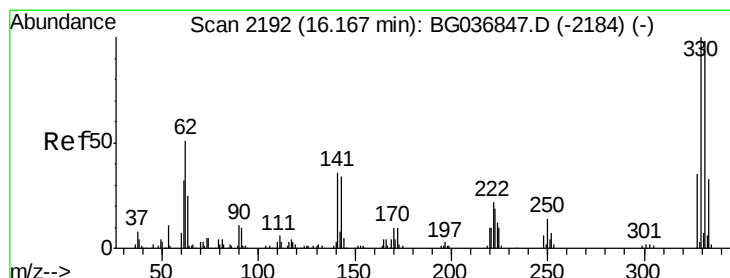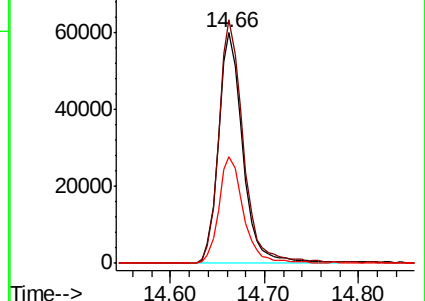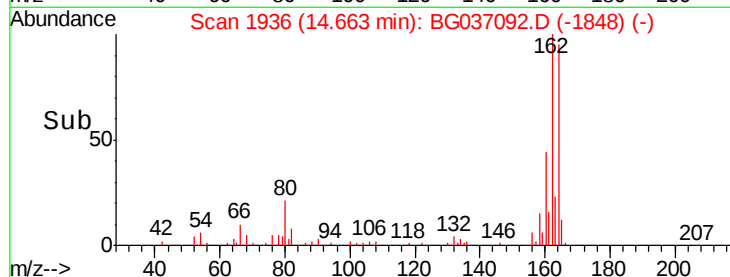

#41

2,4,6-Tribromophenol

Concen: 121.705 ng

RT: 16.16 min Scan# 2190

Delta R.T. -0.01 min

Lab File: BG037092.D

Acq: 2 Oct 2018 1:26


Tgt Ion:330 Resp: 158335

Ion Ratio Lower Upper

330 100

332 96.9 75.4 113.2



141 38.6 30.7 46.1

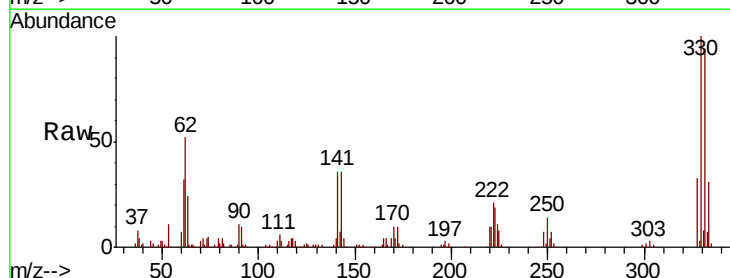


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



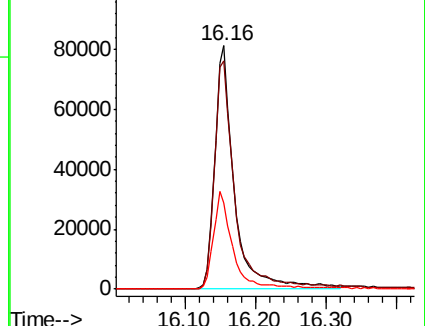
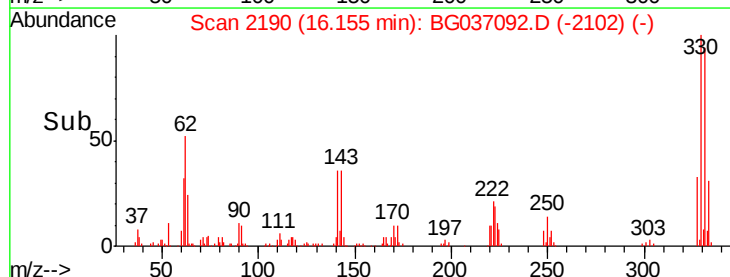


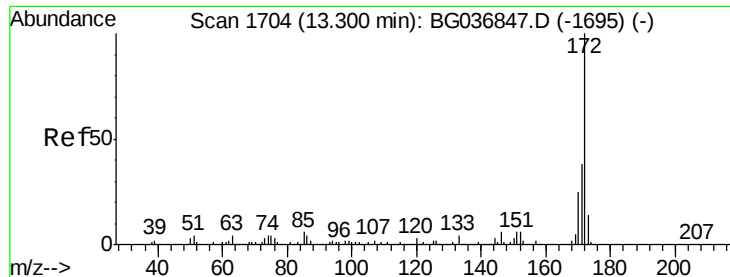

#44
 2-Fluorobiphenyl
 Concen: 87.666 ng
 RT: 13.29 min Scan# 1702
 Delta R.T. -0.01 min
 Lab File: BG037092.D
 Acq: 2 Oct 2018 1:26




Instrument :
 BNA_G
 ClientSampleId :
 PB113379BL


Tgt Ion:172 Resp: 640030
 Ion Ratio Lower Upper
 172 100
 171 37.8 31.3 46.9
 170 25.4 21.0 31.6

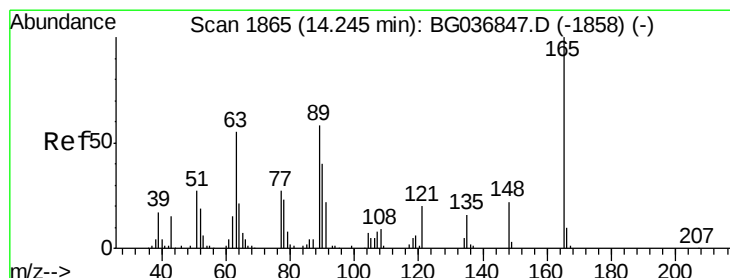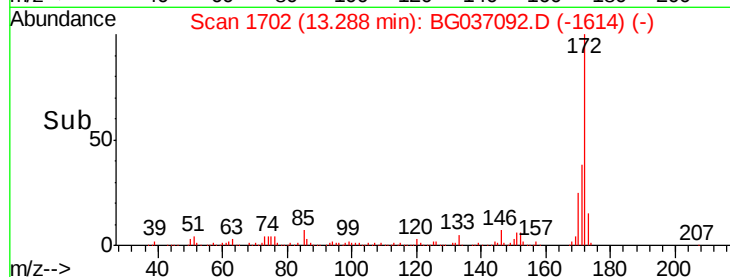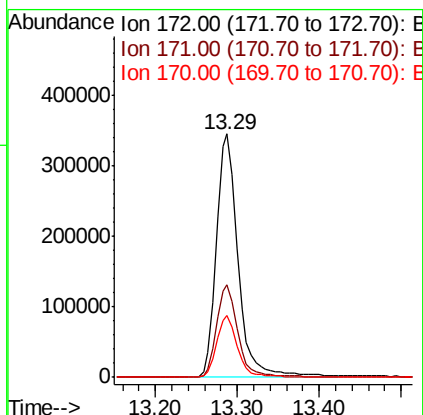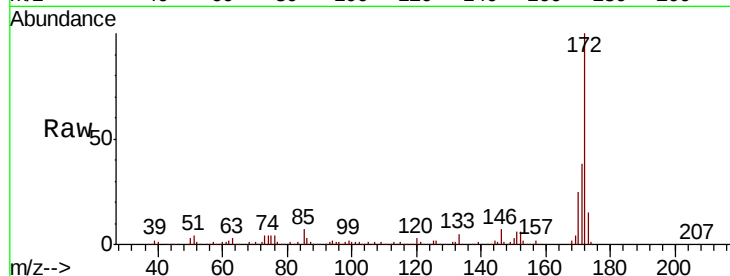

#50
 2,6-Dinitrotoluene
 Concen: 7.020 ng
 RT: 14.66 min Scan# 1936
 Delta R.T. 0.42 min
 Lab File: BG037092.D
 Acq: 2 Oct 2018 1:26

Tgt Ion:165 Resp: 13406
 Ion Ratio Lower Upper
 165 100
 63 2.1 50.1 75.1#
 89 0.0 47.8 71.6#

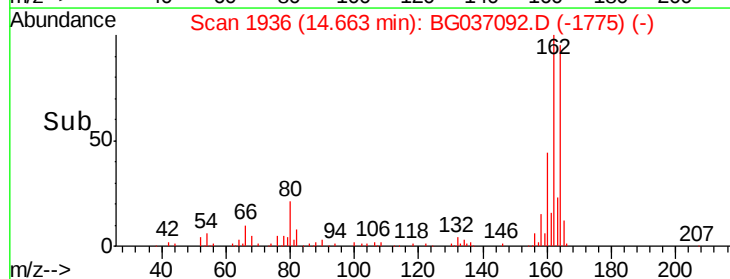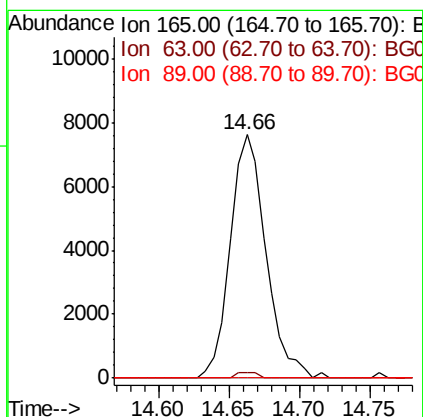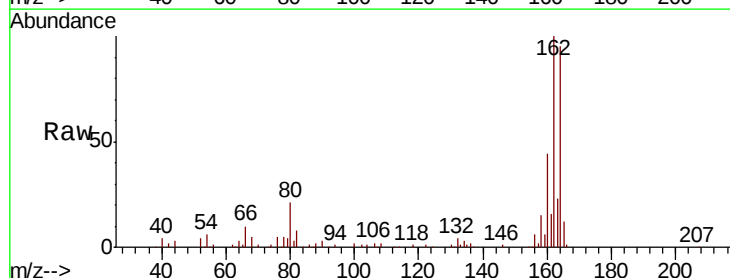


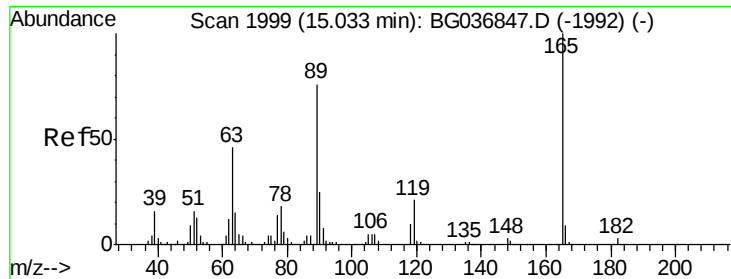




#56
 2,4-Dinitrotoluene
 Concen: 5.031 ng
 RT: 14.66 min Scan# 1936
 Delta R.T. -0.37 min
 Lab File: BG037092.D
 Acq: 2 Oct 2018 1:26

Instrument :
 BNA_G
 ClientSampleId :
 PB113379BL

Tgt Ion:	165	Resp:	13406
Ion	Ratio	Lower	Upper
165	100		
63	2.1	40.1	60.1#
89	0.0	63.7	95.5#
182	0.0	2.5	3.7#

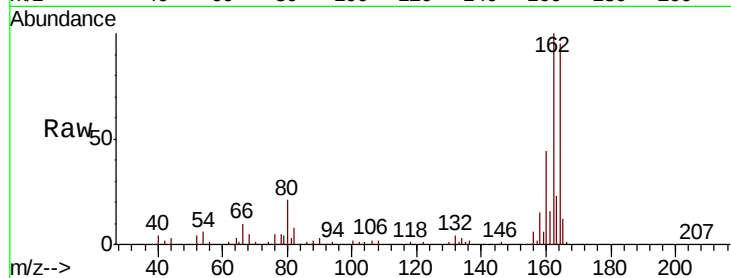


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC
 Ion 182.00 (181.70 to 182.70): E

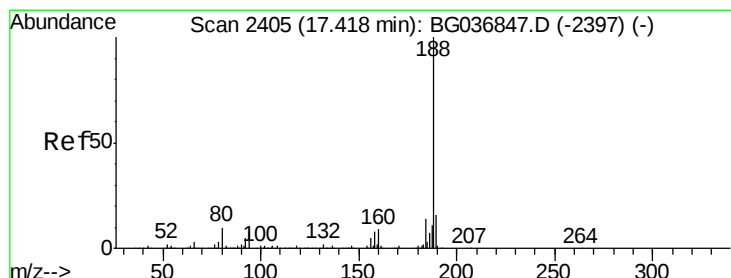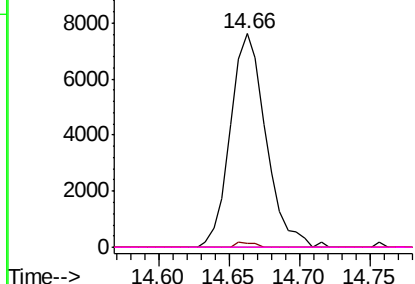
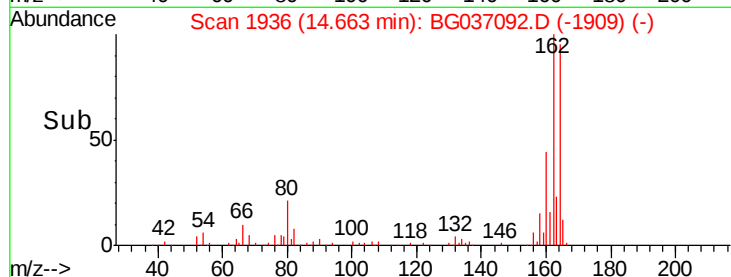



#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.41 min Scan# 2404
 Delta R.T. -0.01 min
 Lab File: BG037092.D
 Acq: 2 Oct 2018 1:26

Tgt Ion:	188	Resp:	288064
Ion	Ratio	Lower	Upper
188	100		
94	7.8	6.7	10.1
80	9.6	8.1	12.1

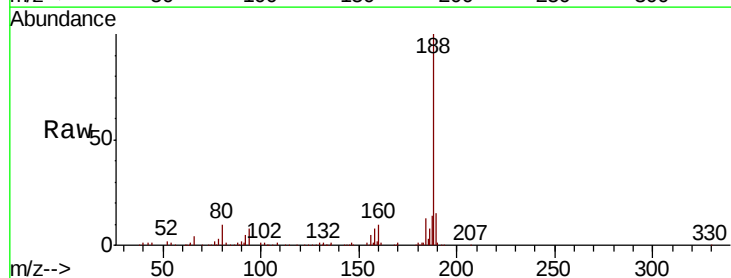

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC

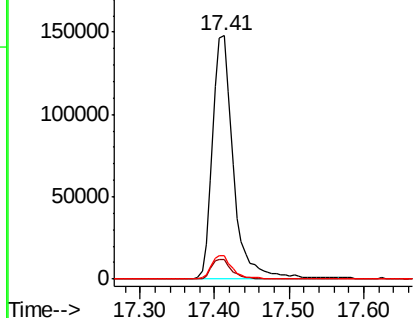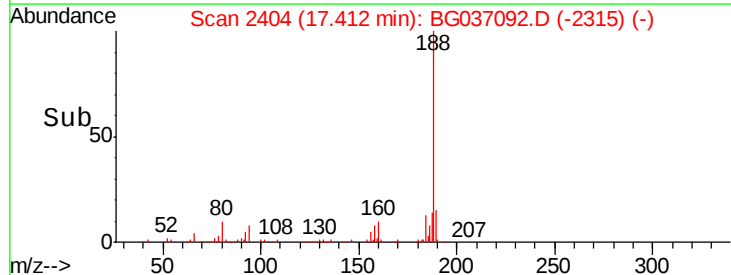


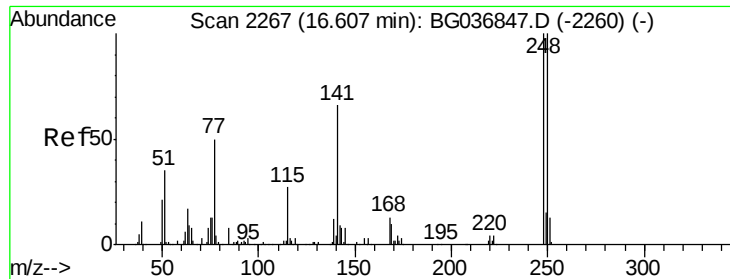




#66
 4-Bromophenyl-phenylether
 Concen: 3.412 ng
 RT: 16.16 min Scan# 2190
 Delta R.T. -0.45 min
 Lab File: BG037092.D
 Acq: 2 Oct 2018 1:26

Instrument :
 BNA_G
 ClientSampleId :
 PB113379BL

Tgt Ion:248 Resp: 11181
 Ion Ratio Lower Upper
 248 100
 250 202.0 78.1 117.1#
 141 510.8 53.7 80.5#

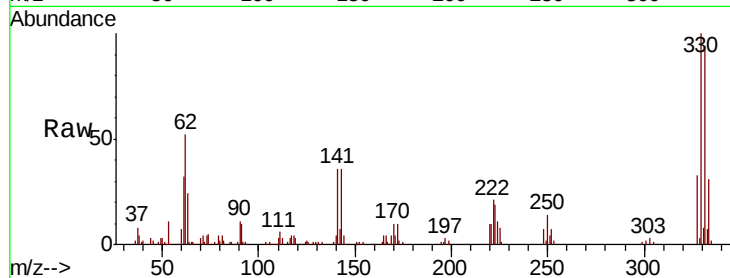


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

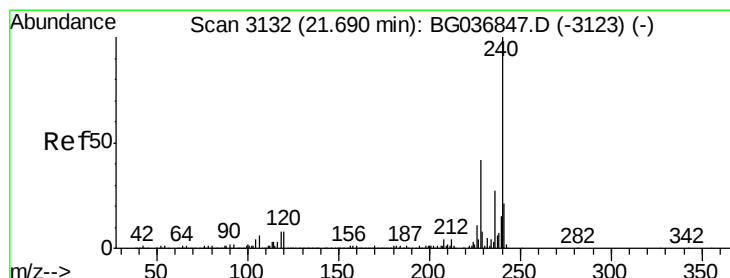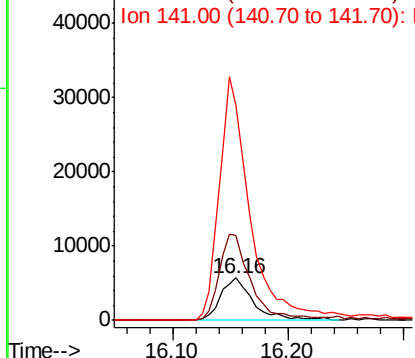
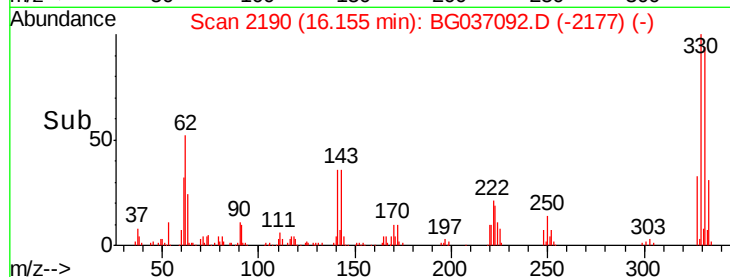



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.67 min Scan# 3129
 Delta R.T. -0.02 min
 Lab File: BG037092.D
 Acq: 2 Oct 2018 1:26

Tgt Ion:240 Resp: 320719
 Ion Ratio Lower Upper
 240 100
 120 9.0 6.9 10.3
 236 25.3 21.2 31.8

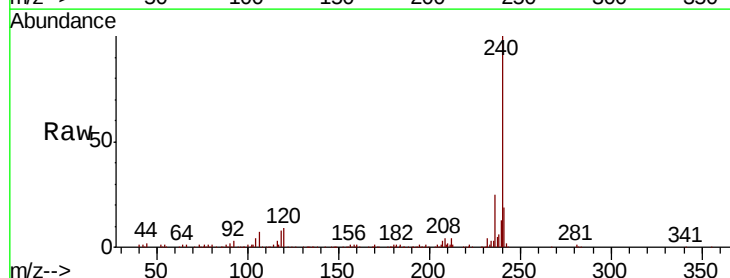

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

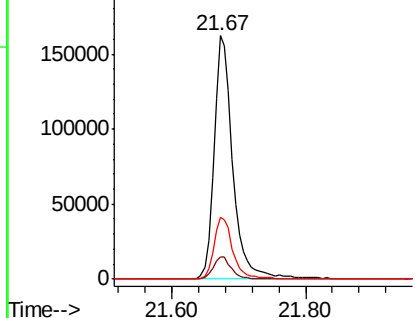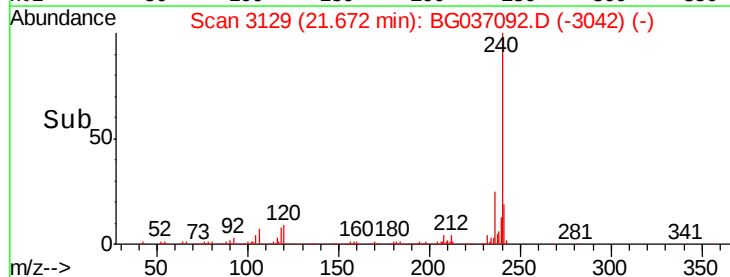

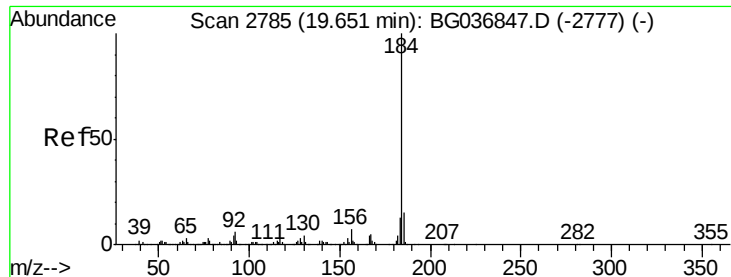

#76

Benzidine

Concen: 2.051 ng

RT: 20.02 min Scan# 2847

Delta R.T. 0.36 min

Lab File: BG037092.D

Acq: 2 Oct 2018 1:26

Instrument :

BNA_G

ClientSampleId :

PB113379BL


Tgt Ion:184 Resp: 19885

Ion Ratio Lower Upper

184 100

185 19.0 12.6 18.8#




183 9.4 10.9 16.3#

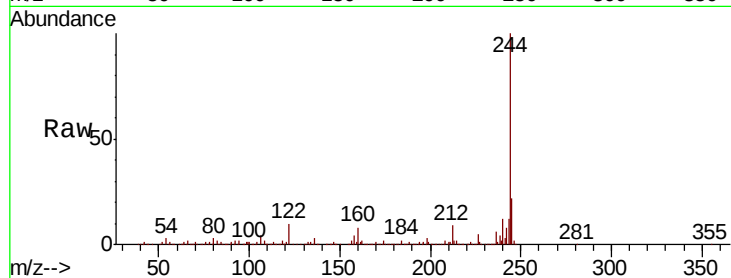

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

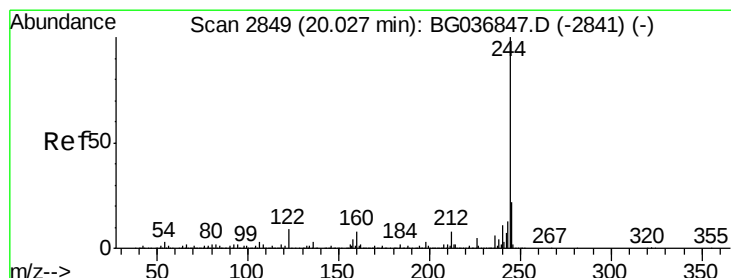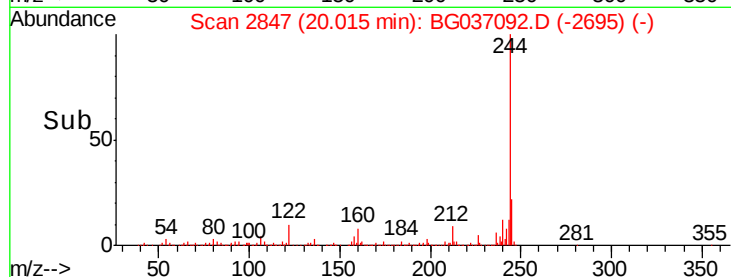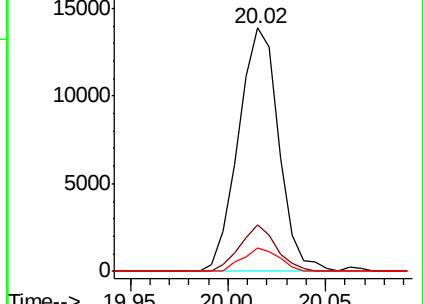

#78

Terphenyl-d14

Concen: 97.892 ng

RT: 20.02 min Scan# 2847

Delta R.T. -0.01 min

Lab File: BG037092.D

Acq: 2 Oct 2018 1:26


Tgt Ion:244 Resp: 1193988

Ion Ratio Lower Upper

244 100

212 8.5 7.0 10.6



122 10.0 7.1 10.7

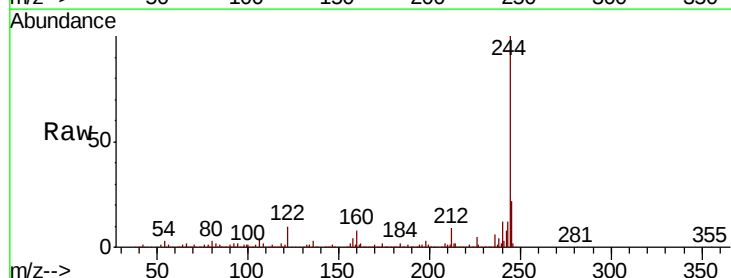


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

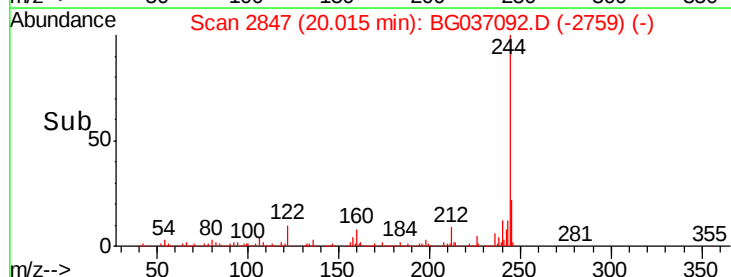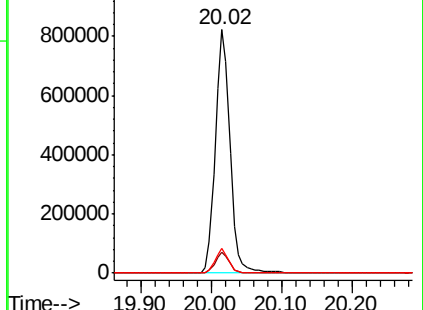

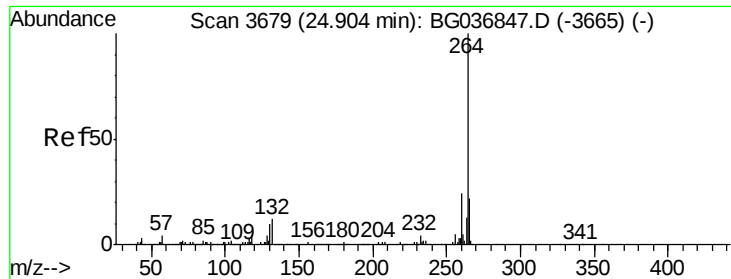

#86
Perylene-d12
Concen: 20.000 ng
RT: 24.88 min Scan# 3675
Delta R.T. -0.02 min
Lab File: BG037092.D
Acq: 2 Oct 2018 1:26

Instrument :
BNA_G
ClientSampleId :
PB113379BL

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.0	19.6	29.4
265	21.5	17.4	26.0

