
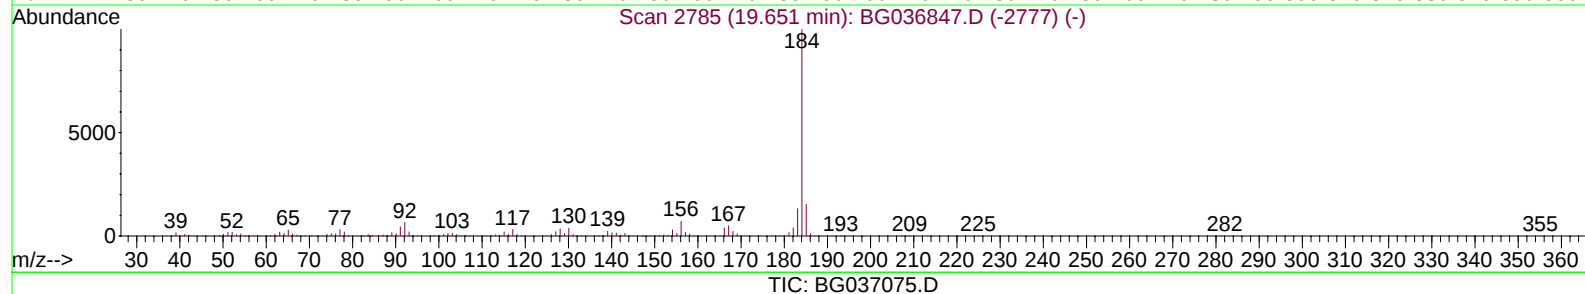
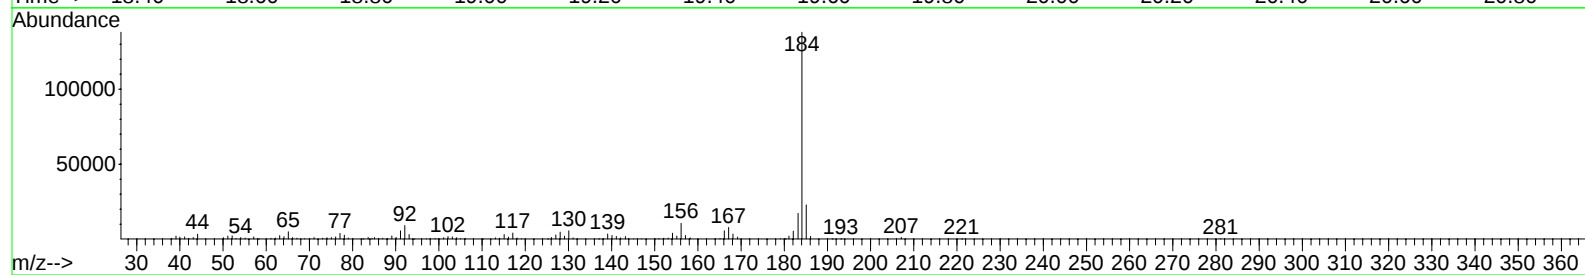


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG100118\
 Data File : BG037075.D
 Acq On : 1 Oct 2018 14:27
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 15:17:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 24 10:41:23 2018
 Response via : Initial Calibration

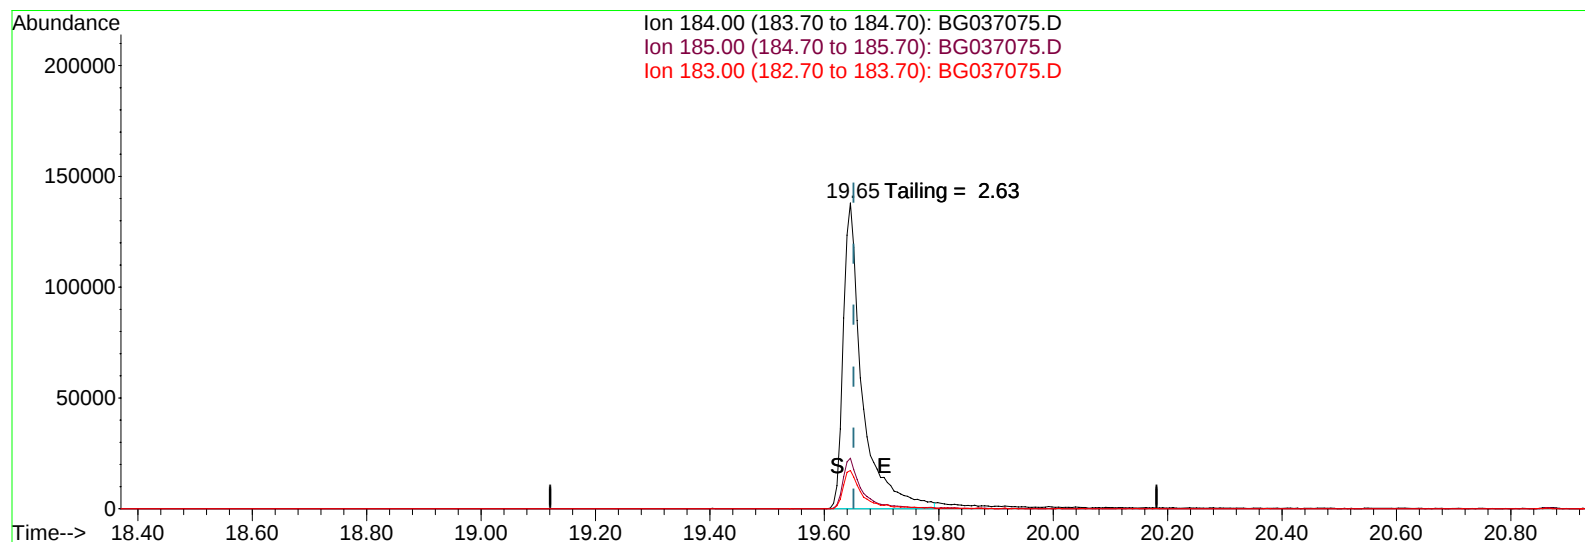

(76) Benzidine




19.645min (-0.006) 127573.58ng

response 331660

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.55
183.00	13.60	12.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG100118\
Data File : BG037075.D
Acq On : 1 Oct 2018 14:27
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 15:00:16 2018
Quant Title :
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

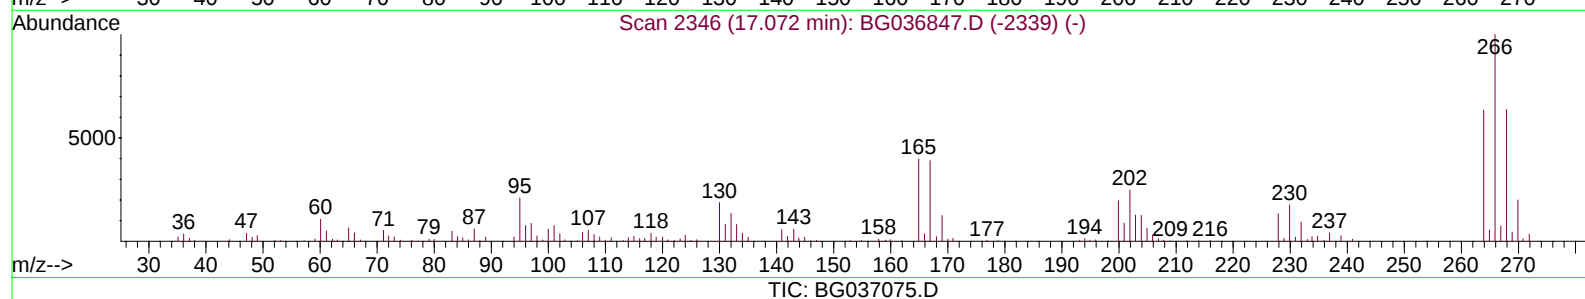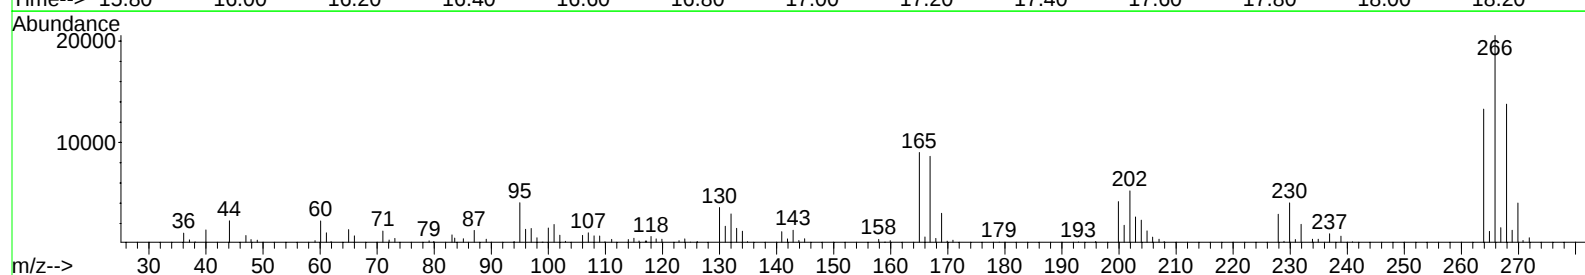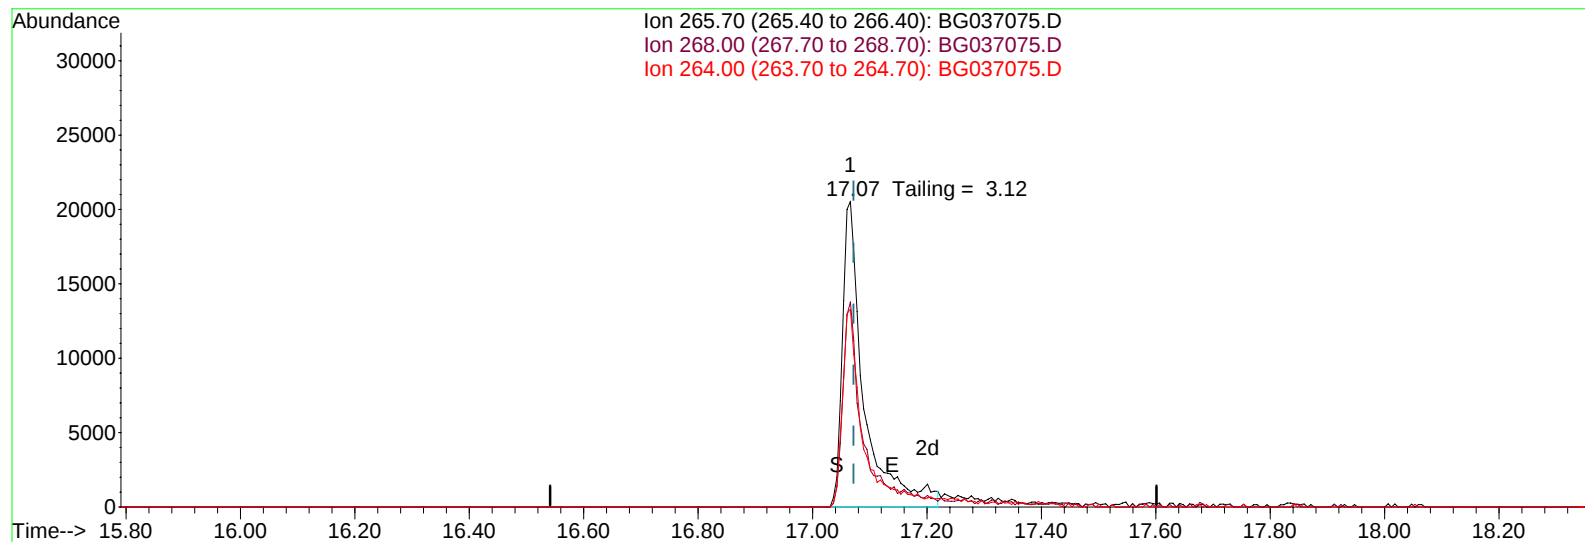

TIC: BG037075.D

(69) Pentachlorophenol (C)

17.066min (-0.006) 117018.95ng

response 51786

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	67.07
264.00	61.10	64.68
0.00	0.00	0.00