


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100118\
Data File : BG037075.D
Acq On : 1 Oct 2018 14:27
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 24 10:41:23 2018

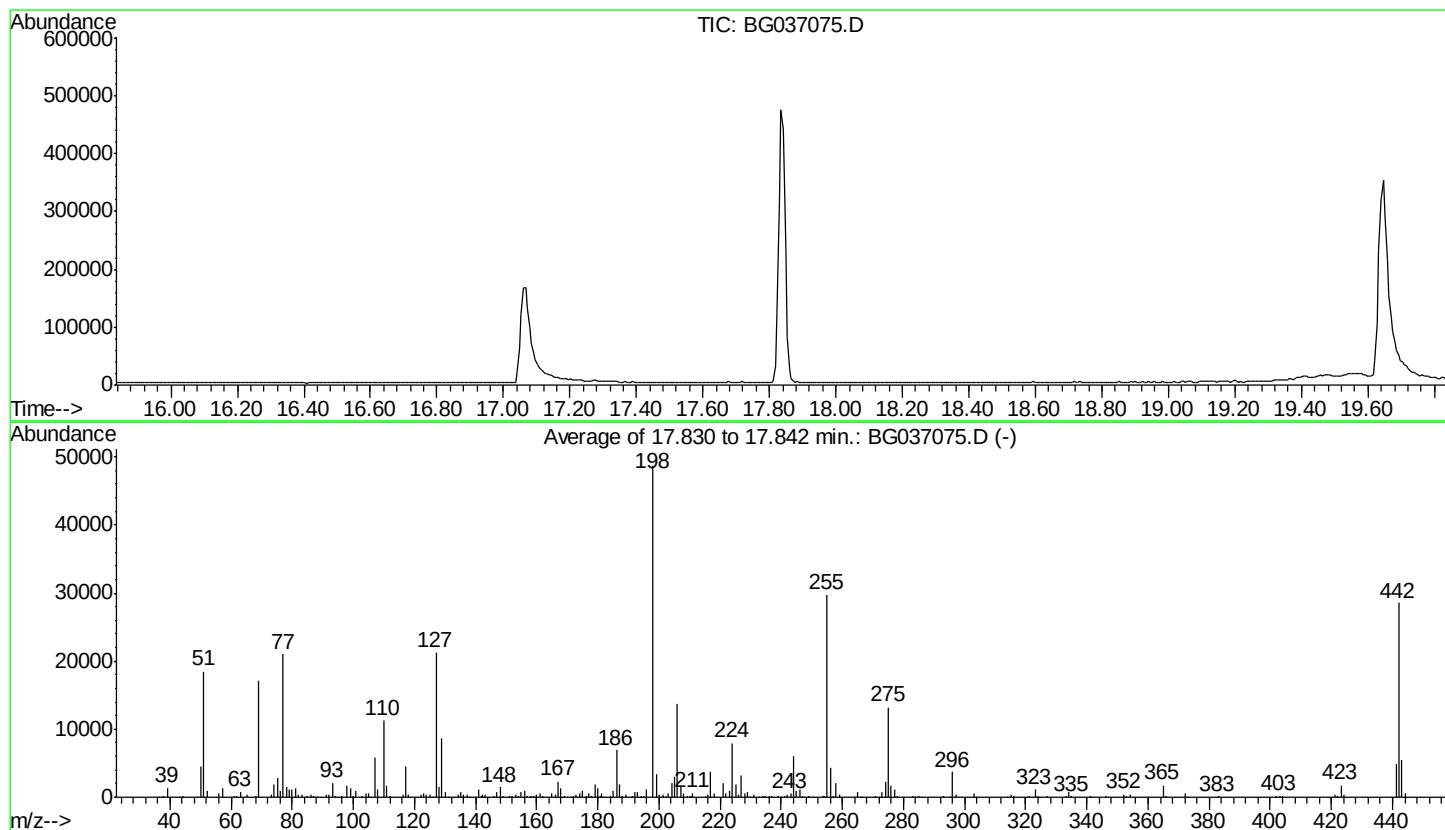

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	18442	PASS
68	69	0.00	2	0.9	148	PASS
69	198	0.00	100	35.3	17214	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.5	21178	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48720	PASS
199	198	5	9	7.0	3428	PASS
275	198	10	60	27.1	13202	PASS
365	198	1	100	3.5	1694	PASS
441	198	0.01	100	10.0	4863	PASS
442	198	50	100	58.7	28578	PASS
443	442	15	24	19.2	5500	PASS