


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100118\
Data File : BG037094.D
Acq On : 2 Oct 2018 3:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 24 10:41:23 2018

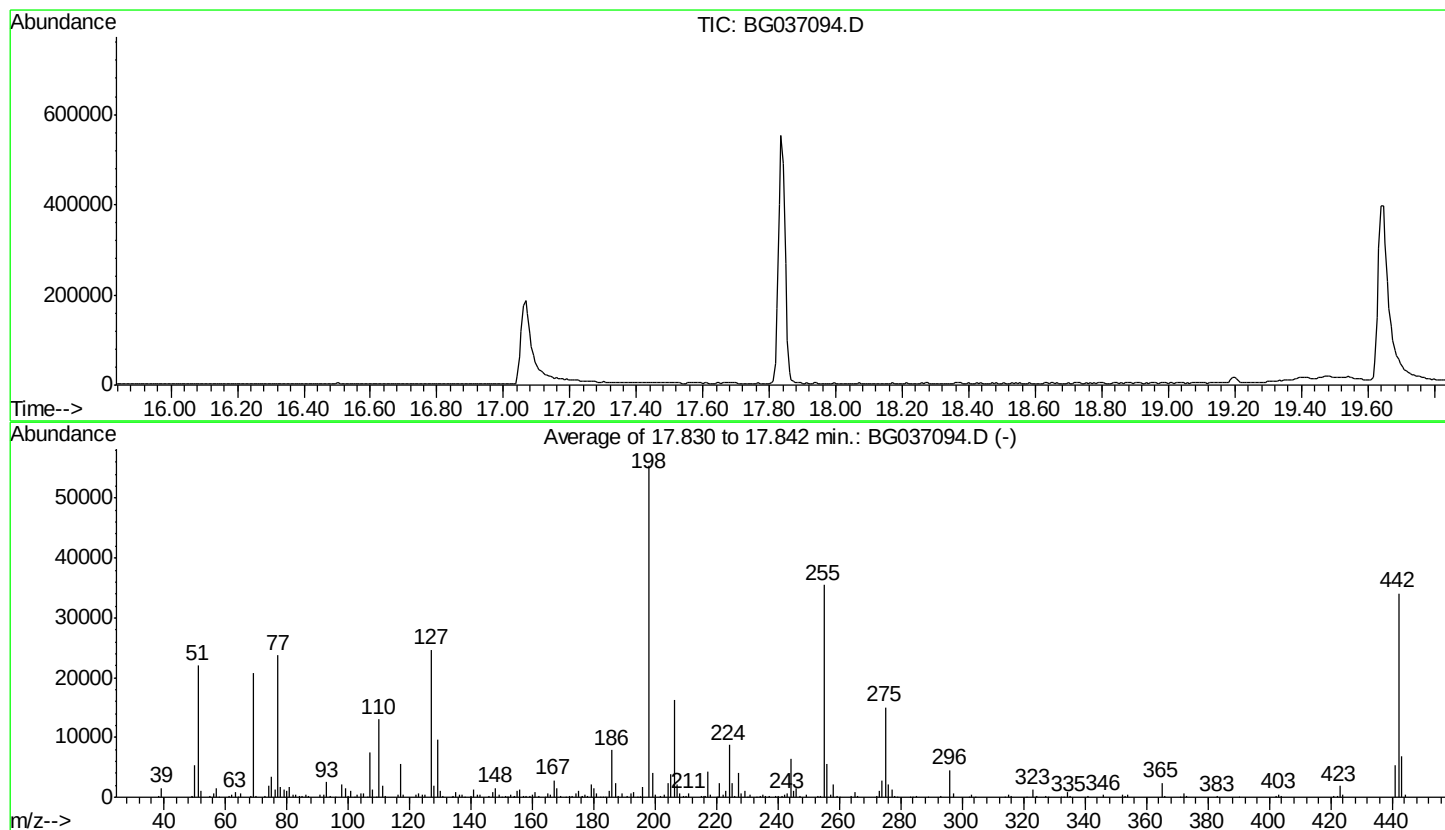

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	22037	PASS
68	69	0.00	2	0.9	184	PASS
69	198	0.00	100	37.4	20728	PASS
70	69	0.00	2	0.6	122	PASS
127	198	10	80	44.5	24666	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55450	PASS
199	198	5	9	7.2	4008	PASS
275	198	10	60	27.1	15008	PASS
365	198	1	100	4.2	2356	PASS
441	198	0.01	100	9.8	5452	PASS
442	198	50	100	61.5	34096	PASS
443	442	15	24	19.9	6783	PASS