


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100219\
 Data File : BG042982.D
 Acq On : 2 Oct 2019 12:35
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 25 15:35:52 2019

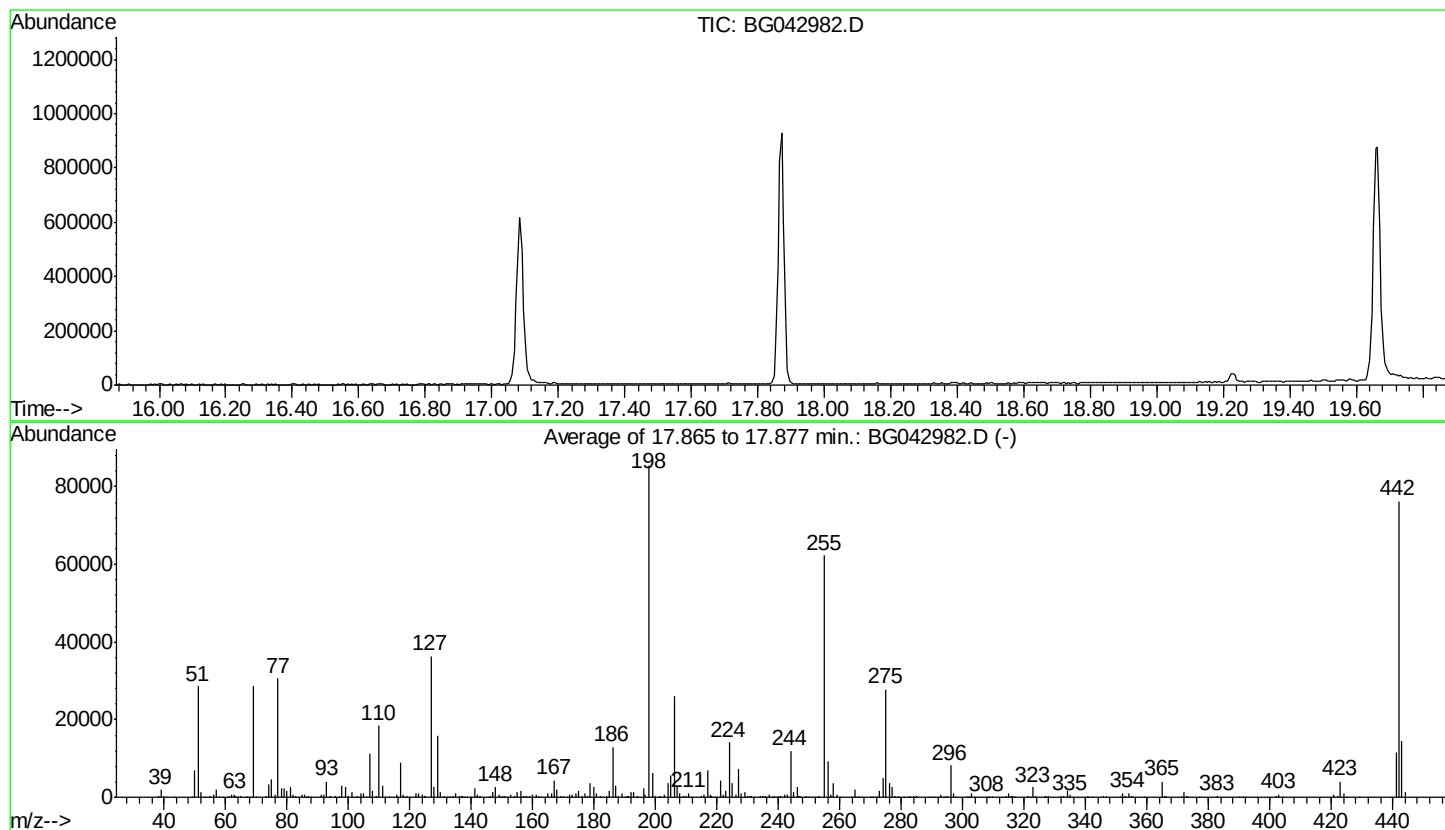

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	28690	PASS
68	69	0.00	2	0.4	108	PASS
69	198	0.00	100	33.5	28656	PASS
70	69	0.00	2	0.5	143	PASS
127	198	10	80	42.5	36312	PASS
197	198	0.00	2	0.7	559	PASS
198	198	100	100	100.0	85450	PASS
199	198	5	9	7.3	6259	PASS
275	198	10	60	32.6	27874	PASS
365	198	1	100	4.7	4012	PASS
441	198	0.01	100	13.5	11561	PASS
442	198	50	100	89.3	76338	PASS
443	442	15	24	18.8	14375	PASS