


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100219\
 Data File : BG043000.D
 Acq On : 3 Oct 2019 1:30
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 25 15:35:52 2019

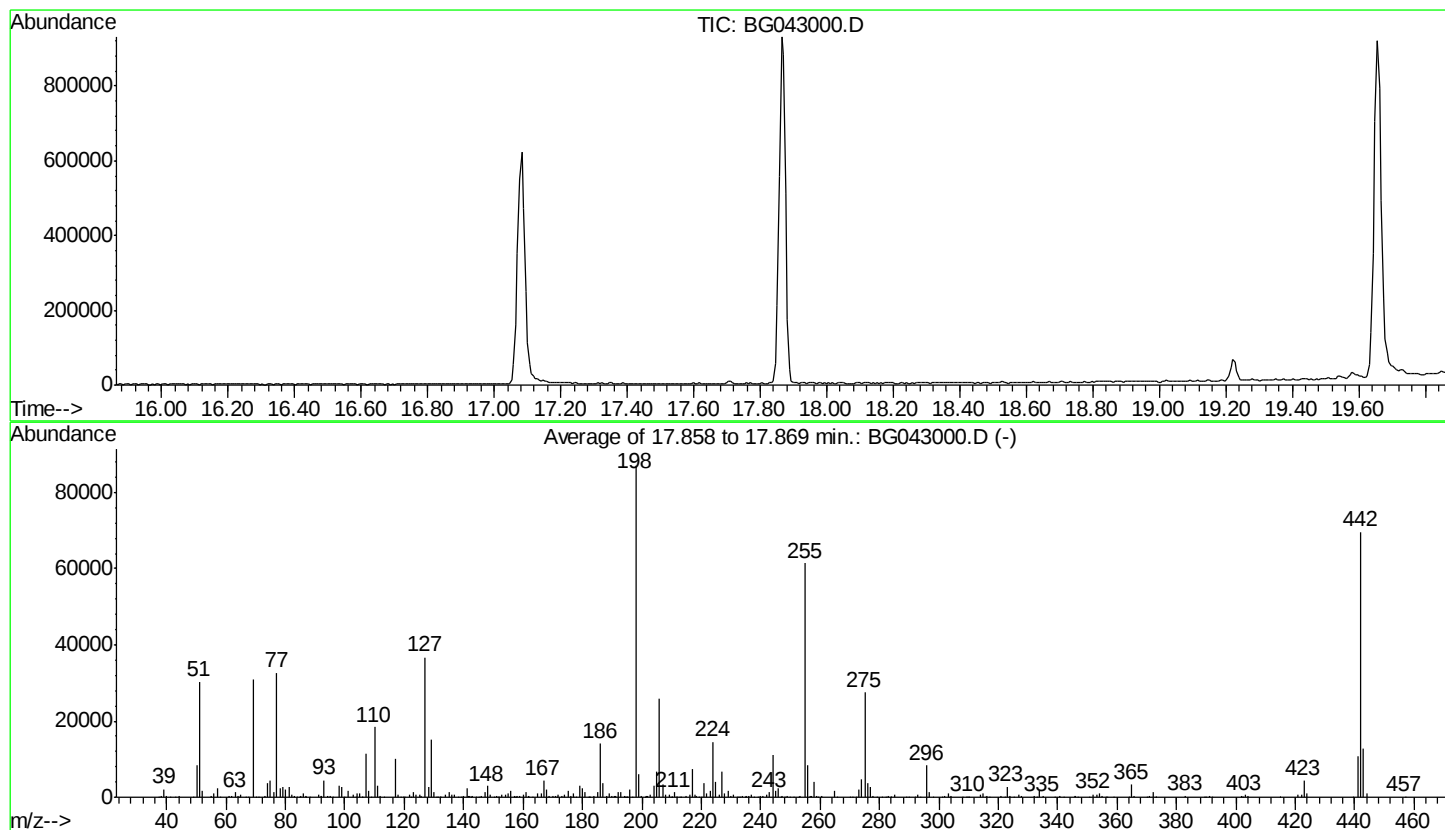

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	30306	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.5	30877	PASS
70	69	0.00	2	0.4	135	PASS
127	198	10	80	42.1	36653	PASS
197	198	0.00	2	0.1	112	PASS
198	198	100	100	100.0	87061	PASS
199	198	5	9	7.0	6107	PASS
275	198	10	60	31.6	27472	PASS
365	198	1	100	3.8	3316	PASS
441	198	0.01	100	12.5	10905	PASS
442	198	50	100	79.9	69597	PASS
443	442	15	24	18.4	12820	PASS