

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
 Data File : BG059247.D
 Acq On : 2 Oct 2023 13:01
 Operator : MA/JU
 Sample : PB155829BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK829

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.528	21	24	29	rVB4	14250	17586	1.10%	0.111%
2	3.963	93	98	114	rBV	222282	391960	24.44%	2.465%
3	4.785	236	238	241	rVB3	2170	2359	0.15%	0.015%
4	5.173	300	304	306	rBV4	1801	2796	0.17%	0.018%
5	5.767	403	405	408	rBV3	2715	2822	0.18%	0.018%
6	5.802	408	411	413	rBV3	2502	3269	0.20%	0.021%
7	6.066	454	456	459	rVB2	3162	2703	0.17%	0.017%
8	6.342	501	503	506	rBV3	2777	3099	0.19%	0.019%
9	6.466	521	524	527	rBV4	2403	2340	0.15%	0.015%
10	6.677	558	560	564	rBV4	2843	2213	0.14%	0.014%
11	7.147	635	640	642	rVB2	3185	4052	0.25%	0.025%
12	7.359	669	676	686	rBV	233952	410623	25.60%	2.582%
13	7.447	689	691	695	rVB2	2766	2435	0.15%	0.015%
14	7.553	702	709	717	rBV	195452	333469	20.79%	2.097%
15	7.747	735	742	749	rBV	220735	383627	23.92%	2.413%
16	7.929	772	773	776	rBV	2889	2161	0.13%	0.014%
17	7.993	782	784	786	rBV	2874	3154	0.20%	0.020%
18	8.228	818	824	833	rBV	171081	292937	18.26%	1.842%
19	8.317	837	839	843	rBV2	2160	2305	0.14%	0.014%
20	8.763	912	915	916	rVB2	2641	2625	0.16%	0.017%
21	8.787	916	919	924	rBV3	2940	5330	0.33%	0.034%
22	8.922	934	942	953	rBV2	285549	496871	30.98%	3.125%
23	9.210	987	991	997	rBV3	2419	3625	0.23%	0.023%
24	9.427	1021	1028	1037	rVB2	226683	396065	24.69%	2.491%
25	9.838	1095	1098	1102	rBV2	1656	2232	0.14%	0.014%
26	10.056	1132	1135	1138	rBV	1797	2661	0.17%	0.017%
27	10.144	1143	1150	1159	rVV	177997	324399	20.22%	2.040%
28	10.355	1182	1186	1188	rVB2	2493	3308	0.21%	0.021%
29	10.673	1233	1240	1248	rBV	273340	495099	30.87%	3.114%
30	11.031	1296	1301	1302	rBV2	3354	4120	0.26%	0.026%
31	11.072	1302	1308	1316	rVB	264284	459177	28.63%	2.888%
32	11.137	1316	1319	1321	rBV	1740	2180	0.14%	0.014%
33	11.219	1326	1333	1347	rBV	300753	547236	34.12%	3.442%
34	11.530	1384	1386	1388	rBV2	3235	2545	0.16%	0.016%
35	11.660	1404	1408	1411	rBV	1860	2480	0.15%	0.016%
36	11.807	1429	1433	1434	rBV	2620	3140	0.20%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
 Data File : BG059247.D
 Acq On : 2 Oct 2023 13:01
 Operator : MA/JU
 Sample : PB155829BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK829

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

37	12.030	1467	1471	1473	rVB2	2065	2644	0.16%	0.017%
38	12.118	1484	1486	1489	rVB2	2425	2266	0.14%	0.014%
39	12.206	1499	1501	1505	rBV2	1963	2176	0.14%	0.014%
40	12.541	1555	1558	1562	rVB	2651	2506	0.16%	0.016%

41	12.641	1569	1575	1577	rBV5	5093	9294	0.58%	0.058%
42	12.717	1585	1588	1591	rVB	2478	2852	0.18%	0.018%
43	12.752	1591	1594	1596	rBV	2802	2870	0.18%	0.018%
44	13.364	1696	1698	1701	rBV	2282	2902	0.18%	0.018%
45	13.693	1751	1754	1757	rBV3	4926	4833	0.30%	0.030%

46	13.745	1760	1763	1764	rBV3	2727	2924	0.18%	0.018%
47	13.792	1767	1771	1774	rBV2	1801	2572	0.16%	0.016%
48	13.839	1777	1779	1783	rBV2	1922	2348	0.15%	0.015%
49	14.092	1820	1822	1824	rVB	3478	2761	0.17%	0.017%
50	14.262	1843	1851	1859	rBV	519052	762708	47.55%	4.797%

51	14.439	1877	1881	1883	rVB2	2685	2418	0.15%	0.015%
52	14.568	1896	1903	1911	rBV	615425	955887	59.59%	6.012%
53	14.797	1939	1942	1946	rBV3	3853	5245	0.33%	0.033%
54	14.868	1946	1954	1961	rBV	412792	627552	39.12%	3.947%
55	15.056	1980	1986	1993	rBV	221827	352086	21.95%	2.214%

56	15.526	2063	2066	2070	rBV3	2757	4531	0.28%	0.028%
57	15.696	2092	2095	2099	rBV3	3744	5273	0.33%	0.033%
58	15.855	2115	2122	2130	rVB	787471	1164118	72.57%	7.321%
59	15.908	2130	2131	2134	rBV2	2366	2238	0.14%	0.014%
60	15.960	2134	2140	2148	rBV	198412	294373	18.35%	1.851%

61	16.172	2172	2176	2177	rBV2	2745	2777	0.17%	0.017%
62	16.201	2177	2181	2183	rVB3	3535	3753	0.23%	0.024%
63	16.278	2191	2194	2195	rBV2	2404	2652	0.17%	0.017%
64	16.348	2203	2206	2209	rVB2	2892	2674	0.17%	0.017%
65	16.536	2236	2238	2241	rBV2	2468	2463	0.15%	0.015%

66	16.795	2281	2282	2285	rVB	3468	2350	0.15%	0.015%
67	16.842	2288	2290	2294	rVB3	1776	2430	0.15%	0.015%
68	17.083	2328	2331	2333	rVB	2789	2899	0.18%	0.018%
69	17.347	2373	2376	2377	rVB	2803	2599	0.16%	0.016%
70	17.412	2381	2387	2390	rVV2	3275	5732	0.36%	0.036%

71	17.494	2399	2401	2404	rBV	2586	2728	0.17%	0.017%
72	17.617	2415	2422	2431	rVB	518354	760278	47.40%	4.781%
73	17.711	2431	2438	2448	rBV2	849152	1296229	80.81%	8.152%
74	17.876	2464	2466	2470	rVB2	3340	4167	0.26%	0.026%
75	17.970	2480	2482	2485	rBV	3391	3341	0.21%	0.021%

76	17.993	2485	2486	2488	rBV	2411	2163	0.13%	0.014%
----	--------	------	------	------	-----	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
 Data File : BG059247.D
 Acq On : 2 Oct 2023 13:01
 Operator : MA/JU
 Sample : PB155829BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK829

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

77	18.540	2577	2579	2582	rBV	2469	3192	0.20%	0.020%
78	18.640	2593	2596	2599	rBV3	2513	3584	0.22%	0.023%
79	18.681	2602	2603	2606	rVB	4056	2327	0.15%	0.015%
80	18.710	2606	2608	2609	rBV2	3553	2316	0.14%	0.015%
81	18.734	2609	2612	2616	rBV4	2292	3445	0.21%	0.022%
82	18.851	2630	2632	2634	rBV2	3043	2424	0.15%	0.015%
83	18.898	2637	2640	2644	rVB4	2566	3758	0.23%	0.024%
84	18.963	2648	2651	2652	rBV3	2933	3284	0.20%	0.021%
85	19.104	2673	2675	2678	rBV3	2917	3182	0.20%	0.020%
86	19.186	2687	2689	2690	rBV	2485	2476	0.15%	0.016%
87	19.374	2718	2721	2722	rBV3	4147	4735	0.30%	0.030%
88	19.409	2725	2727	2730	rVB4	3638	3277	0.20%	0.021%
89	19.503	2742	2743	2745	rBV2	4240	2376	0.15%	0.015%
90	19.550	2748	2751	2755	rVV5	13433	19914	1.24%	0.125%
91	19.615	2756	2762	2768	rVB4	10543	21712	1.35%	0.137%
92	19.991	2819	2826	2832	rBV	1052703	1505417	93.85%	9.468%
93	20.120	2847	2848	2850	rVB2	4734	2267	0.14%	0.014%
94	20.144	2850	2852	2853	rBV2	4622	3684	0.23%	0.023%
95	20.220	2863	2865	2867	rBV2	4107	3630	0.23%	0.023%
96	21.084	3009	3012	3013	rBV3	7518	7993	0.50%	0.050%
97	21.912	3147	3153	3165	rBV2	458505	831716	51.85%	5.231%
98	23.029	3341	3343	3344	rVB2	7681	3682	0.23%	0.023%
99	25.156	3693	3705	3718	rBV2	532750	1604061	100.00%	10.088%
100	25.396	3737	3746	3763	rVB3	293603	918646	57.27%	5.777%




Sum of corrected areas: 15900713

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
Data File : BG059247.D
Acq On : 2 Oct 2023 13:01
Operator : MA/JU
Sample : PB155829BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK829

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

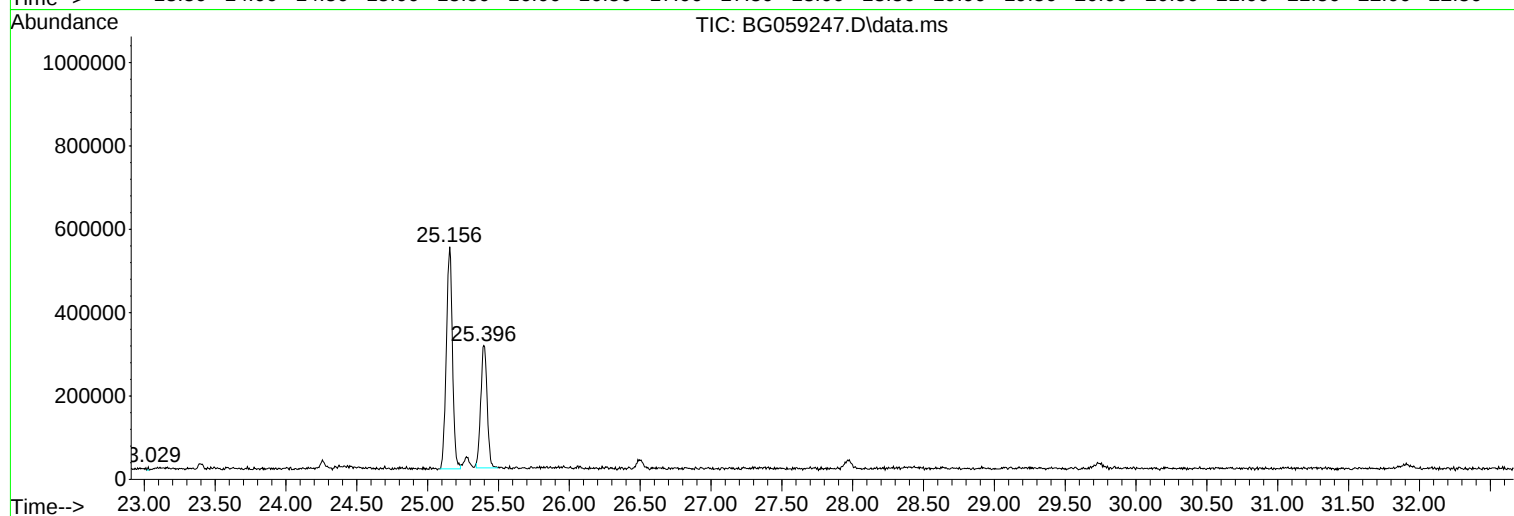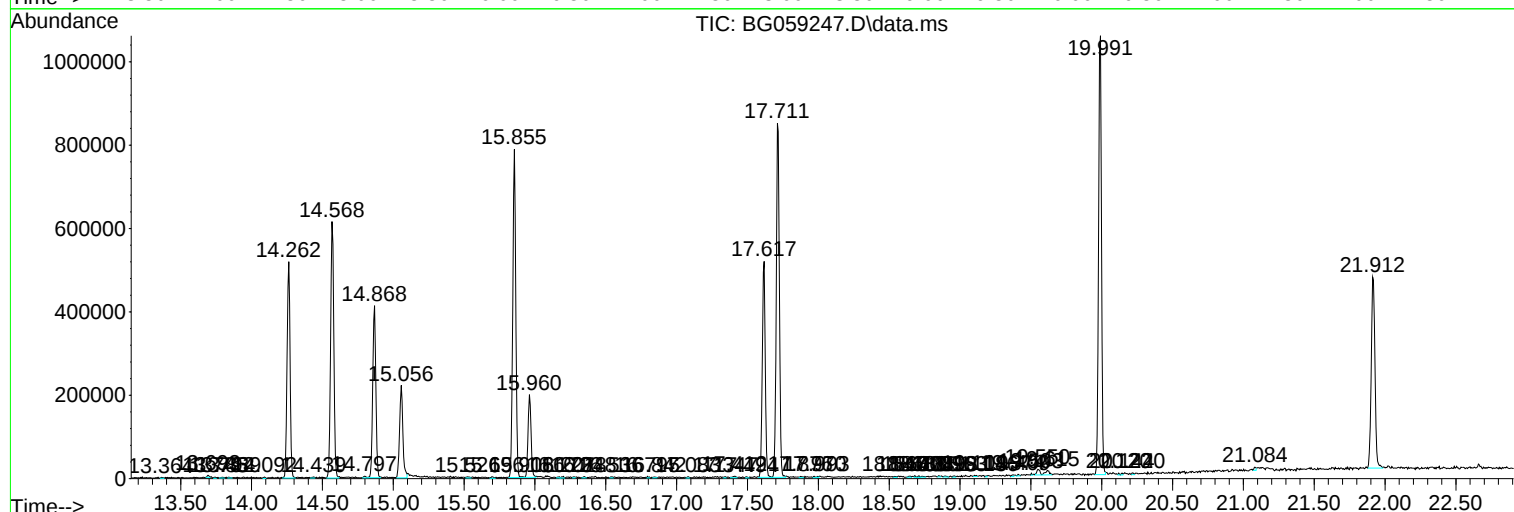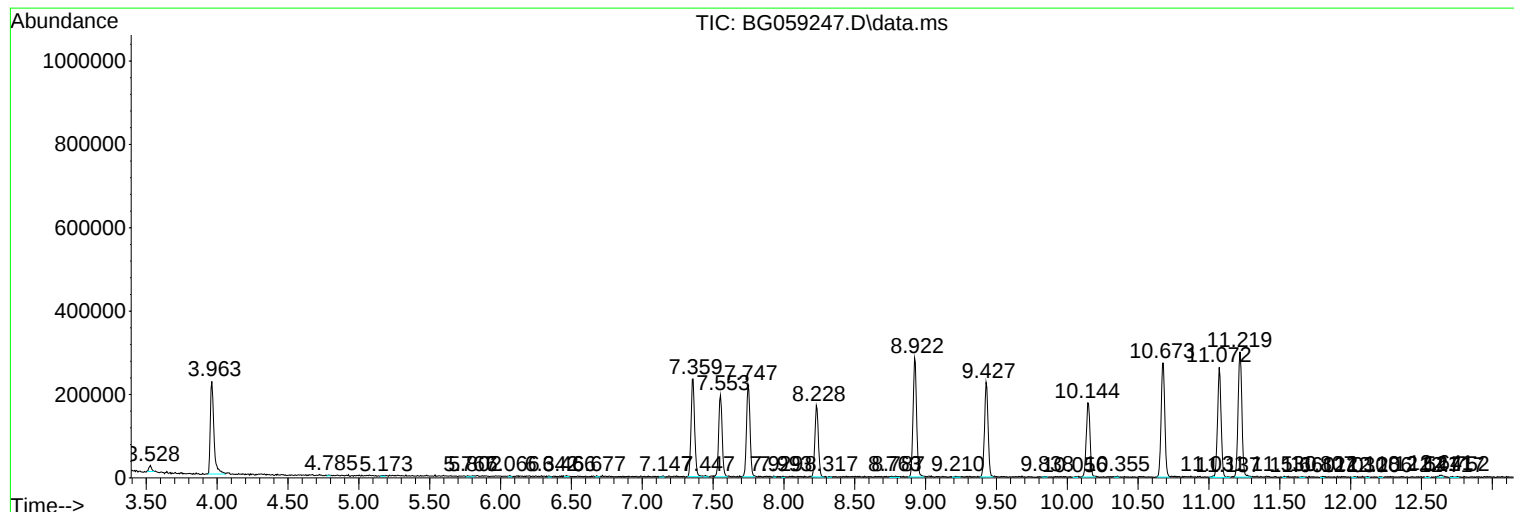

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
Data File : BG059247.D
Acq On : 2 Oct 2023 13:01
Operator : MA/JU
Sample : PB155829BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK829

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
Data File : BG059247.D
Acq On : 2 Oct 2023 13:01
Operator : MA/JU
Sample : PB155829BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK829

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------