

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
 Data File : BG059249.D
 Acq On : 2 Oct 2023 14:26
 Operator : MA/JU
 Sample : 04480-22
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBJE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059249.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.489	11	17	33	rBV	886970	1680903	14.54%	6.646%
2	3.964	94	98	106	rBV	41963	76080	0.66%	0.301%
3	4.176	128	134	140	rBV4	7469	13351	0.12%	0.053%
4	4.840	239	247	262	rBV	6417955	11559881	100.00%	45.703%
5	7.355	669	675	681	rVB	37608	60846	0.53%	0.241%
6	7.548	702	708	716	rVB	132780	220564	1.91%	0.872%
7	7.748	735	742	753	rVB	121355	204840	1.77%	0.810%
8	8.230	817	824	831	rBV	184298	309841	2.68%	1.225%
9	8.923	934	942	950	rBV2	103900	184192	1.59%	0.728%
10	9.429	1019	1028	1038	rVB	156161	282451	2.44%	1.117%
11	10.145	1141	1150	1159	rBV	121063	218578	1.89%	0.864%
12	10.674	1230	1240	1248	rBV2	171312	316957	2.74%	1.253%
13	11.074	1299	1308	1316	rBV	282436	499947	4.32%	1.977%
14	11.221	1325	1333	1341	rBV	164142	297227	2.57%	1.175%
15	14.258	1845	1850	1856	rBV	383822	547195	4.73%	2.163%
16	14.570	1895	1903	1910	rBV	433281	689705	5.97%	2.727%
17	14.869	1947	1954	1961	rVB	449904	699283	6.05%	2.765%
18	15.057	1979	1986	1991	rBV3	24399	50675	0.44%	0.200%
19	15.850	2114	2121	2128	rBV	570929	855511	7.40%	3.382%
20	15.962	2134	2140	2147	rVB	154770	220391	1.91%	0.871%
21	17.613	2413	2421	2428	rBV	555048	844064	7.30%	3.337%
22	17.713	2428	2438	2449	rVB2	649290	966185	8.36%	3.820%
23	18.430	2553	2560	2565	rBV2	17770	28300	0.24%	0.112%
24	19.552	2746	2751	2755	rBV5	8352	14748	0.13%	0.058%
25	19.617	2761	2762	2770	rVB5	13418	17464	0.15%	0.069%
26	19.693	2772	2775	2779	rVV5	9218	12198	0.11%	0.048%
27	19.834	2794	2799	2803	rBV4	16631	22466	0.19%	0.089%
28	19.987	2818	2825	2834	rBV	824651	1154300	9.99%	4.564%
29	20.880	2973	2977	2980	rVB6	9532	13497	0.12%	0.053%
30	21.462	3073	3076	3080	rBV6	6854	13267	0.11%	0.052%
31	21.914	3147	3153	3162	rBV2	512609	893159	7.73%	3.531%
32	22.020	3170	3171	3177	rVB6	9059	12301	0.11%	0.049%
33	22.525	3252	3257	3260	rBV7	8619	16023	0.14%	0.063%
34	23.406	3404	3407	3413	rVB8	12584	20385	0.18%	0.081%
35	23.594	3434	3439	3446	rBV6	16762	38384	0.33%	0.152%
36	24.258	3546	3552	3556	rBV6	14317	23925	0.21%	0.095%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
Data File : BG059249.D
Acq On : 2 Oct 2023 14:26
Operator : MA/JU
Sample : 04480-22
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJE7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Title : SVOA CALIBRATION

37	25.151	3693	3704	3716	rBV3	403572	1182971	10.23%	4.677%
38	25.392	3736	3745	3757	rVB3	318676	988134	8.55%	3.907%
39	26.497	3926	3933	3935	rBV7	15444	31482	0.27%	0.124%
40	30.445	4602	4605	4608	rBV5	8762	11682	0.10%	0.046%




Sum of corrected areas: 25293353

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
Data File : BG059249.D
Acq On : 2 Oct 2023 14:26
Operator : MA/JU
Sample : 04480-22
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

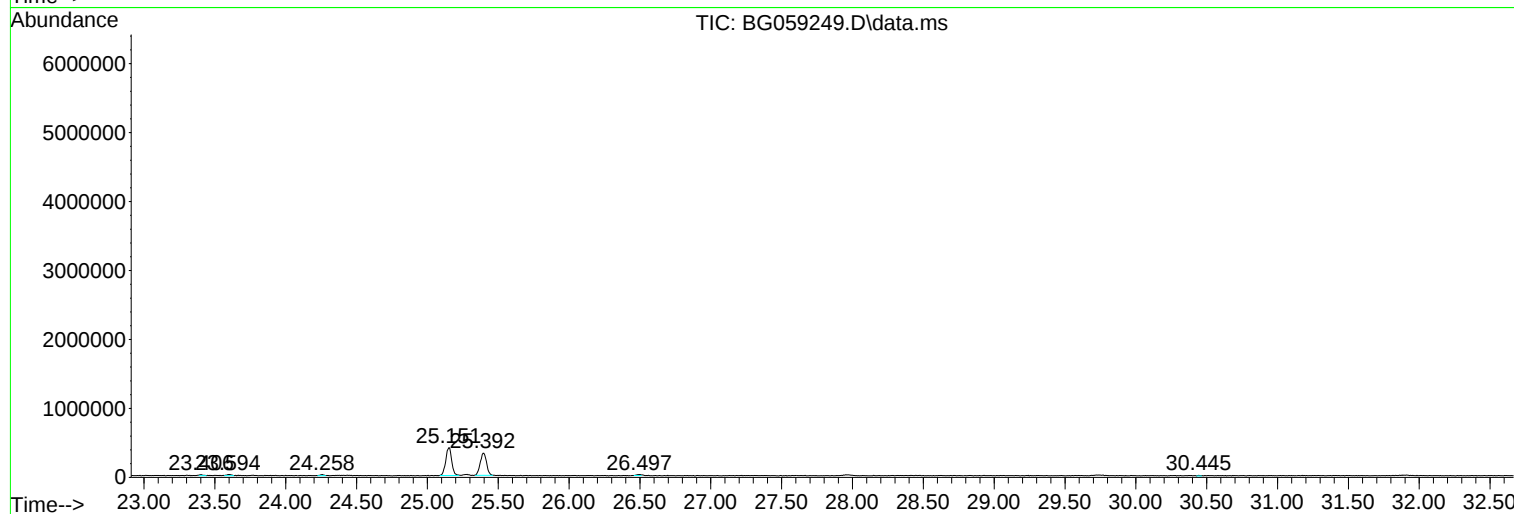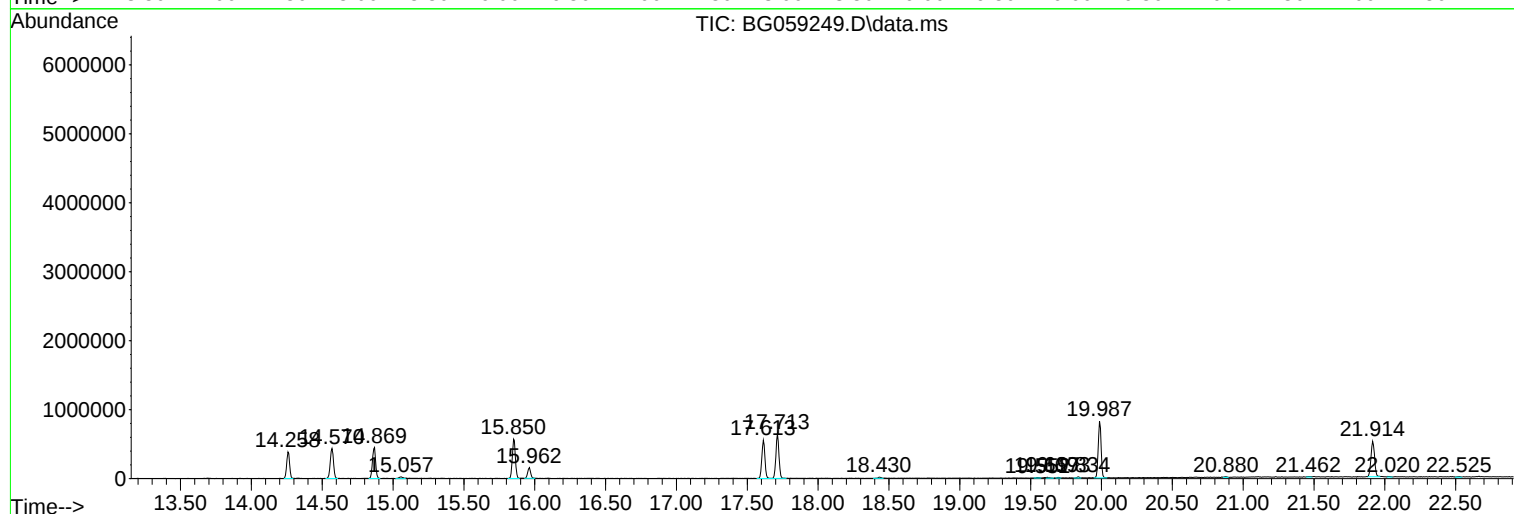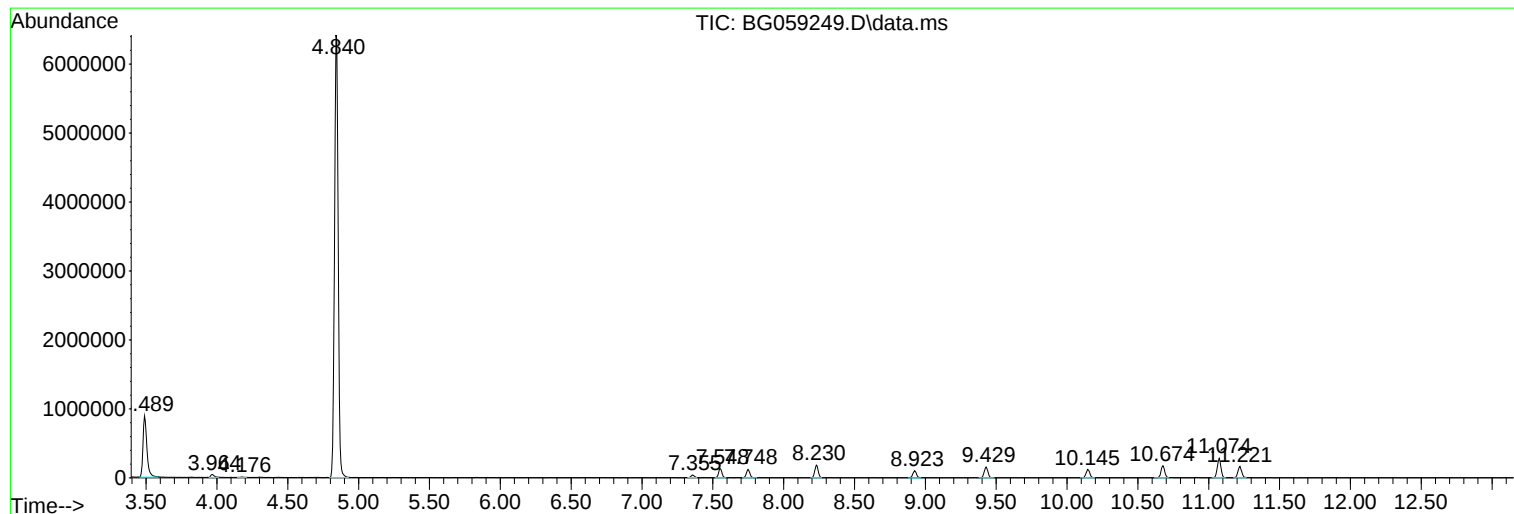

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
Data File : BG059249.D
Acq On : 2 Oct 2023 14:26
Operator : MA/JU
Sample : 04480-22
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJE7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.840	746.18 ng/ul	11559900	1,4-Dichlorobenzene-d4	8.230

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	32

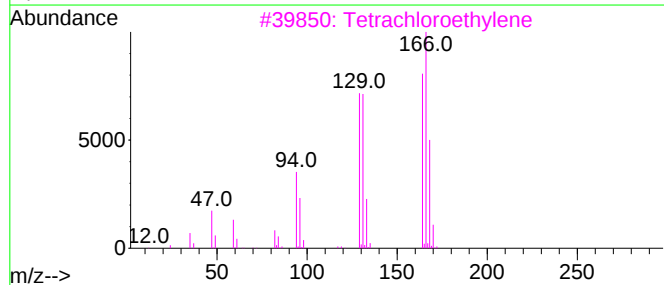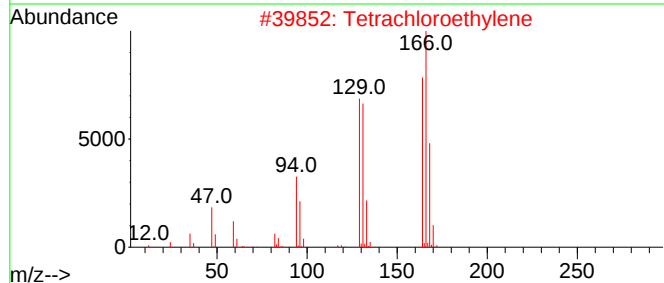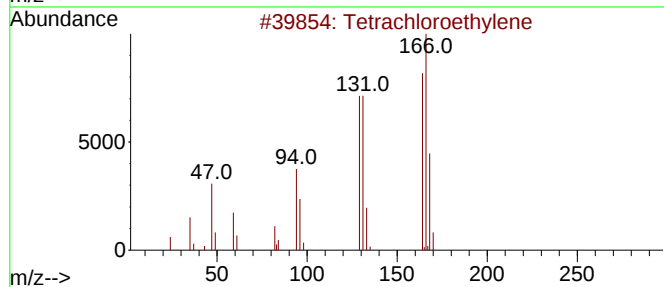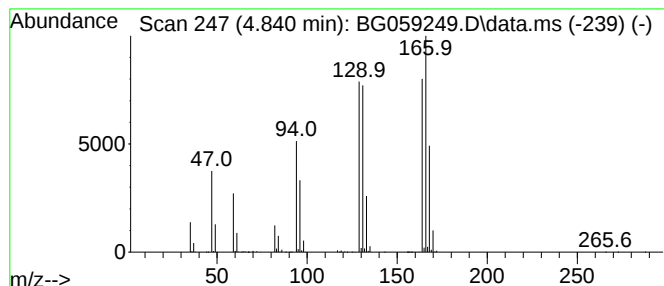

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
Data File : BG059249.D
Acq On : 2 Oct 2023 14:26
Operator : MA/JU
Sample : 04480-22
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.840	746.2	ng/ul	11559900	1	8.230	309841	20.0