

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
 Data File : BG059250.D
 Acq On : 2 Oct 2023 15:29
 Operator : MA/JU
 Sample : 04480-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBHS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.528	19	24	28	rBV4	13944	24688	2.11%	0.194%
2	3.757	59	63	65	rBV4	3612	5615	0.48%	0.044%
3	3.963	94	98	106	rBV2	54714	88272	7.55%	0.692%
4	4.180	132	135	141	rVB4	10922	16034	1.37%	0.126%
5	4.297	153	155	159	rVB2	6244	6392	0.55%	0.050%
6	4.421	174	176	178	rBV2	3607	3524	0.30%	0.028%
7	4.621	207	210	213	rBV2	2484	3140	0.27%	0.025%
8	4.838	243	247	252	rVB6	10808	17582	1.50%	0.138%
9	4.932	260	263	267	rVB5	3241	4432	0.38%	0.035%
10	5.003	273	275	280	rVB3	2882	3539	0.30%	0.028%
11	5.108	289	293	294	rBV2	2562	2626	0.22%	0.021%
12	5.760	401	404	407	rVB3	3081	3346	0.29%	0.026%
13	5.784	407	408	411	rBV2	3481	3733	0.32%	0.029%
14	5.843	415	418	422	rVV3	3160	4290	0.37%	0.034%
15	5.948	434	436	439	rBV3	2642	2451	0.21%	0.019%
16	6.377	505	509	512	rBV2	1579	2560	0.22%	0.020%
17	6.607	545	548	551	rVV2	3507	3465	0.30%	0.027%
18	6.977	607	611	614	rBV	2208	2459	0.21%	0.019%
19	7.353	669	675	683	rBV3	42328	77348	6.61%	0.607%
20	7.547	703	708	715	rBV	144195	235827	20.16%	1.850%
21	7.746	735	742	750	rVB2	126147	226350	19.35%	1.775%
22	7.934	771	774	777	rBV	2025	2559	0.22%	0.020%
23	8.228	817	824	835	rVB	188872	319127	27.29%	2.503%
24	8.463	860	864	866	rVB3	3080	3263	0.28%	0.026%
25	8.510	870	872	874	rVB2	2960	2619	0.22%	0.021%
26	8.528	874	875	881	rBV2	1903	2728	0.23%	0.021%
27	8.833	924	927	931	rVB2	2414	3073	0.26%	0.024%
28	8.921	936	942	953	rVV	114275	192439	16.45%	1.509%
29	9.297	1003	1006	1010	rBV	2229	3592	0.31%	0.028%
30	9.427	1020	1028	1036	rBV	163620	294116	25.15%	2.307%
31	9.568	1051	1052	1056	rVB	3613	2734	0.23%	0.021%
32	10.003	1123	1126	1130	rBV	1378	2588	0.22%	0.020%
33	10.144	1142	1150	1159	rVV2	131267	234333	20.04%	1.838%
34	10.384	1187	1191	1192	rBV2	2699	2909	0.25%	0.023%
35	10.478	1205	1207	1211	rVB2	2400	2485	0.21%	0.019%
36	10.672	1233	1240	1248	rVB	199272	340740	29.13%	2.672%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
 Data File : BG059250.D
 Acq On : 2 Oct 2023 15:29
 Operator : MA/JU
 Sample : 04480-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBHS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

37	11.072	1300	1308	1317	rVB	294663	507735	43.41%	3.982%
38	11.219	1325	1333	1342	rBV2	181312	342586	29.29%	2.687%
39	11.489	1374	1379	1381	rBV2	1755	2826	0.24%	0.022%
40	12.312	1517	1519	1524	rVB	1994	2776	0.24%	0.022%
41	12.635	1565	1574	1576	rBV2	3927	7250	0.62%	0.057%
42	12.735	1588	1591	1593	rVB	3085	2928	0.25%	0.023%
43	12.981	1629	1633	1634	rBV	2371	3155	0.27%	0.025%
44	13.175	1662	1666	1668	rBV	2695	3527	0.30%	0.028%
45	13.645	1742	1746	1749	rVB	2373	2685	0.23%	0.021%
46	13.692	1749	1754	1759	rBV2	8353	14018	1.20%	0.110%
47	14.080	1817	1820	1824	rBV2	2044	2669	0.23%	0.021%
48	14.262	1844	1851	1857	rBV	383527	566038	48.40%	4.439%
49	14.568	1895	1903	1909	rVV	470985	710892	60.78%	5.575%
50	14.779	1935	1939	1941	rBV	2631	3562	0.30%	0.028%
51	14.797	1941	1942	1947	rVV3	4131	4560	0.39%	0.036%
52	14.867	1947	1954	1962	rVV	446105	710344	60.74%	5.571%
53	15.055	1981	1986	1993	rBV2	27111	49089	4.20%	0.385%
54	15.484	2056	2059	2062	rBV	2935	3475	0.30%	0.027%
55	15.596	2073	2078	2083	rBV2	2911	3855	0.33%	0.030%
56	15.649	2085	2087	2090	rVB2	3092	2509	0.21%	0.020%
57	15.854	2114	2122	2128	rBV	570216	895494	76.57%	7.023%
58	15.960	2134	2140	2147	rBV2	164844	238707	20.41%	1.872%
59	16.084	2157	2161	2165	rBV3	5003	5691	0.49%	0.045%
60	16.236	2184	2187	2190	rBV2	2778	3854	0.33%	0.030%
61	16.366	2206	2209	2212	rBV2	2829	3933	0.34%	0.031%
62	16.483	2226	2229	2234	rBV	2521	5104	0.44%	0.040%
63	16.518	2234	2235	2238	rVV	2483	2702	0.23%	0.021%
64	16.877	2295	2296	2300	rBV2	2048	2594	0.22%	0.020%
65	17.176	2344	2347	2348	rBV	3313	3463	0.30%	0.027%
66	17.476	2395	2398	2401	rBV	3038	3957	0.34%	0.031%
67	17.611	2414	2421	2430	rVV	576622	849772	72.66%	6.665%
68	17.711	2431	2438	2446	rVV	674059	1021094	87.31%	8.008%
69	17.776	2448	2449	2454	rVB3	2949	4001	0.34%	0.031%
70	18.299	2537	2538	2540	rBV	2818	2543	0.22%	0.020%
71	18.375	2548	2551	2552	rBV2	3103	2697	0.23%	0.021%
72	18.428	2555	2560	2567	rBV4	28372	40866	3.49%	0.321%
73	18.845	2629	2631	2636	rVB3	4655	5329	0.46%	0.042%
74	18.992	2654	2656	2658	rBV3	3237	2674	0.23%	0.021%
75	19.221	2693	2695	2699	rBV3	1989	2610	0.22%	0.020%
76	19.380	2721	2722	2725	rBV2	3670	3097	0.26%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
 Data File : BG059250.D
 Acq On : 2 Oct 2023 15:29
 Operator : MA/JU
 Sample : 04480-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBHS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

77	19.456	2733	2735	2736	rBV2	4639	3036	0.26%	0.024%
78	19.556	2747	2752	2756	rBV5	9688	14965	1.28%	0.117%
79	19.597	2756	2759	2761	rBV4	8908	12690	1.09%	0.100%
80	19.697	2773	2776	2782	rVB5	10217	14597	1.25%	0.114%
81	19.791	2790	2792	2793	rBV	3165	2748	0.23%	0.022%
82	19.838	2796	2800	2803	rVV2	23511	27535	2.35%	0.216%
83	19.903	2809	2811	2812	rBV2	3844	3364	0.29%	0.026%
84	19.938	2815	2817	2819	rBV2	5382	4614	0.39%	0.036%
85	19.985	2819	2825	2832	rVV	832812	1169522	100.00%	9.172%
86	20.091	2841	2843	2844	rVB	5310	2553	0.22%	0.020%
87	20.114	2844	2847	2849	rBV4	3450	3764	0.32%	0.030%
88	20.214	2862	2864	2867	rBV4	4864	6859	0.59%	0.054%
89	20.725	2946	2951	2955	rBV7	8200	17176	1.47%	0.135%
90	20.872	2974	2976	2979	rVB4	16580	17971	1.54%	0.141%
91	21.912	3147	3153	3163	rVB	544472	878865	75.15%	6.893%
92	23.393	3402	3405	3413	rVB5	24625	46138	3.95%	0.362%
93	24.256	3546	3552	3557	rBV4	28907	62726	5.36%	0.492%
94	25.144	3694	3703	3715	rVB	408247	1153828	98.66%	9.049%
95	25.267	3720	3724	3725	rBV3	24144	29295	2.50%	0.230%
96	25.390	3735	3745	3756	rVB2	326054	969183	82.87%	7.601%
97	25.502	3762	3764	3765	rBV2	7024	4348	0.37%	0.034%
98	26.489	3926	3932	3943	rVB3	32703	98023	8.38%	0.769%
99	29.691	4475	4477	4478	rBV2	9873	6829	0.58%	0.054%
100	31.466	4777	4779	4782	rBV3	7244	6050	0.52%	0.047%




Sum of corrected areas: 12750318

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
Data File : BG059250.D
Acq On : 2 Oct 2023 15:29
Operator : MA/JU
Sample : 04480-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBHS8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

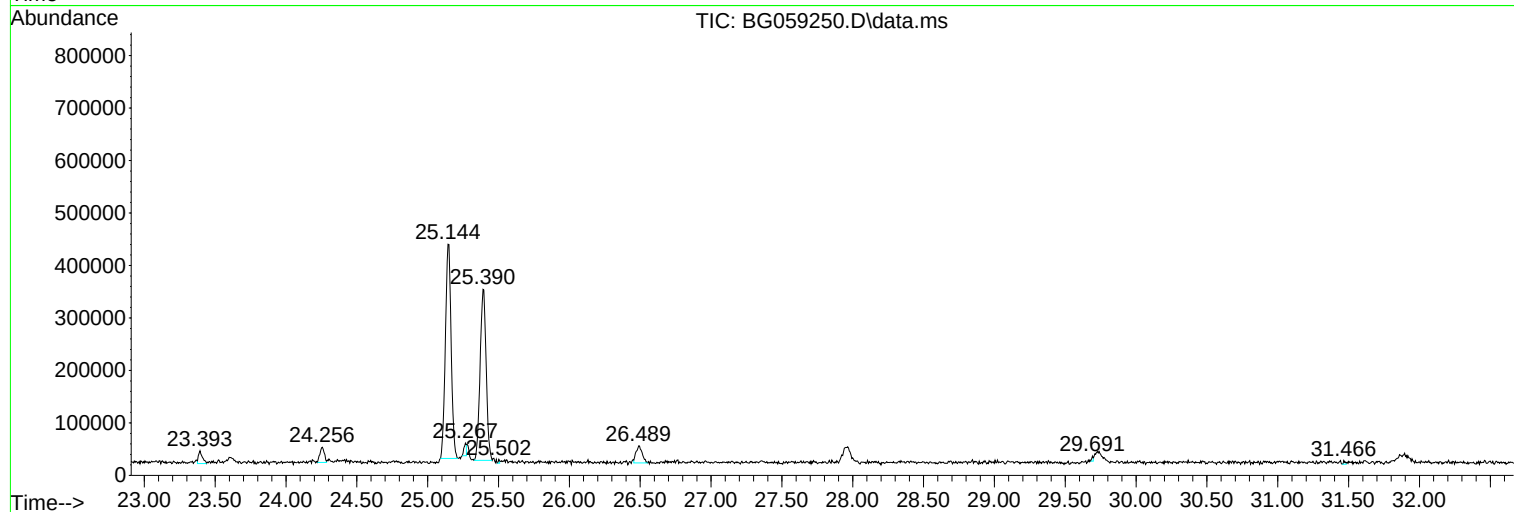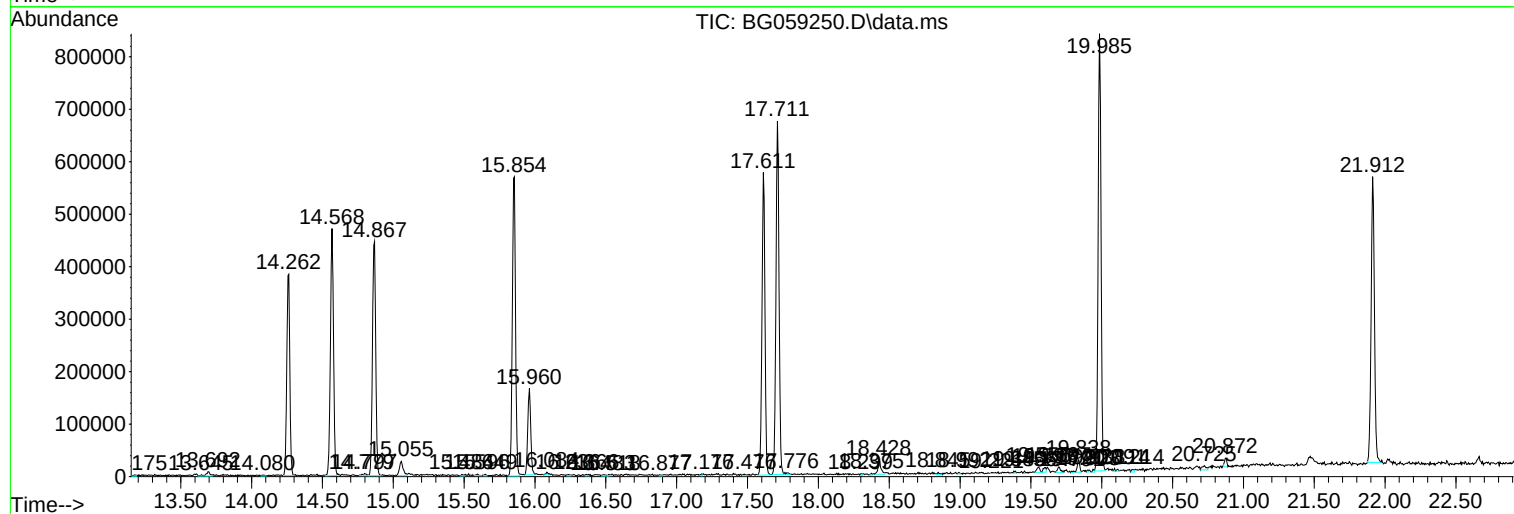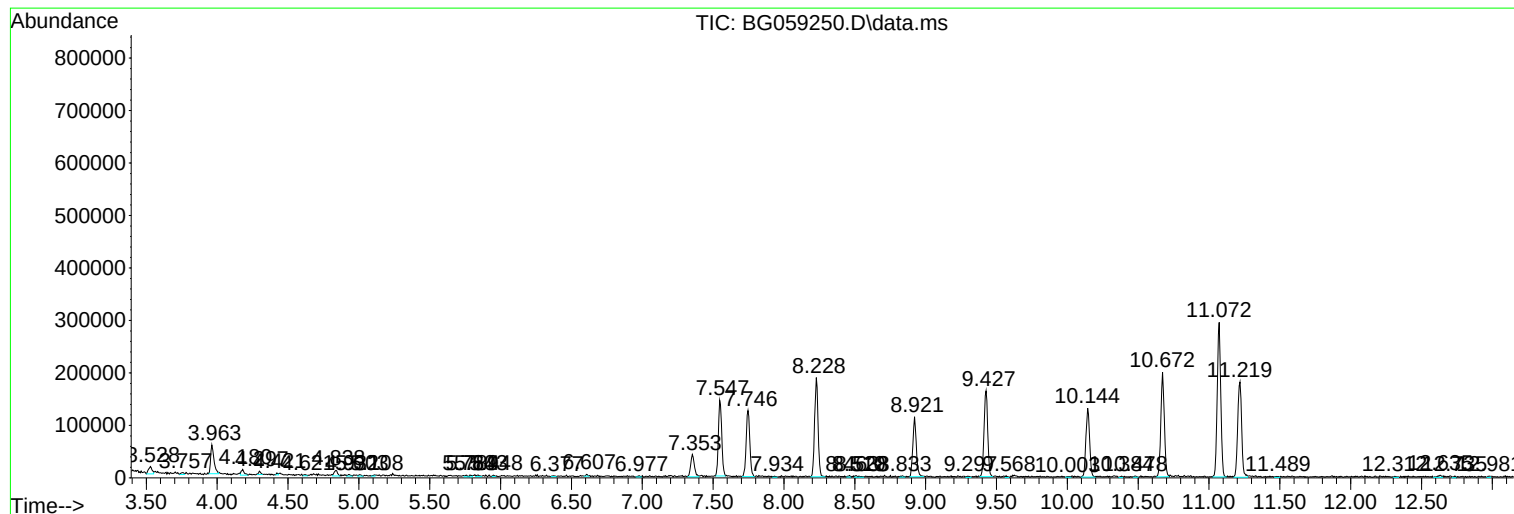

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
Data File : BG059250.D
Acq On : 2 Oct 2023 15:29
Operator : MA/JU
Sample : 04480-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBHS8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
26.489	2.02 ng/ul	98023	Perylene-d12	25.390

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Eicosane	282	C20H42	000112-95-8	62
2			Sulfurous acid, butyl undecyl ester	292	C15H32O3S	1000309-17-8	59
3			Di-n-decylsulfone	346	C20H42O2S	111530-37-1	59
4			Pentadecane	212	C15H32	000629-62-9	53
5			5-Butyl-5-ethylheptadecane	324	C23H48	1000360-43-0	53

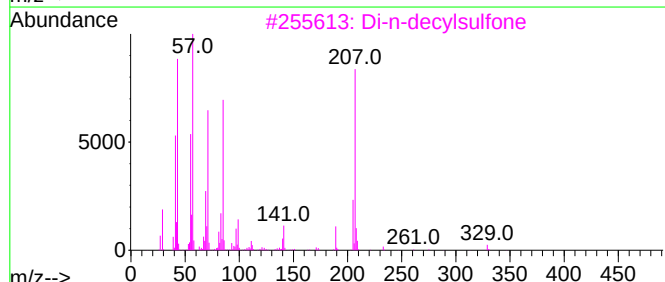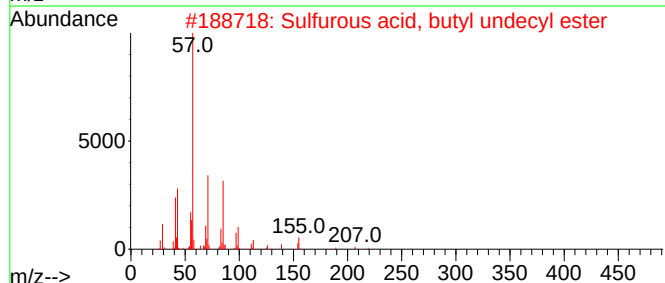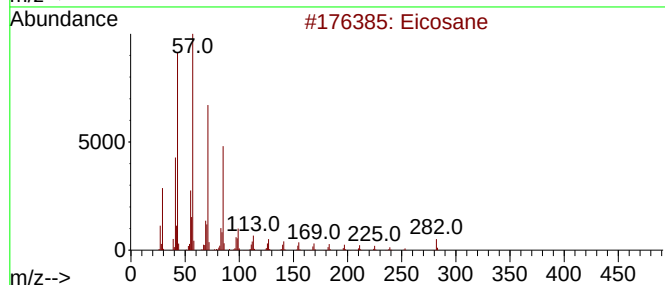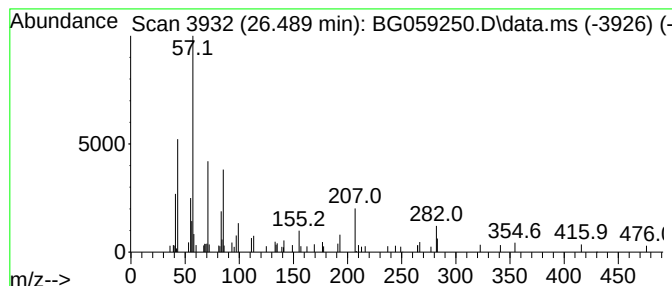

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
Data File : BG059250.D
Acq On : 2 Oct 2023 15:29
Operator : MA/JU
Sample : 04480-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBHS8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	26.489	2.0	ng/u1	98023	6	25.390	969183	20.0