

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
 Data File : BG059251.D
 Acq On : 2 Oct 2023 16:16
 Operator : MA/JU
 Sample : 04480-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBJY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059251.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.467	11	13	15	rBV2	3692	3468	0.22%	0.023%
2	3.526	19	23	27	rVV4	13747	18886	1.20%	0.126%
3	3.708	52	54	56	rBV3	2972	3230	0.20%	0.022%
4	3.961	93	97	105	rBV	87294	149411	9.46%	1.000%
5	4.173	129	133	138	rVB7	8821	14947	0.95%	0.100%
6	4.437	173	178	179	rBV3	3595	4388	0.28%	0.029%
7	4.690	220	221	225	rBV3	3227	2813	0.18%	0.019%
8	4.831	243	245	247	rBV2	2633	2667	0.17%	0.018%
9	5.001	272	274	277	rVB2	2322	2197	0.14%	0.015%
10	5.083	286	288	291	rVB2	2552	2511	0.16%	0.017%
11	5.236	312	314	319	rVB4	2921	2835	0.18%	0.019%
12	5.553	367	368	371	rBV3	2780	2178	0.14%	0.015%
13	6.111	460	463	464	rBV3	3169	2595	0.16%	0.017%
14	6.323	495	499	502	rBV4	1944	2700	0.17%	0.018%
15	6.599	544	546	550	rVB4	2678	3340	0.21%	0.022%
16	7.145	635	639	642	rBV3	2368	4046	0.26%	0.027%
17	7.192	642	647	649	rBV3	3472	3484	0.22%	0.023%
18	7.357	668	675	682	rVB2	79084	136207	8.63%	0.912%
19	7.469	693	694	698	rBV2	2062	2250	0.14%	0.015%
20	7.551	701	708	715	rVB	172165	277583	17.58%	1.858%
21	7.651	721	725	727	rVB3	2497	2778	0.18%	0.019%
22	7.745	734	741	751	rBV	156334	275925	17.48%	1.847%
23	8.021	786	788	790	rBV2	2772	2459	0.16%	0.016%
24	8.121	804	805	809	rVB3	3124	2284	0.14%	0.015%
25	8.232	816	824	830	rBV	188011	321155	20.34%	2.150%
26	8.697	900	903	907	rBV	2017	3403	0.22%	0.023%
27	8.920	935	941	948	rBV	164212	276579	17.52%	1.852%
28	9.225	989	993	996	rVB	2115	3080	0.20%	0.021%
29	9.261	996	999	1001	rBV	2409	2785	0.18%	0.019%
30	9.425	1020	1027	1034	rBV	204011	350955	22.23%	2.350%
31	9.478	1034	1036	1040	rVB2	3125	4138	0.26%	0.028%
32	9.531	1043	1045	1050	rBV2	2086	2367	0.15%	0.016%
33	9.719	1075	1077	1081	rVB2	2640	3730	0.24%	0.025%
34	9.748	1081	1082	1085	rBV	2971	2438	0.15%	0.016%
35	10.142	1141	1149	1157	rBV	148892	272174	17.24%	1.822%
36	10.218	1159	1162	1166	rVV2	2009	3062	0.19%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
 Data File : BG059251.D
 Acq On : 2 Oct 2023 16:16
 Operator : MA/JU
 Sample : 04480-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBJY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

37	10.312	1176	1178	1181	rVB2	2294	2459	0.16%	0.016%
38	10.442	1198	1200	1203	rVB	2109	2124	0.13%	0.014%
39	10.536	1213	1216	1218	rBV	2429	2374	0.15%	0.016%
40	10.671	1232	1239	1249	rBV	220628	402175	25.48%	2.693%
41	10.741	1249	1251	1254	rVB	2206	2140	0.14%	0.014%
42	10.841	1263	1268	1272	rBV2	1911	3959	0.25%	0.027%
43	10.912	1275	1280	1283	rBV	1778	3517	0.22%	0.024%
44	10.947	1283	1286	1294	rVB2	2331	5536	0.35%	0.037%
45	11.070	1299	1307	1319	rVB	284461	516529	32.72%	3.458%
46	11.217	1324	1332	1341	rVV	223400	414058	26.23%	2.772%
47	11.305	1345	1347	1349	rVV	3096	3000	0.19%	0.020%
48	11.335	1349	1352	1354	rVB3	1947	2308	0.15%	0.015%
49	11.399	1360	1363	1365	rBV	1971	2251	0.14%	0.015%
50	11.699	1411	1414	1416	rBV	3473	2782	0.18%	0.019%
51	11.916	1447	1451	1454	rVB	2017	3889	0.25%	0.026%
52	12.163	1489	1493	1496	rVB	1566	2109	0.13%	0.014%
53	12.204	1496	1500	1502	rBV2	2849	2367	0.15%	0.016%
54	12.633	1570	1573	1576	rBV2	3160	3204	0.20%	0.021%
55	12.856	1610	1611	1614	rBV2	2713	2528	0.16%	0.017%
56	13.468	1713	1715	1720	rVB	3517	4673	0.30%	0.031%
57	13.685	1748	1752	1758	rBV3	5494	10009	0.63%	0.067%
58	13.832	1775	1777	1779	rBV2	3437	2927	0.19%	0.020%
59	13.920	1790	1792	1796	rVB	2045	2386	0.15%	0.016%
60	14.184	1835	1837	1839	rVB	3346	3270	0.21%	0.022%
61	14.208	1839	1841	1843	rBV2	2226	2921	0.19%	0.020%
62	14.261	1844	1850	1860	rVB	480715	689330	43.67%	4.615%
63	14.566	1895	1902	1913	rVB2	537788	838308	53.10%	5.613%
64	14.866	1946	1953	1960	rVB	469578	720790	45.66%	4.826%
65	15.054	1977	1985	1992	rBV	67424	121648	7.71%	0.814%
66	15.354	2034	2036	2041	rBV3	1704	2532	0.16%	0.017%
67	15.453	2050	2053	2058	rBV3	2680	4252	0.27%	0.028%
68	15.506	2058	2062	2063	rBV	2268	2170	0.14%	0.015%
69	15.630	2081	2083	2085	rBV	3169	2769	0.18%	0.019%
70	15.853	2114	2121	2128	rBV	695992	1072142	67.92%	7.178%
71	15.959	2133	2139	2146	rVB	234796	330653	20.95%	2.214%
72	16.153	2168	2172	2174	rBV	1948	2519	0.16%	0.017%
73	16.217	2181	2183	2187	rVB2	2335	2559	0.16%	0.017%
74	16.670	2257	2260	2263	rBV2	2087	2261	0.14%	0.015%
75	16.858	2290	2292	2296	rBV2	1731	2165	0.14%	0.014%
76	16.946	2305	2307	2309	rBV2	3823	2110	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
 Data File : BG059251.D
 Acq On : 2 Oct 2023 16:16
 Operator : MA/JU
 Sample : 04480-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBJY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

77	17.069	2326	2328	2330	rBV	2632	2120	0.13%	0.014%
78	17.193	2343	2349	2350	rBV3	2177	3450	0.22%	0.023%
79	17.463	2394	2395	2399	rBV	1882	2152	0.14%	0.014%
80	17.610	2414	2420	2429	rBV	596097	908108	57.52%	6.080%
81	17.710	2429	2437	2448	rVV	870108	1276200	80.84%	8.544%
82	17.839	2457	2459	2462	rBV2	3876	3235	0.20%	0.022%
83	17.933	2473	2475	2481	rBV2	2754	4670	0.30%	0.031%
84	18.426	2555	2559	2569	rBV5	22815	41501	2.63%	0.278%
85	18.644	2590	2596	2597	rBV3	4198	4757	0.30%	0.032%
86	18.990	2651	2655	2657	rBV2	3193	4088	0.26%	0.027%
87	19.220	2692	2694	2695	rBV2	4035	3066	0.19%	0.021%
88	19.549	2747	2750	2753	rVB3	12075	13280	0.84%	0.089%
89	19.619	2760	2762	2766	rVB2	9987	9467	0.60%	0.063%
90	19.695	2770	2775	2777	rBV3	10338	13996	0.89%	0.094%
91	19.837	2795	2799	2800	rBV4	11054	12695	0.80%	0.085%
92	19.983	2818	2824	2832	rBV	1061271	1545184	97.88%	10.345%
93	20.218	2862	2864	2866	rBV3	3380	3782	0.24%	0.025%
94	20.265	2870	2872	2874	rBV3	3972	2821	0.18%	0.019%
95	20.871	2973	2975	2982	rVB5	10412	11139	0.71%	0.075%
96	21.470	3072	3077	3084	rBV8	17847	48929	3.10%	0.328%
97	21.911	3146	3152	3163	rBV2	555888	978878	62.01%	6.554%
98	25.142	3692	3702	3715	rBV2	549770	1578652	100.00%	10.569%
99	25.389	3734	3744	3755	rVB2	369024	1087863	68.91%	7.283%
100	31.646	4808	4809	4811	rBV2	7123	3324	0.21%	0.022%




Sum of corrected areas: 14936108

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
Data File : BG059251.D
Acq On : 2 Oct 2023 16:16
Operator : MA/JU
Sample : 04480-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

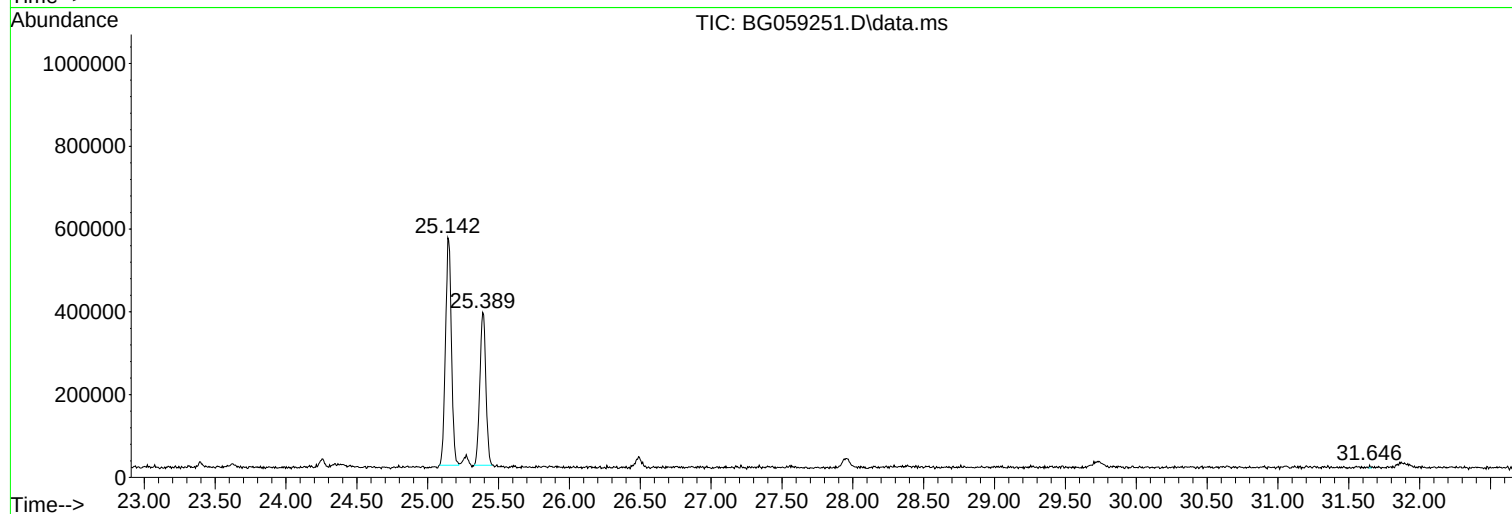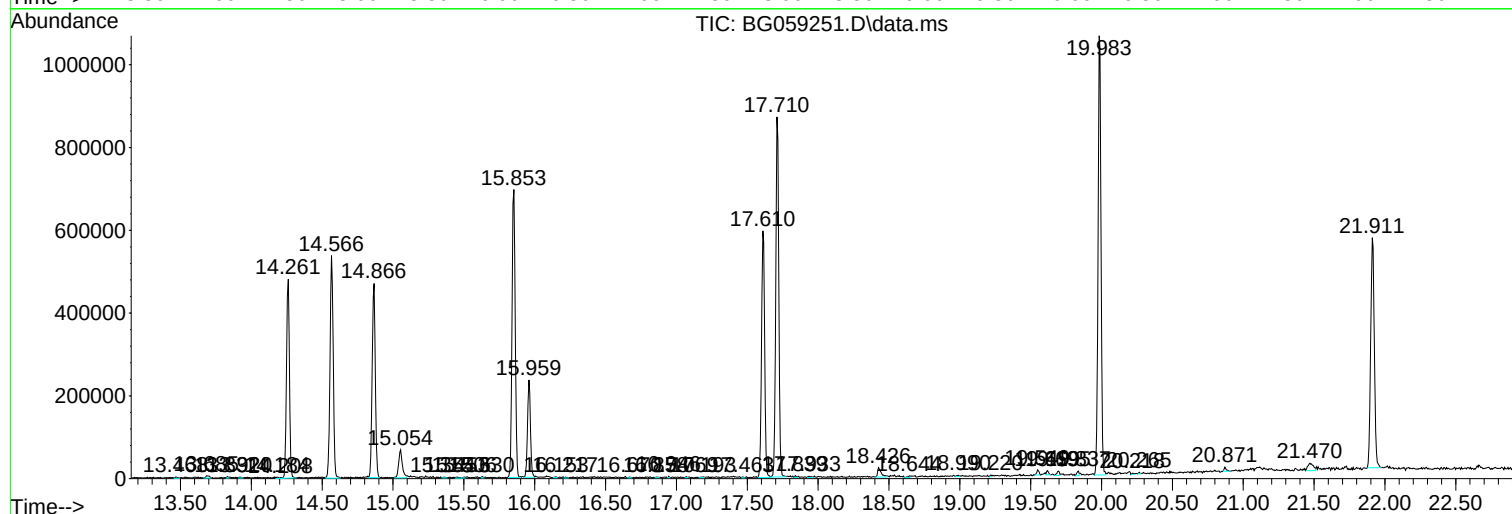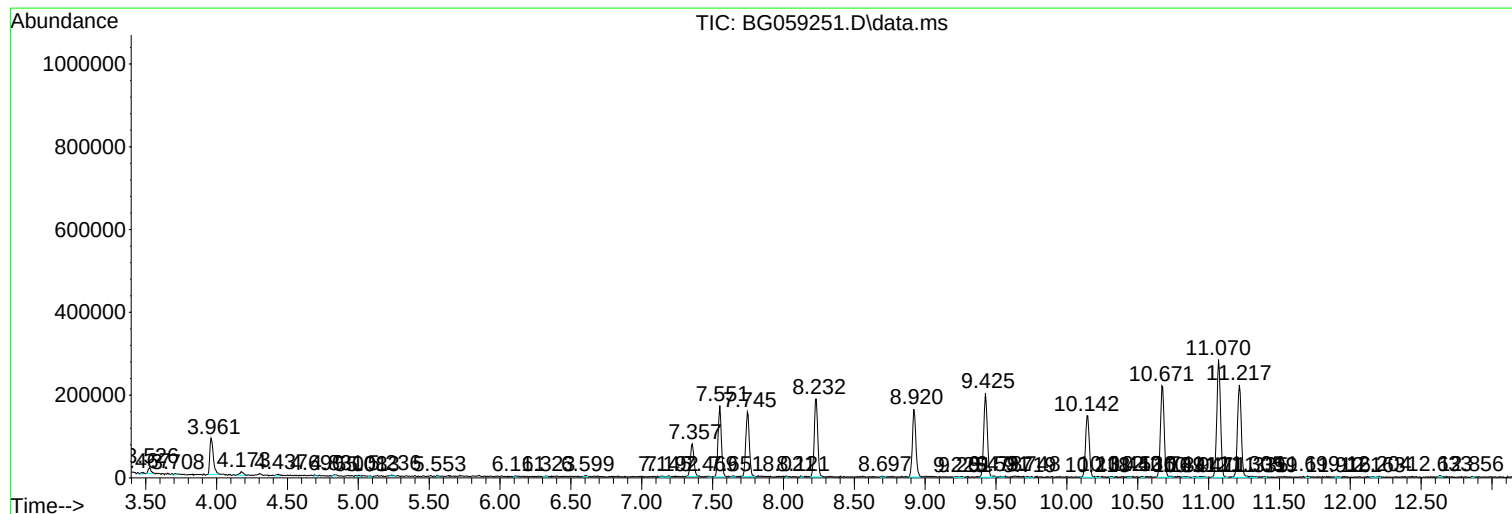

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
Data File : BG059251.D
Acq On : 2 Oct 2023 16:16
Operator : MA/JU
Sample : 04480-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100223\
Data File : BG059251.D
Acq On : 2 Oct 2023 16:16
Operator : MA/JU
Sample : 04480-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------