

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG100318\
 Data File : BG037130.D
 Acq On : 3 Oct 2018 11:33
 Operator : JU/SJ
 Sample : J5123-13
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B51

Quant Time: Oct 03 12:26:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG082118MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 23 01:44:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	48817	20.00	ng/ul	-0.04
18) Naphthalene-d8	10.84	136	204411	20.00	ng/ul	-0.04
36) Acenaphthene-d10	14.66	164	121600	20.00	ng/ul	-0.04
62) Phenanthrene-d10	17.41	188	248829	20.00	ng/ul	-0.03
78) Chrysene-d12	21.68	240	283826	20.00	ng/ul	-0.04
86) Perylene-d12	24.88	264	294496	20.00	ng/ul	-0.06

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL
5) Phenol-d5	0.00	99	0	0.00	ng/ul
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul
44) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul
47) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
58) Fluorene-d10	0.00	176	0d	0.00	ng/ul
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul
79) Pyrene-d10	0.00	212	0d	0.00	ng/ul
90) Benzo(a)pyrene-d12	0.00	264	0	0.00	ng/ul


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
77) Fluoranthene	19.46	202	17673	1.179	ng/ul#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG100318\
Data File : BG037130.D
Acq On : 3 Oct 2018 11:33
Operator : JU/SJ
Sample : J5123-13
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B51

Quant Time: Oct 03 12:26:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG082118MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 23 01:44:31 2018
Response via : Initial Calibration

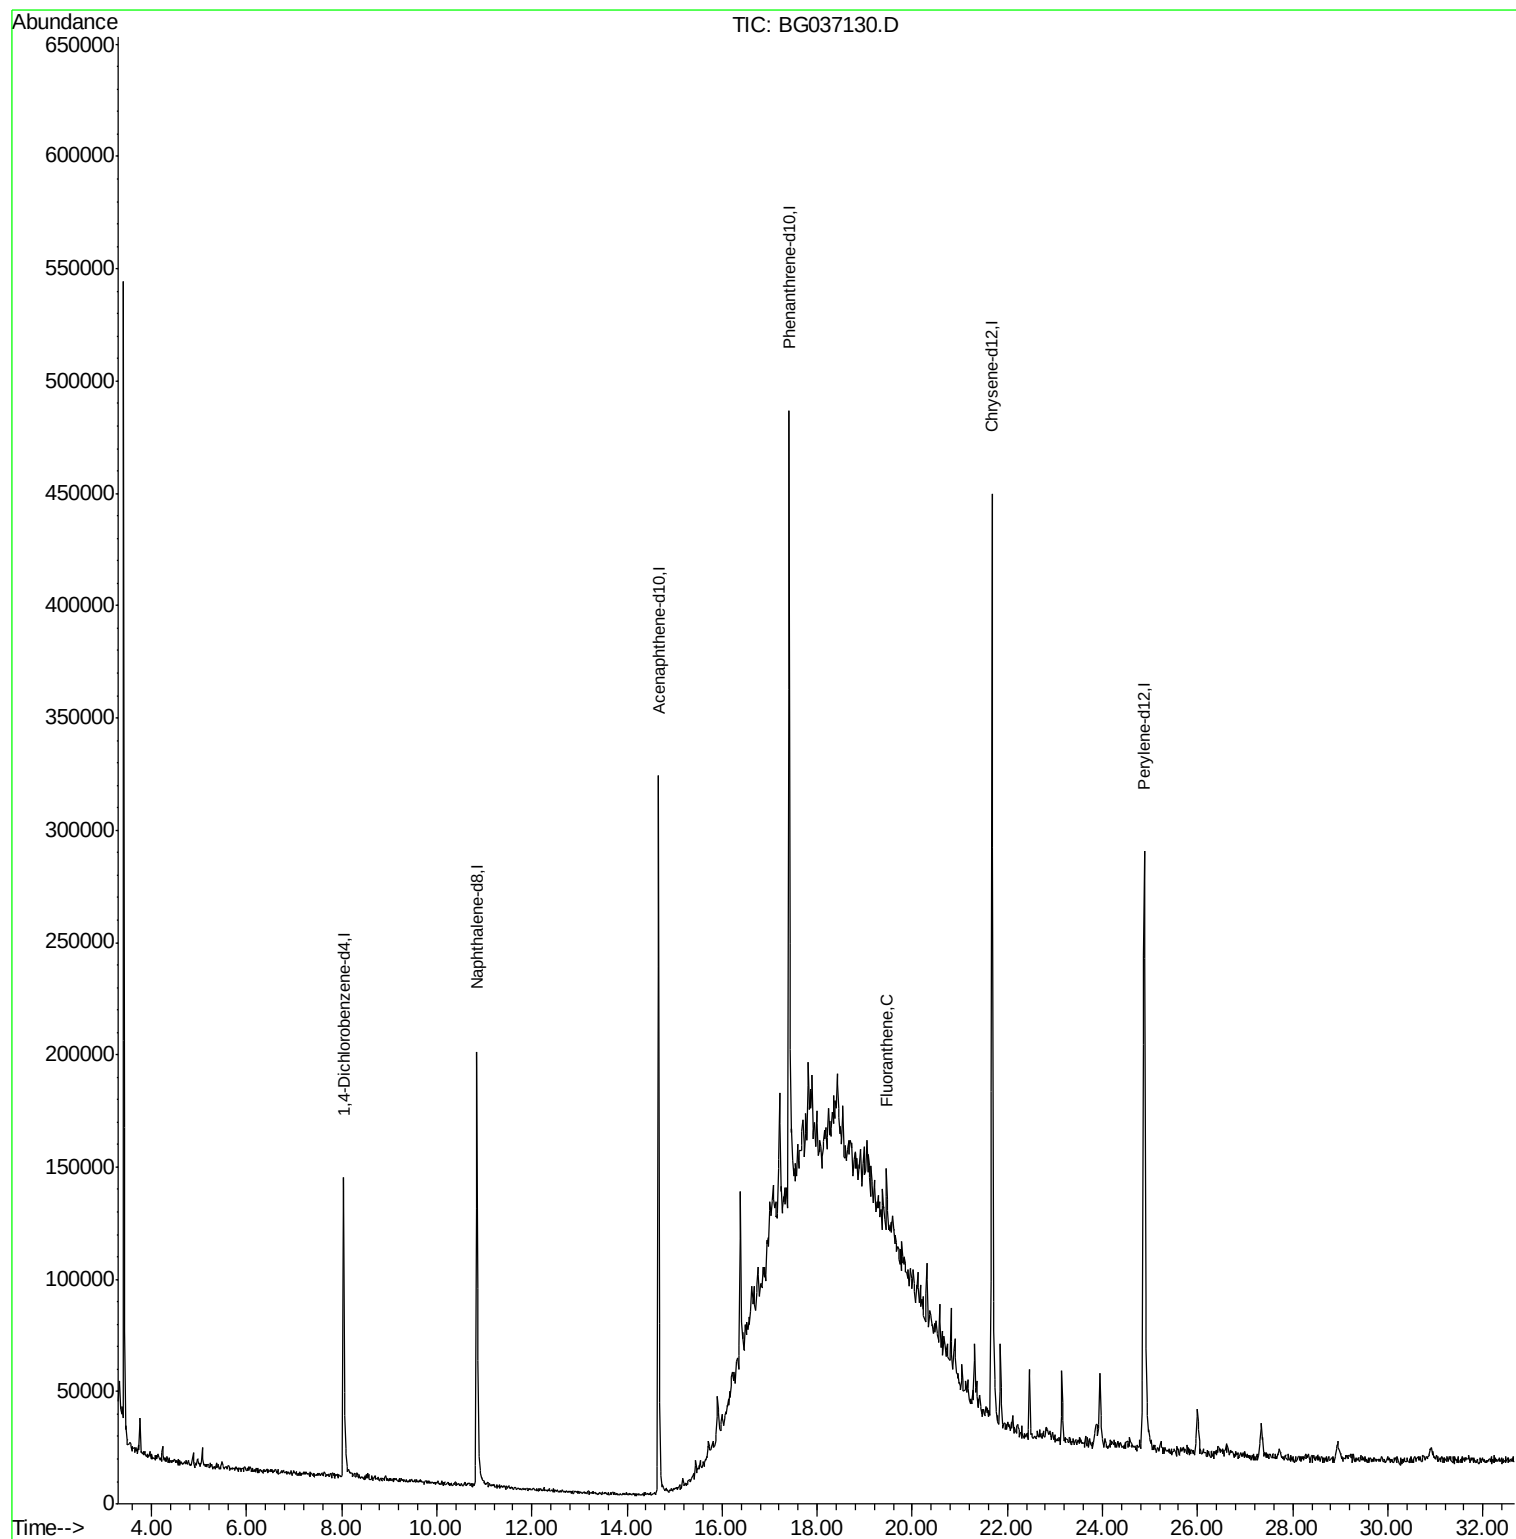


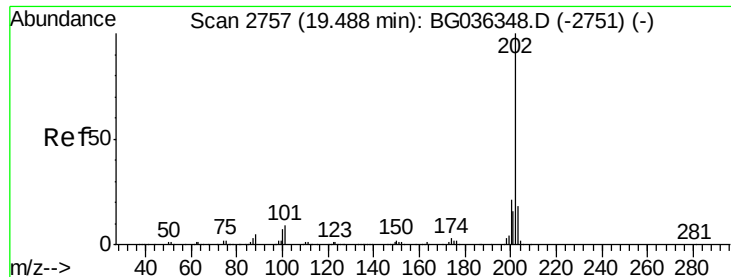

#77
 Fluoranthene
 Concen: 1.179 ng/ul
 RT: 19.46 min Scan# 2752
 Delta R.T. -0.03 min
 Lab File: BG037130.D
 Acq: 3 Oct 2018 11:33

Instrument :
 BNA_G
 ClientSampleId :
 C0B51

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.4	6.1	9.1#
100	9.5	4.6	7.0#

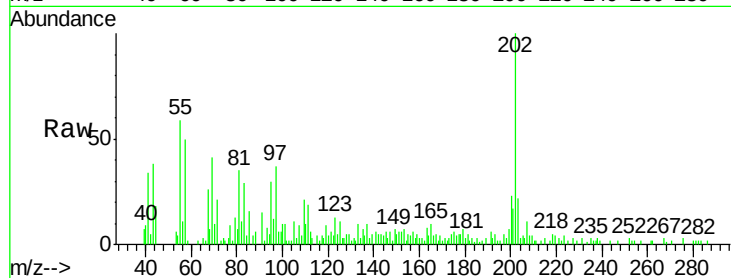

Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

