
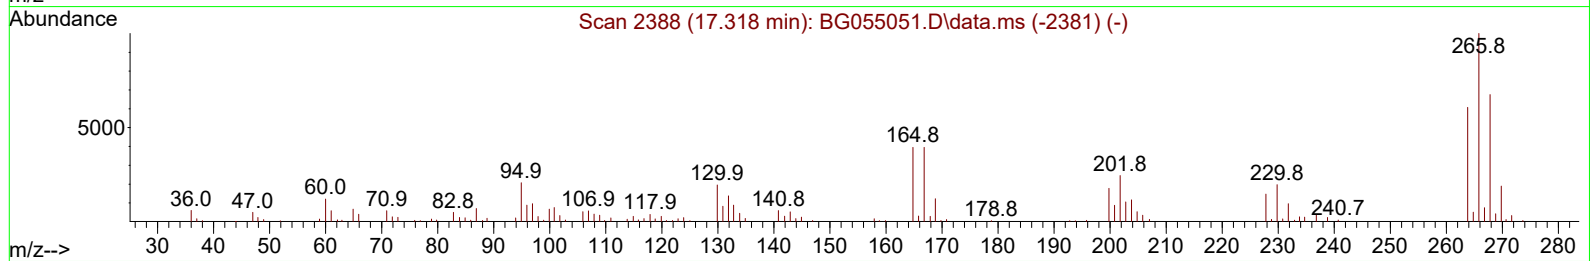
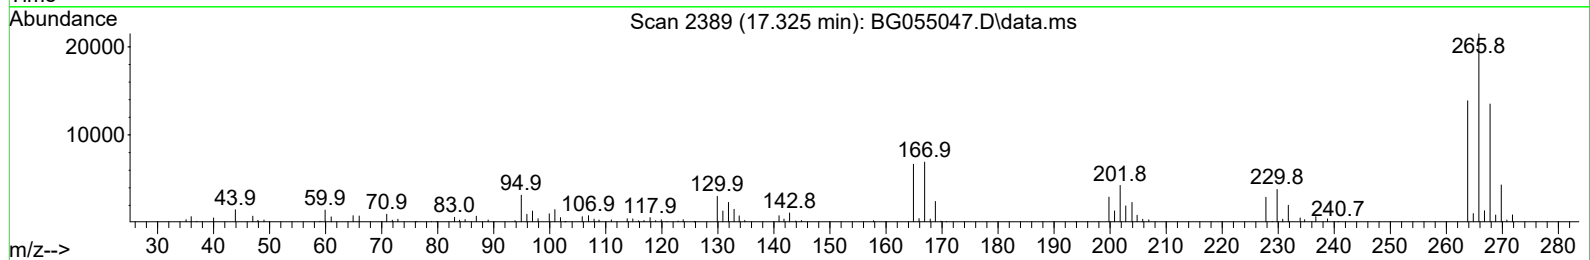


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100322\
Data File : BG055047.D
Acq On : 3 Oct 2022 16:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 04 07:46:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 07:12:22 2022
Response via : Initial Calibration

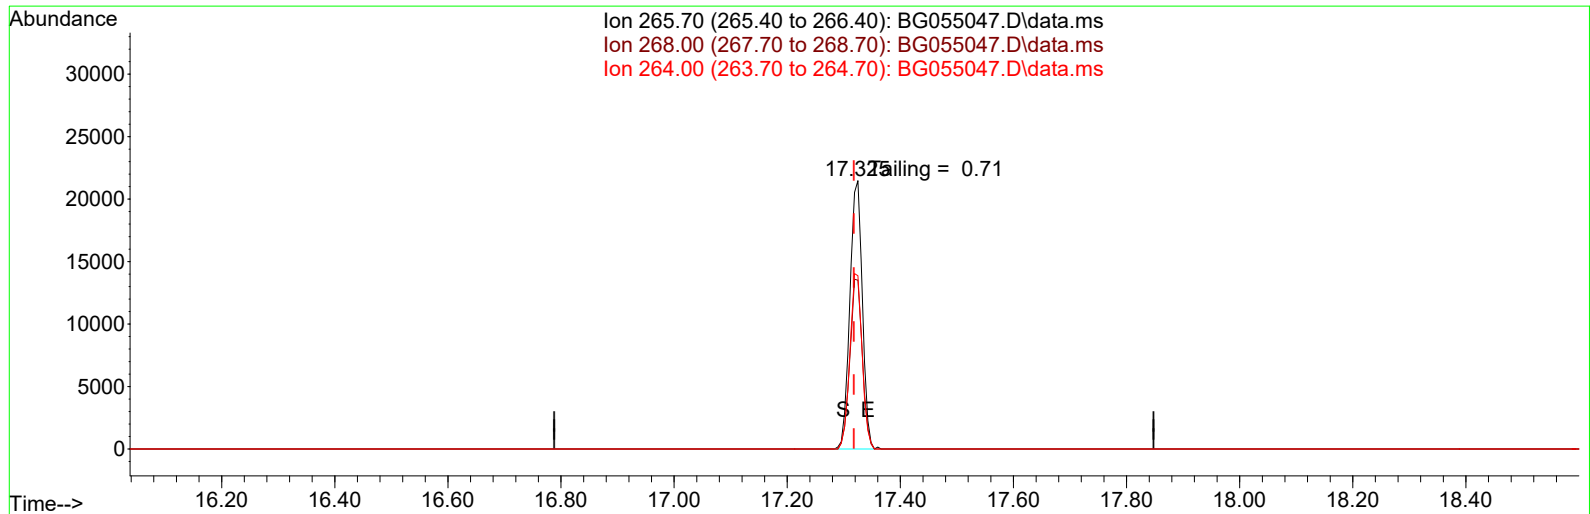

TIC: BG055047.D\data.ms

(70) Pentachlorophenol (C)




17.325min (+ 0.007) 16713.52 ng

response 32927

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	62.93
264.00	60.80	64.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100322\
Data File : BG055047.D
Acq On : 3 Oct 2022 16:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 04 07:46:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 07:12:22 2022
Response via : Initial Calibration

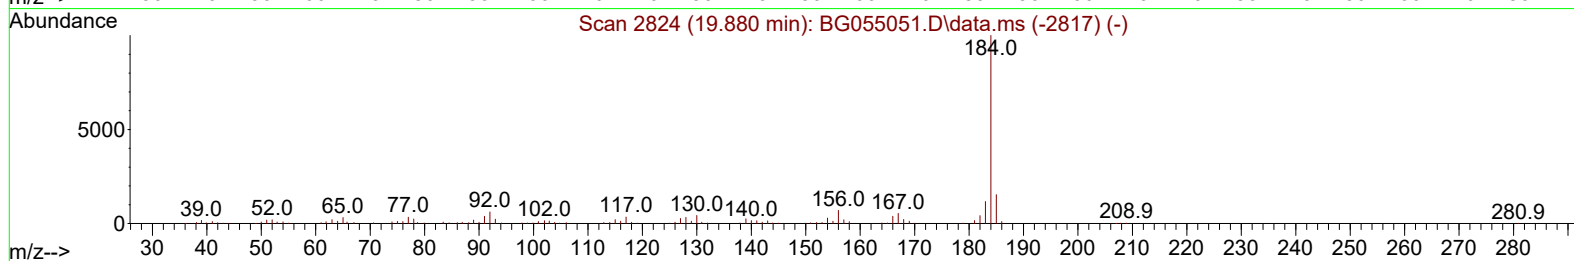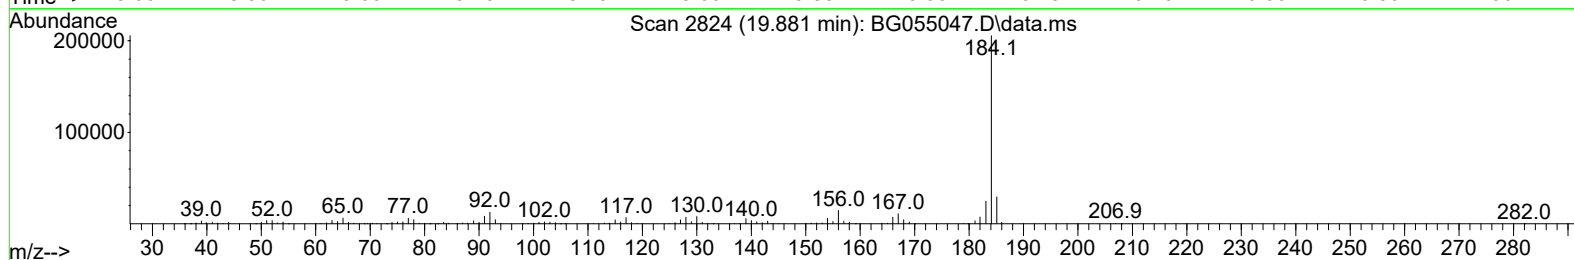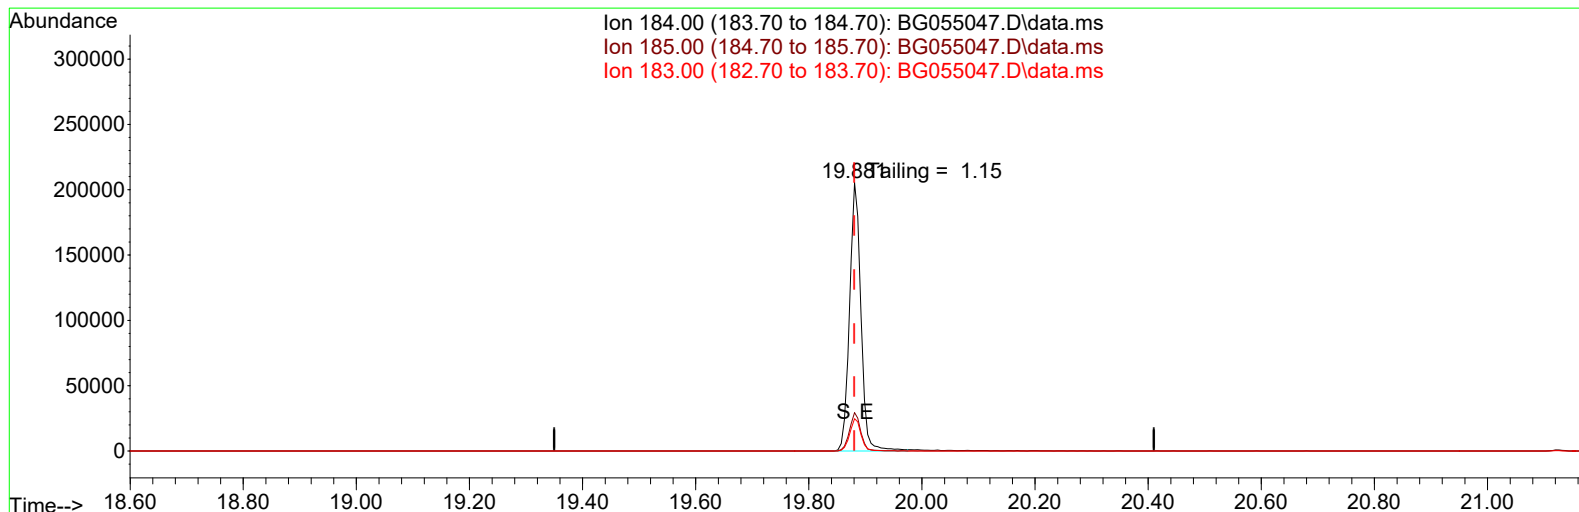

TIC: BG055047.D\data.ms

(77) Benzidine

19.881min (+ 0.001) 0.00 ng

response 289883

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.33
183.00	11.70	12.09
0.00	0.00	0.00