
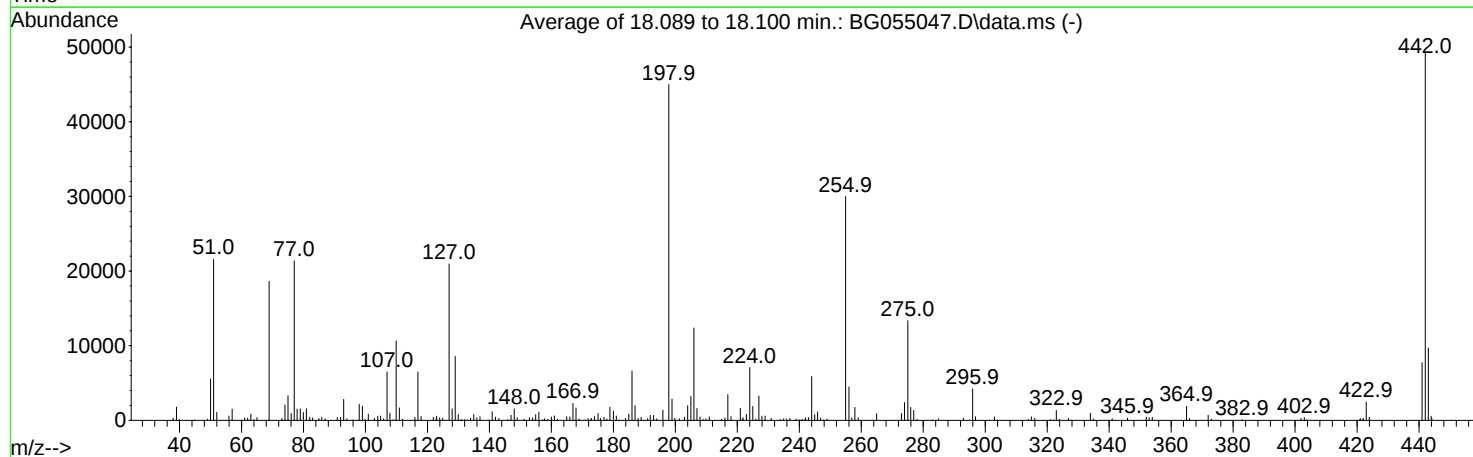


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100322\
 Data File : BG055047.D
 Acq On : 3 Oct 2022 16:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 04 07:12:22 2022

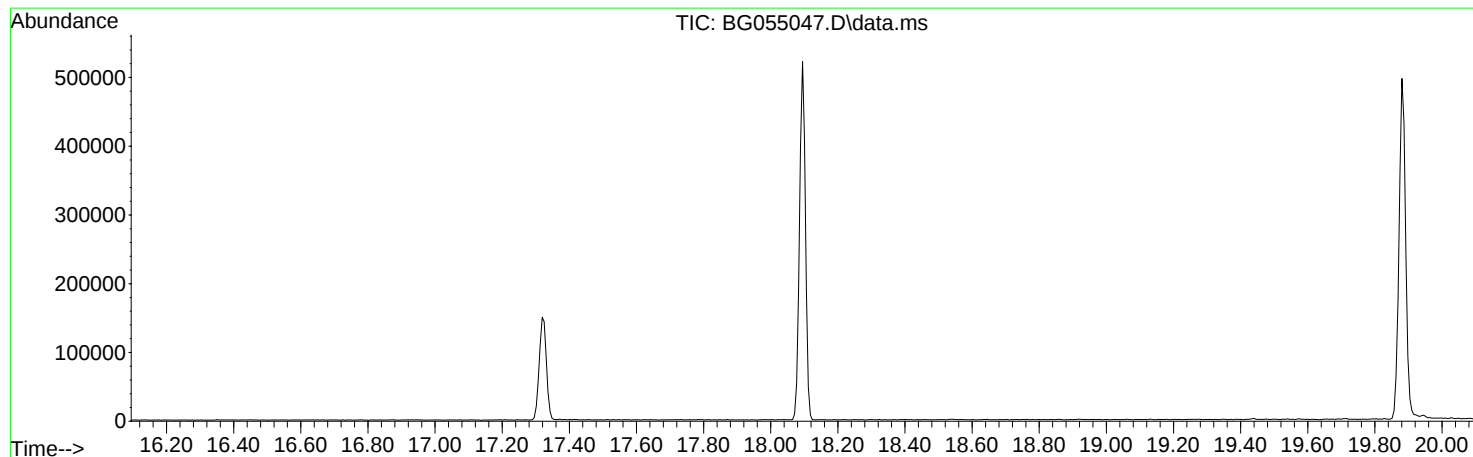




AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.9	21573	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.4	18632	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.6	20955	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44995	PASS
199	198	5	9	6.4	2862	PASS
275	198	10	60	29.7	13362	PASS
365	198	1	100	4.2	1876	PASS
441	198	0.01	100	17.2	7729	PASS
442	442	50	100	100.0	49277	PASS
443	442	15	24	19.7	9699	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100322\
Data File : BG055047.D
Acq On : 3 Oct 2022 16:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 04 07:46:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 07:12:22 2022
Response via : Initial Calibration

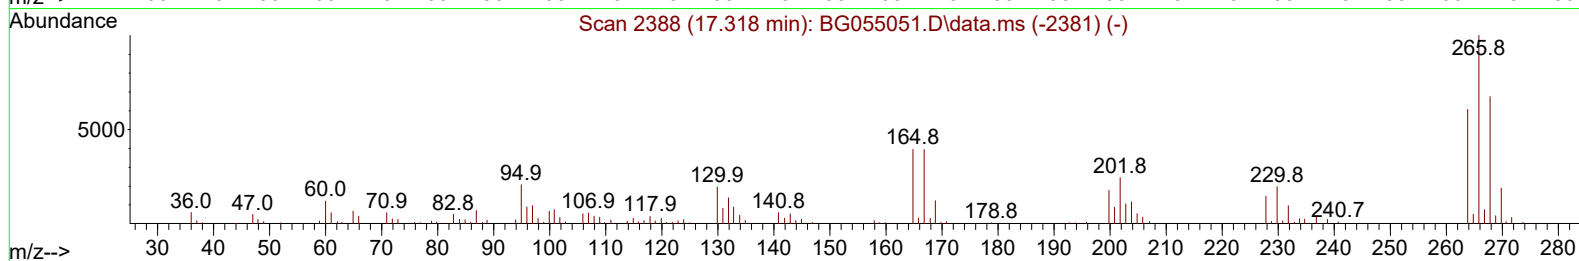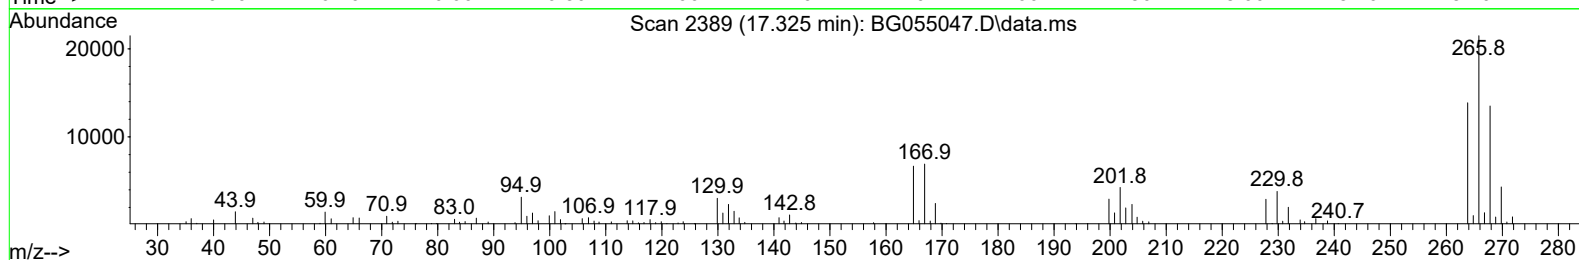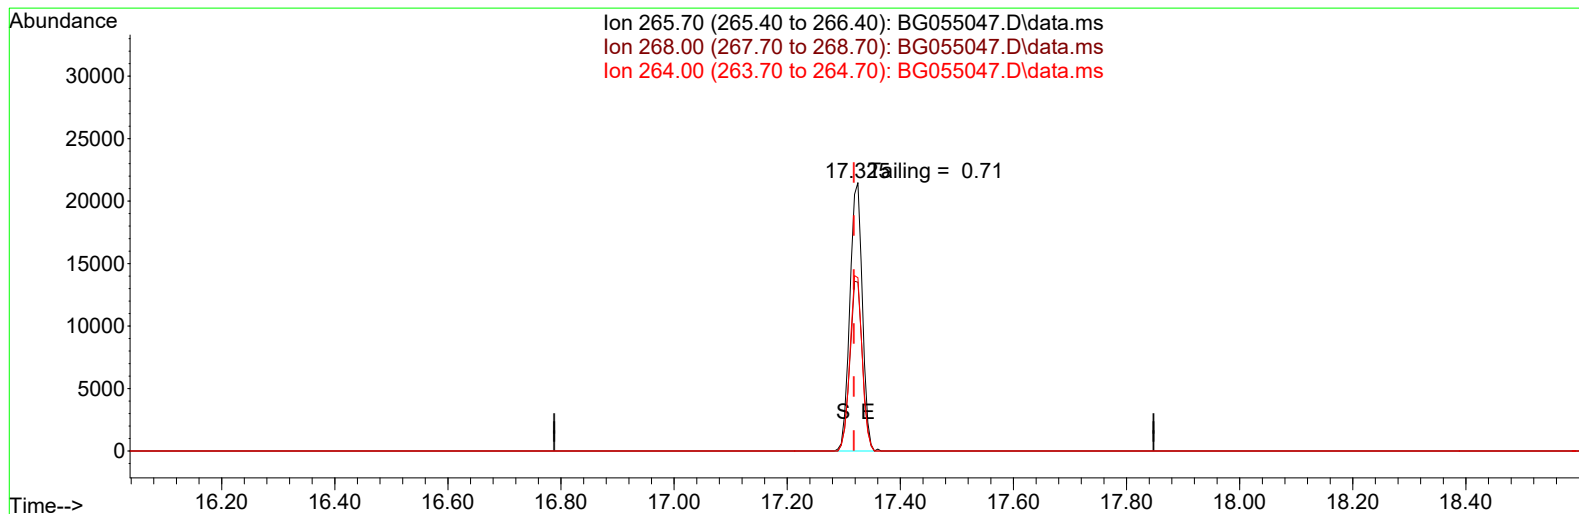

TIC: BG055047.D\data.ms

(70) Pentachlorophenol (C)

17.325min (+ 0.007) 16713.52 ng




response 32927

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	62.93
264.00	60.80	64.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100322\
 Data File : BG055047.D
 Acq On : 3 Oct 2022 16:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 04 07:46:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 04 07:12:22 2022
 Response via : Initial Calibration

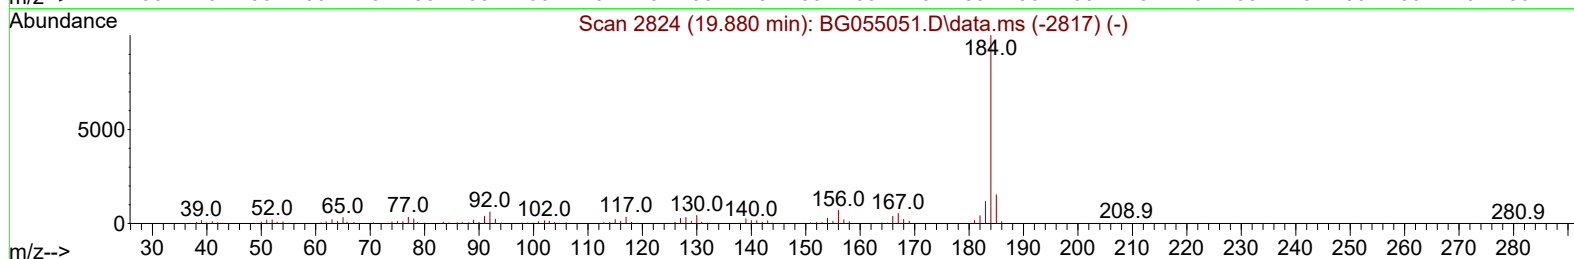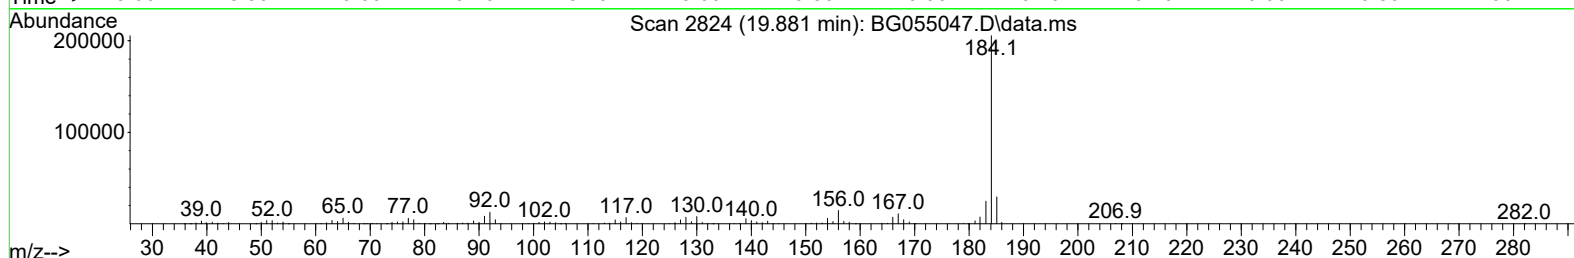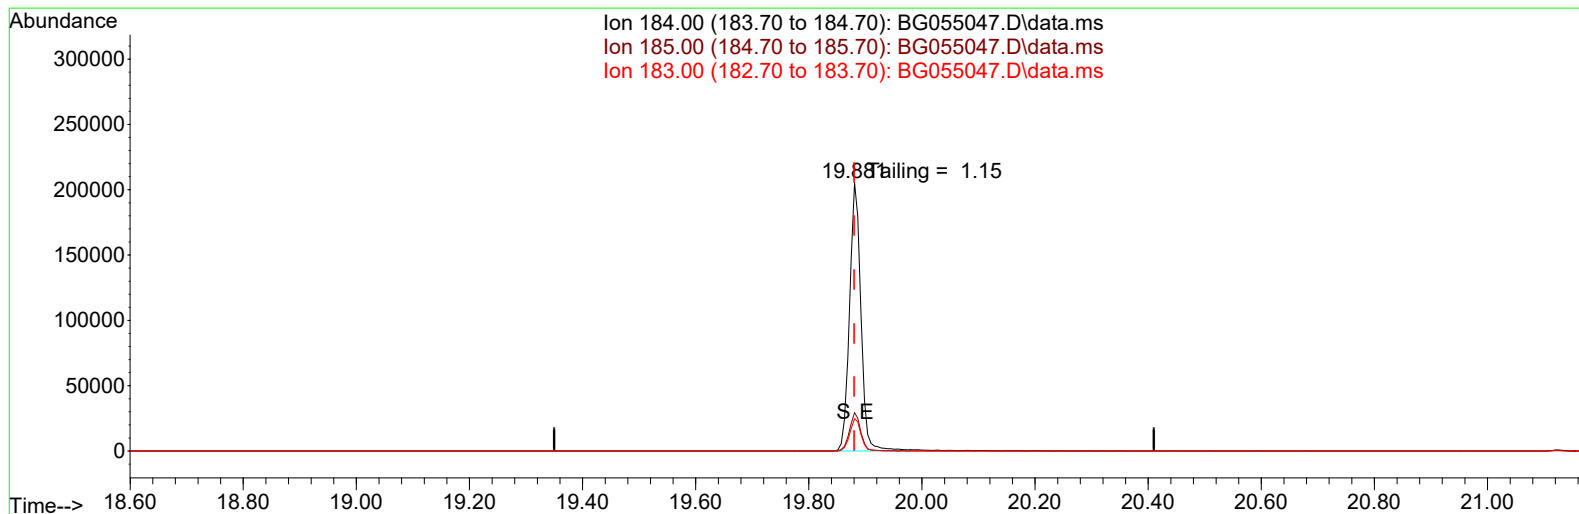

TIC: BG055047.D\data.ms

(77) Benzidine

19.881min (+ 0.001) 0.00 ng

response 289883

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.33
183.00	11.70	12.09
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/3/2022	BNA_G	BG055047.D
Compound Name	Response	Retention Time
DDT	103350	21.126
DDD	769	20.721
DDE	0	19.09
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
769	104119	0.74

Instrument :
BNA_G
ClientSampleId :
DFTPP