
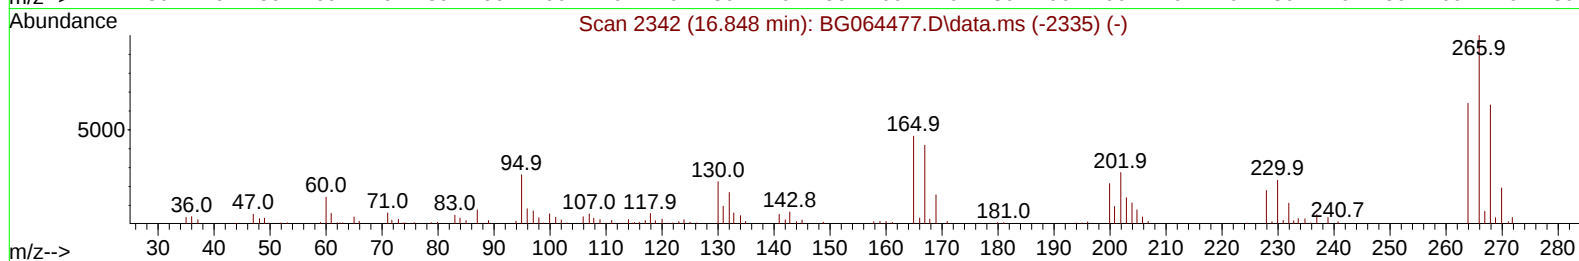
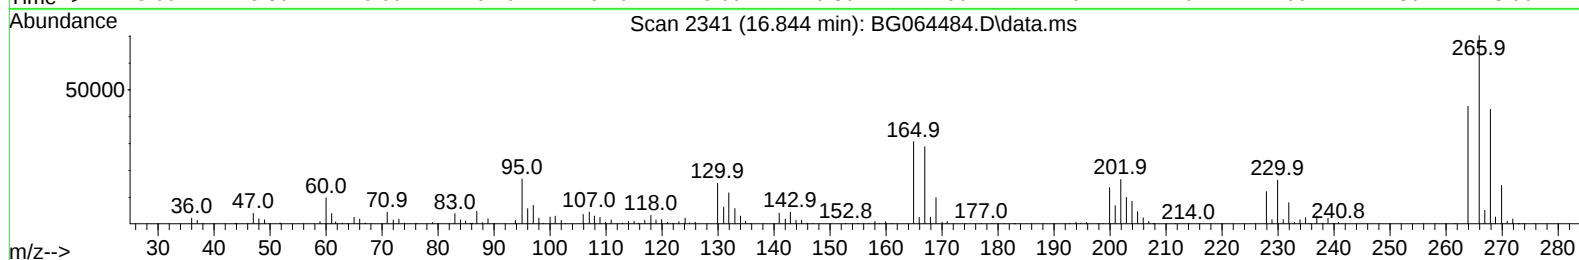


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100325\
Data File : BG064484.D
Acq On : 3 Oct 2025 12:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 13:30:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

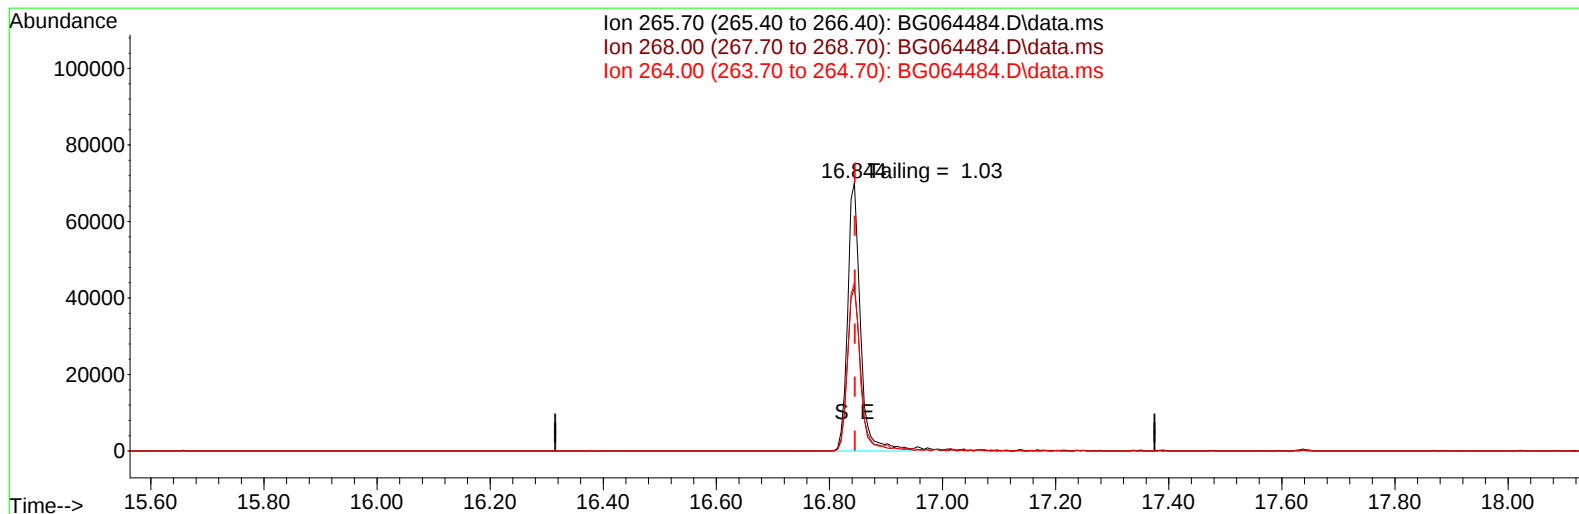

TIC: BG064484.D\data.ms

(70) Pentachlorophenol (C)




16.844min (-0.001) 67536.73 ng

response 110600

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	60.92
264.00	64.00	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100325\
Data File : BG064484.D
Acq On : 3 Oct 2025 12:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 13:30:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

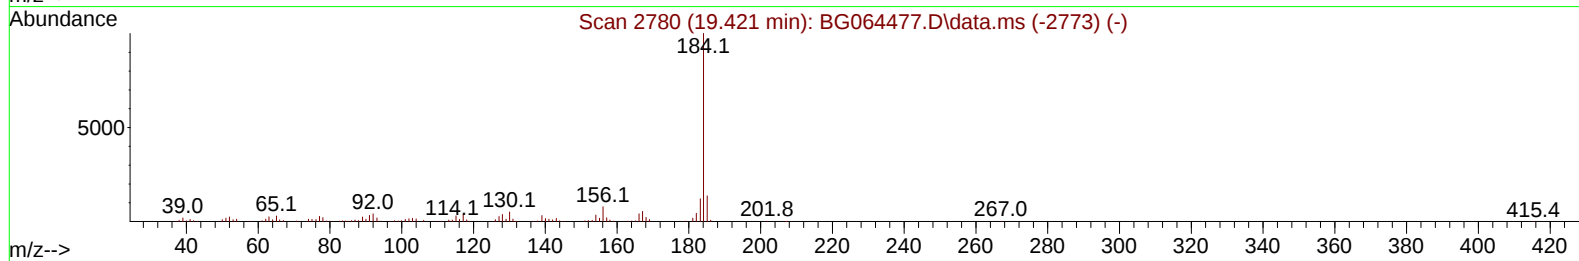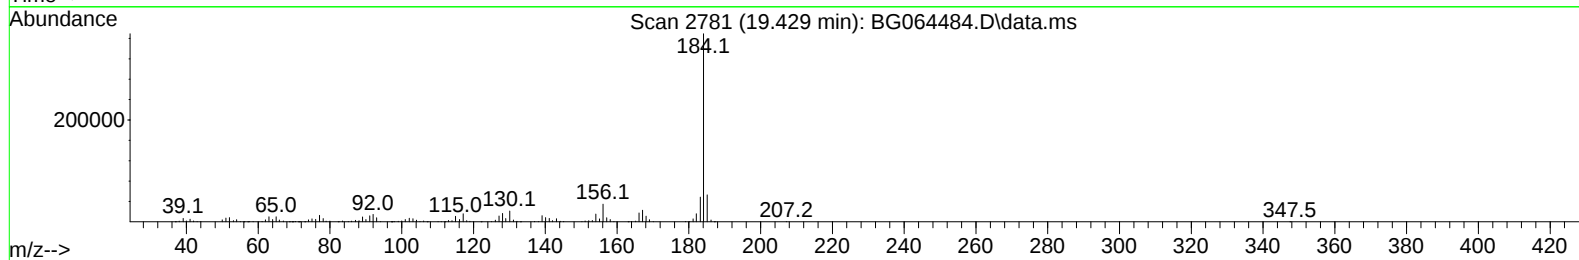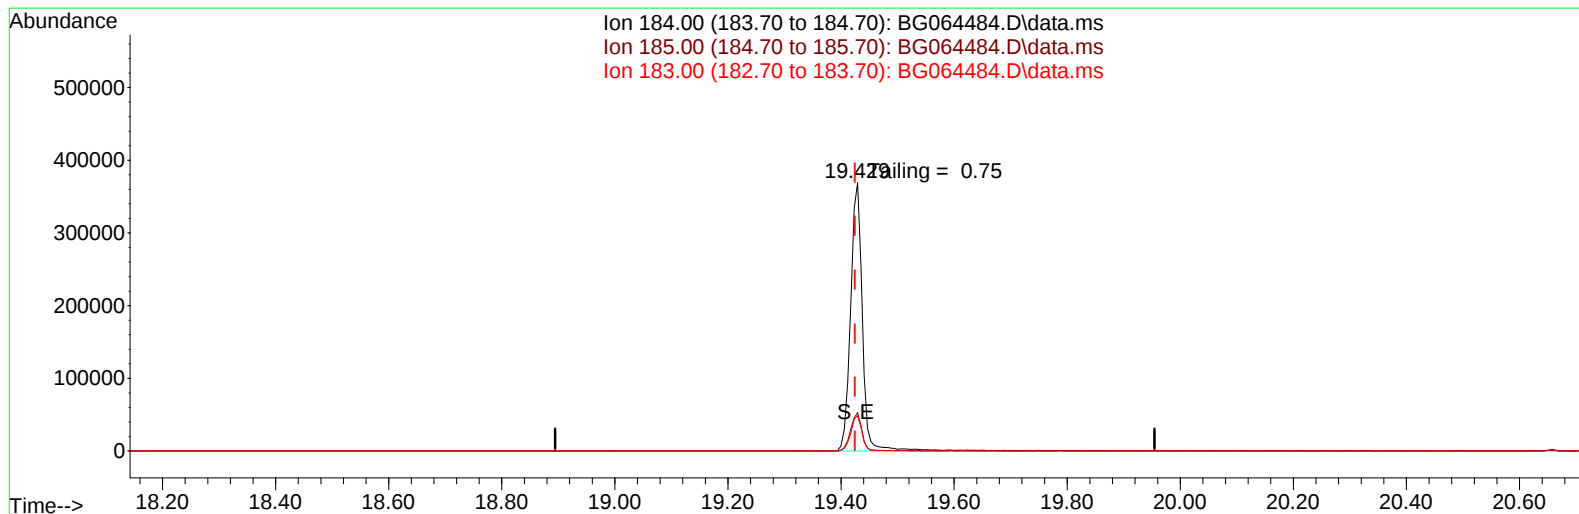

TIC: BG064484.D\data.ms

(77) Benzidine**19.429min (+ 0.004) 28542.55 ng****response 531970**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.34
183.00	12.20	13.17
0.00	0.00	0.00