

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100418\
 Data File : BG037150.D
 Acq On : 4 Oct 2018 7:32
 Operator : JU/SJ
 Sample : J5192-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 AU-05-100218-A

Quant Time: Oct 04 09:18:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 24 10:41:23 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	53646	20.00	ng	0.00
21) Naphthalene-d8	10.84	136	215747	20.00	ng	-0.02
38) Acenaphthene-d10	14.66	164	126658	20.00	ng	-0.01
63) Phenanthrene-d10	17.41	188	299087	20.00	ng	-0.01
75) Chrysene-d12	21.67	240	325531	20.00	ng	-0.02
86) Perylene-d12	24.88	264	311098	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	340427	121.70	ng	0.00
7) Phenol-d6	7.20	99	408605	94.41	ng	-0.01
23) Nitrobenzene-d5	9.20	82	339451	84.26	ng	-0.01
41) 2,4,6-Tribromophenol	16.15	330	147938	97.62	ng	-0.02
44) 2-Fluorobiphenyl	13.29	172	678532	79.79	ng	-0.01
78) Terphenyl-d14	20.01	244	1116090	90.15	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.20	70	45446	12.623	ng	# 75
50) 2,6-Dinitrotoluene	14.66	165	16276	7.317	ng	# 21
56) 2,4-Dinitrotoluene	14.66	165	16276	5.244	ng	# 19
66) 4-Bromophenyl-phenylether	16.15	248	9868	2.901	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100418\
Data File : BG037150.D
Acq On : 4 Oct 2018 7:32
Operator : JU/SJ
Sample : J5192-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
AU-05-100218-A

Quant Time: Oct 04 09:18:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

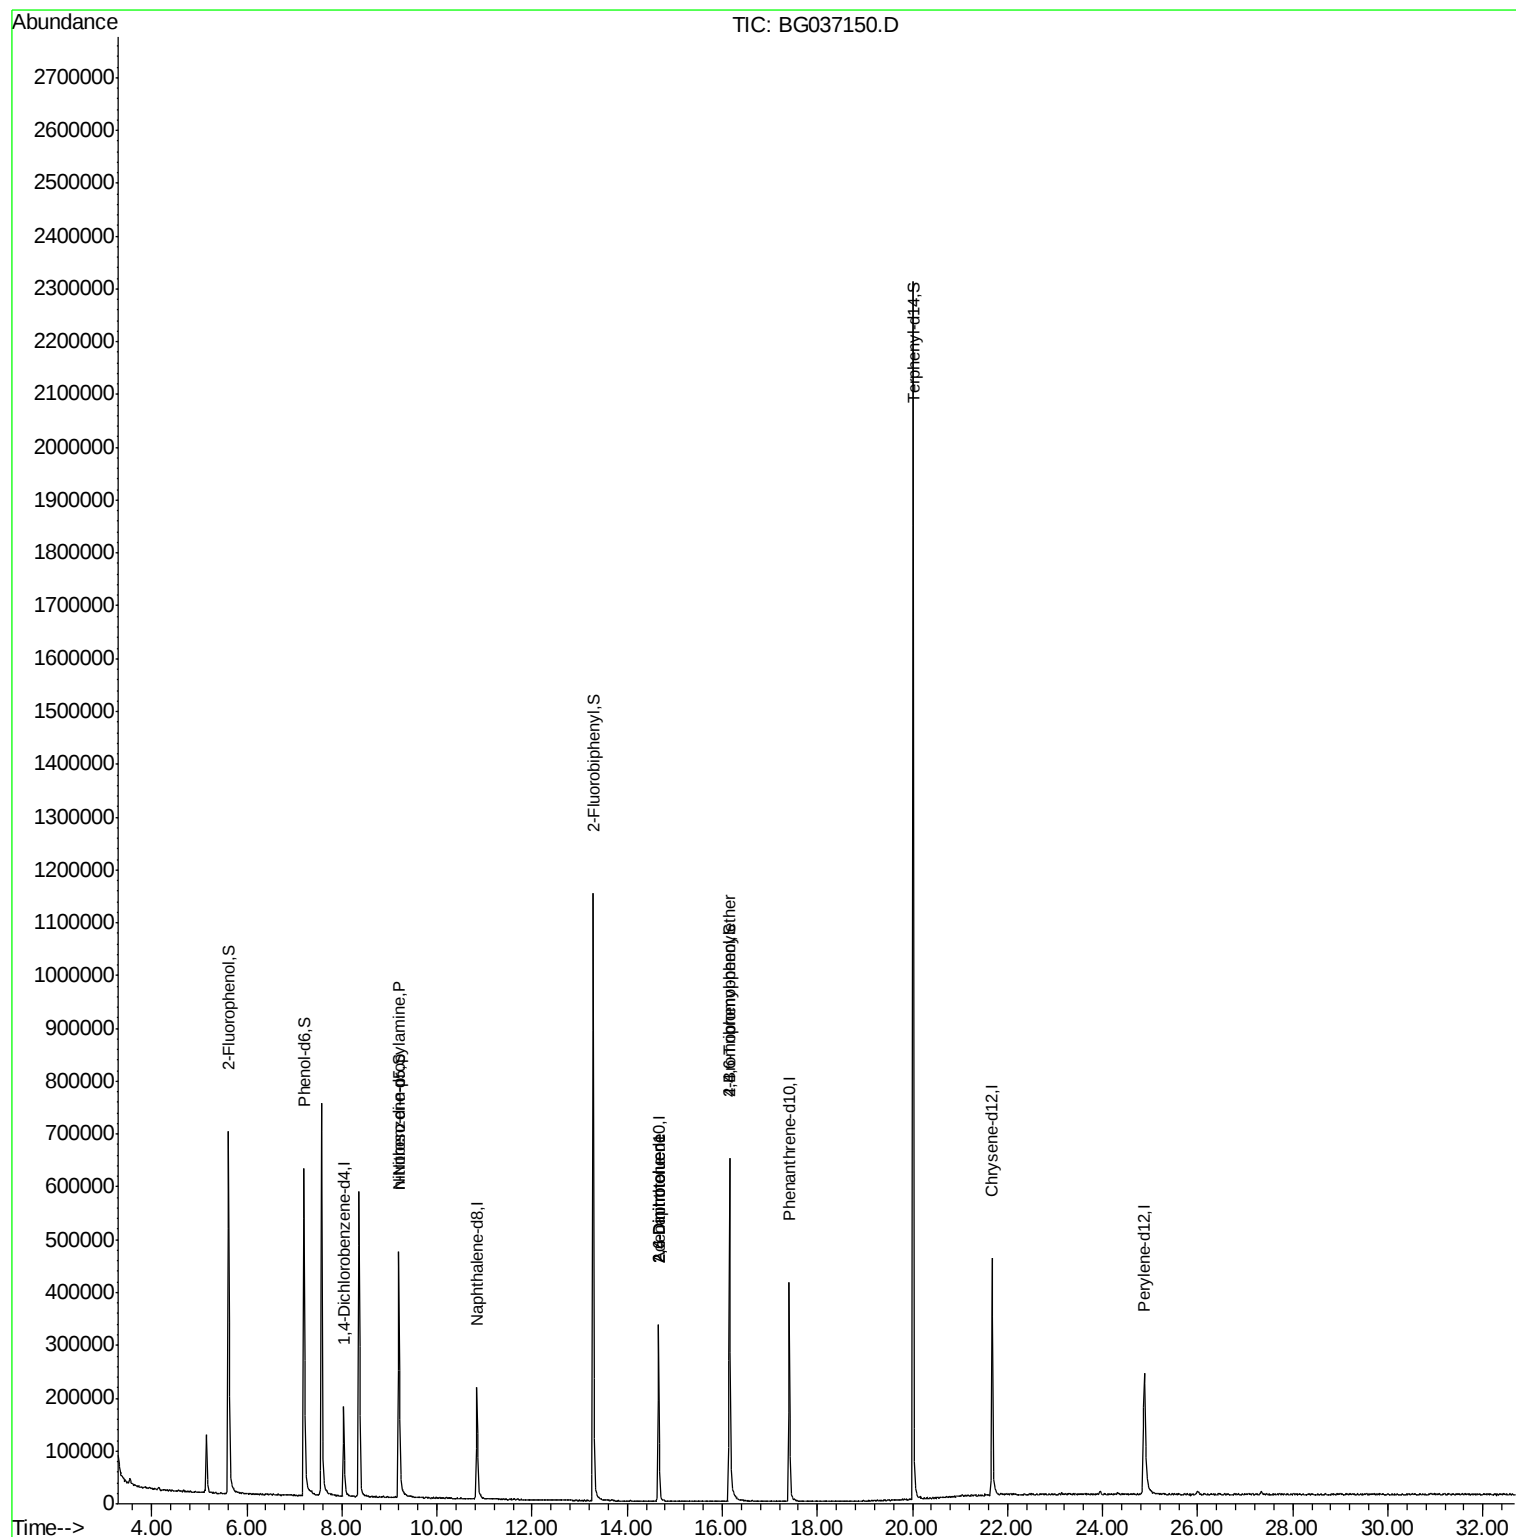

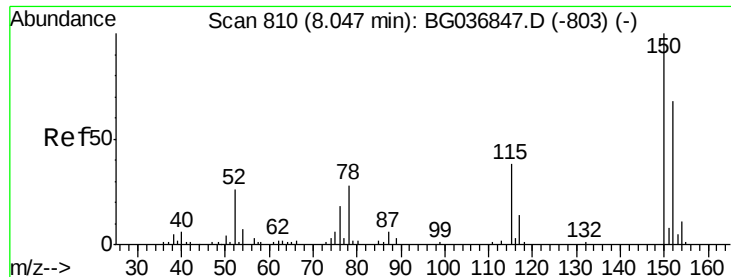

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.04 min Scan# 809

Delta R.T. -0.01 min

Lab File: BG037150.D

Acq: 4 Oct 2018 7:32

Instrument :

BNA_G

ClientSampleId :

AU-05-100218-A


Tgt Ion:152 Resp: 53646

Ion Ratio Lower Upper

152 100

150 154.2 119.5 179.3




115 61.7 44.5 66.7



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

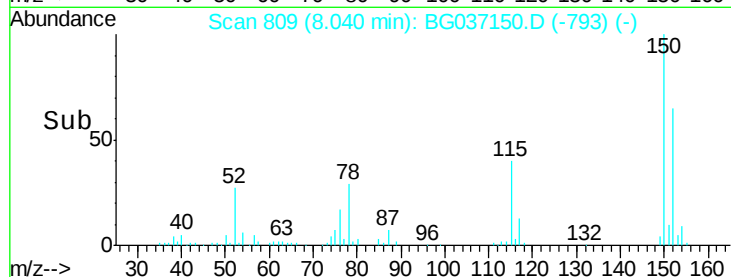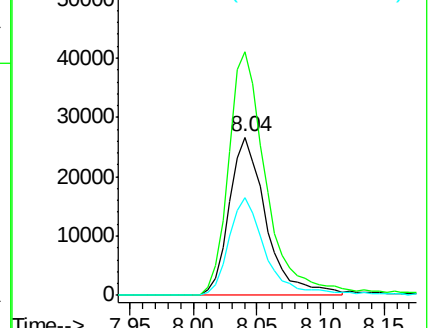

#5

2-Fluorophenol

Concen: 121.699 ng

RT: 5.62 min Scan# 397

Delta R.T. -0.00 min

Lab File: BG037150.D

Acq: 4 Oct 2018 7:32


Tgt Ion:112 Resp: 340427

Ion Ratio Lower Upper

112 100

64 69.2 57.2 85.8



63 37.6 30.8 46.2





Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

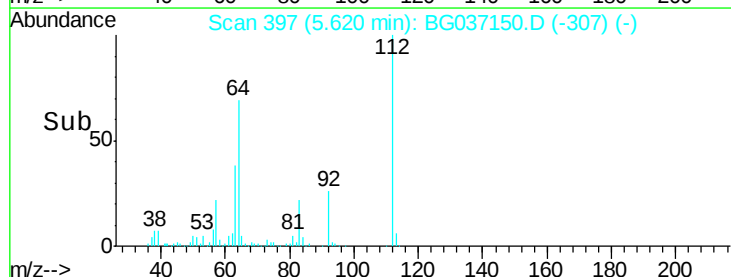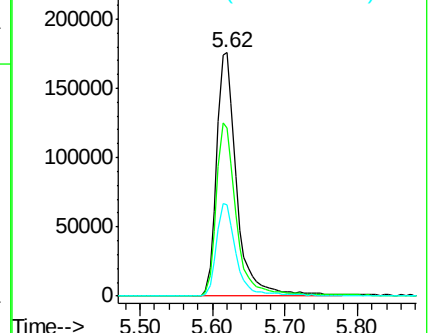

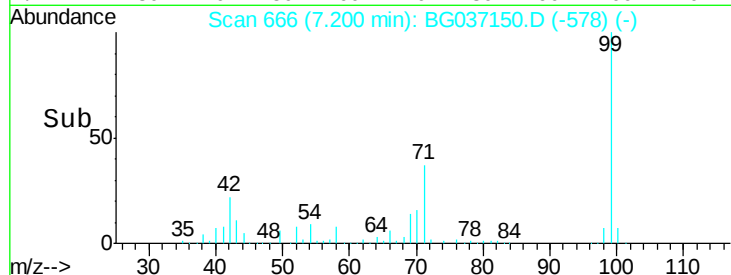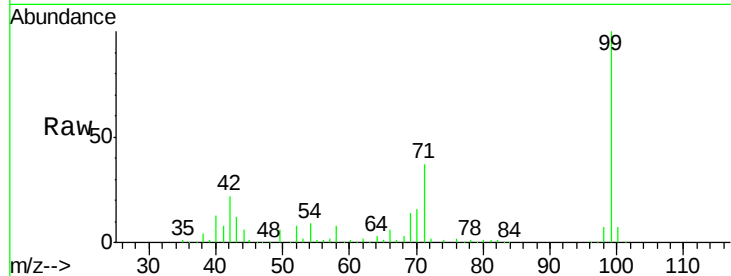

#7

Phenol-d6

Concen: 94.412 ng

RT: 7.20 min Scan# 666

Delta R.T. -0.01 min

Lab File: BG037150.D

Acq: 4 Oct 2018 7:32

Instrument :

BNA_G

ClientSampleId :

AU-05-100218-A





Tgt Ion: 99 Resp: 408605

Ion Ratio Lower Upper

99 100

42 21.8 16.5 24.7

71 36.6 29.4 44.2

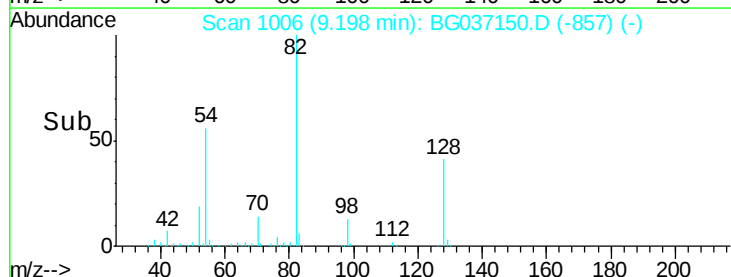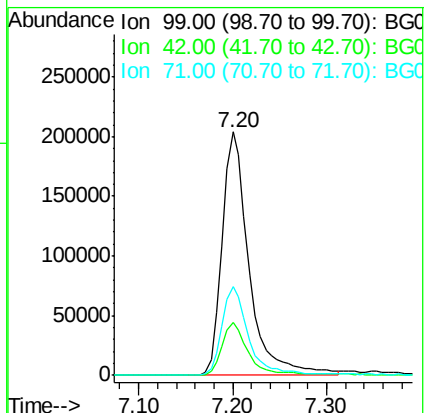

#19

n-Nitroso-di-n-propylamine

Concen: 12.623 ng

RT: 9.20 min Scan# 1006

Delta R.T. 0.35 min

Lab File: BG037150.D

Acq: 4 Oct 2018 7:32

Tgt Ion: 70 Resp: 45446


Ion Ratio Lower Upper

70 100

42 52.9 56.2 84.4#

101 0.0 7.8 11.6#

130 2.4 16.2 24.2#

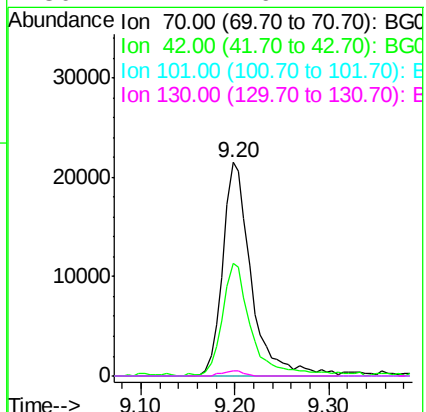







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.84 min Scan# 1285
Delta R.T. -0.02 min
Lab File: BG037150.D
Acq: 4 Oct 2018 7:32

Instrument :
BNA_G
ClientSampleId :
AU-05-100218-A

Tgt Ion:	136	Resp:	215747
Ion	Ratio	Lower	Upper
136	100		
137	11.6	8.8	13.2
54	10.4	9.2	13.8
68	6.9	5.8	8.6

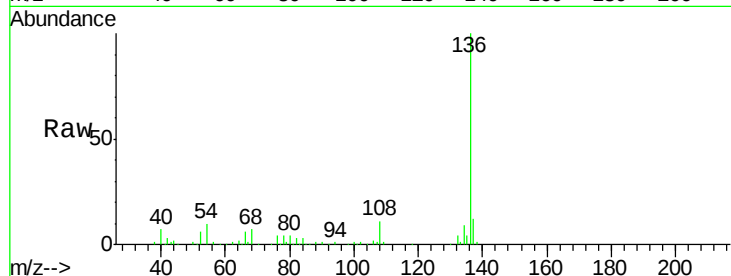


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

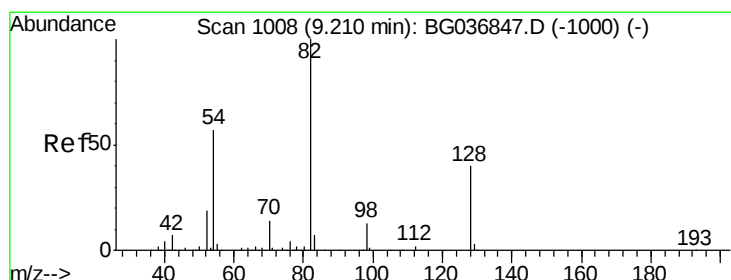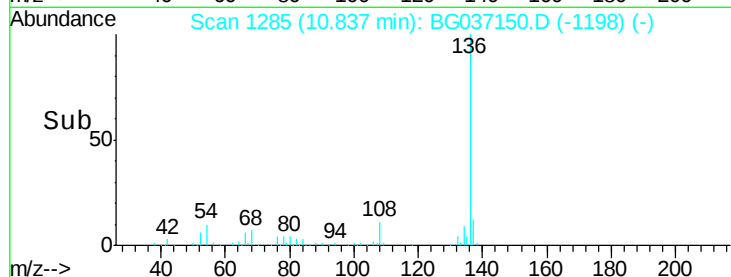
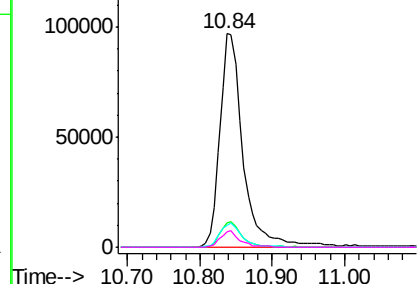



#23
Nitrobenzene-d5
Concen: 84.256 ng
RT: 9.20 min Scan# 1006
Delta R.T. -0.01 min
Lab File: BG037150.D
Acq: 4 Oct 2018 7:32

Tgt Ion:	82	Resp:	339451
Ion	Ratio	Lower	Upper
82	100		
128	41.2	33.3	49.9
54	56.5	45.1	67.7



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

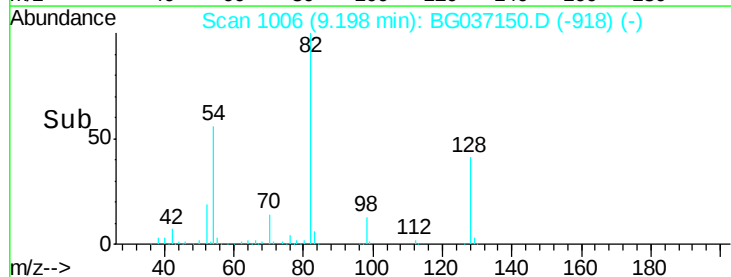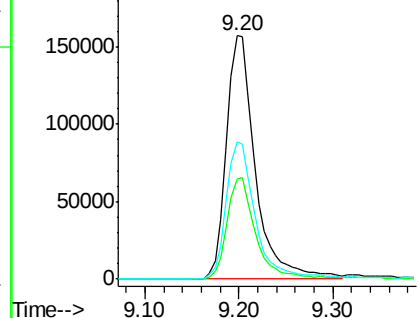

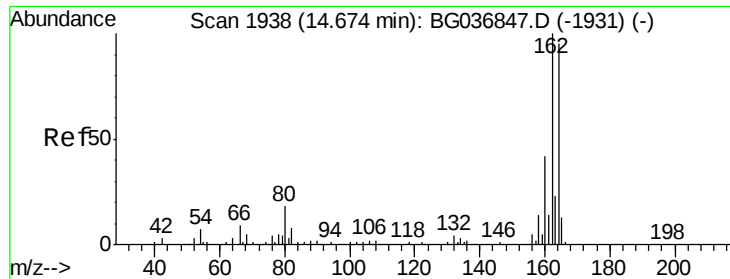

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.66 min Scan# 1936

Delta R.T. -0.01 min

Lab File: BG037150.D

Acq: 4 Oct 2018 7:32

Instrument :

BNA_G

ClientSampleId :

AU-05-100218-A


Tgt Ion:164 Resp: 126658

Ion Ratio Lower Upper

164 100

162 106.3 80.7 121.1




160 47.1 35.3 52.9

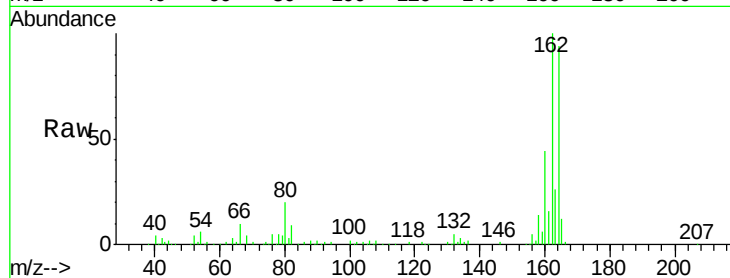

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

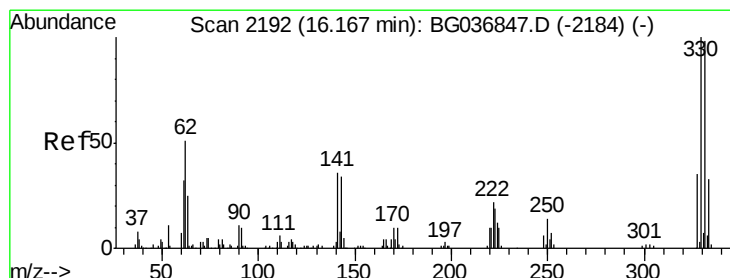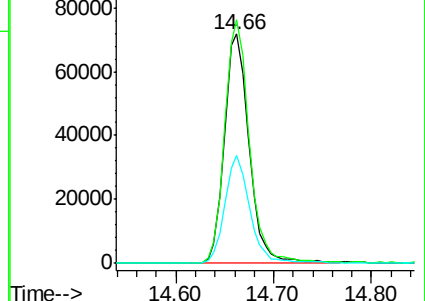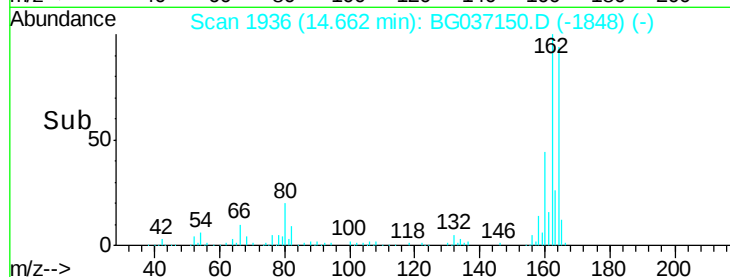

#41

2,4,6-Tribromophenol

Concen: 97.624 ng

RT: 16.15 min Scan# 2189

Delta R.T. -0.02 min

Lab File: BG037150.D

Acq: 4 Oct 2018 7:32


Tgt Ion:330 Resp: 147938

Ion Ratio Lower Upper

330 100

332 94.6 75.4 113.2



141 39.9 30.7 46.1

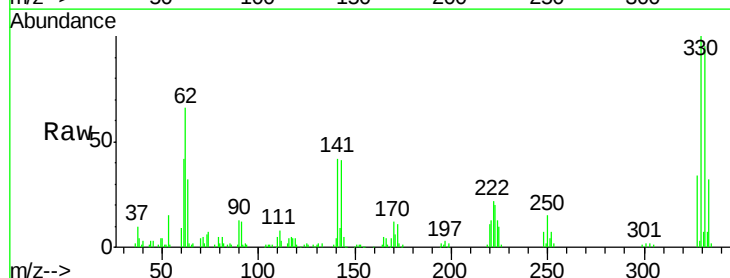

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



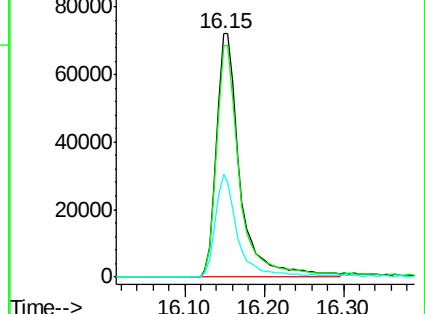
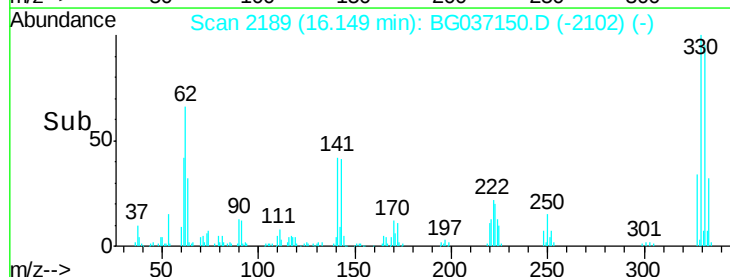




#44
 2-Fluorobiphenyl
 Concen: 79.790 ng
 RT: 13.29 min Scan# 1702
 Delta R.T. -0.01 min
 Lab File: BG037150.D
 Acq: 4 Oct 2018 7:32




Instrument :
 BNA_G
 ClientSampleId :
 AU-05-100218-A


Tgt Ion:172 Resp: 678532
 Ion Ratio Lower Upper
 172 100
 171 37.1 31.3 46.9
 170 24.6 21.0 31.6

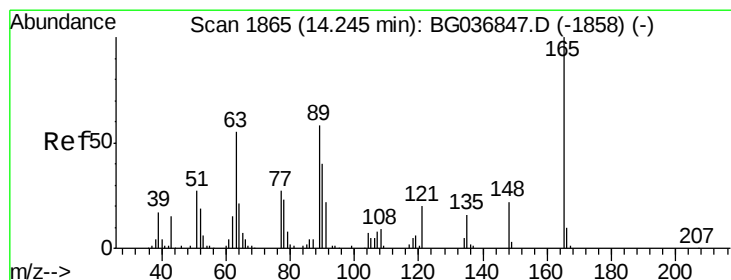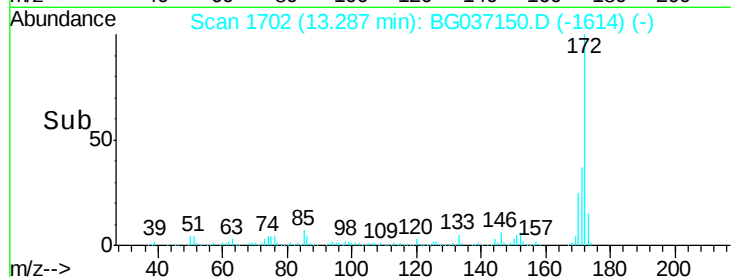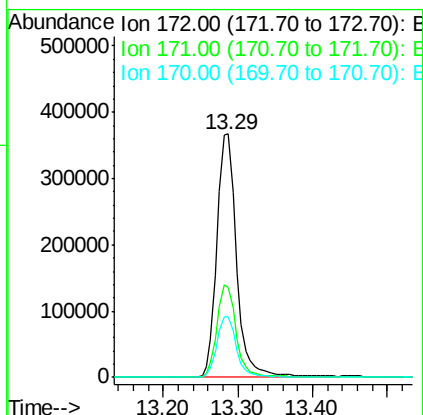

#50
 2,6-Dinitrotoluene
 Concen: 7.317 ng
 RT: 14.66 min Scan# 1936
 Delta R.T. 0.42 min
 Lab File: BG037150.D
 Acq: 4 Oct 2018 7:32

Tgt Ion:165 Resp: 16276
 Ion Ratio Lower Upper
 165 100
 63 0.0 50.1 75.1#
 89 1.8 47.8 71.6#

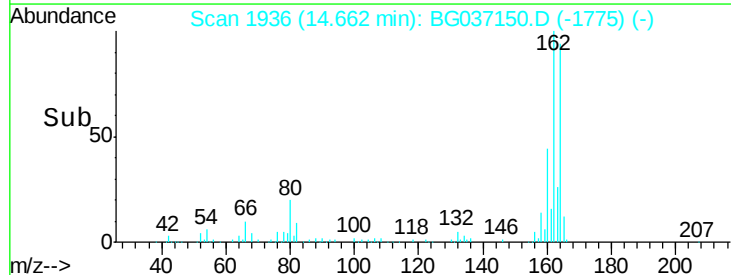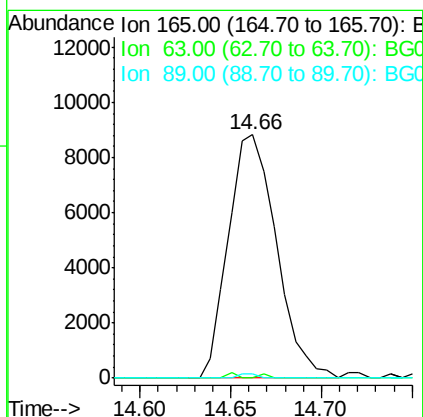


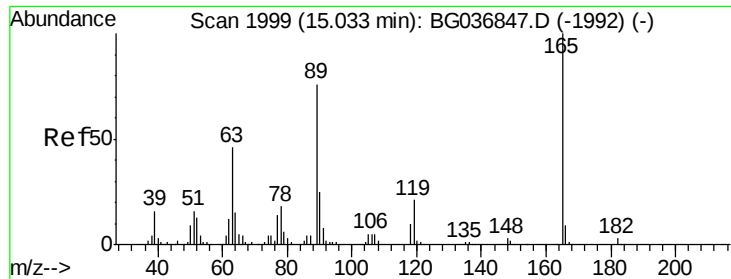




#56
2,4-Dinitrotoluene
Concen: 5.244 ng
RT: 14.66 min Scan# 1936
Delta R.T. -0.37 min
Lab File: BG037150.D
Acq: 4 Oct 2018 7:32

Instrument :
BNA_G
ClientSampleId :
AU-05-100218-A

Tgt Ion:165 Resp: 16276
Ion Ratio Lower Upper
165 100
63 0.0 40.1 60.1#
89 1.8 63.7 95.5#
182 0.0 2.5 3.7#




Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BGC
Ion 89.00 (88.70 to 89.70): BGC
Ion 182.00 (181.70 to 182.70): E

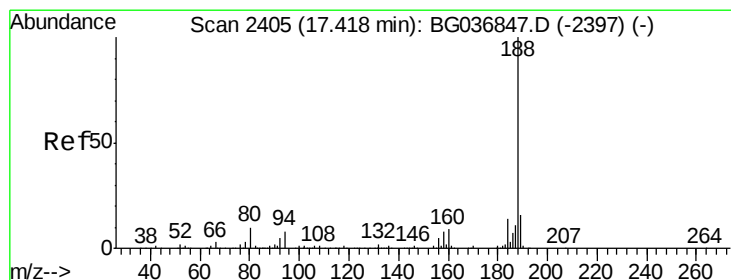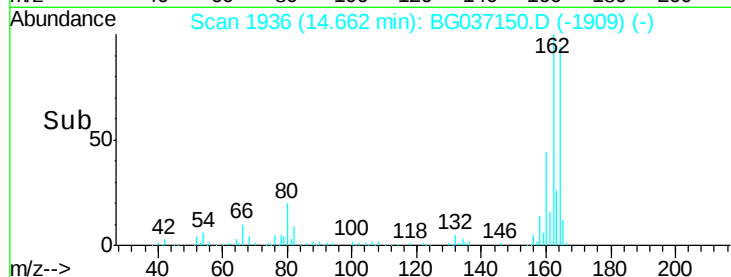
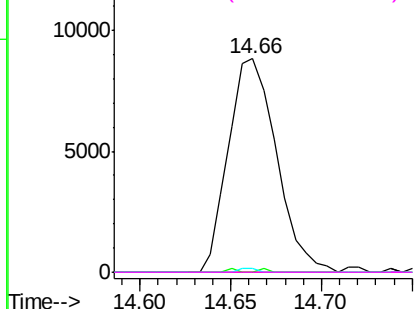


#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.41 min Scan# 2403
Delta R.T. -0.01 min
Lab File: BG037150.D
Acq: 4 Oct 2018 7:32

Tgt Ion:188 Resp: 299087
Ion Ratio Lower Upper
188 100
94 8.2 6.7 10.1
80 10.5 8.1 12.1

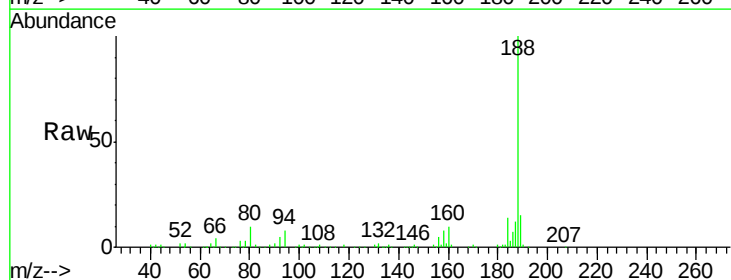

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

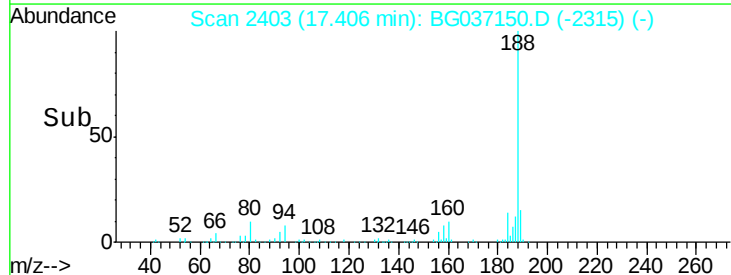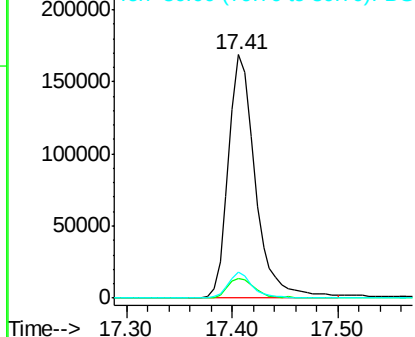







#66
4-Bromophenyl-phenylether
Concen: 2.901 ng
RT: 16.15 min Scan# 2189
Delta R.T. -0.46 min
Lab File: BG037150.D
Acq: 4 Oct 2018 7:32

Instrument :
BNA_G
ClientSampleId :
AU-05-100218-A

Tgt Ion:248 Resp: 9868
Ion Ratio Lower Upper
248 100
250 202.5 78.1 117.1#
141 587.9 53.7 80.5#

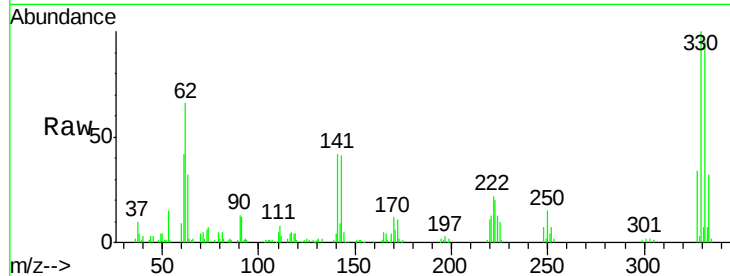


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

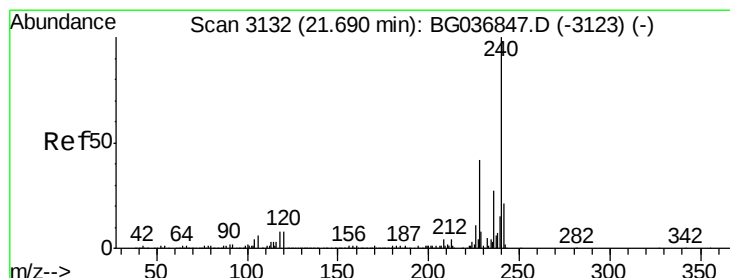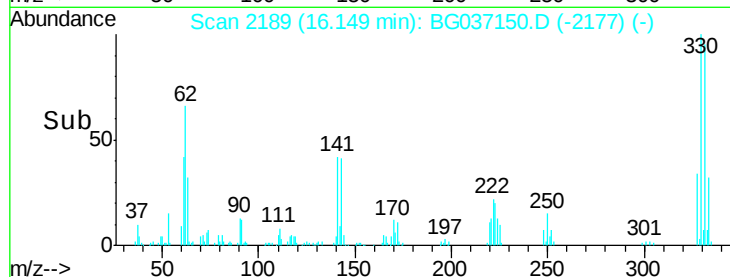
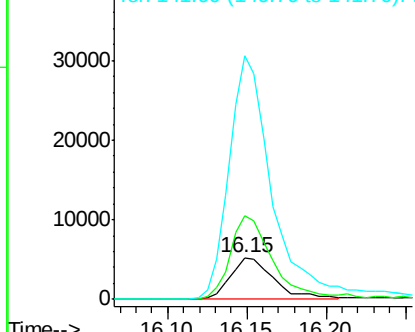



#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.67 min Scan# 3129
Delta R.T. -0.02 min
Lab File: BG037150.D
Acq: 4 Oct 2018 7:32

Tgt Ion:240 Resp: 325531
Ion Ratio Lower Upper
240 100
120 9.0 6.9 10.3
236 25.5 21.2 31.8

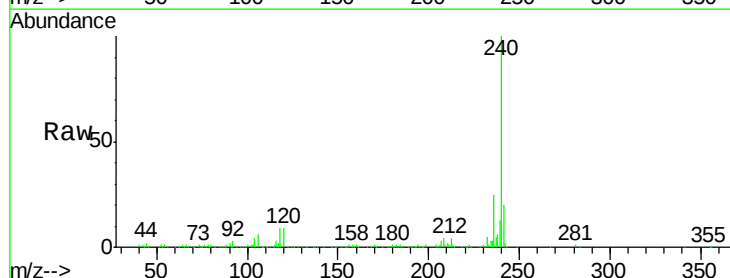

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



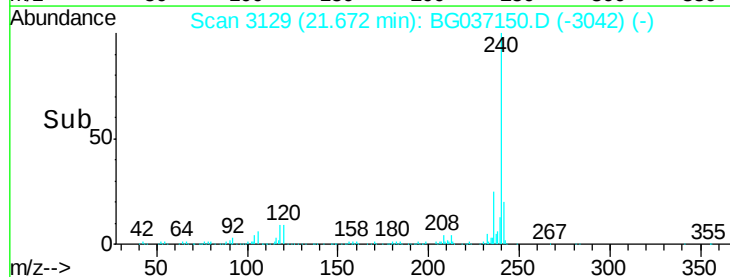
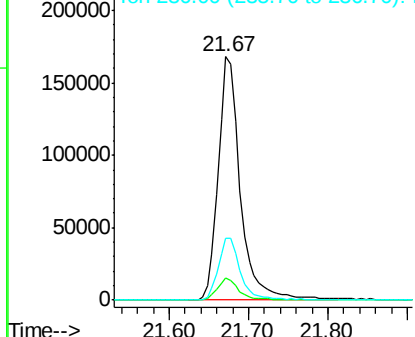


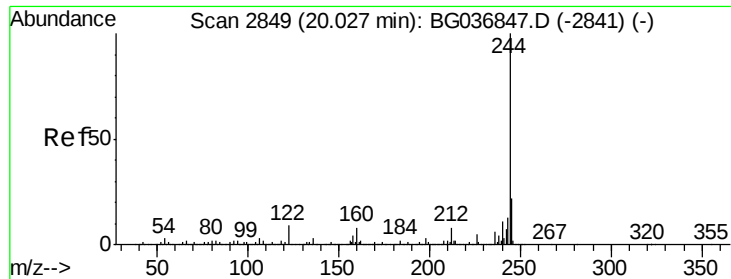

#78
 Terphenyl-d14
 Concen: 90.153 ng
 RT: 20.01 min Scan# 2847
 Delta R.T. -0.01 min
 Lab File: BG037150.D
 Acq: 4 Oct 2018 7:32

Instrument :
 BNA_G
 ClientSampleId :
 AU-05-100218-A

Tgt Ion:244 Resp: 1116090
 Ion Ratio Lower Upper
 244 100
 212 8.5 7.0 10.6
 122 9.8 7.1 10.7

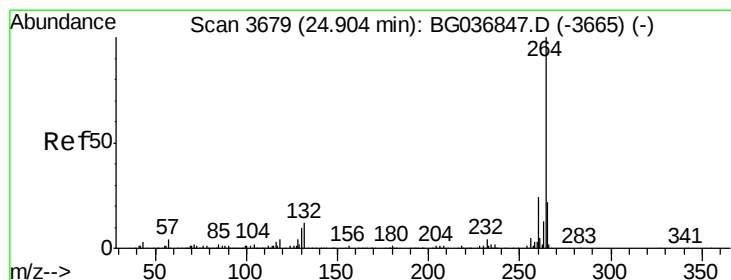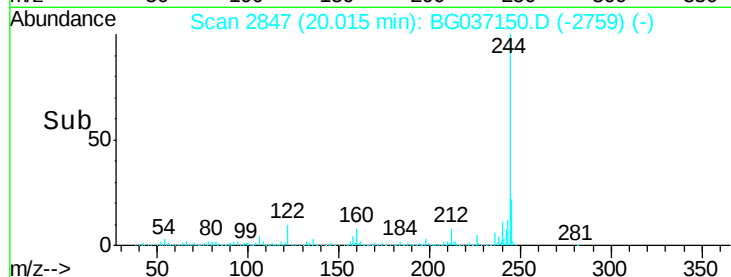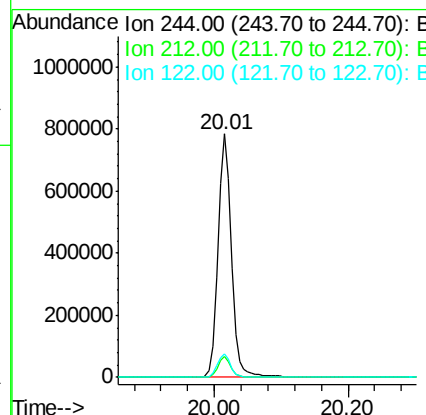

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.88 min Scan# 3675
 Delta R.T. -0.02 min
 Lab File: BG037150.D
 Acq: 4 Oct 2018 7:32

Tgt Ion:264 Resp: 311098
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.6 29.4
 265 21.5 17.4 26.0

