

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100418\
Data File : BG037134.D
Acq On : 3 Oct 2018 15:27
Operator : JU/SJ
Sample : PB113454BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB113454BL

Quant Time: Oct 03 18:05:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	53266	20.00	ng	0.00
21) Naphthalene-d8	10.84	136	223016	20.00	ng	-0.01
38) Acenaphthene-d10	14.66	164	132840	20.00	ng	-0.01
63) Phenanthrene-d10	17.41	188	320925	20.00	ng	-0.01
75) Chrysene-d12	21.67	240	323282	20.00	ng	-0.02
86) Perylene-d12	24.88	264	314856	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	345518	124.40	ng	0.00
7) Phenol-d6	7.20	99	464761	108.15	ng	-0.01
23) Nitrobenzene-d5	9.20	82	307549	73.85	ng	-0.01
41) 2,4,6-Tribromophenol	16.15	330	145139	91.32	ng	-0.02
44) 2-Fluorobiphenyl	13.28	172	674281	75.60	ng	-0.02
78) Terphenyl-d14	20.02	244	1024348	83.32	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100418\
Data File : BG037134.D
Acq On : 3 Oct 2018 15:27
Operator : JU/SJ
Sample : PB113454BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB113454BL

Quant Time: Oct 03 18:05:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

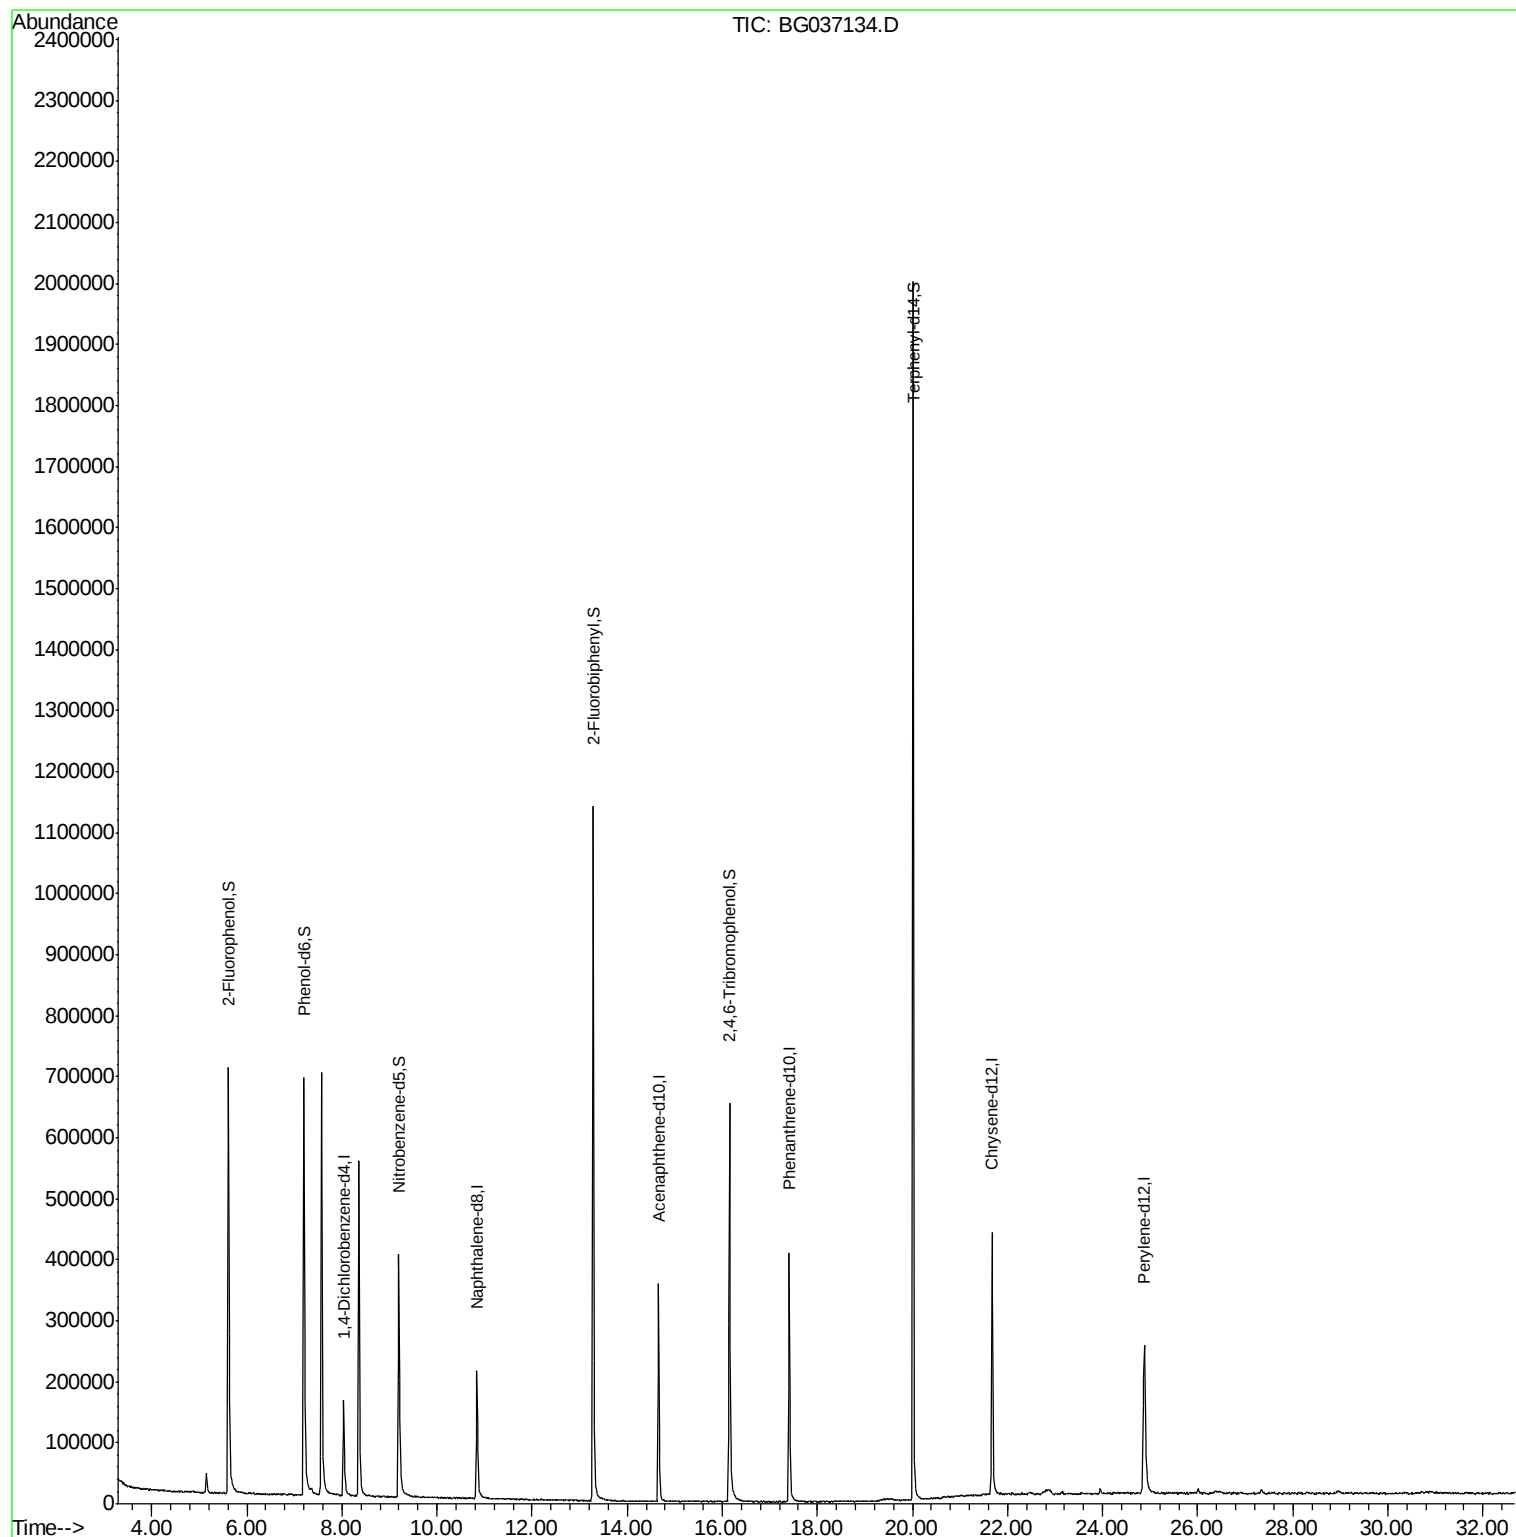

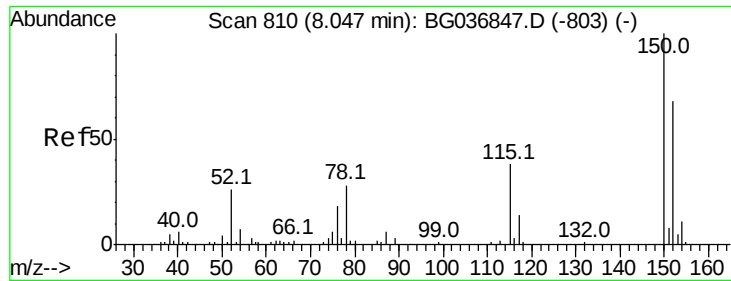


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.04 min Scan# 809
Delta R.T. -0.01 min
Lab File: BG037134.D
Acq: 3 Oct 2018 15:27

Instrument :
BNA_G
ClientSampled :
PB113454BL

Tot Ion	Ratio	Lower	Upper
152	100		
150	150.9	119.5	179.3
115	60.8	44.5	66.7



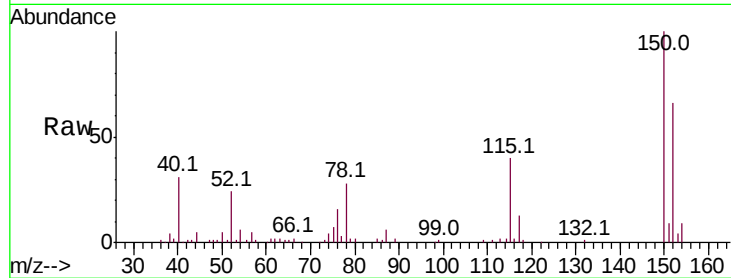


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

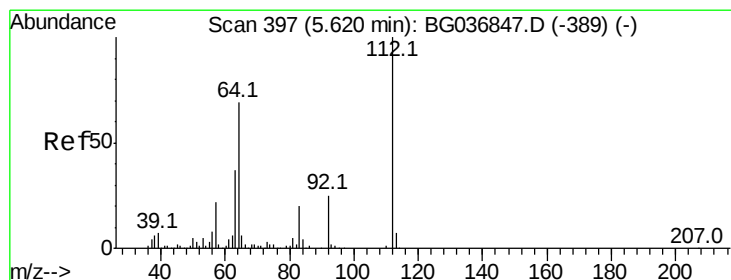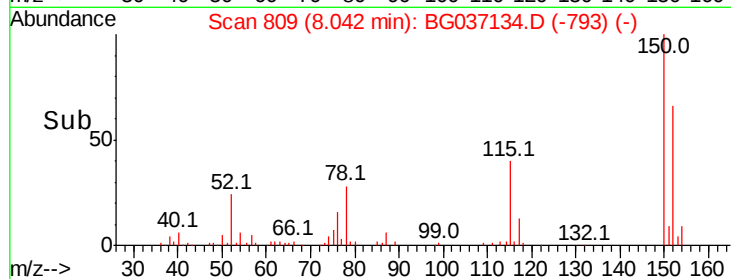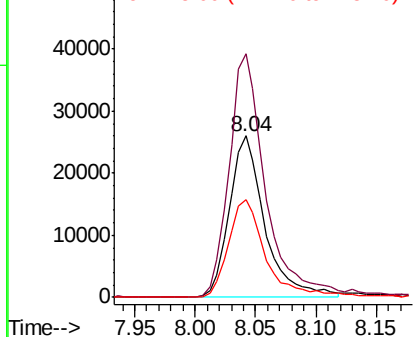

#5

2-Fluorophenol
Concen: 124.400 ng
RT: 5.62 min Scan# 396
Delta R.T. -0.01 min
Lab File: BG037134.D
Acq: 3 Oct 2018 15:27

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.4	57.2	85.8
63	37.3	30.8	46.2


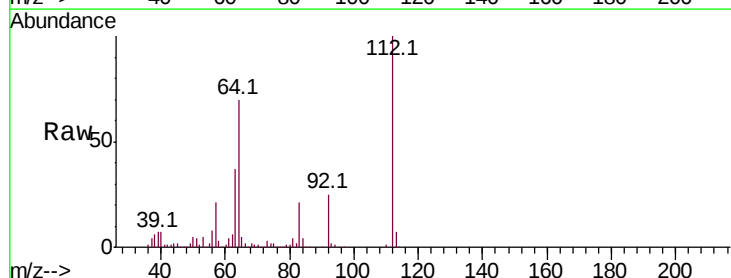


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

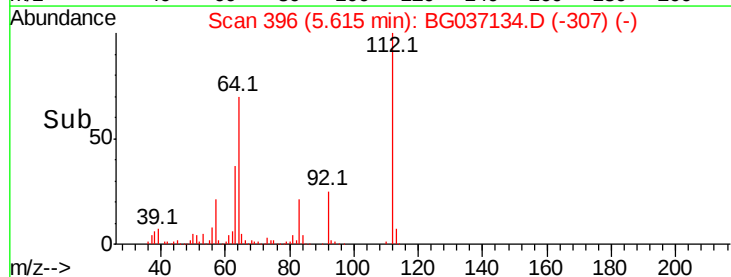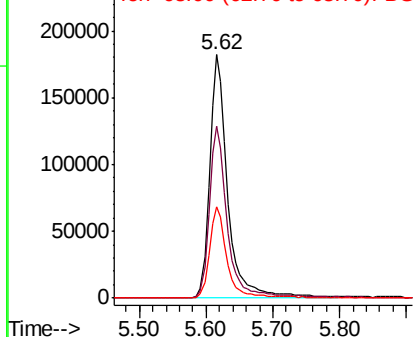



#7

Phenol-d6

Concen: 108.154 ng

RT: 7.20 min Scan# 666

Delta R.T. -0.01 min

Lab File: BG037134.D

Acq: 3 Oct 2018 15:27

Instrument :

BNA_G

ClientSampleId :

PB113454BL


Tot Ion: 99 Resp: 464761

Ion Ratio Lower Upper



99 100

42 20.7 16.5 24.7

71 35.7 29.4 44.2

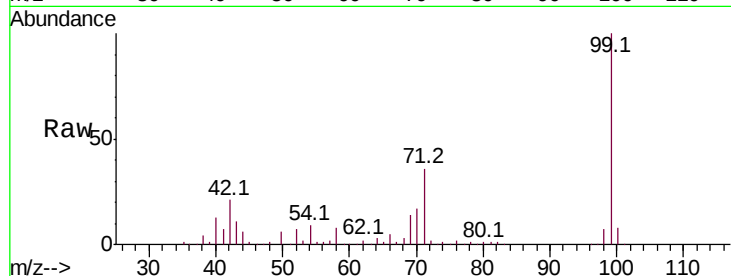

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

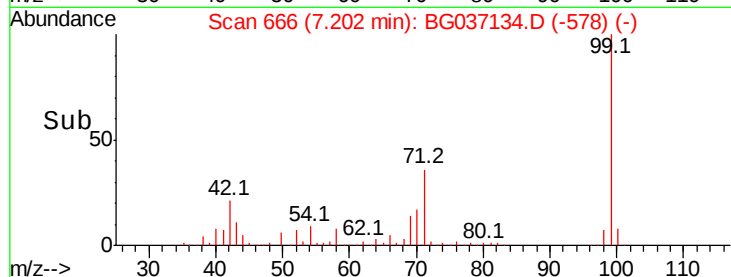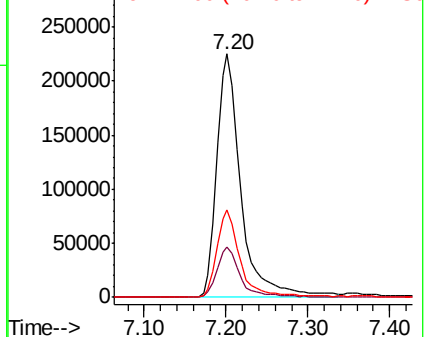

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.84 min Scan# 1286

Delta R.T. -0.01 min

Lab File: BG037134.D

Acq: 3 Oct 2018 15:27

Tgt Ion: 136 Resp: 223016


Ion Ratio Lower Upper

136 100



137 11.4 8.8 13.2

54 10.4 9.2 13.8

68 6.9 5.8 8.6

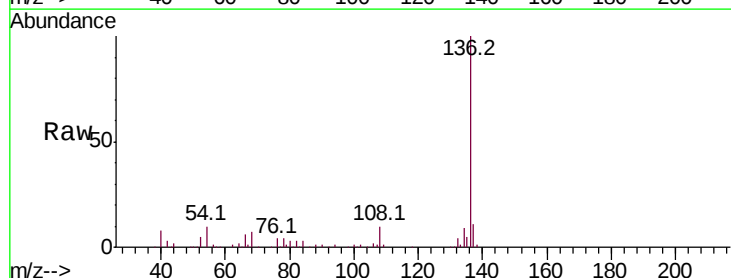

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


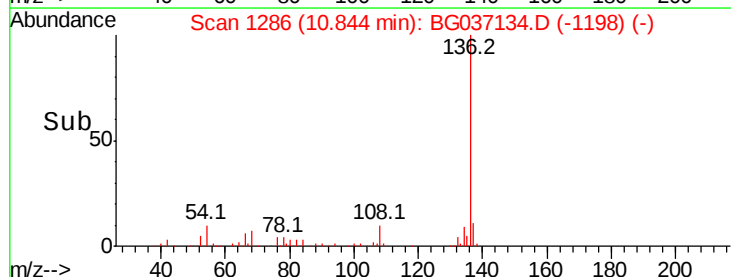
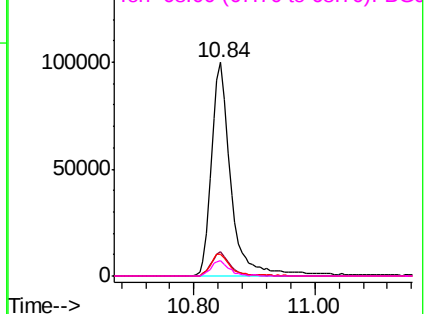




#23
Nitrobenzene-d5
Concen: 73.849 ng
RT: 9.20 min Scan# 1006
Delta R.T. -0.01 min
Lab File: BG037134.D
Acq: 3 Oct 2018 15:27




Instrument :
BNA_G
ClientSampleId :
PB113454BL

Tot Ion: 82 Resp: 307549
Ion Ratio Lower Upper
82 100
128 40.4 33.3 49.9
54 57.3 45.1 67.7

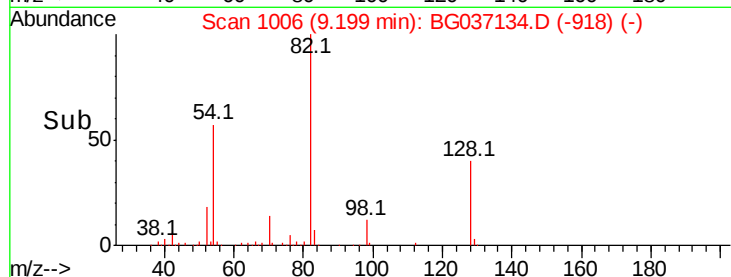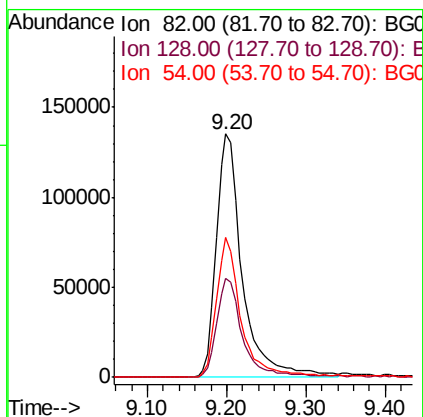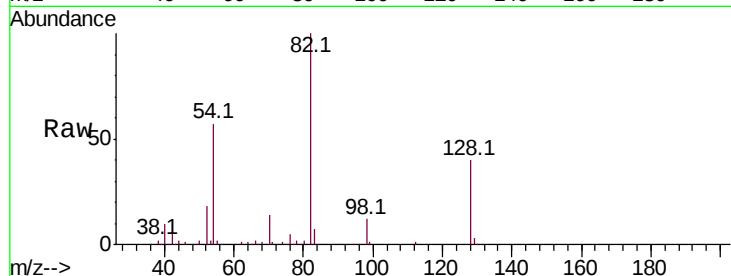

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.66 min Scan# 1936
Delta R.T. -0.01 min
Lab File: BG037134.D
Acq: 3 Oct 2018 15:27

Tgt Ion:164 Resp: 132840
Ion Ratio Lower Upper
164 100
162 100.8 80.7 121.1
160 44.0 35.3 52.9

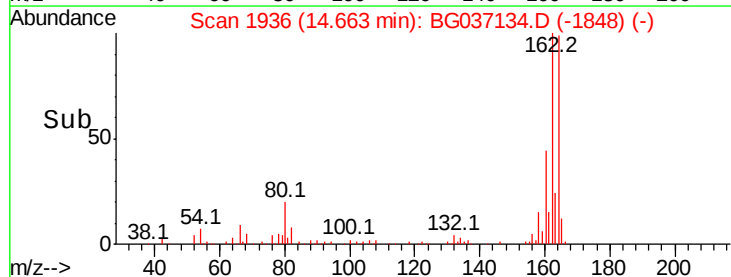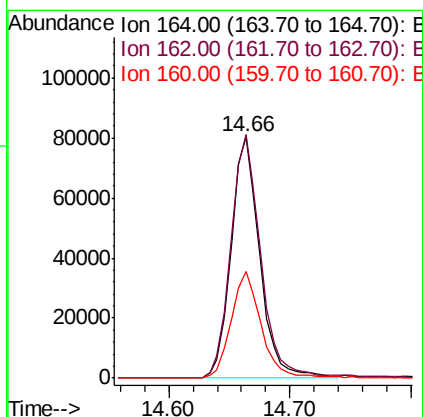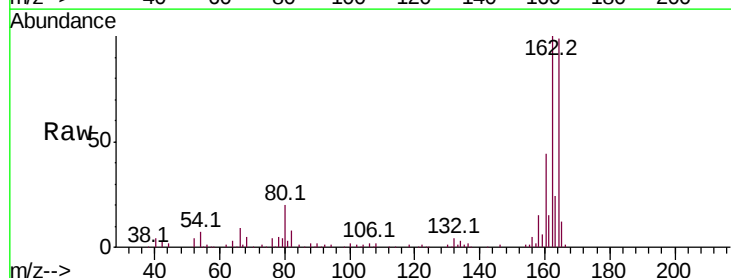




#41
 2,4,6-Tribromophenol
 Concen: 91.320 ng
 RT: 16.15 min Scan# 2189
 Delta R.T. -0.02 min
 Lab File: BG037134.D
 Acq: 3 Oct 2018 15:27

Instrument :
 BNA_G
 ClientSampleId :
 PB113454BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.6	75.4	113.2
141	38.1	30.7	46.1


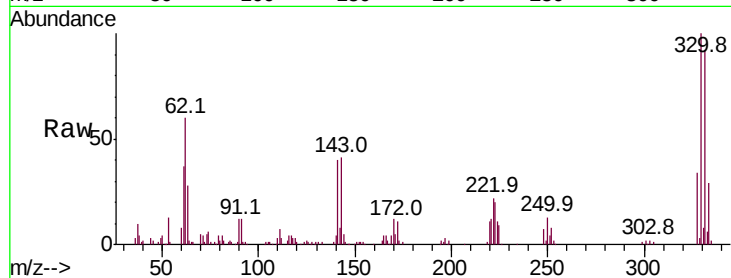


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

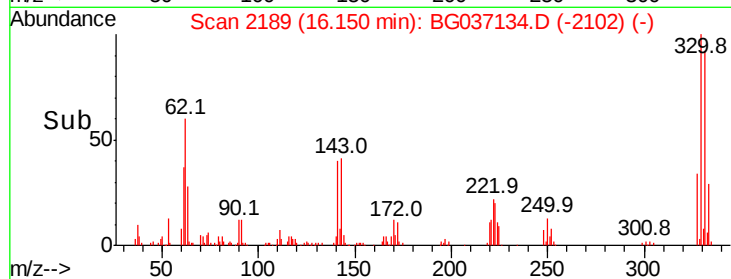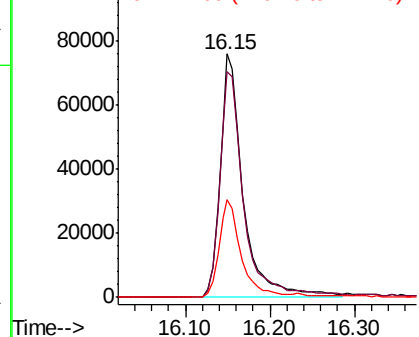

#44
 2-Fluorobiphenyl
 Concen: 75.600 ng
 RT: 13.28 min Scan# 1701
 Delta R.T. -0.02 min
 Lab File: BG037134.D
 Acq: 3 Oct 2018 15:27

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.1	31.3	46.9
170	24.4	21.0	31.6


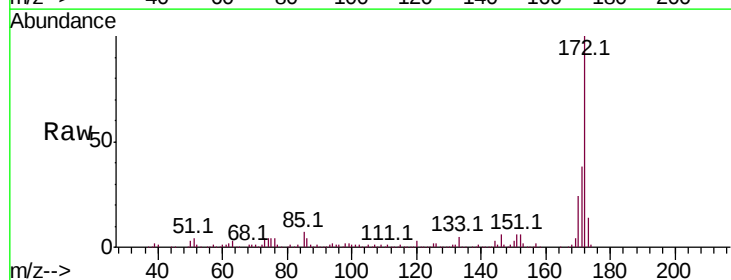


Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



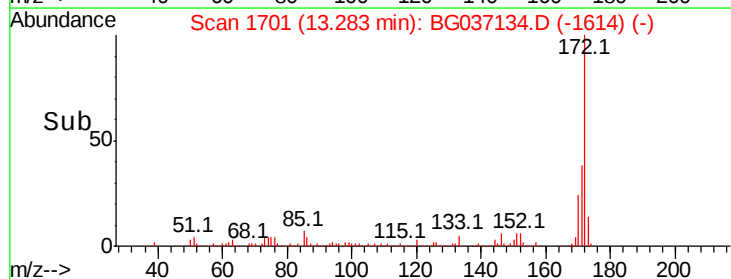
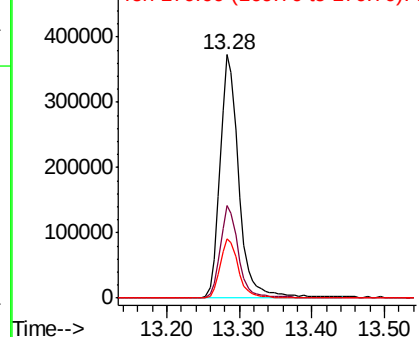




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.41 min Scan# 2403
Delta R.T. -0.01 min
Lab File: BG037134.D
Acq: 3 Oct 2018 15:27




Instrument :
BNA_G
ClientSampleId :
PB113454BL

Tot Ion:188 Resp: 320925
Ion Ratio Lower Upper
188 100
94 9.0 6.7 10.1
80 9.8 8.1 12.1

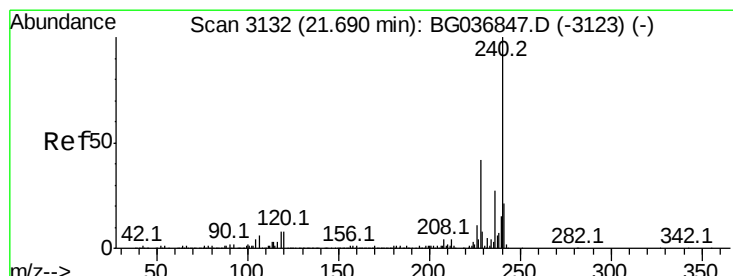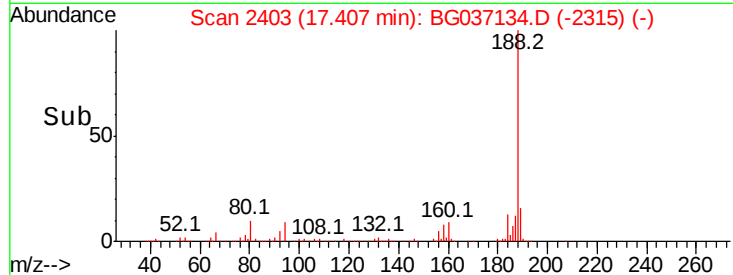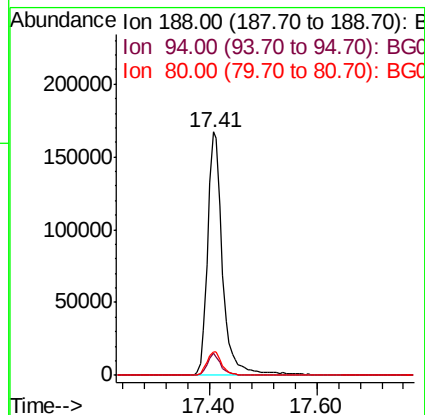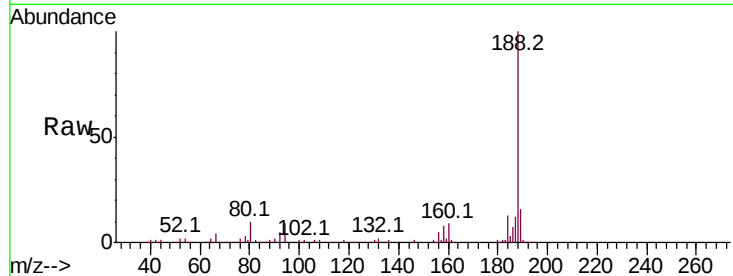

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.67 min Scan# 3129
Delta R.T. -0.02 min
Lab File: BG037134.D
Acq: 3 Oct 2018 15:27

Tgt Ion:240 Resp: 323282
Ion Ratio Lower Upper
240 100
120 9.2 6.9 10.3
236 25.8 21.2 31.8

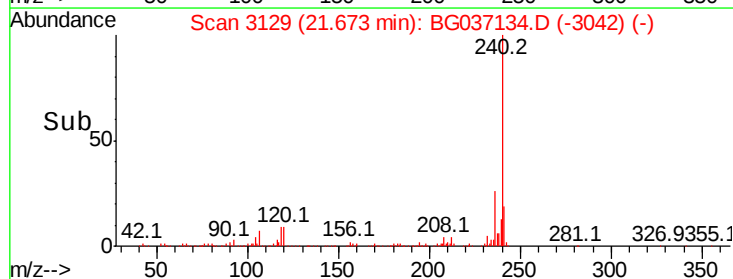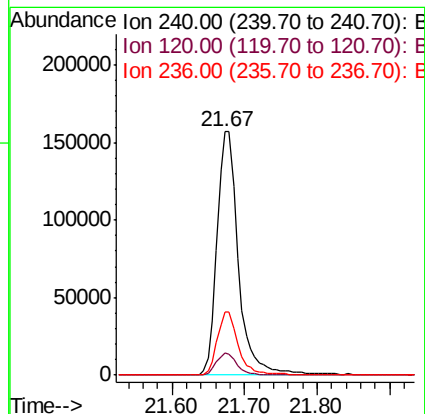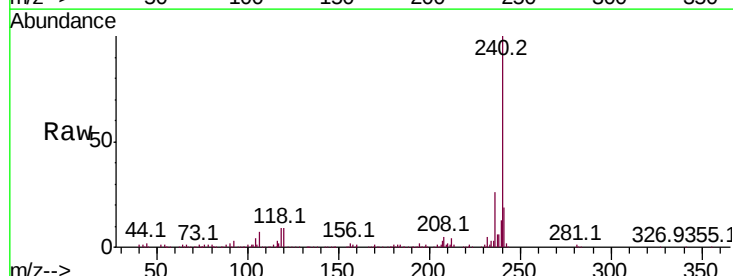



#78

Terphenyl-d14

Concen: 83.318 ng

RT: 20.02 min Scan# 2847

Delta R.T. -0.01 min

Lab File: BG037134.D

Acq: 3 Oct 2018 15:27

Instrument :





BNA_G

ClientSampleId :

PB113454BL

Tot Ion:244 Resp: 1024348

Ion	Ratio	Lower	Upper
244	100		
212	8.4	7.0	10.6
122	9.3	7.1	10.7

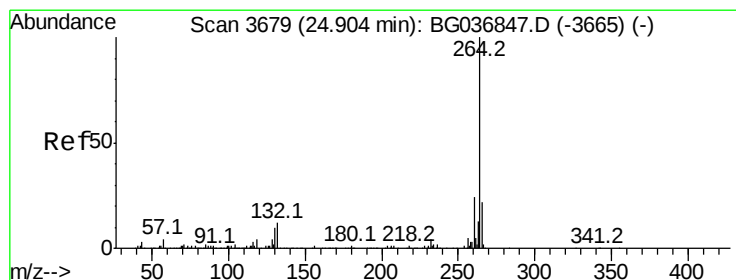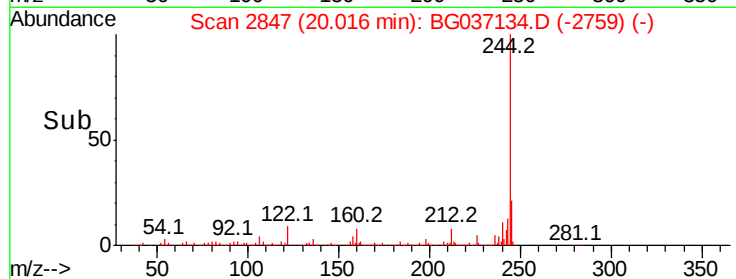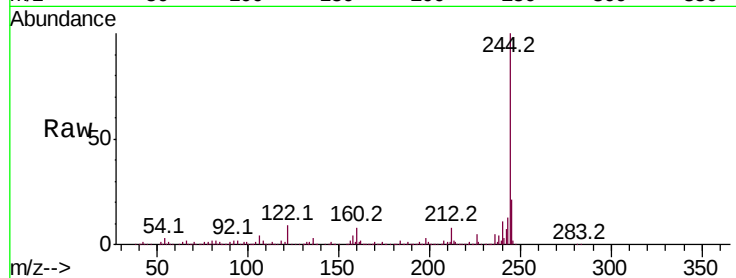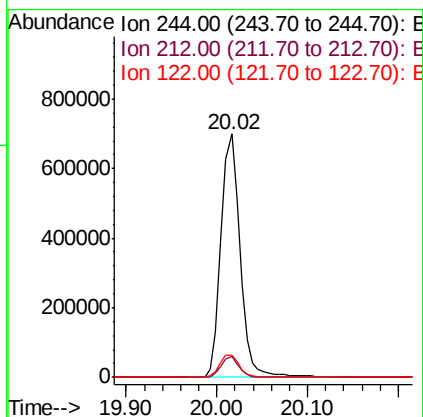

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.88 min Scan# 3675

Delta R.T. -0.02 min

Lab File: BG037134.D

Acq: 3 Oct 2018 15:27

Tgt Ion:264 Resp: 314856

Ion	Ratio	Lower	Upper
264	100		
260	22.7	19.6	29.4
265	22.1	17.4	26.0

