


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100419\
 Data File : BG043029.D
 Acq On : 4 Oct 2019 15:44
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 25 15:35:52 2019

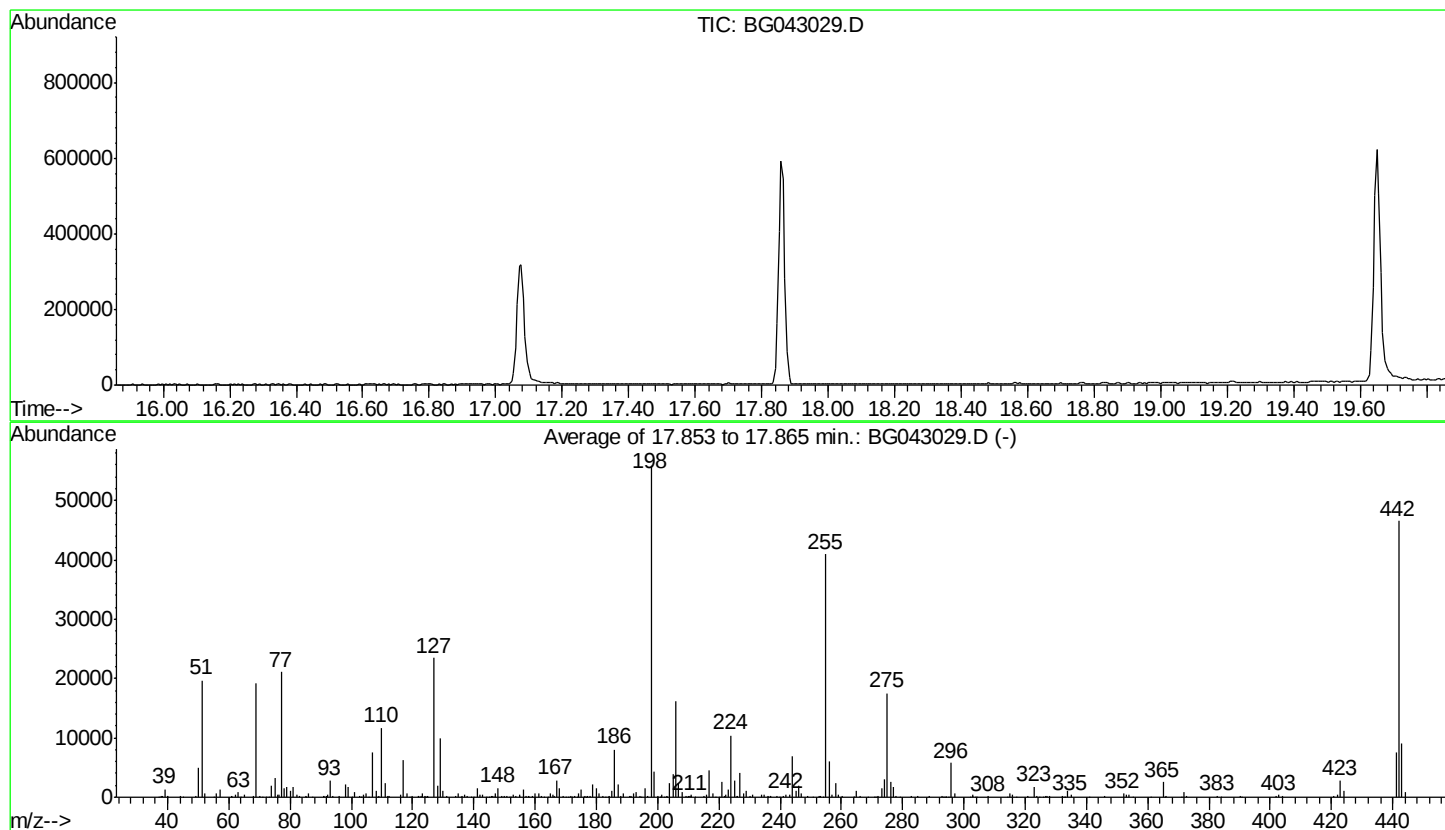

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	19736	PASS
68	69	0.00	2	0.8	146	PASS
69	198	0.00	100	34.4	19232	PASS
70	69	0.00	2	1.0	187	PASS
127	198	10	80	41.9	23429	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55893	PASS
199	198	5	9	7.6	4273	PASS
275	198	10	60	31.3	17512	PASS
365	198	1	100	4.5	2537	PASS
441	198	0.01	100	13.5	7558	PASS
442	198	50	100	83.2	46530	PASS
443	442	15	24	19.7	9155	PASS