

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100422\
 Data File : BG055064.D
 Acq On : 4 Oct 2022 15:29
 Operator : CG/JU
 Sample : N4943-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 05 00:31:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 04 07:12:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.340	152	28725	20.000	ng	0.00
21) Naphthalene-d8	11.172	136	125376	20.000	ng	0.00
39) Acenaphthene-d10	14.950	164	93211	20.000	ng	0.00
64) Phenanthrene-d10	17.682	188	229542	20.000	ng	0.00
76) Chrysene-d12	21.977	240	230916	20.000	ng	0.00
86) Perylene-d12	25.438	264	246456	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.861	112	169194	130.828	ng	0.00
7) Phenol-d6	7.471	99	237384	122.508	ng	0.00
23) Nitrobenzene-d5	9.509	82	143922	68.593	ng	0.00
42) 2,4,6-Tribromophenol	16.425	330	123093	127.222	ng	0.00
45) 2-Fluorobiphenyl	13.581	172	349414	58.521	ng	0.00
79) Terphenyl-d14	20.256	244	645868	56.532	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.381	88	2540	3.471	ng	# 1
19) n-Nitroso-di-n-propyla...	9.509	70	19988	10.649	ng	# 79
31) Naphthalene	11.225	128	140101	21.173	ng	99
33) 4-Chloroaniline	11.225	127	17968	6.567	ng	# 34
36) 4-Chloro-3-methylphenol	11.959	107	145	2.966	ng	# 22
37) 2-Methylnaphthalene	12.800	142	59515	12.205	ng	99
38) 1-Methylnaphthalene	13.017	142	33181	6.995	ng	96
46) 1,1'-Biphenyl	13.787	154	18581	2.907	ng	96
48) 2-Nitroaniline	13.787	65	66	4.123	ng	# 7
51) 2,6-Dinitrotoluene	14.944	165	13986	13.508	ng	# 14
52) Acenaphthene	15.009	154	60984	11.517	ng	98
55) Dibenzofuran	15.338	168	103916	12.301	ng	97
56) 4-Nitrophenol	15.338	139	39511	36.875	ng	# 2
57) 2,4-Dinitrotoluene	15.261	165	552	3.893	ng	# 15
58) Fluorene	15.984	166	102249	15.125	ng	99
67) 4-Bromophenyl-phenylether	16.419	248	7452	3.070	ng	# 1
71) Phenanthrene	17.723	178	440051	36.496	ng	99
72) Anthracene	17.811	178	45854	3.910	ng	97
75) Fluoranthene	19.709	202	267485	17.782	ng	99
77) Benzidine	20.256	184	9754	2.452	ng	# 90
78) Pyrene	20.068	202	181523	11.822	ng	99
80) Butylbenzylphthalate	20.949	149	54	4.849	ng	# 53
81) Benzo(a)anthracene	21.954	228	49483	3.373	ng	97
83) Chrysene	22.024	228	34305	2.426	ng	95
84) Bis(2-ethylhexyl)phtha...	21.848	149	1318	4.269	ng	# 95
85) Di-n-octyl phthalate	23.140	149	58	4.345	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100422\
Data File : BG055064.D
Acq On : 4 Oct 2022 15:29
Operator : CG/JU
Sample : N4943-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 05 00:31:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 07:12:22 2022
Response via : Initial Calibration




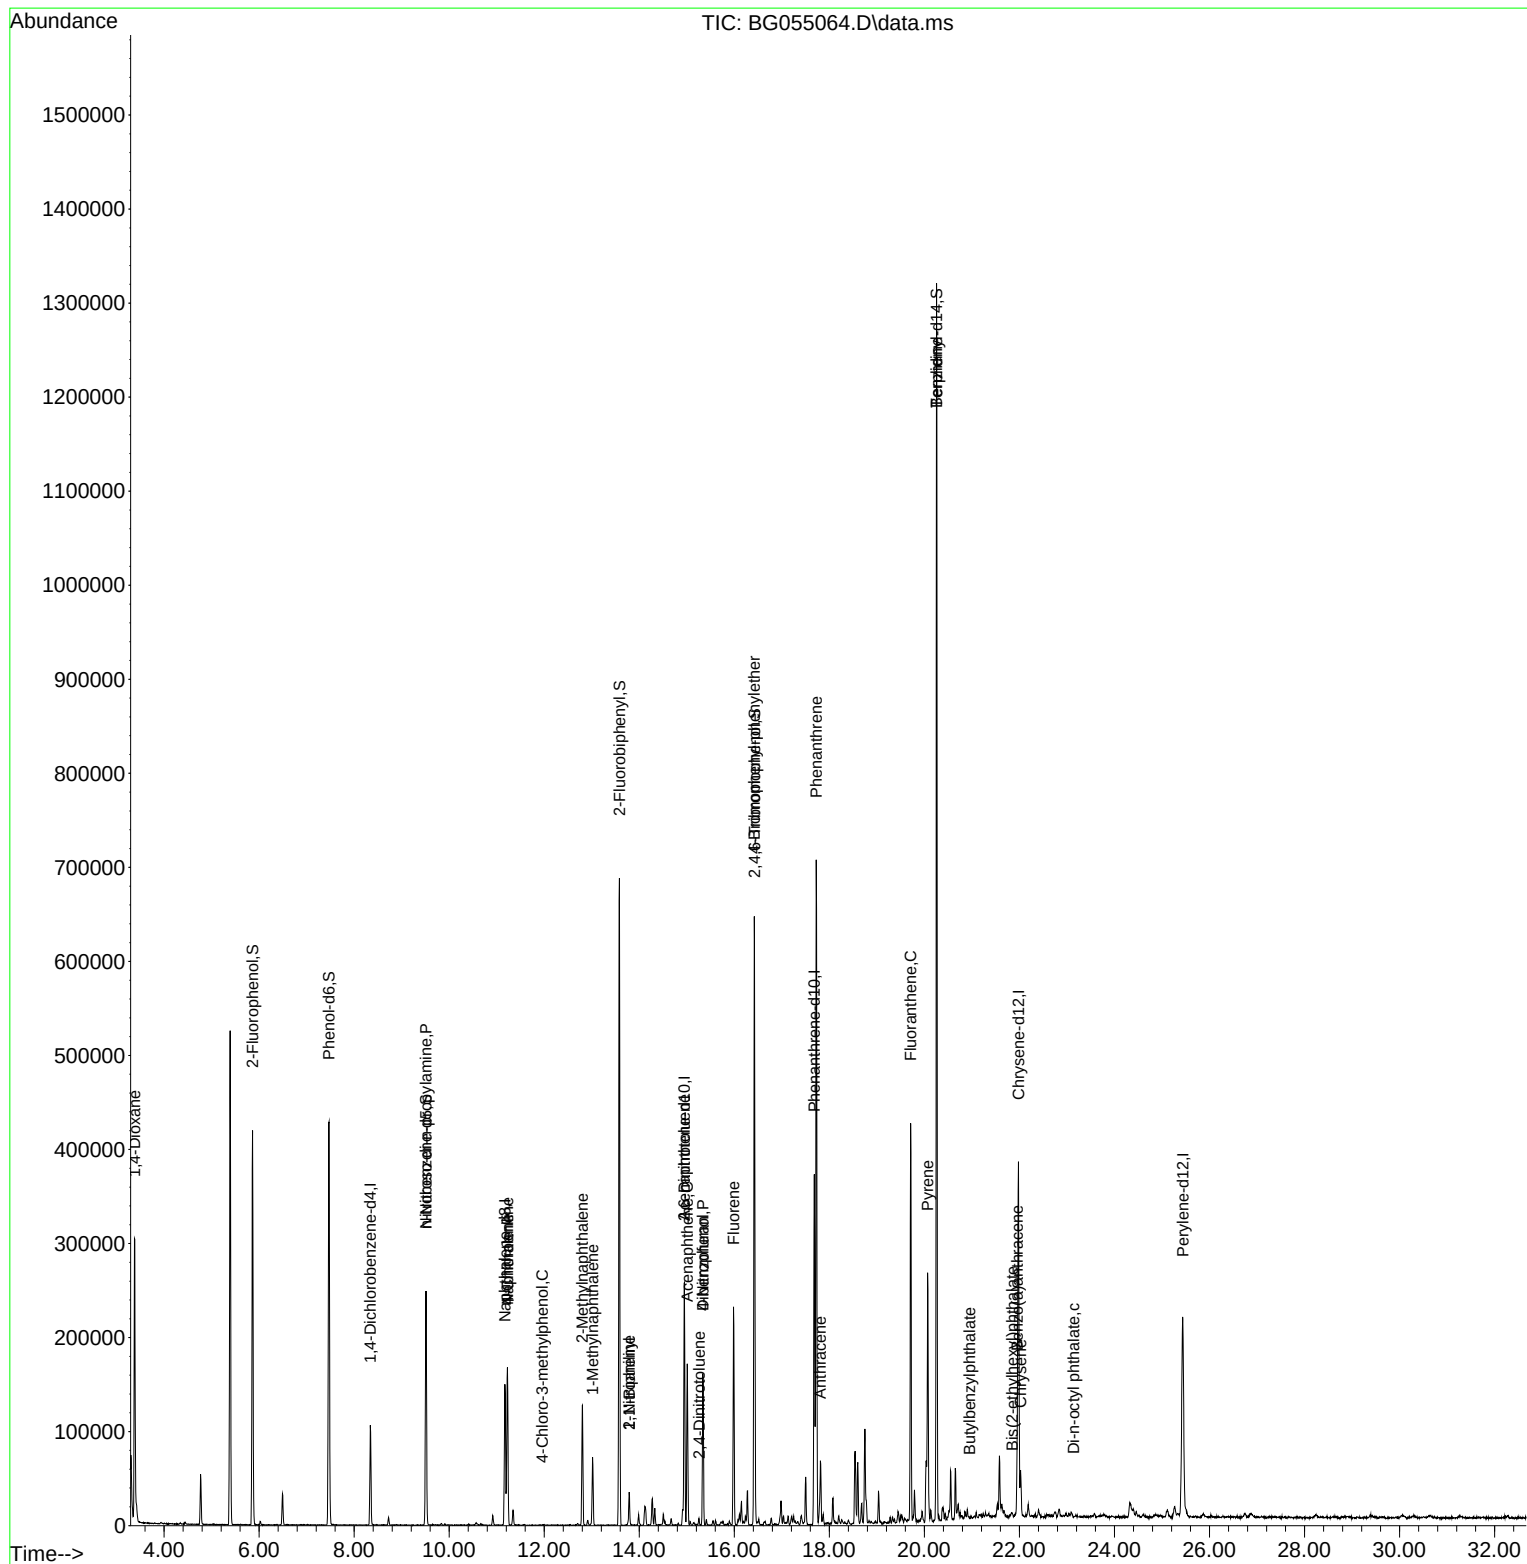




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.340 min Scan# 80
 Delta R.T. -0.001 min
 Lab File: BG055064.D
 Acq: 4 Oct 2022 15:29




Instrument :
 BNA_G
 ClientSampleId :


Tgt Ion:152 Resp: 28725
 Ion Ratio Lower Upper
 152 100
 150 147.6 128.0 192.0
 115 58.1 47.7 71.5

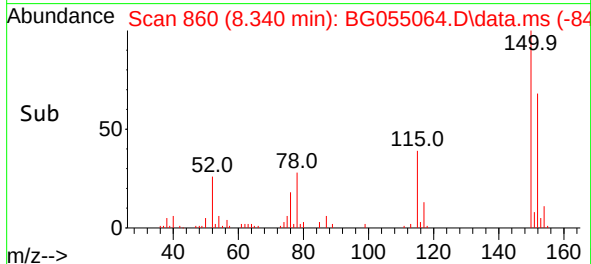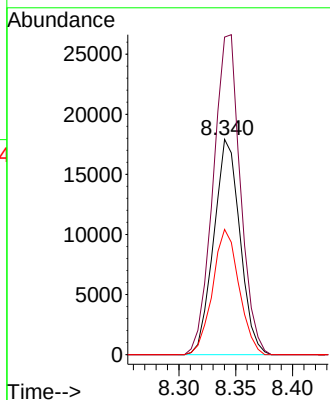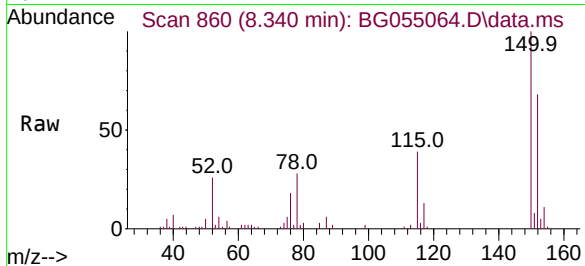

#2
 1,4-Dioxane
 Concen: 3.471 ng
 RT: 3.381 min Scan# 16
 Delta R.T. -0.312 min
 Lab File: BG055064.D
 Acq: 4 Oct 2022 15:29

Tgt Ion: 88 Resp: 2540
 Ion Ratio Lower Upper
 88 100
 58 75.7 62.6 94.0
 43 2923.6 29.0 43.6#


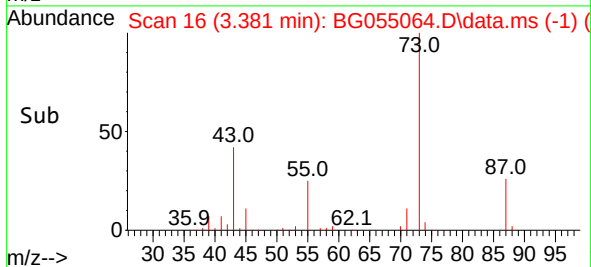
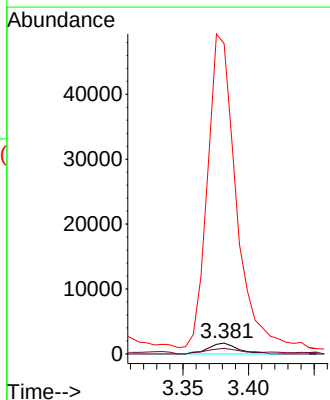
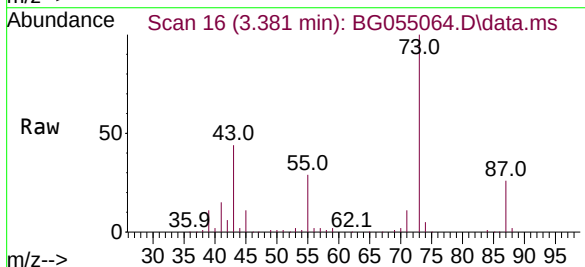




#5
2-Fluorophenol
Concen: 130.828 ng
RT: 5.861 min Scan# 437
Delta R.T. 0.006 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29




Instrument :
BNA_G
ClientSampleId :


Tgt Ion:112 Resp: 169194
Ion Ratio Lower Upper
112 100
64 65.9 54.5 81.7
63 36.4 30.5 45.7

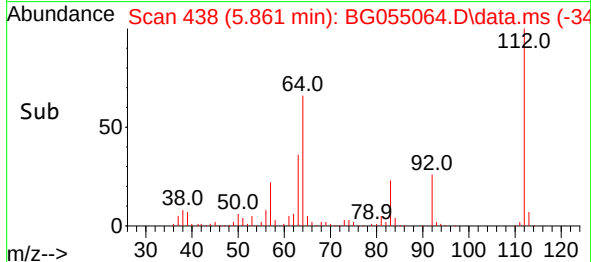

#7
Phenol-d6
Concen: 122.508 ng
RT: 7.471 min Scan# 712
Delta R.T. 0.006 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29

Tgt Ion: 99 Resp: 237384
Ion Ratio Lower Upper
99 100
42 23.2 18.6 28.0
71 38.4 31.2 46.8

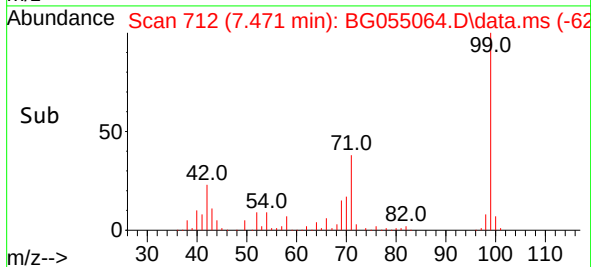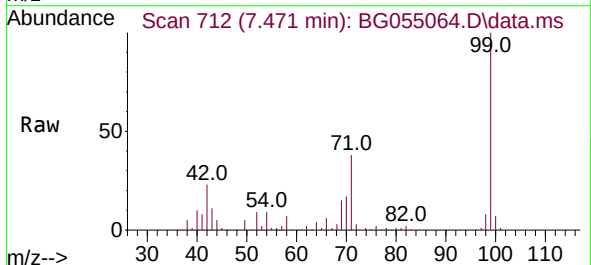



#19

n-Nitroso-di-n-propylamine

Concen: 10.649 ng

RT: 9.509 min Scan# 1059

Delta R.T. 0.364 min


Lab File: BG055064.D

Acq: 4 Oct 2022 15:29

Instrument :

BNA_G

ClientSampleId :



Tgt Ion: 70 Resp: 19988




Ion Ratio Lower Upper

70 100

42 54.7 55.8 83.6#

101 0.0 7.1 10.7#

130 2.1 12.9 19.3#

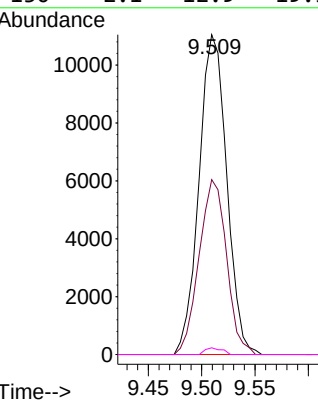

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.172 min Scan# 1342

Delta R.T. -0.001 min

Lab File: BG055064.D

Acq: 4 Oct 2022 15:29

Tgt Ion: 136 Resp: 125376




Ion Ratio Lower Upper


136 100

137 10.8 8.7 13.1

54 10.4 8.2 12.4

68 5.4 4.9 7.3

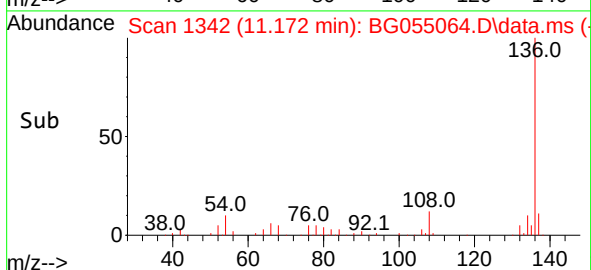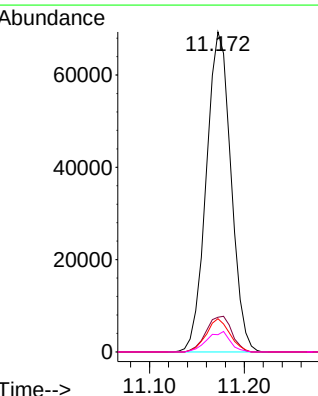



#23

Nitrobenzene-d5

Concen: 68.593 ng

RT: 9.509 min Scan# 1059

Delta R.T. -0.001 min

Lab File: BG055064.D

Acq: 4 Oct 2022 15:29

Instrument :

BNA_G

ClientSampleId :





Tgt Ion: 82 Resp: 143922

Ion Ratio Lower Upper

82 100

128 39.2 29.5 44.3

54 57.5 46.7 70.1

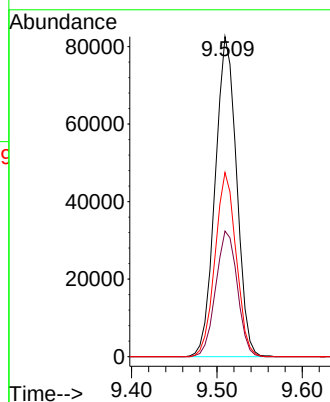

#31

Naphthalene

Concen: 21.173 ng

RT: 11.225 min Scan# 1351

Delta R.T. -0.001 min

Lab File: BG055064.D

Acq: 4 Oct 2022 15:29




Tgt Ion: 128 Resp: 140101


Ion Ratio Lower Upper

128 100

129 10.7 8.7 13.1


127 13.4 10.9 16.3

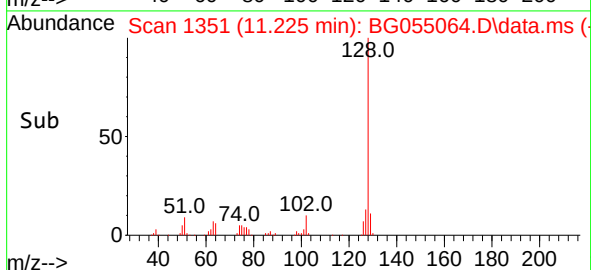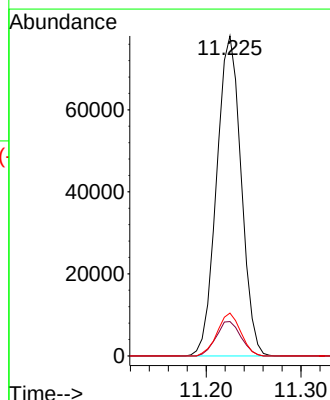






#33
4-Chloroaniline
Concen: 6.567 ng
RT: 11.225 min Scan# 1476
Delta R.T. -0.095 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29

Instrument :
BNA_G
ClientSampleId :







Tgt Ion:127	Resp:	17968
Ion	Ratio	Lower Upper
127	100	
129	80.4	26.4 39.6#
65	0.0	28.6 43.0#
92	0.0	16.2 24.2#

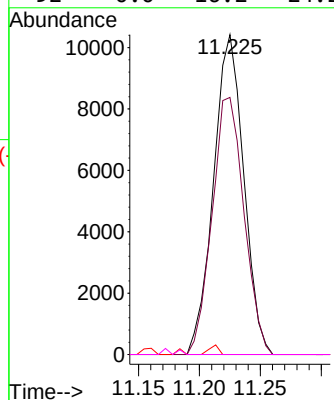

#36
4-Chloro-3-methylphenol
Concen: 2.966 ng
RT: 11.959 min Scan# 1476
Delta R.T. -0.442 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29

Tgt Ion:107	Resp:	145
Ion	Ratio	Lower Upper
107	100	
144	0.0	19.7 29.5#
142	0.0	59.3 88.9#

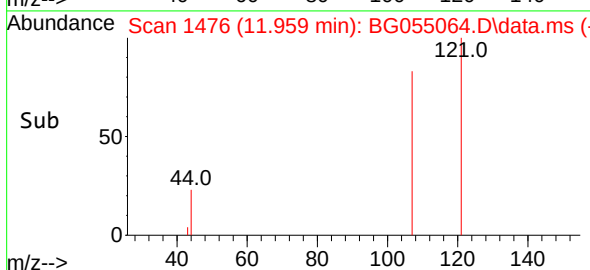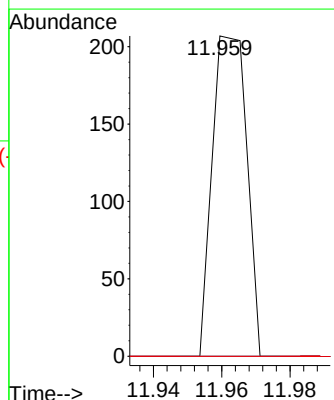



#37

2-Methylnaphthalene

Concen: 12.205 ng

RT: 12.800 min Scan# 1619

Delta R.T. -0.000 min


Lab File: BG055064.D

Acq: 4 Oct 2022 15:29

Instrument :

BNA_G

ClientSampleId :






Tgt Ion:142 Resp: 59515

Ion Ratio Lower Upper

142 100

141 93.9 75.0 112.4

115 36.9 31.7 47.5

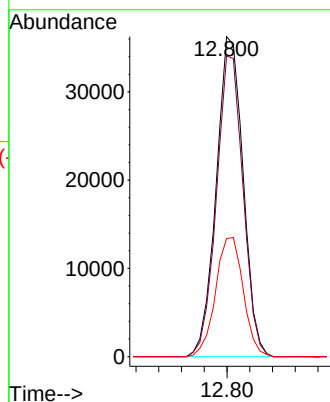

#38

1-Methylnaphthalene

Concen: 6.995 ng

RT: 13.017 min Scan# 1656

Delta R.T. -0.001 min

Lab File: BG055064.D

Acq: 4 Oct 2022 15:29




Tgt Ion:142 Resp: 33181


Ion Ratio Lower Upper

142 100

141 90.2 75.5 113.3


116 4.9 3.4 5.2

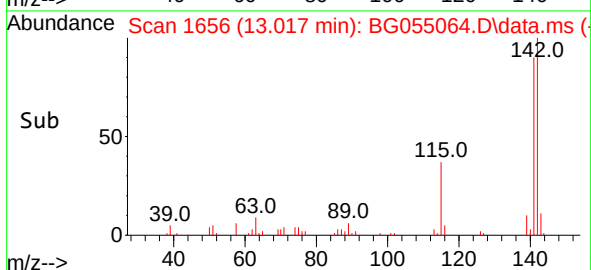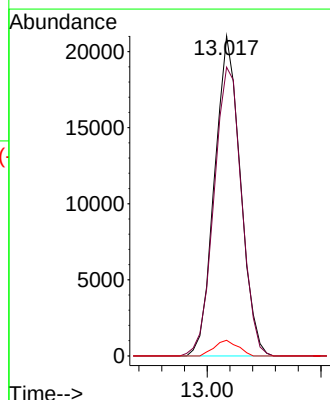






#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.950 min Scan# 1985
Delta R.T. -0.001 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29


Instrument :
BNA_G
ClientSampleId :





Tgt Ion:164 Resp: 93211
Ion Ratio Lower Upper
164 100
162 106.2 85.5 128.3
160 46.5 35.5 53.3

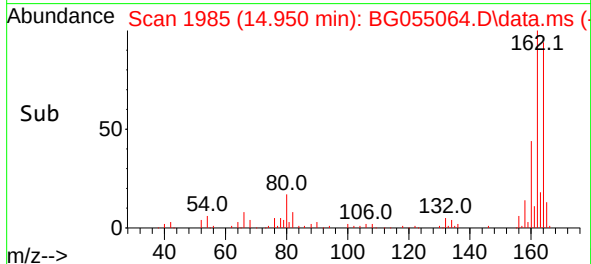


#42
2,4,6-Tribromophenol
Concen: 127.222 ng
RT: 16.425 min Scan# 2236
Delta R.T. -0.000 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29

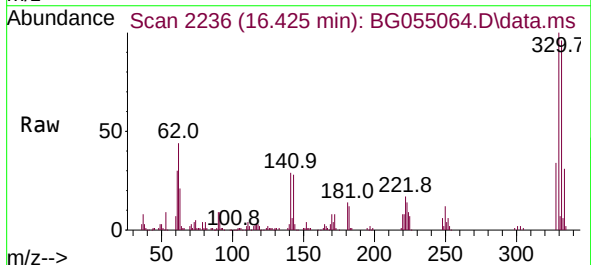


Tgt Ion:330 Resp: 123093
Ion Ratio Lower Upper
330 100
332 96.6 77.4 116.0
141 31.5 25.0 37.4

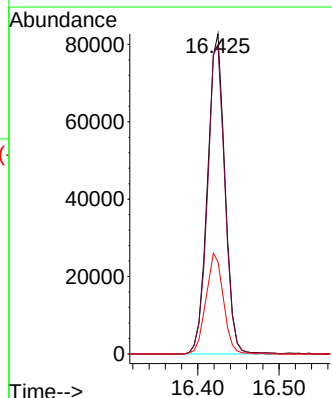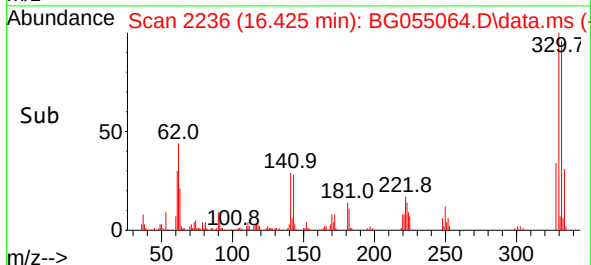






#45
2-Fluorobiphenyl
Concen: 58.521 ng
RT: 13.581 min Scan# 1752
Delta R.T. -0.001 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29


Instrument :
BNA_G
ClientSampleId :





Tgt Ion:172 Resp: 349414
Ion Ratio Lower Upper
172 100
171 37.2 30.1 45.1
170 24.9 20.0 30.0

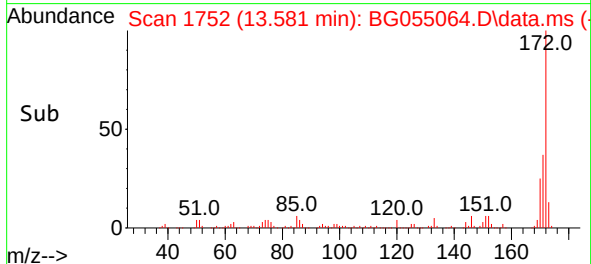


#46
1,1'-Biphenyl
Concen: 2.907 ng
RT: 13.787 min Scan# 1787
Delta R.T. -0.001 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29

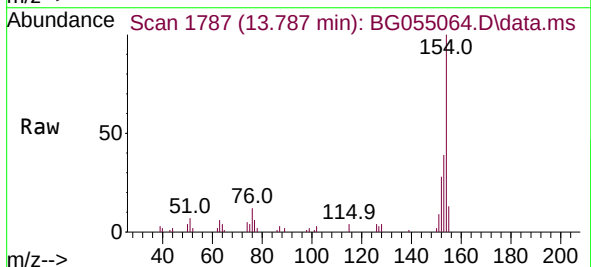

Tgt Ion:154 Resp: 18581
Ion Ratio Lower Upper
154 100
153 39.4 22.0 62.0
76 11.9 0.0 33.3



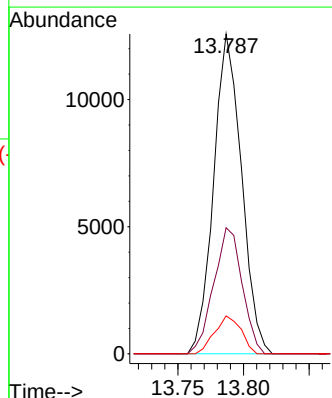
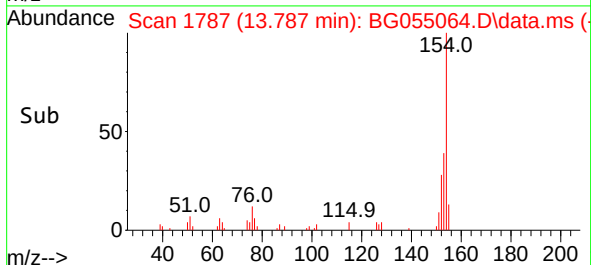




#48
2-Nitroaniline
Concen: 4.123 ng
RT: 13.787 min Scan# 11
Delta R.T. -0.235 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29




Instrument :
BNA_G
ClientSampleId :


Tgt Ion: 65 Resp: 66
Ion Ratio Lower Upper
65 100
92 0.0 50.9 76.3#
138 0.0 79.5 119.3#

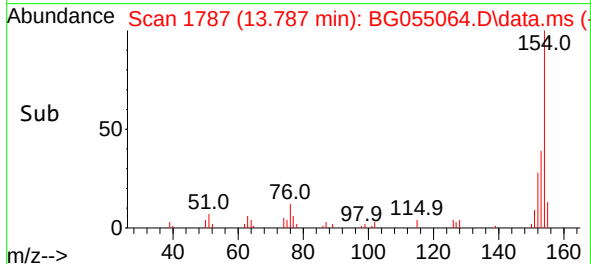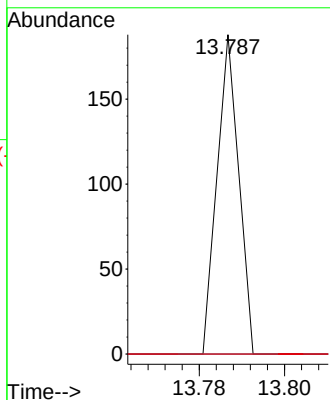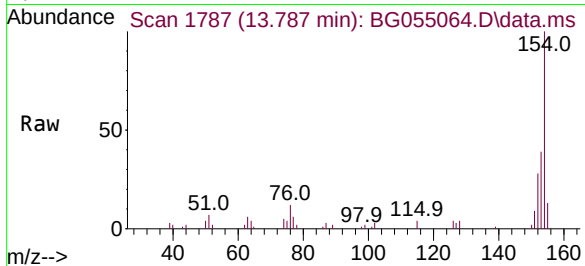

#51
2,6-Dinitrotoluene
Concen: 13.508 ng
RT: 14.944 min Scan# 1984
Delta R.T. 0.434 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29


Tgt Ion:165 Resp: 13986
Ion Ratio Lower Upper
165 100
63 0.0 56.2 84.4#
89 1.9 60.4 90.6#

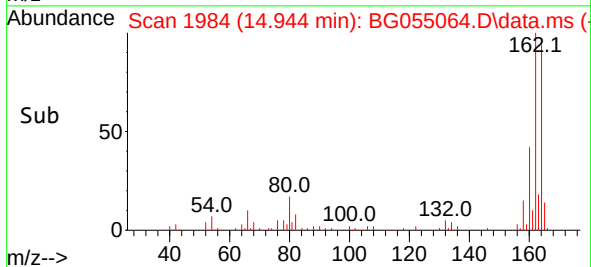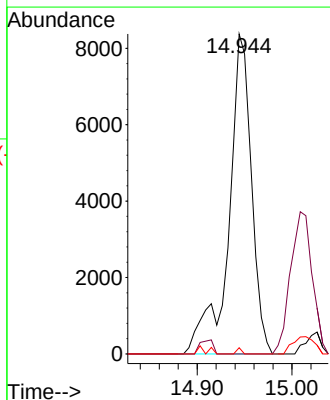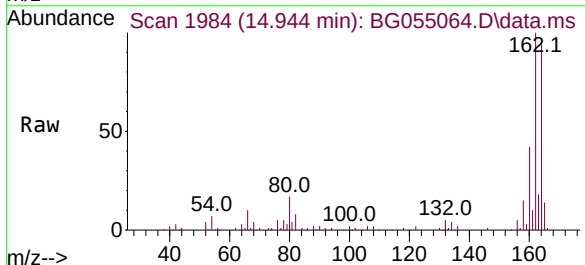






#52
Acenaphthene
Concen: 11.517 ng
RT: 15.009 min Scan# 1996
Delta R.T. -0.006 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29


Instrument :
BNA_G
ClientSampleId :





Tgt Ion:154 Resp: 60984
Ion Ratio Lower Upper
154 100
153 116.9 91.4 137.0
152 57.5 45.3 67.9

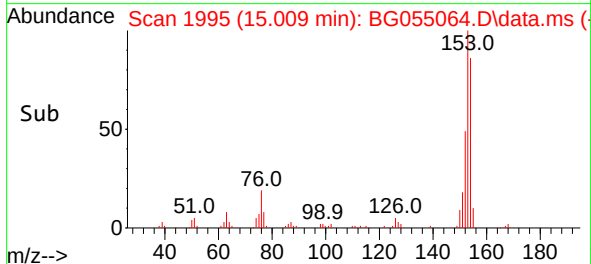


#55
Dibenzofuran
Concen: 12.301 ng
RT: 15.338 min Scan# 2051
Delta R.T. -0.006 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29

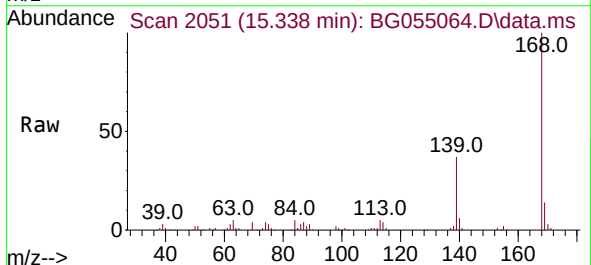

Tgt Ion:168 Resp: 103916
Ion Ratio Lower Upper
168 100
139 36.5 31.0 46.4
169 14.3 10.6 16.0




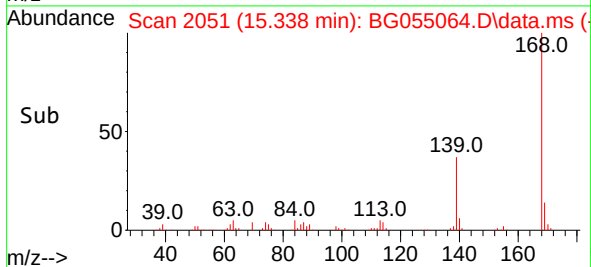




#56
4-Nitrophenol
Concen: 36.875 ng
RT: 15.338 min Scan# 2013
Delta R.T. 0.223 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29




Instrument :
BNA_G
ClientSampleId :


Tgt Ion:139 Resp: 39511
Ion Ratio Lower Upper
139 100
109 1.2 66.6 106.6#
65 1.4 88.5 128.5#

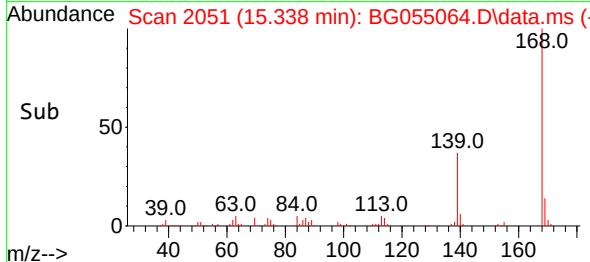

#57
2,4-Dinitrotoluene
Concen: 3.893 ng
RT: 15.261 min Scan# 2038
Delta R.T. -0.025 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29


Tgt Ion:165 Resp: 552
Ion Ratio Lower Upper
165 100
63 0.0 44.2 66.2#
89 0.0 69.0 103.6#
182 0.0 2.2 3.4#

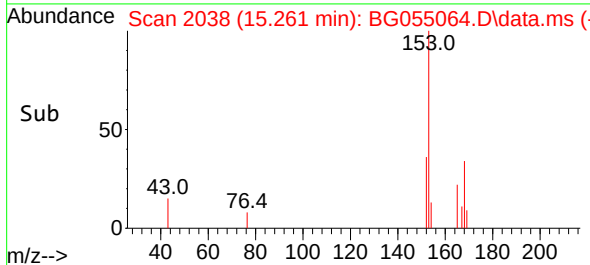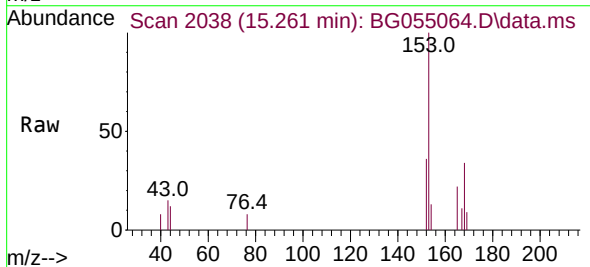






#58
 Fluorene
 Concen: 15.125 ng
 RT: 15.984 min Scan# 2161
 Delta R.T. -0.001 min
 Lab File: BG055064.D
 Acq: 4 Oct 2022 15:29


Instrument :
 BNA_G
 ClientSampleId :





Tgt Ion:166 Resp: 102249
 Ion Ratio Lower Upper
 166 100
 165 102.5 82.6 123.8
 167 14.2 11.8 17.8

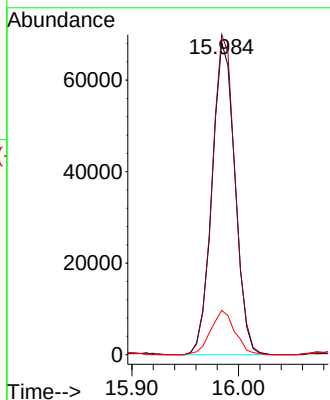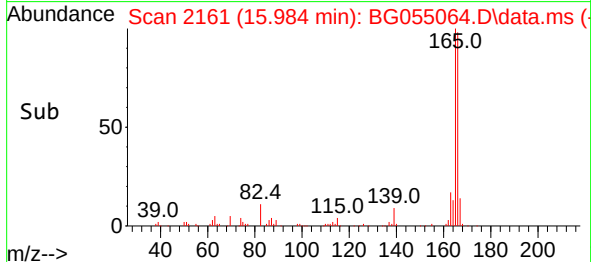


#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.682 min Scan# 2450
 Delta R.T. -0.001 min
 Lab File: BG055064.D
 Acq: 4 Oct 2022 15:29

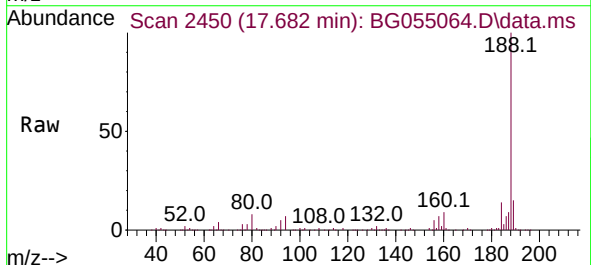

Tgt Ion:188 Resp: 229542
 Ion Ratio Lower Upper
 188 100
 94 7.1 6.2 9.2
 80 8.4 7.2 10.8

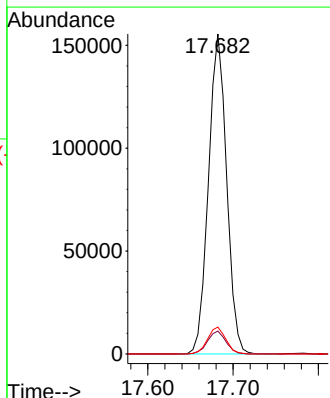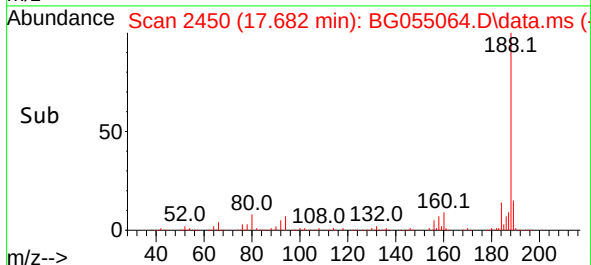



#67

4-Bromophenyl-phenylether

Concen: 3.070 ng

RT: 16.419 min Scan# 21

Delta R.T. -0.447 min


Lab File: BG055064.D

Acq: 4 Oct 2022 15:29

Instrument :

BNA_G

ClientSampleId :






Tgt Ion:248 Resp: 7452

Ion Ratio Lower Upper

248 100

250 189.5 81.7 122.5#

141 505.1 53.7 80.5#

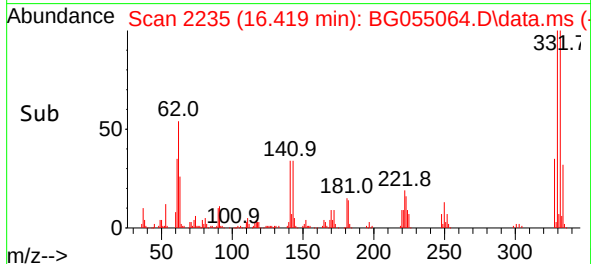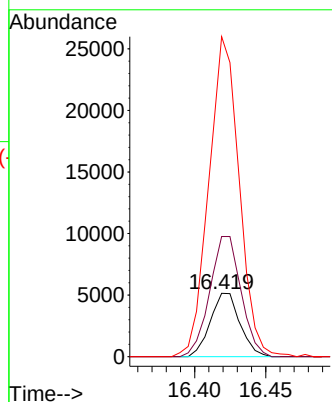

#71

Phenanthrene

Concen: 36.496 ng

RT: 17.723 min Scan# 2457

Delta R.T. -0.001 min

Lab File: BG055064.D

Acq: 4 Oct 2022 15:29




Tgt Ion:178 Resp: 440051


Ion Ratio Lower Upper

178 100

176 19.2 15.8 23.6


179 16.1 13.2 19.8

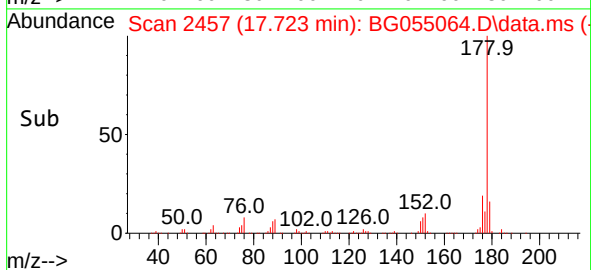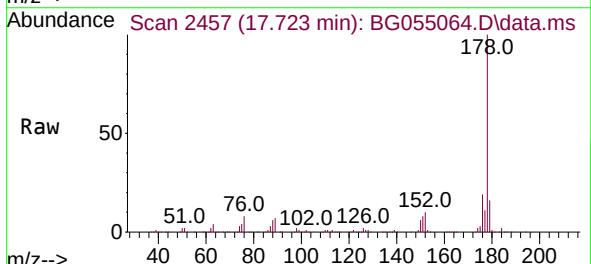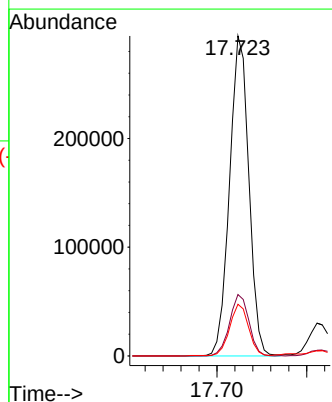






#72
 Anthracene
 Concen: 3.910 ng
 RT: 17.811 min Scan# 2473
 Delta R.T. -0.006 min
 Lab File: BG055064.D
 Acq: 4 Oct 2022 15:29


Instrument :
 BNA_G
 ClientSampleId :





Tgt Ion:178 Resp: 45854
 Ion Ratio Lower Upper
 178 100
 176 17.1 15.7 23.5
 179 15.3 12.5 18.7

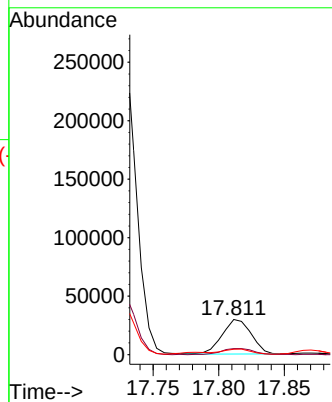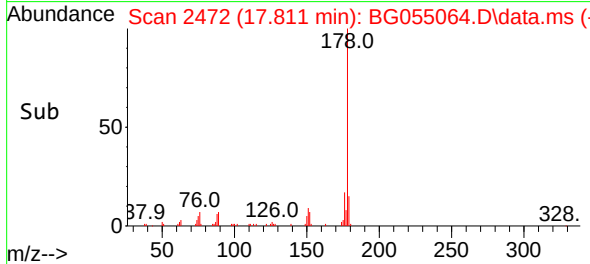


#75
 Fluoranthene
 Concen: 17.782 ng
 RT: 19.709 min Scan# 2795
 Delta R.T. -0.000 min
 Lab File: BG055064.D
 Acq: 4 Oct 2022 15:29

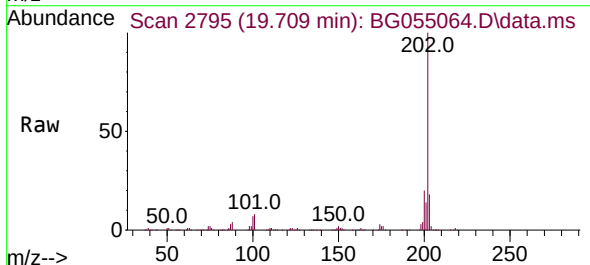

Tgt Ion:202 Resp: 267485
 Ion Ratio Lower Upper
 202 100
 101 8.4 0.0 28.9
 203 18.0 0.0 37.7

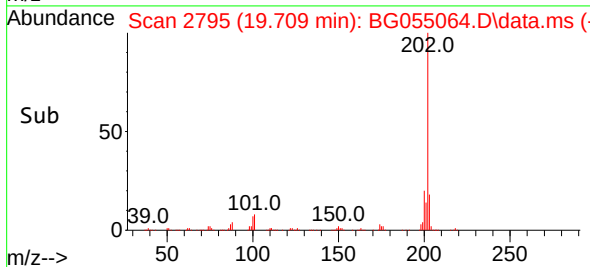

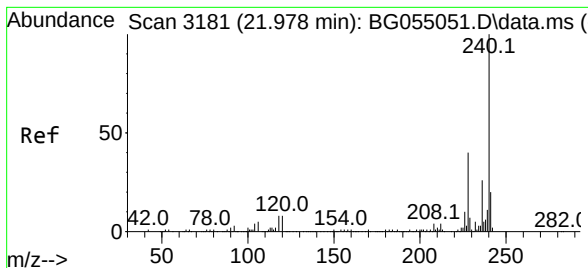

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.977 min Scan# 31

Delta R.T. -0.001 min


Lab File: BG055064.D

Acq: 4 Oct 2022 15:29

Instrument :

BNA_G

ClientSampleId :

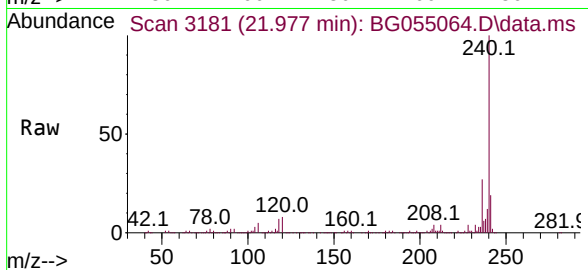




Tgt Ion:240 Resp: 230916

Ion Ratio Lower Upper

240 100

120 7.7 6.2 9.4

236 26.6 20.6 30.8

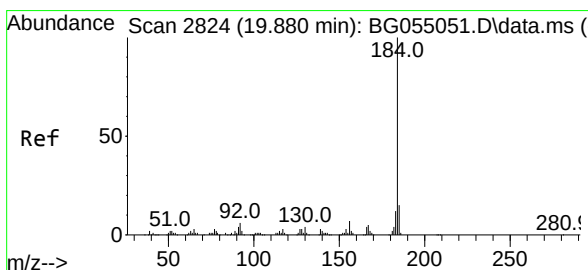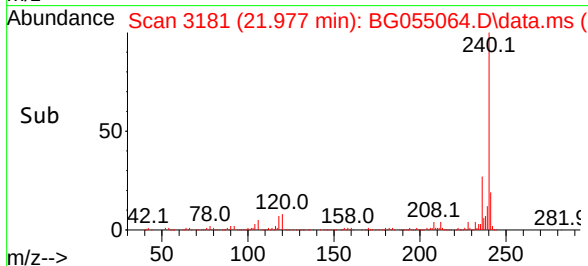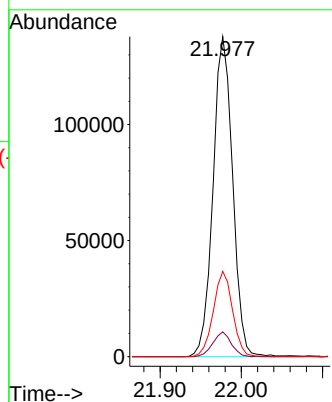

#77

Benzidine

Concen: 2.452 ng

RT: 20.256 min Scan# 2888

Delta R.T. 0.376 min

Lab File: BG055064.D

Acq: 4 Oct 2022 15:29




Tgt Ion:184 Resp: 9754


Ion Ratio Lower Upper

184 100

185 18.1 12.2 18.4

183 6.0 9.4 14.0#


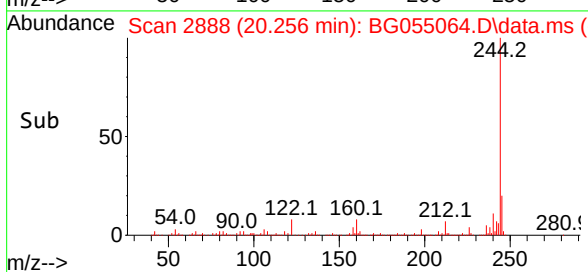
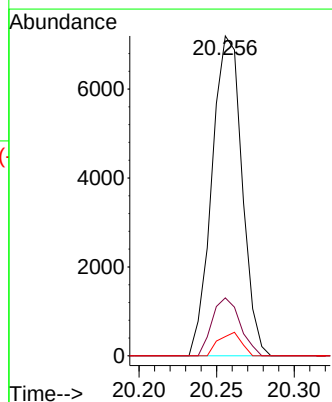
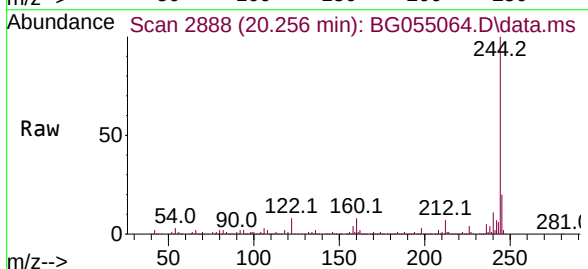




#78
 Pyrene
 Concen: 11.822 ng
 RT: 20.068 min Scan# 2856
 Delta R.T. -0.006 min
 Lab File: BG055064.D
 Acq: 4 Oct 2022 15:29




Instrument :
 BNA_G
 ClientSampleId :


Tgt Ion:202 Resp: 181523
 Ion Ratio Lower Upper
 202 100
 200 20.4 16.6 25.0
 203 17.0 14.0 21.0

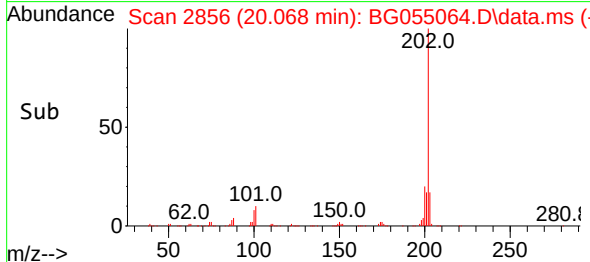

#79
 Terphenyl-d14
 Concen: 56.532 ng
 RT: 20.256 min Scan# 2888
 Delta R.T. -0.000 min
 Lab File: BG055064.D
 Acq: 4 Oct 2022 15:29

Tgt Ion:244 Resp: 645868
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.0 9.0
 122 8.2 6.6 10.0


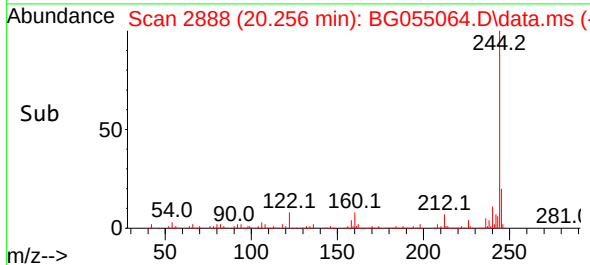

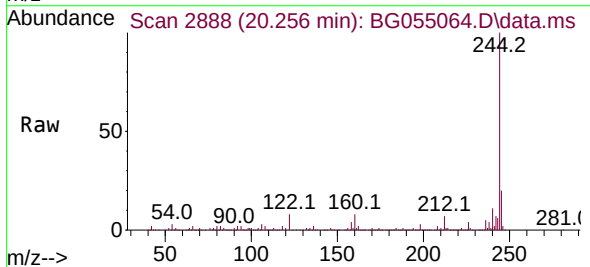




#80
Butylbenzylphthalate
Concen: 4.849 ng
RT: 20.949 min Scan# 3005
Delta R.T. 0.005 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29




Instrument :
BNA_G
ClientSampleId :


Tgt Ion	Ratio	Lower	Upper
149	100		
91	112.3	57.8	86.8#
206	0.0	16.9	25.3#

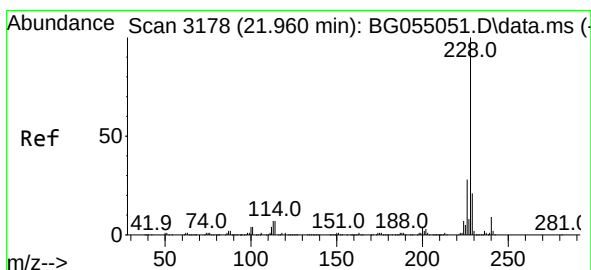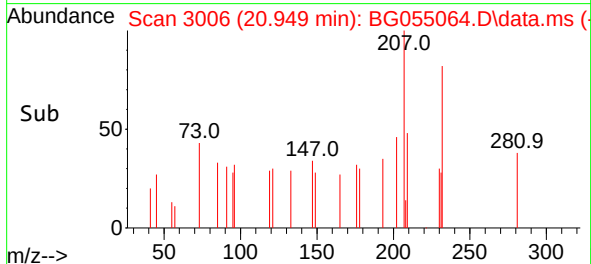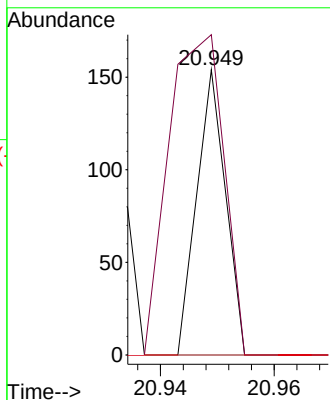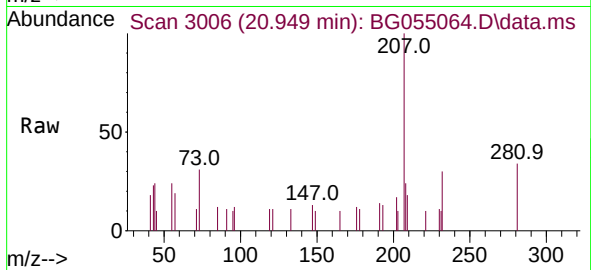

#81
Benzo(a)anthracene
Concen: 3.373 ng
RT: 21.954 min Scan# 3177
Delta R.T. -0.006 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29

Tgt Ion	Ratio	Lower	Upper
228	100		
226	27.5	22.4	33.6
229	18.8	16.7	25.1


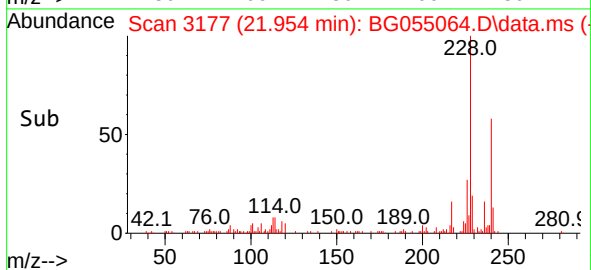
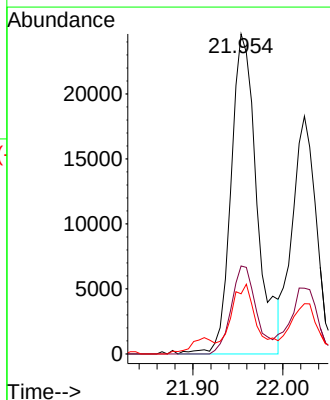
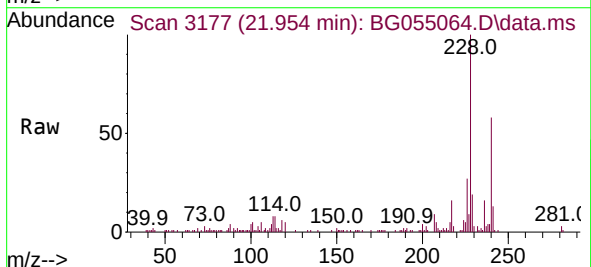




#83
Chrysene
Concen: 2.426 ng
RT: 22.024 min Scan# 3190
Delta R.T. -0.006 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29




Instrument :
BNA_G
ClientSampleId :


Tgt Ion:228 Resp: 34305
Ion Ratio Lower Upper
228 100
226 27.6 25.3 37.9
229 21.1 16.1 24.1

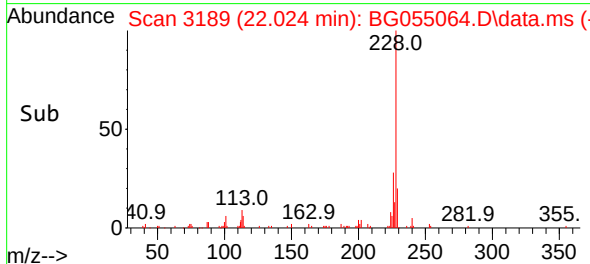

#84
Bis(2-ethylhexyl)phthalate
Concen: 4.269 ng
RT: 21.848 min Scan# 3159
Delta R.T. -0.000 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29

Tgt Ion:149 Resp: 1318
Ion Ratio Lower Upper
149 100
167 28.1 21.0 31.4
279 0.0 3.4 5.2#


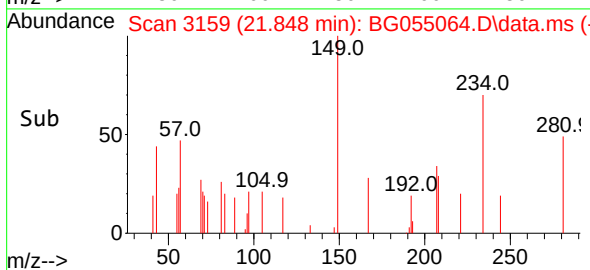

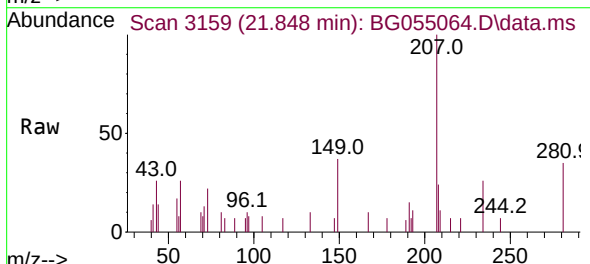




#85
Di-n-octyl phthalate
Concen: 4.345 ng
RT: 23.140 min Scan# 3380
Delta R.T. -0.007 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29

Instrument :
BNA_G
ClientSampleId :

Tgt Ion:149 Resp: 58
Ion Ratio Lower Upper
149 100
167 0.0 1.3 1.9#
43 277.6 10.2 15.4#

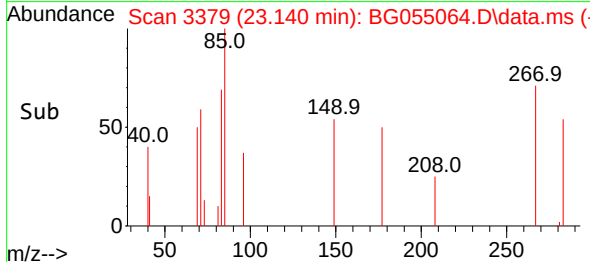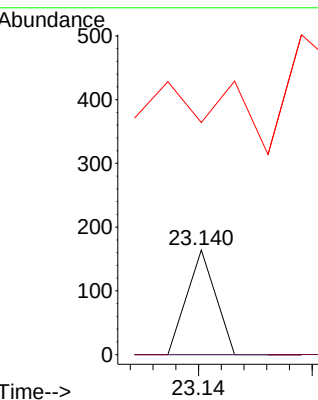

#86
Perylene-d12
Concen: 20.000 ng
RT: 25.438 min Scan# 3770
Delta R.T. 0.005 min
Lab File: BG055064.D
Acq: 4 Oct 2022 15:29

Tgt Ion:264 Resp: 246456
Ion Ratio Lower Upper
264 100
260 23.1 19.7 29.5
265 21.0 17.8 26.6

