
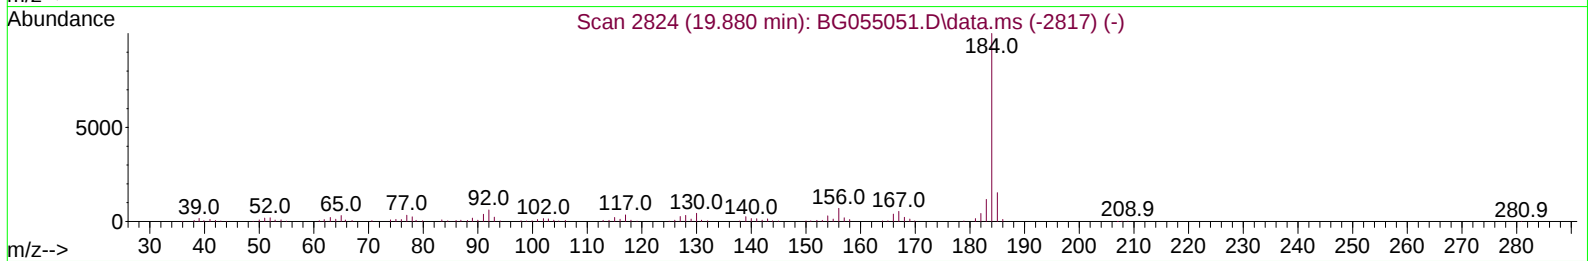
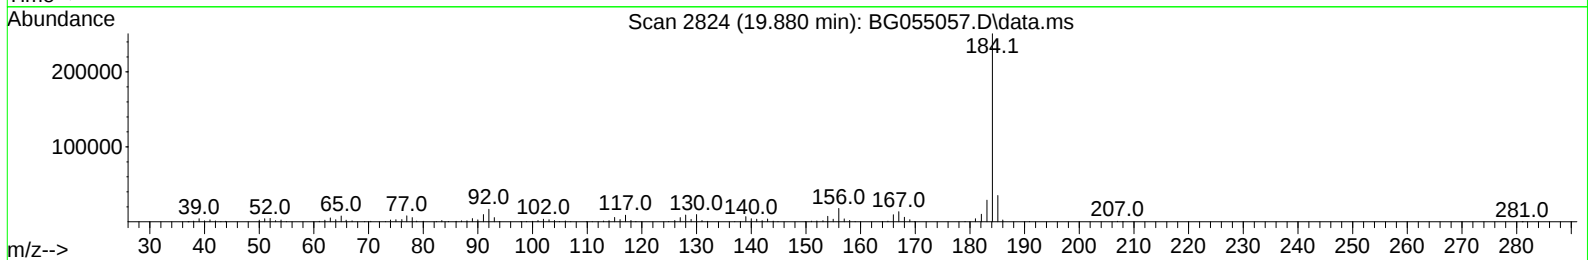


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100422\
 Data File : BG055057.D
 Acq On : 4 Oct 2022 10:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 02:07:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 04 07:12:22 2022
 Response via : Initial Calibration

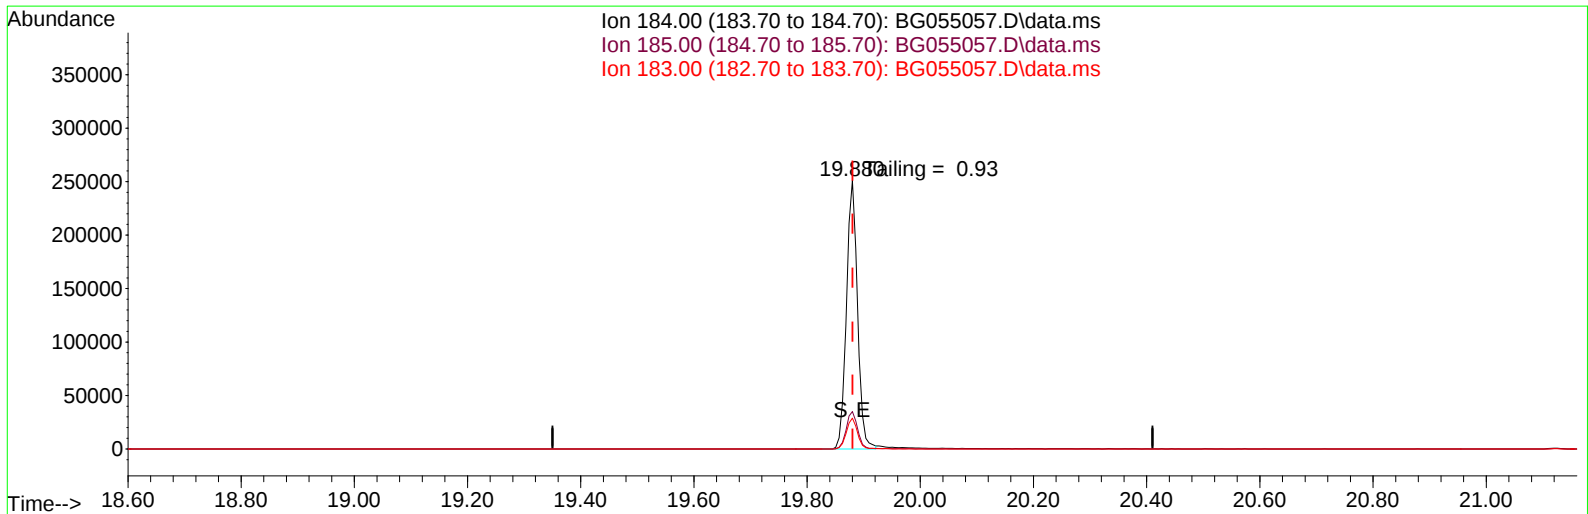




TIC: BG055057.D\data.ms

(77) Benzidine**19.880min (+ 0.000) 104211.85 ng****response 346487**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	13.94
183.00	11.70	11.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100422\
Data File : BG055057.D
Acq On : 4 Oct 2022 10:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 02:07:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 07:12:22 2022
Response via : Initial Calibration

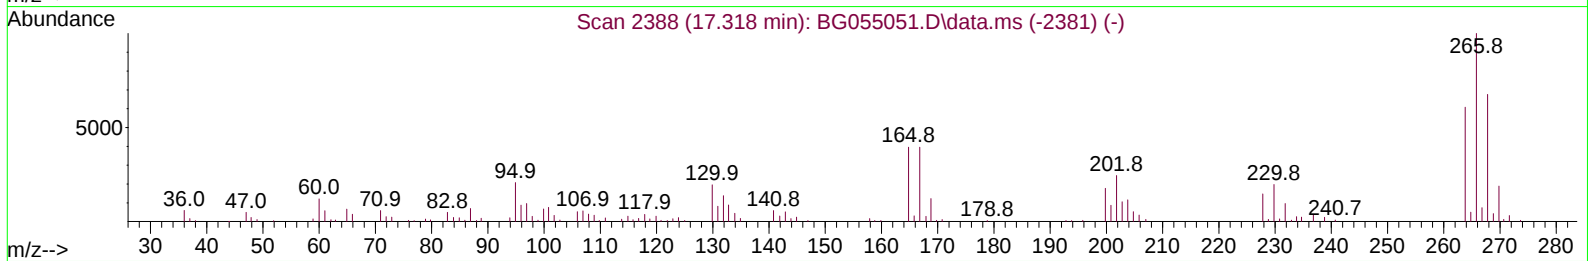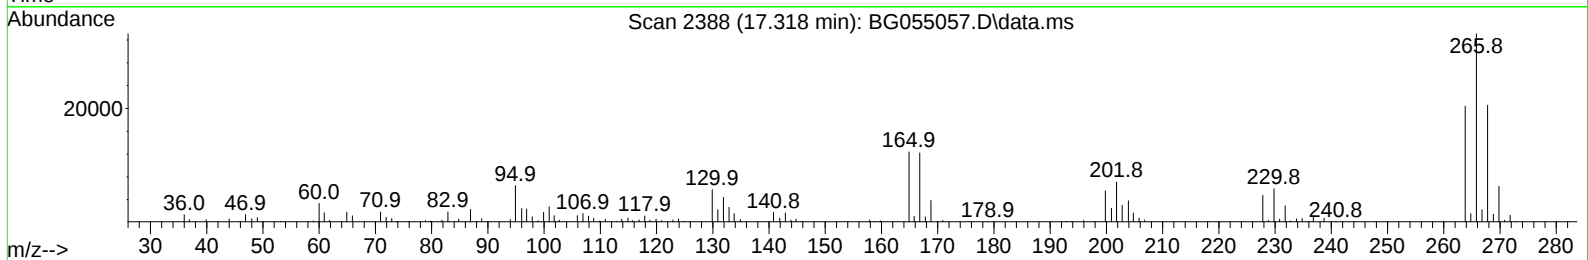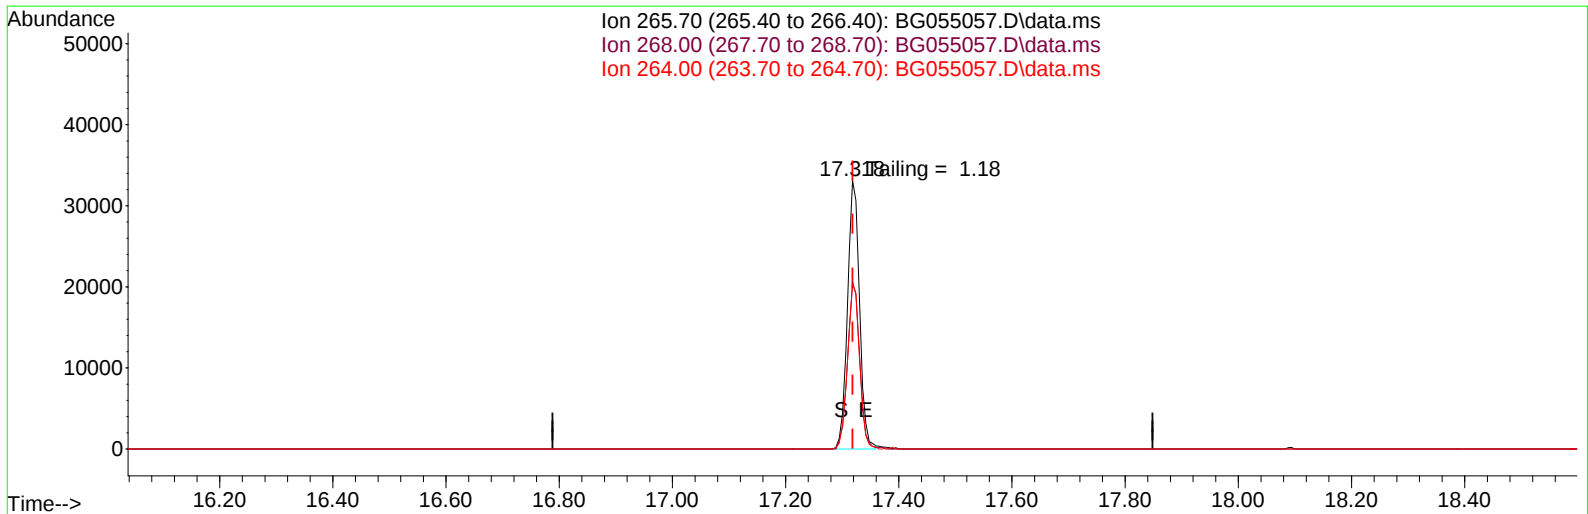

TIC: BG055057.D\data.ms

(70) Pentachlorophenol (C)

17.318min (+ 0.000) 39768.52 ng

response 49164

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	62.09
264.00	60.80	61.58
0.00	0.00	0.00