

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100422\
 Data File : BG055059.D
 Acq On : 4 Oct 2022 11:56
 Operator : CG/JU
 Sample : PB148039BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB148039BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	11	15	22	rVB	21161	27392	1.07%	0.303%
2	5.855	429	437	448	rBV	452080	712665	27.90%	7.890%
3	7.465	703	711	720	rBV	468607	782341	30.62%	8.662%
4	8.340	852	860	867	rVB	91939	153198	6.00%	1.696%
5	9.509	1051	1059	1068	rBV	248946	445784	17.45%	4.936%
6	11.172	1333	1342	1350	rBV	127512	228953	8.96%	2.535%
7	13.581	1745	1752	1760	rVB	780235	1188624	46.53%	13.160%
8	14.944	1976	1984	1991	rVB	224041	354224	13.87%	3.922%
9	16.419	2228	2235	2253	rVB	535214	797774	31.23%	8.833%
10	17.682	2443	2450	2457	rVB	340909	510424	19.98%	5.651%
11	20.255	2882	2888	2898	rBV	1921832	2554799	100.00%	28.286%
12	21.977	3173	3181	3190	rBV	365948	629956	24.66%	6.975%
13	25.432	3758	3769	3789	rVB2	214831	645979	25.28%	7.152%




Sum of corrected areas: 9032113

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100422\
Data File : BG055059.D
Acq On : 4 Oct 2022 11:56
Operator : CG/JU
Sample : PB148039BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB148039BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

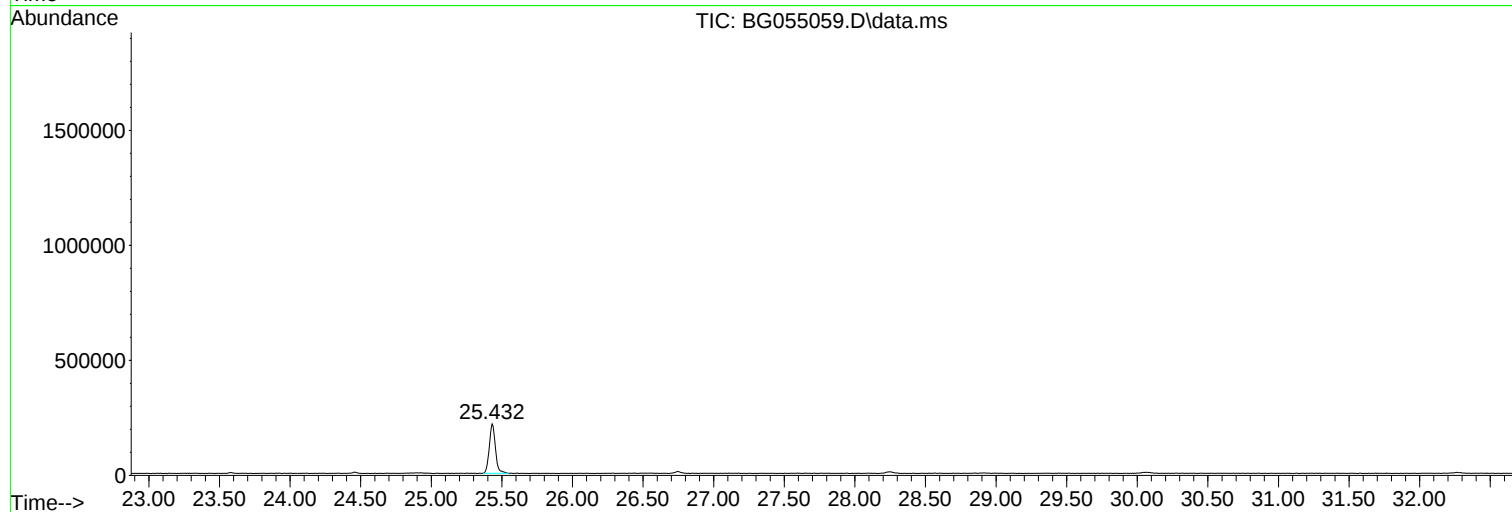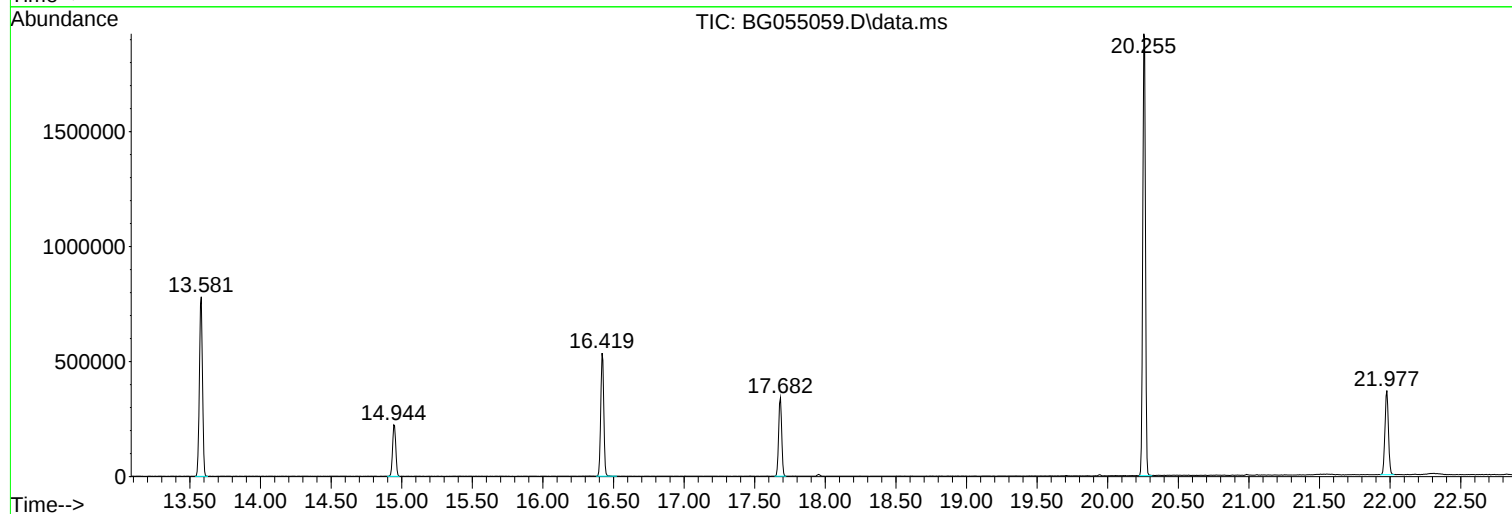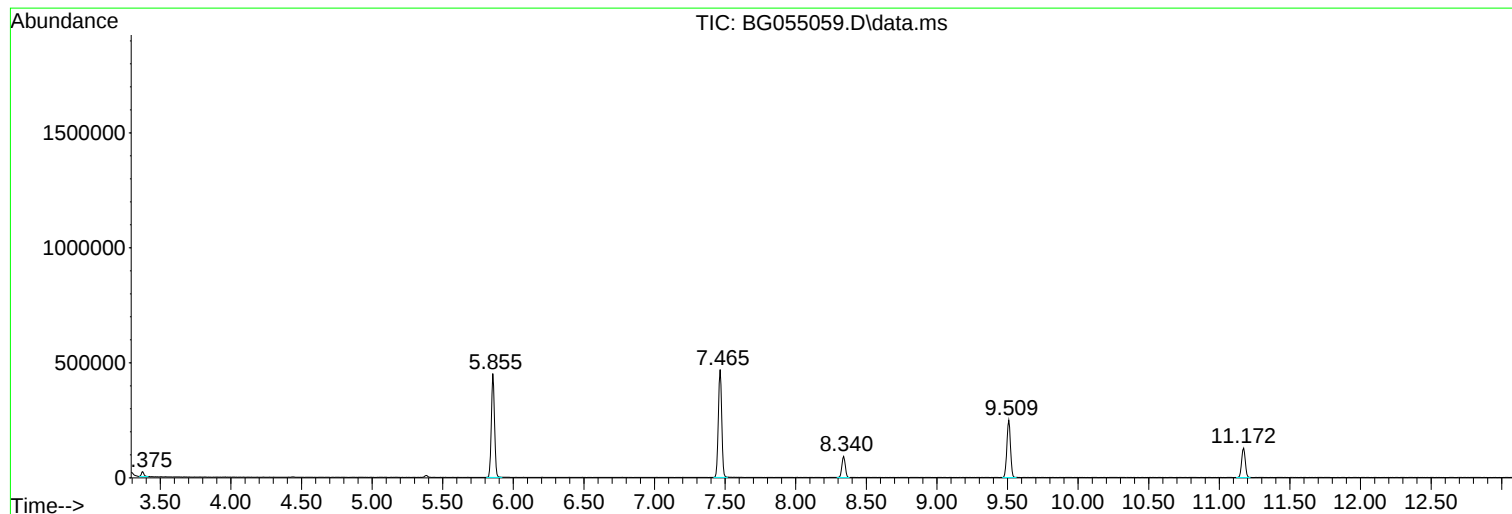

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100422\
Data File : BG055059.D
Acq On : 4 Oct 2022 11:56
Operator : CG/JU
Sample : PB148039BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB148039BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.375	3.58 ng	27392	1,4-Dichlorobenzene-d4	8.340

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
2			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12
3			N-Ethylformamide	73	C3H7NO	000627-45-2	9
4			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	9
5			2-Acetamido-N-methylacetamide	130	C5H10N2O2	007606-79-3	9

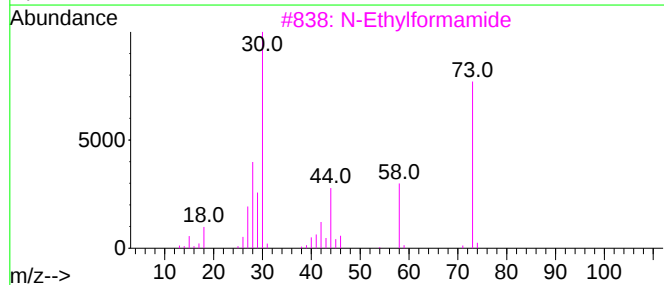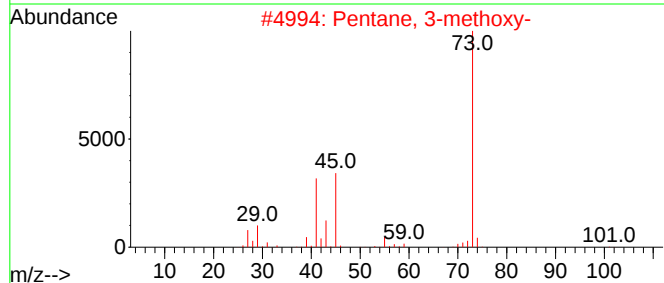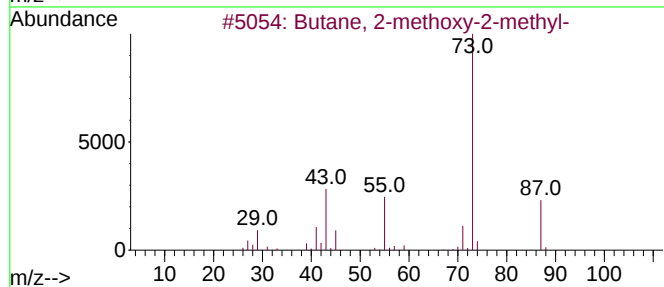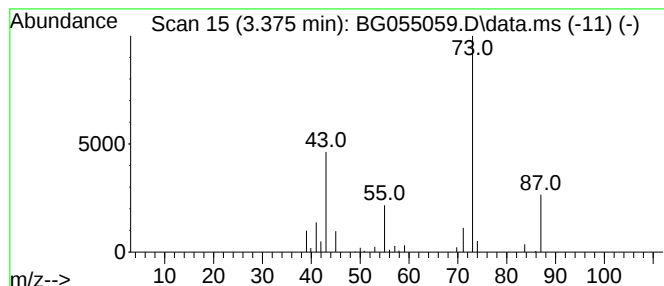

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100422\
Data File : BG055059.D
Acq On : 4 Oct 2022 11:56
Operator : CG/JU
Sample : PB148039BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB148039BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.375	3.6	ng	27392	1	8.340	153198	20.0