

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100423\
 Data File : BG059275.D
 Acq On : 4 Oct 2023 10:53
 Operator : MA/JU
 Sample : PB155829BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK829

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059275.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.528	21	24	28	rVB4	18476	22767	1.40%	0.133%
2	3.963	92	98	109	rBV	240190	422491	25.93%	2.462%
3	4.345	162	163	165	rBV2	3673	2511	0.15%	0.015%
4	4.445	178	180	183	rVB3	2533	2703	0.17%	0.016%
5	4.662	214	217	219	rBV3	3859	3530	0.22%	0.021%
6	4.739	228	230	232	rBV2	3045	2920	0.18%	0.017%
7	5.520	361	363	365	rVB3	2952	2412	0.15%	0.014%
8	5.755	402	403	405	rBV2	2925	2577	0.16%	0.015%
9	5.996	442	444	447	rBV3	2590	2948	0.18%	0.017%
10	6.419	511	516	517	rBV	2490	2767	0.17%	0.016%
11	7.118	630	635	636	rBV3	2545	2567	0.16%	0.015%
12	7.271	656	661	663	rBV3	2314	4094	0.25%	0.024%
13	7.353	668	675	687	rBV	279473	471274	28.92%	2.747%
14	7.553	702	709	719	rVB	208199	359959	22.09%	2.098%
15	7.747	735	742	748	rBV2	240876	422285	25.92%	2.461%
16	8.047	790	793	795	rBV	2814	3240	0.20%	0.019%
17	8.182	811	816	817	rVB2	2767	4207	0.26%	0.025%
18	8.229	817	824	835	rBV	186581	332621	20.41%	1.939%
19	8.658	894	897	899	rBV2	2208	2399	0.15%	0.014%
20	8.705	904	905	910	rBV2	2462	2586	0.16%	0.015%
21	8.922	935	942	950	rBV	314479	556243	34.14%	3.242%
22	9.245	993	997	999	rBV2	2250	3429	0.21%	0.020%
23	9.327	1008	1011	1014	rVB	1802	2582	0.16%	0.015%
24	9.427	1017	1028	1036	rBV	249544	444576	27.29%	2.591%
25	9.727	1076	1079	1082	rVB	2353	2920	0.18%	0.017%
26	10.144	1143	1150	1159	rBV	202800	363086	22.28%	2.116%
27	10.297	1175	1176	1179	rBV	2979	2429	0.15%	0.014%
28	10.673	1233	1240	1248	rBV	310649	551927	33.87%	3.217%
29	10.808	1261	1263	1268	rVB2	2866	3704	0.23%	0.022%
30	10.849	1268	1270	1273	rBV	2531	2638	0.16%	0.015%
31	11.072	1298	1308	1317	rBV	286445	516981	31.73%	3.013%
32	11.219	1325	1333	1346	rBV	322453	609058	37.38%	3.550%
33	11.877	1442	1445	1447	rBV2	3380	4602	0.28%	0.027%
34	12.177	1493	1496	1500	rVB2	1697	2647	0.16%	0.015%
35	12.224	1500	1504	1508	rBV2	2551	3960	0.24%	0.023%
36	12.471	1543	1546	1548	rBV2	2062	2385	0.15%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100423\
 Data File : BG059275.D
 Acq On : 4 Oct 2023 10:53
 Operator : MA/JU
 Sample : PB155829BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK829

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

37	12.624	1570	1572	1575	rBV2	3500	4223	0.26%	0.025%
38	12.700	1584	1585	1588	rBV	4461	2619	0.16%	0.015%
39	12.747	1588	1593	1595	rBV	2445	3498	0.21%	0.020%
40	12.841	1606	1609	1613	rBV	2505	2998	0.18%	0.017%

41	13.252	1675	1679	1684	rBV	3248	3369	0.21%	0.020%
42	13.581	1731	1735	1737	rBV	2779	2593	0.16%	0.015%
43	13.652	1744	1747	1750	rBV	3087	3546	0.22%	0.021%
44	13.699	1750	1755	1760	rVB3	8320	11212	0.69%	0.065%
45	14.204	1839	1841	1844	rBV	1891	2641	0.16%	0.015%

46	14.257	1844	1850	1857	rVV	558286	813251	49.91%	4.740%
47	14.504	1889	1892	1894	rBV	1777	2485	0.15%	0.014%
48	14.568	1896	1903	1910	rVV2	632550	1027860	63.08%	5.991%
49	14.862	1947	1953	1963	rVB	448933	712638	43.74%	4.153%
50	15.050	1979	1985	1998	rBV	216667	385307	23.65%	2.246%

51	15.256	2019	2020	2024	rVB3	2958	2636	0.16%	0.015%
52	15.644	2084	2086	2089	rVB2	2999	2898	0.18%	0.017%
53	15.849	2115	2121	2128	rVB	817320	1240229	76.12%	7.228%
54	15.961	2134	2140	2147	rBV	210234	321679	19.74%	1.875%
55	16.090	2160	2162	2165	rVV3	4945	4635	0.28%	0.027%

56	16.137	2168	2170	2172	rVB	2570	2565	0.16%	0.015%
57	16.613	2248	2251	2254	rBV	2380	3472	0.21%	0.020%
58	17.195	2348	2350	2354	rVB	2652	2567	0.16%	0.015%
59	17.406	2385	2386	2389	rVB3	4089	3537	0.22%	0.021%
60	17.612	2413	2421	2428	rBV	564138	826614	50.73%	4.818%

61	17.712	2432	2438	2446	rVV2	924755	1350099	82.86%	7.869%
62	17.900	2468	2470	2472	rBV	2340	2946	0.18%	0.017%
63	18.141	2510	2511	2515	rVB2	2208	2393	0.15%	0.014%
64	18.229	2525	2526	2531	rVB2	2230	2830	0.17%	0.016%
65	18.329	2542	2543	2546	rVV	4191	2834	0.17%	0.017%

66	18.370	2546	2550	2553	rVV2	3068	3718	0.23%	0.022%
67	18.411	2555	2557	2560	rVB2	3270	2552	0.16%	0.015%
68	18.440	2560	2562	2564	rBV	4268	3347	0.21%	0.020%
69	18.758	2614	2616	2619	rBV2	2494	2804	0.17%	0.016%
70	18.787	2619	2621	2623	rBV2	3193	3062	0.19%	0.018%

71	18.846	2629	2631	2635	rVB2	4065	4553	0.28%	0.027%
72	18.887	2635	2638	2639	rBV2	3597	2386	0.15%	0.014%
73	18.910	2639	2642	2645	rVB3	3018	3865	0.24%	0.023%
74	19.098	2672	2674	2679	rBV4	1935	3101	0.19%	0.018%
75	19.139	2679	2681	2683	rVB3	3540	2772	0.17%	0.016%

76	19.163	2683	2685	2686	rBV2	4721	3523	0.22%	0.021%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100423\
 Data File : BG059275.D
 Acq On : 4 Oct 2023 10:53
 Operator : MA/JU
 Sample : PB155829BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK829

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

77	19.269	2702	2703	2705	rVB2	4806	2380	0.15%	0.014%
78	19.380	2719	2722	2723	rBV3	4401	4837	0.30%	0.028%
79	19.433	2729	2731	2734	rVB3	5326	4805	0.29%	0.028%
80	19.468	2734	2737	2740	rBV4	4130	5722	0.35%	0.033%
81	19.551	2748	2751	2755	rBV5	12373	18838	1.16%	0.110%
82	19.615	2755	2762	2769	rVB3	11117	24295	1.49%	0.142%
83	19.915	2811	2813	2816	rVB3	3013	2503	0.15%	0.015%
84	19.986	2819	2825	2833	rVV	1103492	1534498	94.18%	8.943%
85	20.074	2839	2840	2842	rBV2	4041	3231	0.20%	0.019%
86	20.197	2859	2861	2863	rBV3	3455	2899	0.18%	0.017%
87	20.297	2876	2878	2879	rVB2	5452	3497	0.21%	0.020%
88	20.790	2959	2962	2964	rBV3	5340	7570	0.46%	0.044%
89	21.736	3122	3123	3125	rBV2	6441	3118	0.19%	0.018%
90	21.913	3146	3153	3160	rBV3	505877	881223	54.08%	5.136%
91	22.483	3248	3250	3251	rBV2	6161	3030	0.19%	0.018%
92	23.393	3401	3405	3410	rVB7	16145	24174	1.48%	0.141%
93	24.028	3511	3513	3515	rBV3	6163	4845	0.30%	0.028%
94	24.662	3619	3621	3624	rBV3	7545	7954	0.49%	0.046%
95	25.150	3693	3704	3716	rBV2	556736	1629371	100.00%	9.496%
96	25.391	3735	3745	3758	rVB	330440	989474	60.73%	5.767%
97	26.478	3923	3930	3932	rBV6	30363	56431	3.46%	0.329%
98	27.682	4133	4135	4136	rBV	6209	3255	0.20%	0.019%
99	29.386	4423	4425	4427	rBV3	8678	4599	0.28%	0.027%
100	29.474	4438	4440	4441	rVB2	7445	3656	0.22%	0.021%




Sum of corrected areas: 17158087

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100423\
Data File : BG059275.D
Acq On : 4 Oct 2023 10:53
Operator : MA/JU
Sample : PB155829BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK829

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

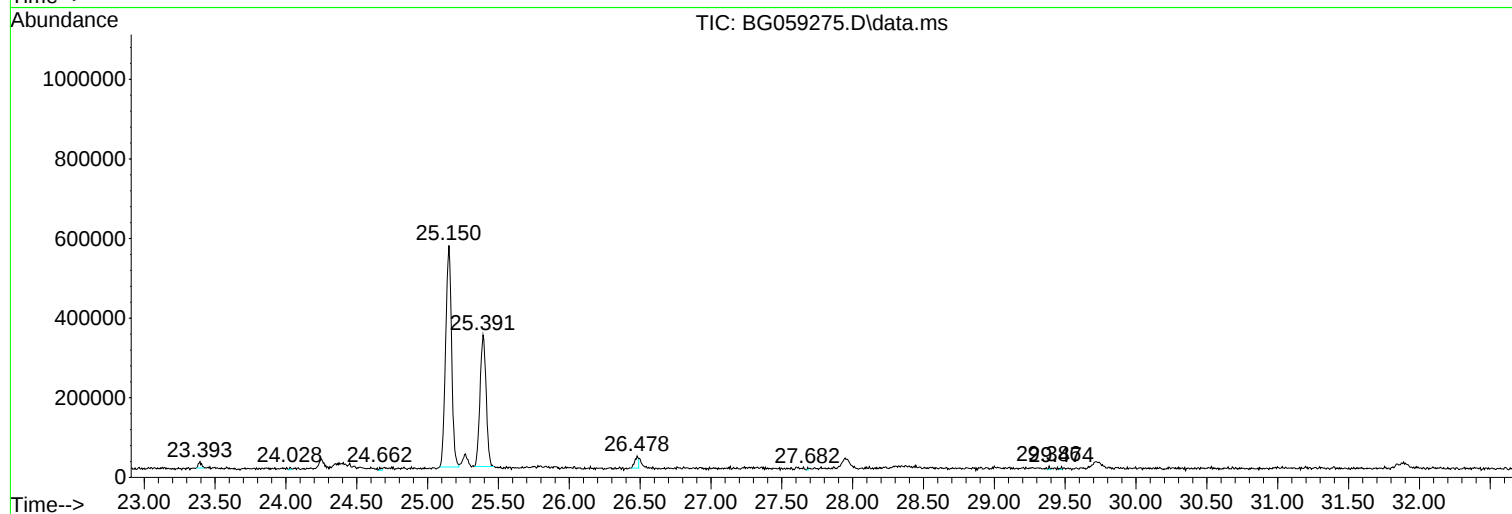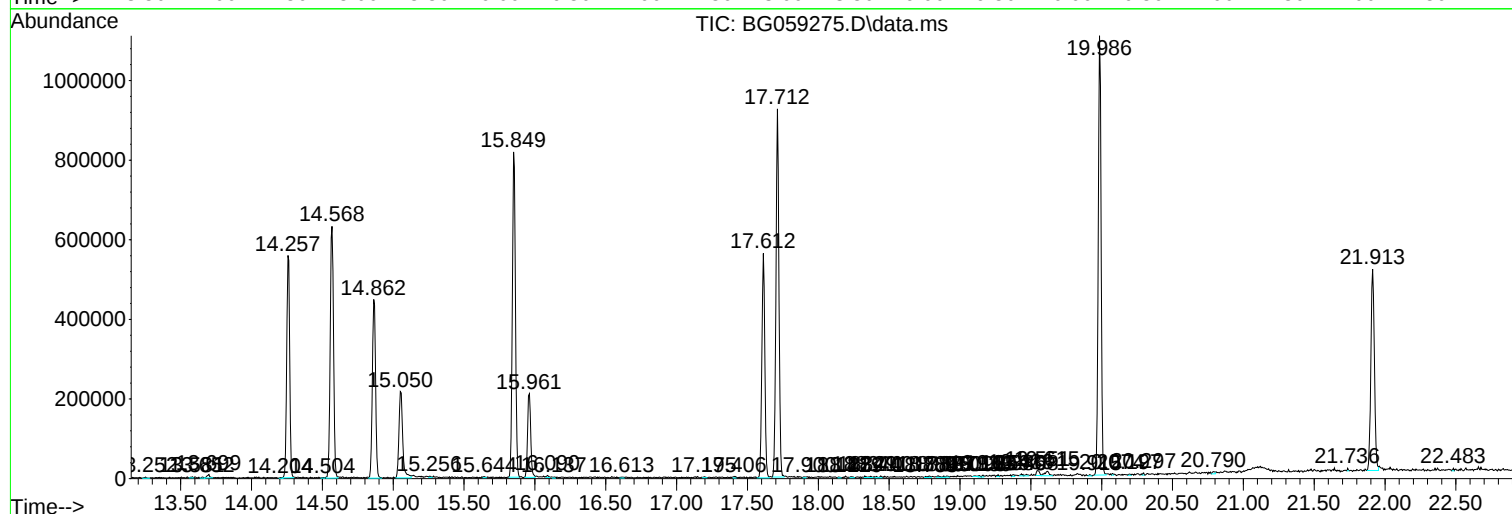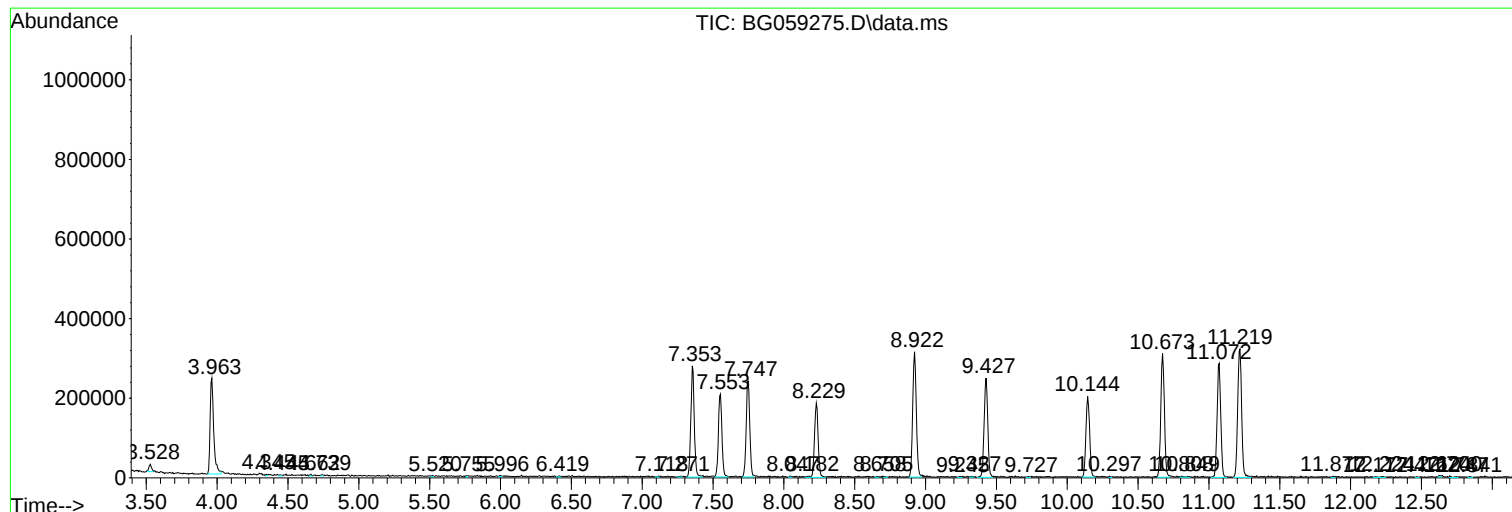

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100423\
Data File : BG059275.D
Acq On : 4 Oct 2023 10:53
Operator : MA/JU
Sample : PB155829BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK829

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100423\
Data File : BG059275.D
Acq On : 4 Oct 2023 10:53
Operator : MA/JU
Sample : PB155829BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK829

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc