

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100423\
 Data File : BG059276.D
 Acq On : 4 Oct 2023 11:34
 Operator : MA/JU
 Sample : PB155820BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK820

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059276.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.529	20	24	30	rVB4	17440	27566	1.62%	0.165%
2	3.964	93	98	106	rBV	267963	440387	25.80%	2.635%
3	4.240	143	145	147	rBV2	2908	2501	0.15%	0.015%
4	4.293	152	154	155	rBV2	3596	2469	0.14%	0.015%
5	4.516	191	192	198	rBV3	2157	3061	0.18%	0.018%
6	4.610	205	208	209	rBV2	3520	3063	0.18%	0.018%
7	4.633	209	212	213	rBV2	3071	3212	0.19%	0.019%
8	4.704	222	224	227	rBV2	2620	2781	0.16%	0.017%
9	4.786	237	238	242	rBV3	2964	4211	0.25%	0.025%
10	5.955	434	437	440	rBV2	1847	2772	0.16%	0.017%
11	6.138	466	468	472	rVB3	2704	3342	0.20%	0.020%
12	6.625	548	551	556	rBV4	2385	3413	0.20%	0.020%
13	6.707	563	565	567	rBV	2170	2629	0.15%	0.016%
14	6.731	567	569	573	rVB2	2291	2952	0.17%	0.018%
15	7.060	623	625	629	rBV2	3863	4278	0.25%	0.026%
16	7.354	668	675	687	rBV	285762	488302	28.61%	2.922%
17	7.548	703	708	717	rVB	222564	370457	21.71%	2.216%
18	7.747	735	742	750	rBV2	257819	437633	25.64%	2.618%
19	7.836	756	757	760	rBV	2775	2985	0.17%	0.018%
20	8.118	801	805	808	rBV2	2269	2641	0.15%	0.016%
21	8.229	816	824	831	rBV2	152686	255537	14.97%	1.529%
22	8.682	899	901	902	rBV2	3373	2446	0.14%	0.015%
23	8.746	908	912	914	rVB2	2486	3322	0.19%	0.020%
24	8.923	934	942	957	rBV	334159	582884	34.15%	3.487%
25	9.128	975	977	981	rVB2	1972	2738	0.16%	0.016%
26	9.163	981	983	985	rBV	3440	3066	0.18%	0.018%
27	9.257	996	999	1000	rBV	2615	2344	0.14%	0.014%
28	9.428	1020	1028	1035	rBV	260075	461123	27.02%	2.759%
29	9.586	1052	1055	1057	rBV	3195	2553	0.15%	0.015%
30	9.968	1117	1120	1124	rBV	1933	2744	0.16%	0.016%
31	10.145	1139	1150	1160	rBV2	211298	388140	22.74%	2.322%
32	10.209	1160	1161	1164	rVB2	2766	2371	0.14%	0.014%
33	10.362	1186	1187	1190	rVB2	2839	2637	0.15%	0.016%
34	10.615	1229	1230	1233	rBV2	2152	2437	0.14%	0.015%
35	10.673	1233	1240	1248	rVV	330798	573257	33.59%	3.430%
36	11.073	1301	1308	1316	rVB	216502	398101	23.33%	2.382%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100423\
 Data File : BG059276.D
 Acq On : 4 Oct 2023 11:34
 Operator : MA/JU
 Sample : PB155820BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK820

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

37	11.220	1324	1333	1344	rBV	335848	621039	36.39%	3.716%
38	11.702	1414	1415	1420	rVB	2911	3180	0.19%	0.019%
39	11.878	1441	1445	1448	rBV	1735	2366	0.14%	0.014%
40	11.990	1463	1464	1467	rVB	2933	2600	0.15%	0.016%

41	12.166	1491	1494	1496	rBV	2444	2542	0.15%	0.015%
42	12.418	1533	1537	1540	rVB	2512	3443	0.20%	0.021%
43	12.583	1563	1565	1569	rBV	2019	2975	0.17%	0.018%
44	12.624	1569	1572	1573	rBV	4417	4500	0.26%	0.027%
45	12.636	1573	1574	1577	rVB2	4549	3051	0.18%	0.018%

46	13.693	1750	1754	1758	rVB2	5516	7785	0.46%	0.047%
47	14.257	1844	1850	1857	rBV	614923	860516	50.42%	5.149%
48	14.369	1864	1869	1875	rVB	2055	4980	0.29%	0.030%
49	14.569	1896	1903	1912	rVB	688786	1078989	63.22%	6.456%
50	14.863	1947	1953	1962	rVB	363014	552260	32.36%	3.304%

51	14.968	1968	1971	1975	rVB	2529	3070	0.18%	0.018%
52	15.051	1978	1985	1994	rBV	242113	407276	23.86%	2.437%
53	15.550	2066	2070	2071	rBV	1996	2831	0.17%	0.017%
54	15.850	2114	2121	2129	rBV	860152	1313449	76.96%	7.858%
55	15.961	2133	2140	2149	rBV	229597	349336	20.47%	2.090%

56	16.091	2159	2162	2164	rBV4	5015	5700	0.33%	0.034%
57	16.173	2175	2176	2182	rVB	1969	2595	0.15%	0.016%
58	16.261	2187	2191	2194	rBV2	3657	3421	0.20%	0.020%
59	16.396	2211	2214	2216	rBV2	2524	2737	0.16%	0.016%
60	16.478	2225	2228	2231	rVB	2314	2596	0.15%	0.016%

61	16.608	2247	2250	2254	rBV	1740	2374	0.14%	0.014%
62	17.401	2382	2385	2388	rBV3	2524	3755	0.22%	0.022%
63	17.612	2413	2421	2430	rBV	437844	659734	38.66%	3.947%
64	17.712	2431	2438	2446	rVV	949944	1422961	83.37%	8.514%
65	17.842	2459	2460	2462	rBV2	4509	2787	0.16%	0.017%

66	18.006	2483	2488	2492	rBV	2486	4383	0.26%	0.026%
67	18.088	2500	2502	2507	rVB2	1756	2391	0.14%	0.014%
68	18.171	2514	2516	2519	rVB2	3812	3205	0.19%	0.019%
69	18.241	2526	2528	2531	rVB	2877	2400	0.14%	0.014%
70	18.370	2548	2550	2552	rVB	3086	2605	0.15%	0.016%

71	18.458	2563	2565	2569	rVB2	3034	3653	0.21%	0.022%
72	18.870	2633	2635	2637	rBV2	2286	2521	0.15%	0.015%
73	19.022	2660	2661	2664	rVB2	3063	2416	0.14%	0.014%
74	19.134	2679	2680	2682	rBV	3709	3175	0.19%	0.019%
75	19.263	2700	2702	2705	rBV3	2692	3450	0.20%	0.021%

76	19.381	2719	2722	2724	rBV4	2283	3030	0.18%	0.018%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100423\
 Data File : BG059276.D
 Acq On : 4 Oct 2023 11:34
 Operator : MA/JU
 Sample : PB155820BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK820

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

77	19.504	2741	2743	2746	rVB3	3941	2444	0.14%	0.015%
78	19.545	2746	2750	2756	rVV3	14237	21225	1.24%	0.127%
79	19.592	2756	2758	2759	rVV2	5705	5134	0.30%	0.031%
80	19.610	2759	2761	2766	rVV3	12192	18429	1.08%	0.110%
81	19.669	2770	2771	2774	rBV	2465	2681	0.16%	0.016%
82	19.763	2786	2787	2790	rVB2	3940	2776	0.16%	0.017%
83	19.986	2818	2825	2831	rBV	1204585	1627485	95.36%	9.737%
84	20.509	2912	2914	2916	rBV3	3898	3717	0.22%	0.022%
85	20.697	2944	2946	2948	rBV3	4699	5186	0.30%	0.031%
86	21.473	3076	3078	3083	rBV6	5079	6153	0.36%	0.037%
87	21.907	3146	3152	3159	rBV2	372303	663990	38.90%	3.973%
88	22.013	3168	3170	3173	rBV4	6743	3693	0.22%	0.022%
89	24.146	3531	3533	3536	rVB4	7047	4336	0.25%	0.026%
90	25.151	3692	3704	3714	rBV2	585537	1706708	100.00%	10.211%
91	25.386	3735	3744	3757	rVB3	253126	761959	44.64%	4.559%
92	30.303	4579	4581	4584	rBV4	7709	9044	0.53%	0.054%
93	32.231	4907	4909	4911	rBV3	6769	4369	0.26%	0.026%


Sum of corrected areas: 16713761

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100423\
Data File : BG059276.D
Acq On : 4 Oct 2023 11:34
Operator : MA/JU
Sample : PB155820BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK820

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

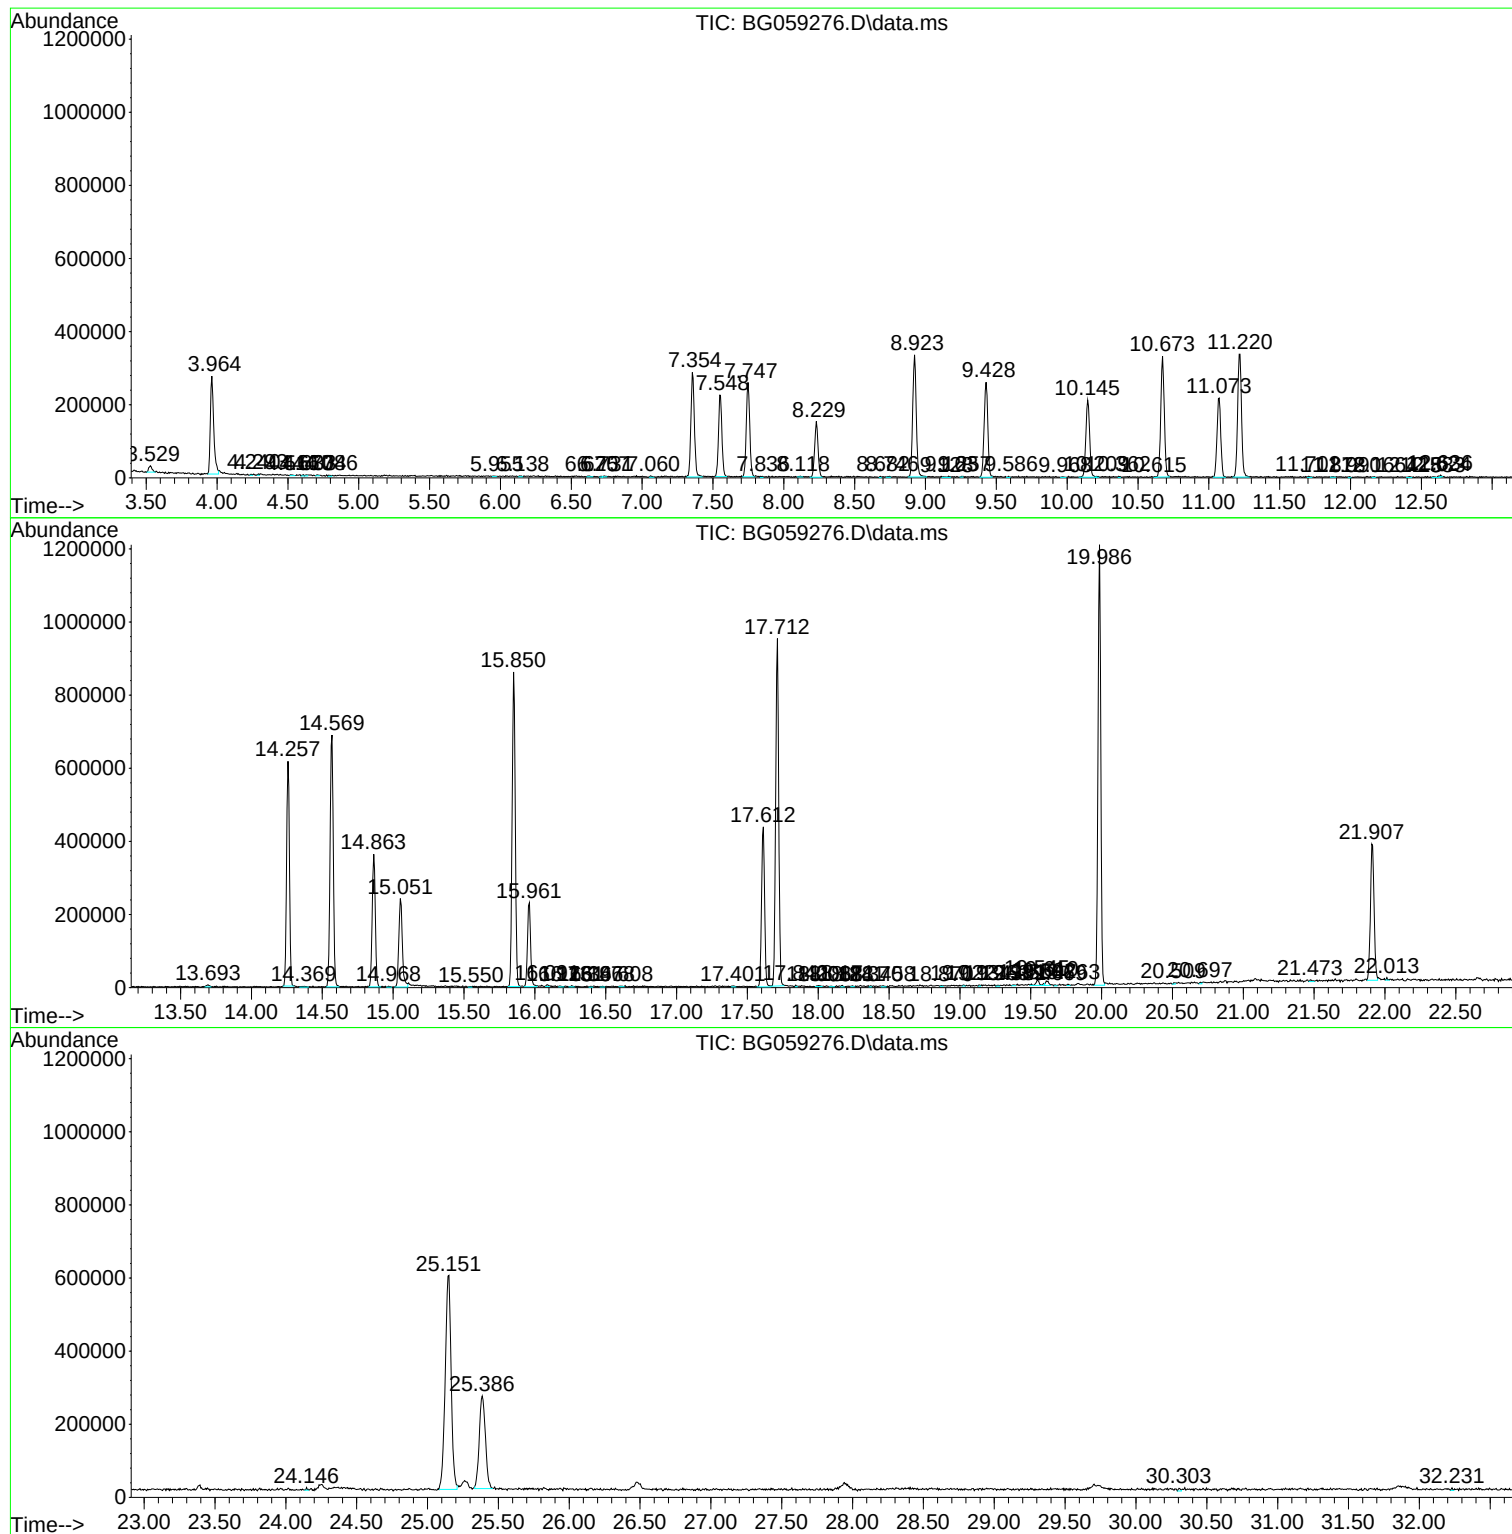

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100423\
Data File : BG059276.D
Acq On : 4 Oct 2023 11:34
Operator : MA/JU
Sample : PB155820BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK820

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100423\
Data File : BG059276.D
Acq On : 4 Oct 2023 11:34
Operator : MA/JU
Sample : PB155820BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK820

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc