


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100423\
 Data File : BG059273.D
 Acq On : 4 Oct 2023 9:00
 Operator : MA/JU
 Sample : DFTPP540
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP540

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION
 Last Update : Thu Sep 28 04:33:25 2023

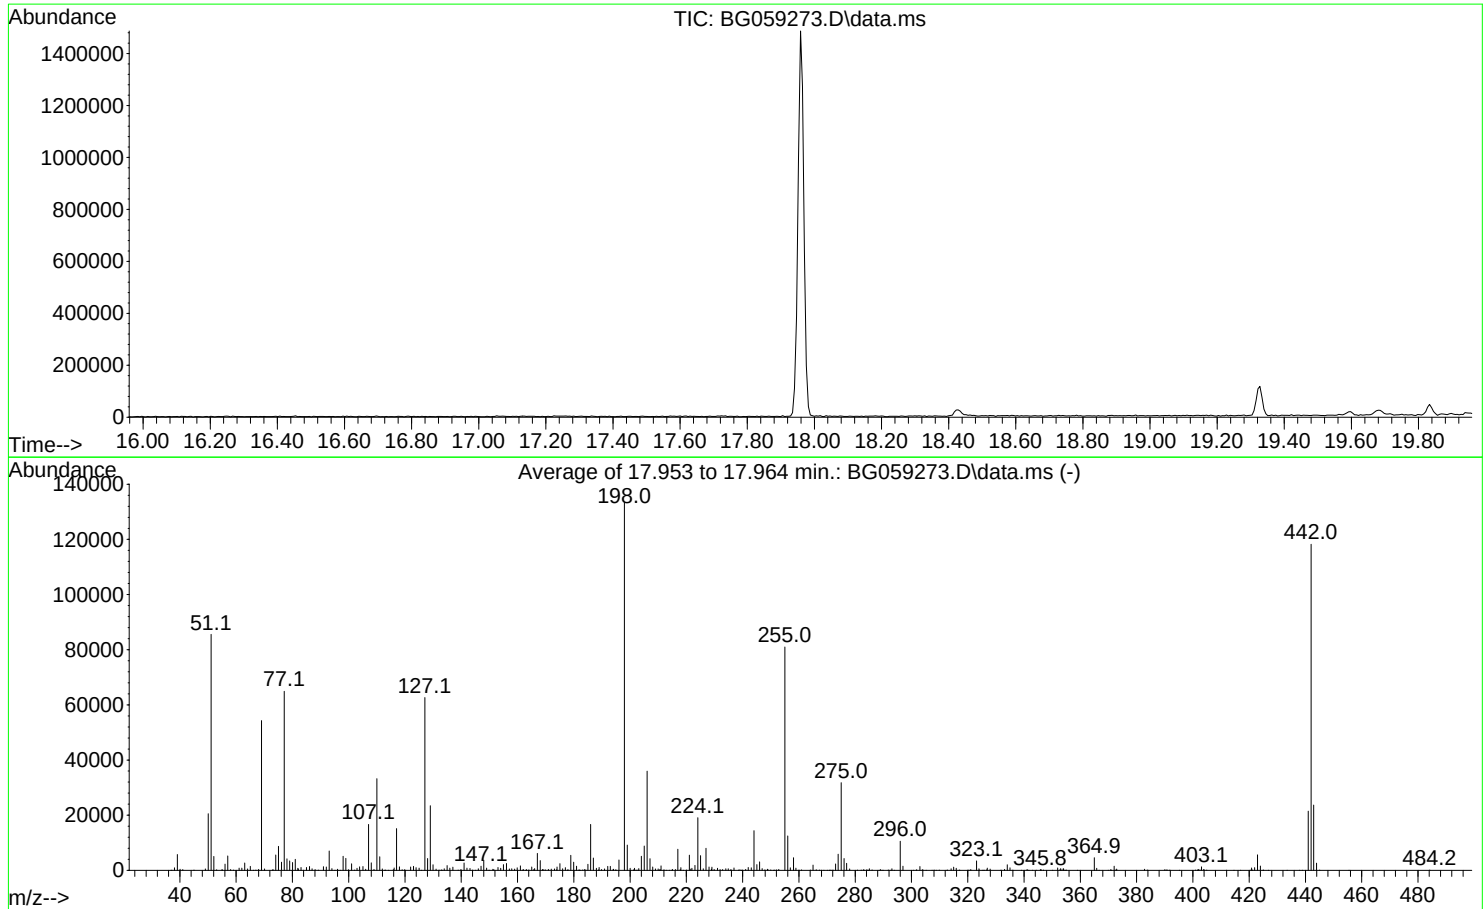

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.1	85552	PASS
68	69	0.00	2	0.7	378	PASS
69	198	0.00	100	40.7	54317	PASS
70	69	0.00	2	1.0	531	PASS
127	198	10	80	47.0	62653	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	133371	PASS
199	198	5	9	6.9	9162	PASS
275	198	10	60	23.8	31781	PASS
365	198	1	100	3.5	4604	PASS
441	198	0.01	100	16.1	21465	PASS
442	198	50	100	88.7	118245	PASS
443	442	15	24	20.0	23672	PASS

m/z	Abundance
44.00	306.0
56.10	175.0
70.60	266.0
71.10	156.0
72.90	206.0
103.80	259.0
181.10	209.0
192.90	180.0
207.20	395.0
252.50	179.0
275.40	189.0
339.40	168.0
350.60	155.0
439.80	219.0
466.50	169.0
501.70	227.0
542.70	167.0

Instrument :
BNA_G
ClientSampleId :
DFTPP540

m/z	Abundance
38.10	945.0
39.10	5000.0
40.00	292.0
41.00	344.0
44.10	402.0
50.10	20048.0
51.10	78984.0
52.10	5263.0
53.10	225.0
54.90	336.0
56.00	2501.0
57.00	5353.0
58.00	408.0
61.00	549.0
62.00	591.0
63.10	2619.0
64.10	493.0
65.10	1231.0
69.00	47184.0
70.10	765.0
72.90	580.0
74.10	4148.0
75.00	7538.0
76.10	2554.0
77.10	55272.0
78.00	3845.0
79.00	2836.0
80.00	2384.0
81.00	3254.0
81.90	870.0
83.00	648.0
85.00	814.0
86.10	1161.0
87.00	718.0
88.00	362.0
91.10	1268.0
92.00	1533.0
93.10	5824.0
94.00	635.0
96.00	834.0
97.00	186.0
98.00	4101.0
99.00	3766.0
101.10	1836.0
102.90	1025.0
104.00	1550.0
105.10	1187.0
106.10	404.0
107.00	15130.0
108.00	2698.0
110.00	32880.0
111.00	4816.0
112.10	344.0
113.10	331.0
114.20	193.0
116.10	1342.0
117.00	13833.0
118.10	1159.0
119.00	257.0
119.90	368.0
122.00	1267.0
123.10	1170.0
123.90	938.0
125.10	968.0
127.10	54648.0
128.00	4085.0
129.00	18448.0
129.90	1837.0
131.00	357.0
133.00	320.0
134.00	570.0
135.00	1268.0
136.00	750.0
137.10	974.0
140.10	218.0
141.00	3305.0
142.00	901.0
143.10	735.0
146.10	692.0
147.10	1452.0
148.00	2449.0
149.10	623.0
149.80	202.0
151.20	343.0
153.00	1116.0
154.10	628.0
155.00	1633.0
156.00	2268.0
157.20	400.0
157.90	663.0
158.90	502.0
159.90	702.0

Instrument :
BNA_G
ClientSampleId :
DFTPP540

161.00	1587.0
162.10	450.0
162.90	263.0
165.10	781.0
165.80	979.0
167.10	5287.0
168.10	3458.0
168.80	440.0
169.90	390.0
171.00	246.0
172.00	350.0
173.00	166.0
173.90	760.0
175.10	1927.0
176.10	298.0
177.00	1027.0
177.80	291.0
179.00	4285.0
179.90	2537.0
180.90	1501.0
181.80	331.0
182.30	194.0
183.90	378.0
184.30	385.0
185.00	2026.0
186.00	13707.0
187.00	3699.0
188.10	671.0
188.80	569.0
189.00	552.0
190.00	252.0
190.90	351.0
192.00	1054.0
193.00	1123.0
193.90	482.0
194.80	365.0
196.00	2246.0
198.00	107056.0
199.00	7607.0
200.00	411.0
201.50	666.0
202.80	405.0
204.00	4168.0
205.00	6679.0
206.00	26648.0
207.00	3227.0
208.10	722.0
209.00	378.0
209.90	555.0
210.40	619.0
211.00	1340.0
211.80	261.0
214.90	245.0
217.00	6554.0
218.10	1319.0
218.90	196.0
221.10	4623.0
221.90	712.0
223.00	1508.0
224.10	13835.0
225.10	2923.0
227.00	6594.0
228.00	973.0
228.90	1328.0
229.80	370.0
231.00	334.0
232.00	345.0
232.90	270.0
234.00	716.0
234.90	426.0
235.70	186.0
237.00	883.0
238.50	329.0
241.10	227.0
242.00	625.0
243.10	944.0
244.10	11799.0
245.00	1423.0
246.00	1930.0
246.90	185.0
248.80	544.0
250.00	169.0
251.40	172.0
255.00	58664.0
256.00	9565.0
257.00	554.0
258.10	2597.0
258.90	708.0
264.20	159.0
265.00	1338.0
266.10	376.0
268.90	170.0
270.80	223.0
273.10	1263.0
273.90	3742.0
275.00	21736.0

Instrument :
BNA_G
ClientSampleId :
DFTPP540

276.00	3400.0
276.90	1438.0
278.10	603.0
280.80	187.0
282.20	157.0
283.20	413.0
284.40	309.0
285.00	372.0
289.00	298.0
291.70	196.0
292.70	273.0
293.90	240.0
296.00	7564.0
296.90	1158.0
303.00	808.0
304.00	187.0
309.90	211.0
312.80	152.0
314.10	331.0
315.00	983.0
315.90	500.0
316.90	196.0
320.40	291.0
321.10	165.0
323.10	2914.0
324.20	435.0
326.70	470.0
327.00	627.0
331.60	157.0
334.00	1643.0
335.10	565.0
335.80	222.0
341.20	206.0
343.10	195.0
345.80	172.0
346.20	159.0
352.10	626.0
353.10	995.0
353.90	572.0
354.50	275.0
365.00	2949.0
365.90	516.0
370.80	226.0
372.00	1185.0
372.90	612.0
382.90	303.0
390.20	202.0
401.60	379.0
402.50	464.0
403.10	687.0
405.00	178.0
417.00	173.0
420.70	481.0
421.20	302.0
422.00	1019.0
423.00	3846.0
424.10	881.0
424.90	210.0
441.00	12691.0
442.00	70128.0
443.00	16017.0
444.00	827.0
455.50	193.0

Instrument :
BNA_G
ClientSampleId :
DFTPP540

m/z	Abundance
36.90	232.0
38.10	905.0
39.10	7292.0
40.10	464.0
41.00	263.0
44.00	163.0
45.00	295.0
49.10	1042.0
50.10	25152.0
51.10	105496.0
52.10	6364.0
53.10	447.0
55.20	328.0
56.00	2244.0
57.10	5329.0
58.10	196.0
61.10	1133.0
62.10	1257.0
63.00	3075.0
64.00	521.0
65.10	1566.0
66.10	173.0
67.00	197.0
69.00	68384.0
70.00	249.0
73.10	897.0
74.10	8196.0
75.10	10436.0
76.10	4038.0
77.10	78328.0
78.10	4671.0
79.10	3692.0
80.10	3887.0
81.00	4894.0
81.90	1488.0
83.10	1624.0
84.00	171.0
85.00	1693.0
86.00	1555.0
86.90	552.0
88.10	239.0
89.20	362.0
91.00	1657.0
92.10	1501.0
93.00	7749.0
94.10	429.0
96.00	391.0
98.00	6406.0
99.00	5230.0
99.90	429.0
101.00	2837.0
102.10	204.0
103.00	545.0
104.00	1748.0
105.00	1692.0
106.10	504.0
107.00	19112.0
108.10	3356.0
109.00	1012.0
110.00	38312.0
111.00	5942.0
111.90	566.0
112.80	168.0
116.20	1226.0
117.00	18832.0
118.00	1082.0
119.00	458.0
119.80	306.0
121.90	1121.0
123.00	2273.0
124.00	1342.0
125.00	742.0
127.00	74896.0
128.00	5601.0
129.00	29824.0
130.00	2702.0
131.10	500.0
132.20	235.0
132.80	152.0
134.00	624.0
135.00	2143.0
136.00	802.0
137.00	1579.0
138.90	306.0
139.80	513.0
140.90	2677.0
141.90	929.0
143.10	709.0
144.10	287.0
145.10	256.0
145.90	627.0
147.10	1777.0

Instrument :
BNA_G
ClientSampleId :
DFTPP540

148.00	5273.0
148.90	1031.0
151.30	386.0
151.70	309.0
153.00	1128.0
154.00	996.0
155.00	2608.0
156.10	2330.0
157.10	911.0
158.00	557.0
159.00	626.0
159.90	1099.0
161.00	1686.0
162.10	423.0
163.10	456.0
164.00	394.0
165.10	1664.0
166.10	1340.0
167.00	6865.0
168.00	4097.0
168.90	446.0
170.90	340.0
172.00	448.0
173.10	1165.0
174.10	2132.0
175.10	2701.0
175.90	888.0
177.00	1106.0
178.00	450.0
179.00	7173.0
180.00	3235.0
181.00	2104.0
182.00	452.0
183.90	540.0
185.00	2324.0
186.00	20296.0
186.90	4560.0
187.90	808.0
189.00	1391.0
189.80	351.0
191.00	821.0
192.10	2010.0
193.00	1968.0
194.10	814.0
195.10	305.0
196.00	5232.0
198.00	159936.0
199.00	10335.0
200.00	876.0
201.50	971.0
202.10	366.0
203.10	1064.0
204.00	5965.0
205.10	10598.0
206.10	45560.0
207.00	5859.0
208.00	1517.0
208.90	919.0
209.90	624.0
211.00	2357.0
212.00	187.0
215.10	724.0
216.10	967.0
216.90	8907.0
218.00	1569.0
221.10	5493.0
222.00	1626.0
223.10	1938.0
224.00	22480.0
225.00	7494.0
226.00	652.0
227.00	9314.0
228.00	1345.0
229.10	1586.0
229.90	259.0
231.10	965.0
231.90	176.0
232.80	260.0
233.90	621.0
234.80	645.0
235.90	523.0
237.00	730.0
239.10	359.0
239.60	233.0
241.00	443.0
242.00	1447.0
243.00	701.0
244.10	17312.0
245.00	2899.0
246.00	3610.0
247.00	723.0
248.00	245.0
249.00	938.0
250.00	289.0
251.50	173.0
252.10	210.0

Instrument :
BNA_G
ClientSampleId :
DFTPP540

252.80	809.0
255.00	93280.0
256.00	14739.0
256.90	1155.0
258.00	5814.0
259.00	989.0
260.90	266.0
264.00	267.0
265.00	2482.0
266.20	293.0
270.10	211.0
271.10	209.0
271.70	200.0
273.00	3408.0
274.00	7525.0
275.00	37216.0
276.00	5682.0
276.90	2699.0
278.10	479.0
280.80	172.0
282.10	208.0
282.90	182.0
284.00	195.0
285.00	1061.0
286.00	243.0
288.50	168.0
288.90	222.0
289.90	220.0
293.00	970.0
296.00	11837.0
297.00	1851.0
301.70	274.0
301.90	256.0
303.00	1624.0
303.80	560.0
308.00	205.0
308.80	160.0
309.90	237.0
312.90	174.0
314.00	810.0
315.00	1070.0
316.00	601.0
317.20	242.0
319.90	233.0
321.10	557.0
323.10	3639.0
323.90	837.0
325.10	162.0
326.00	155.0
327.00	951.0
327.90	764.0
332.00	279.0
333.20	219.0
334.00	2420.0
334.90	1225.0
336.10	198.0
339.10	192.0
339.60	162.0
341.10	659.0
341.70	180.0
344.50	186.0
346.10	491.0
346.90	333.0
350.20	152.0
351.90	1175.0
353.00	977.0
353.90	992.0
354.10	967.0
354.70	238.0
364.90	5545.0
365.80	877.0
366.70	161.0
371.10	358.0
372.10	1951.0
373.00	728.0
382.80	553.0
383.80	318.0
390.00	232.0
390.80	174.0
391.80	231.0
400.90	381.0
401.80	617.0
403.00	1337.0
403.80	457.0
404.10	440.0
404.90	256.0
414.60	168.0
420.90	1340.0
421.90	873.0
422.90	5291.0
423.90	2100.0
425.10	398.0
426.90	178.0
438.90	162.0
441.00	23296.0
442.00	131840.0

Instrument :
BNA_G
ClientSampleId :
DFTPP540

443.00	26376.0
444.00	3198.0
445.10	325.0

Instrument :
BNA_G
ClientSampleId :
DFTPP540

m/z	Abundance
37.20	270.0
38.10	865.0
39.10	4884.0
40.20	413.0
41.10	216.0
44.20	331.0
49.00	510.0
50.10	16424.0
51.10	72176.0
52.10	3562.0
55.00	615.0
56.10	2556.0
57.00	5068.0
58.00	194.0
59.10	302.0
61.00	763.0
62.10	676.0
63.10	2345.0
64.10	595.0
65.00	1612.0
67.10	242.0
68.00	1133.0
69.00	47384.0
70.10	579.0
72.90	350.0
74.10	4355.0
75.10	8077.0
76.20	2379.0
77.10	61240.0
78.10	4086.0
79.10	3736.0
80.10	2294.0
81.00	3844.0
82.10	1555.0
83.10	825.0
85.10	630.0
86.00	1515.0
87.10	540.0
88.00	192.0
91.00	1047.0
92.10	724.0
93.00	7569.0
94.10	863.0
95.10	279.0
96.20	267.0
98.00	4746.0
99.00	4007.0
100.00	334.0
101.00	2569.0
102.10	184.0
103.00	625.0
103.90	1268.0
105.10	1338.0
106.00	387.0
107.10	15729.0
108.10	2208.0
110.00	28512.0
111.10	3985.0
111.90	624.0
115.90	826.0
117.00	12738.0
118.00	1527.0
120.10	250.0
122.10	1210.0
123.00	959.0
124.00	652.0
125.00	757.0
125.80	179.0
127.00	58416.0
128.10	3288.0
129.00	22120.0
130.10	1637.0
131.00	470.0
132.10	211.0
133.20	186.0
133.90	613.0
135.00	1775.0
135.90	868.0
136.90	948.0
139.90	336.0
141.10	2110.0
142.10	631.0
143.10	668.0
146.10	471.0
147.00	1285.0
148.00	3350.0
149.00	885.0
150.10	206.0
151.20	494.0
151.50	505.0
153.10	835.0
154.00	632.0

Instrument :
BNA_G
ClientSampleId :
DFTPP540

155.00	2099.0
156.10	2908.0
157.00	341.0
158.00	503.0
158.90	356.0
159.90	1064.0
161.00	1587.0
161.80	411.0
163.20	401.0
164.10	166.0
165.00	1133.0
166.10	569.0
167.00	6246.0
168.10	3162.0
169.10	865.0
169.80	391.0
170.90	458.0
172.00	634.0
173.00	304.0
174.00	1470.0
175.00	2643.0
176.10	604.0
177.00	874.0
177.90	292.0
178.90	4965.0
180.00	3042.0
181.00	1522.0
181.80	244.0
183.20	459.0
183.90	232.0
185.00	2296.0
186.00	15944.0
187.00	5090.0
188.10	804.0
189.00	1218.0
189.70	231.0
190.90	457.0
192.10	1296.0
193.10	1797.0
194.10	380.0
194.90	153.0
196.10	3836.0
198.00	133120.0
199.00	9544.0
200.10	984.0
201.20	529.0
201.60	563.0
203.10	938.0
204.00	5246.0
205.00	9217.0
206.00	35672.0
207.10	4750.0
208.00	1399.0
209.10	308.0
210.00	445.0
210.70	941.0
211.00	1110.0
212.10	311.0
212.90	272.0
214.00	239.0
215.00	364.0
217.00	7606.0
217.80	911.0
220.10	337.0
221.00	6416.0
221.60	1465.0
223.00	1953.0
224.00	21024.0
225.10	5561.0
226.00	1102.0
227.00	8200.0
228.10	1317.0
229.00	1859.0
229.90	490.0
231.00	885.0
231.90	295.0
233.00	306.0
234.10	415.0
234.90	632.0
235.80	313.0
236.90	962.0
239.00	334.0
239.90	415.0
241.00	478.0
242.00	1113.0
243.00	1096.0
244.00	14015.0
245.10	1941.0
246.00	3736.0
246.90	1071.0
247.80	234.0
248.80	626.0
251.00	158.0
252.00	265.0
252.90	336.0
255.00	91072.0

Instrument :
BNA_G
ClientSampleId :
DFTPP540

256.00	13192.0
257.00	1057.0
258.00	5285.0
259.00	803.0
259.90	245.0
260.10	252.0
260.90	296.0
265.00	2030.0
267.30	348.0
268.00	168.0
271.10	167.0
272.10	407.0
273.00	2245.0
274.00	6402.0
275.00	36392.0
276.10	3809.0
277.00	3547.0
277.90	554.0
282.90	442.0
284.00	287.0
284.70	161.0
285.10	293.0
286.00	275.0
288.90	276.0
289.50	228.0
291.90	325.0
293.10	731.0
296.00	12288.0
297.00	1544.0
300.80	269.0
301.80	394.0
303.00	1726.0
304.10	482.0
305.20	244.0
307.30	158.0
308.10	182.0
312.60	198.0
314.20	573.0
315.00	1358.0
315.90	1253.0
317.10	183.0
321.00	222.0
323.10	3739.0
324.00	941.0
325.50	262.0
326.90	836.0
328.00	721.0
333.00	855.0
334.10	2043.0
335.10	1009.0
341.20	273.0
345.80	628.0
352.00	877.0
352.80	929.0
353.40	445.0
354.00	858.0
355.10	304.0
359.00	204.0
365.00	5319.0
365.80	851.0
369.90	188.0
370.70	432.0
371.90	1344.0
372.70	631.0
382.90	347.0
384.00	178.0
390.00	385.0
390.80	532.0
391.80	222.0
395.30	197.0
402.00	876.0
403.00	1797.0
403.90	622.0
412.00	161.0
420.80	1335.0
421.90	1000.0
423.00	7673.0
424.10	1754.0
433.50	153.0
438.00	215.0
441.00	28408.0
442.00	152768.0
442.90	28624.0
443.90	3746.0
484.20	349.0

Instrument :
BNA_G
ClientSampleId :
DFTPP540