
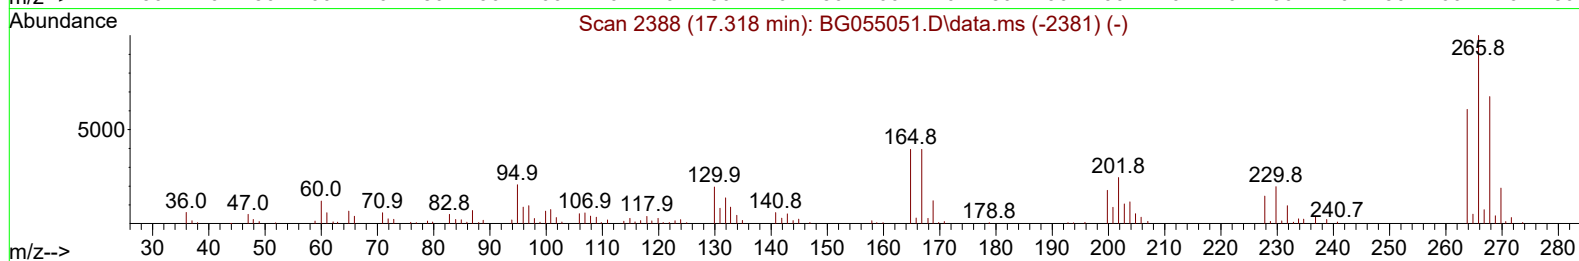
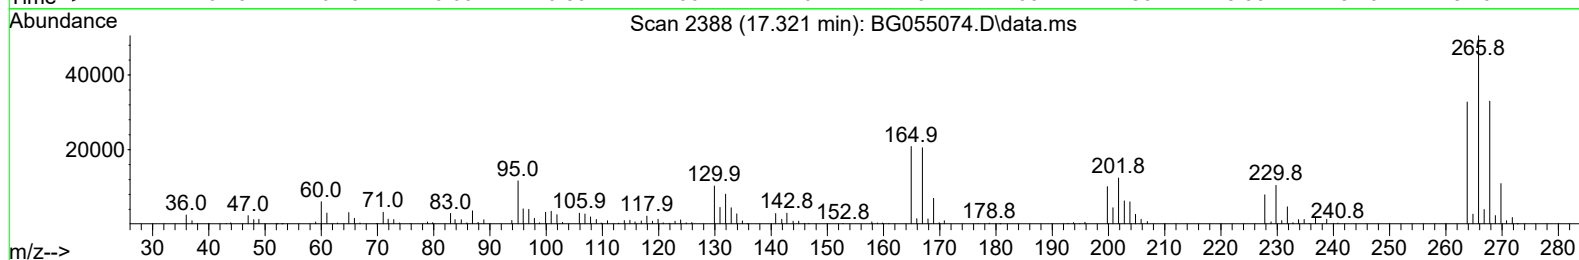


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100522\
Data File : BG055074.D
Acq On : 5 Oct 2022 11:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 04:51:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 07:12:22 2022
Response via : Initial Calibration

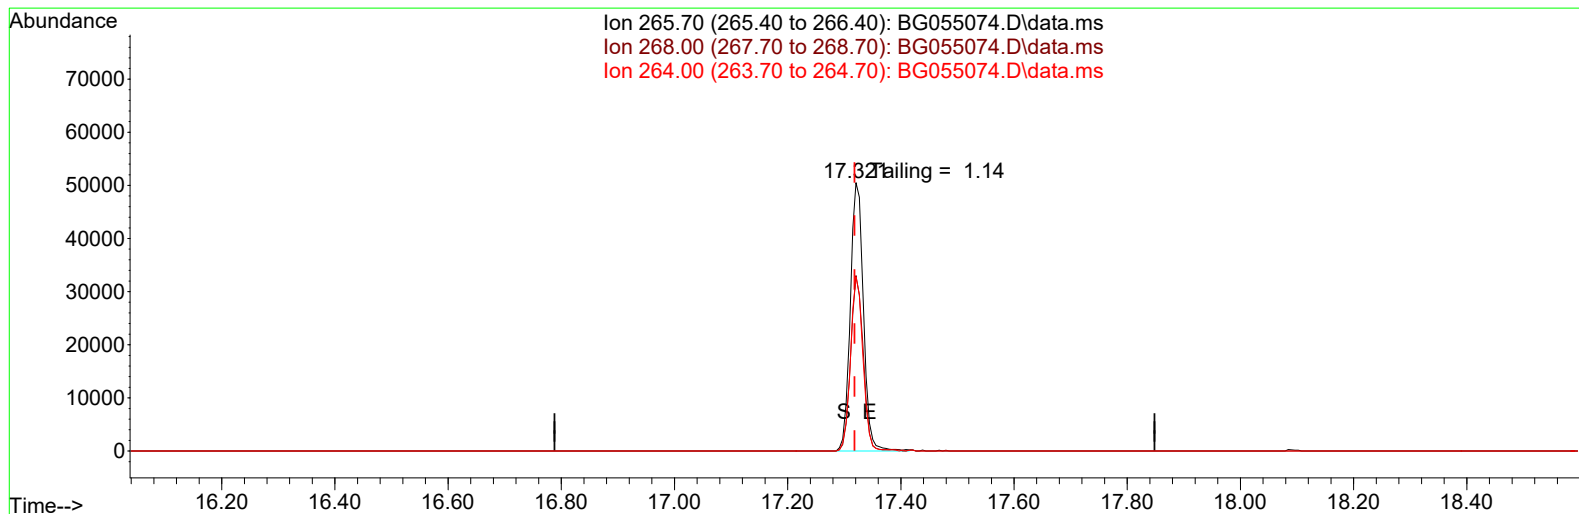

TIC: BG055074.D\data.ms

(70) Pentachlorophenol (C)




17.321min (+ 0.003) 26495.94 ng

response 81188

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	65.34
264.00	60.80	64.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100522\
Data File : BG055074.D
Acq On : 5 Oct 2022 11:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 04:51:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 07:12:22 2022
Response via : Initial Calibration

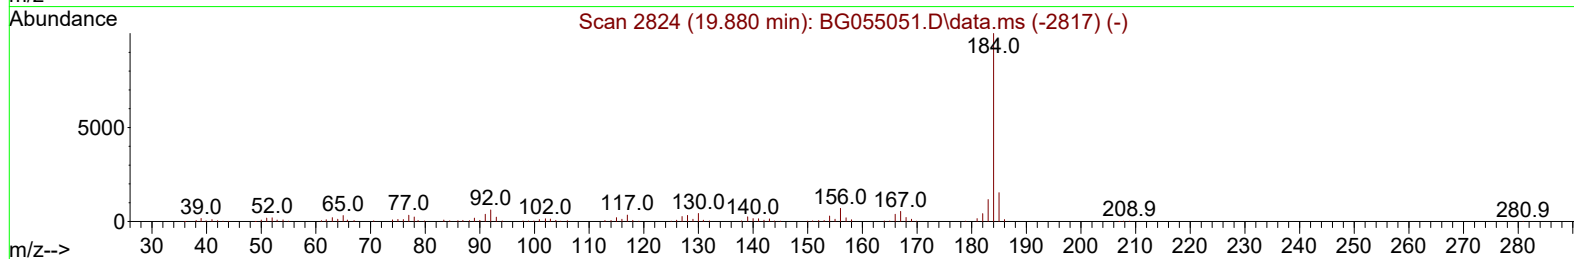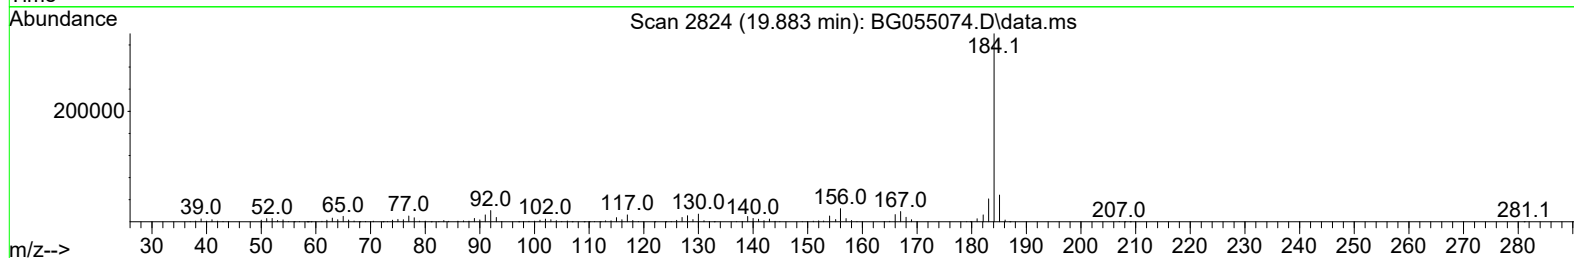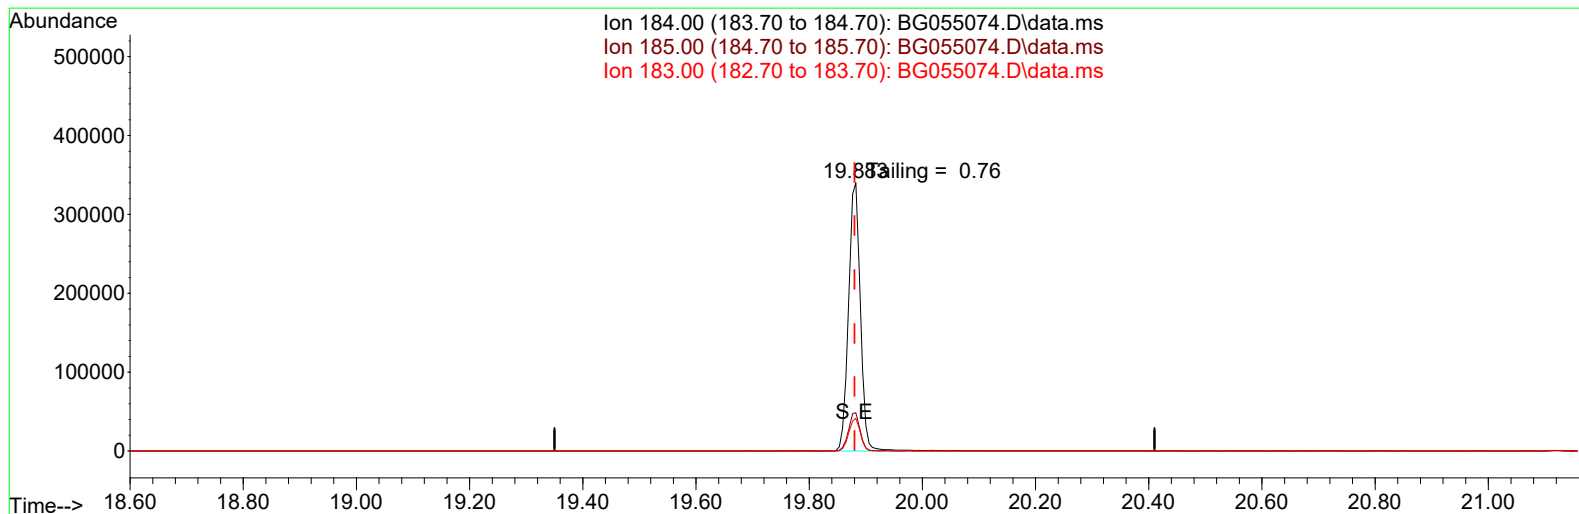

TIC: BG055074.D\data.ms

(77) Benzidine**19.883min (+ 0.003) 24859.54 ng****response 495923**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.27
183.00	11.70	12.20
0.00	0.00	0.00