
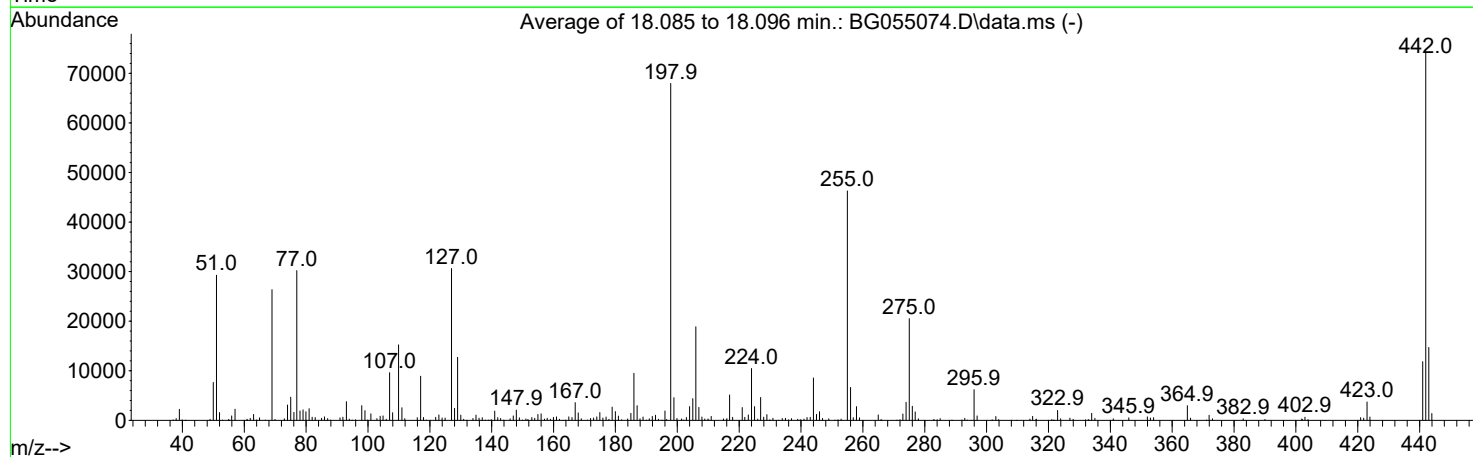


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100522\
 Data File : BG055074.D
 Acq On : 5 Oct 2022 11:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 04 07:12:22 2022

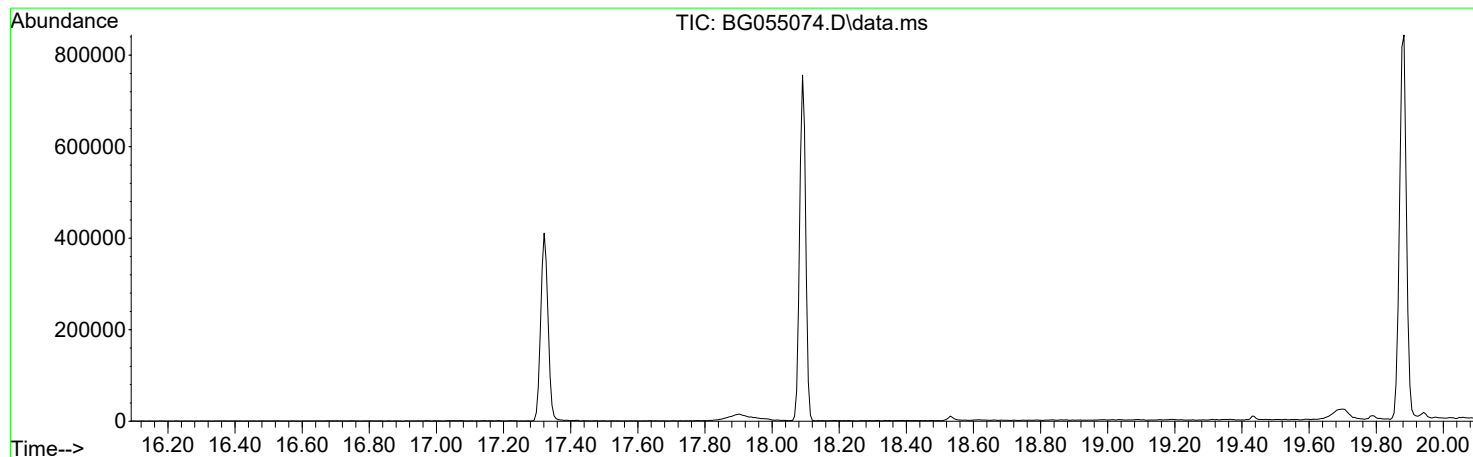




AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	29283	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.8	26384	PASS
70	69	0.00	2	0.7	195	PASS
127	198	10	80	45.1	30643	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67963	PASS
199	198	5	9	6.8	4591	PASS
275	198	10	60	30.2	20515	PASS
365	198	1	100	4.4	2967	PASS
441	198	0.01	100	17.4	11855	PASS
442	442	50	100	100.0	74200	PASS
443	442	15	24	19.8	14718	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100522\
 Data File : BG055074.D
 Acq On : 5 Oct 2022 11:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 06 04:51:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 04 07:12:22 2022
 Response via : Initial Calibration

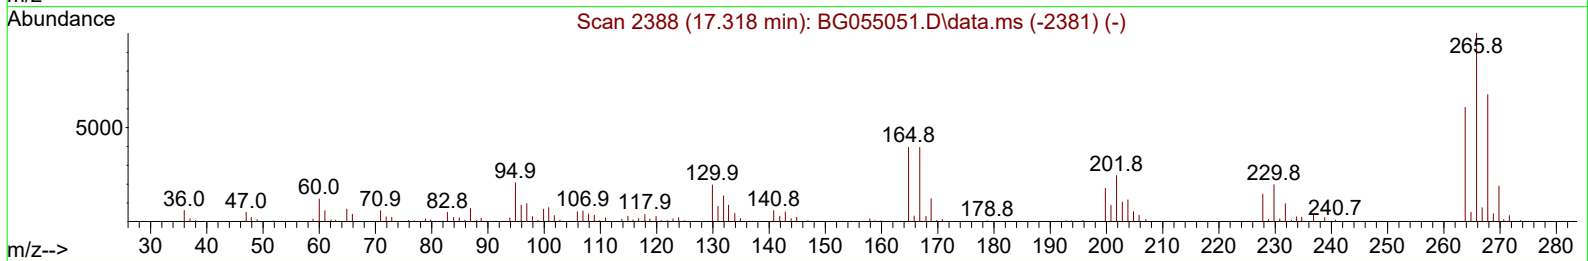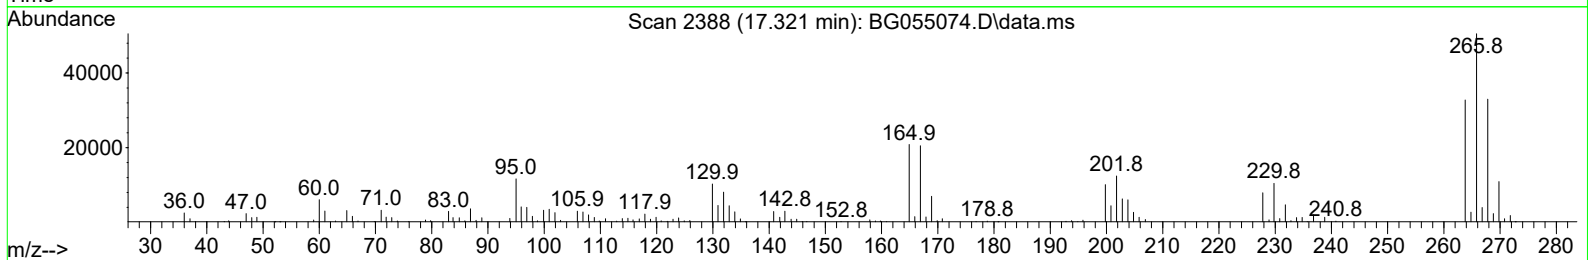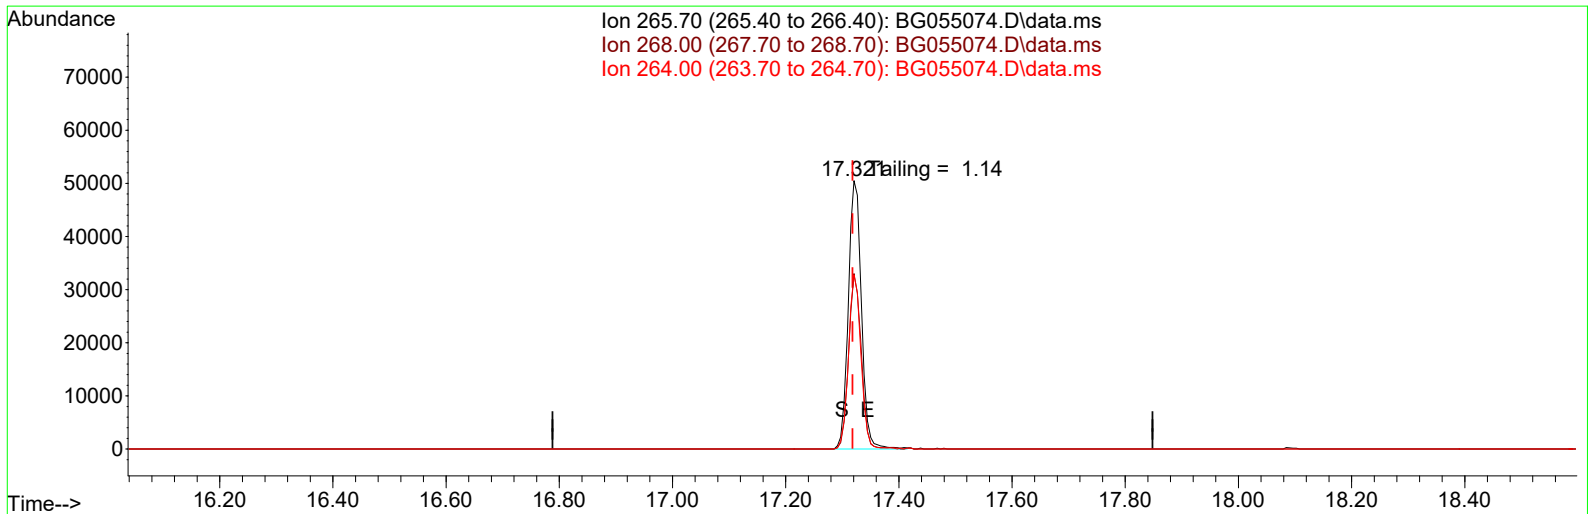

TIC: BG055074.D\data.ms

(70) Pentachlorophenol (C)

17.321min (+ 0.003) 26495.94 ng




response 81188

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	65.34
264.00	60.80	64.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100522\
Data File : BG055074.D
Acq On : 5 Oct 2022 11:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 06 04:51:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 07:12:22 2022
Response via : Initial Calibration

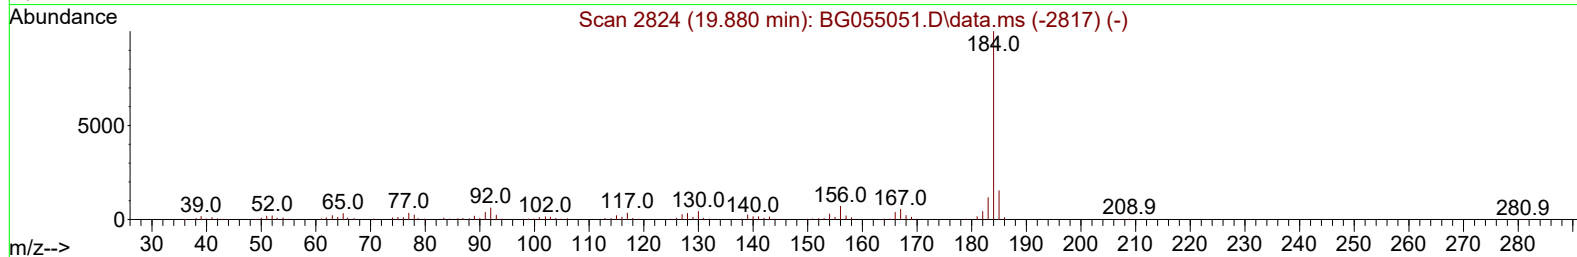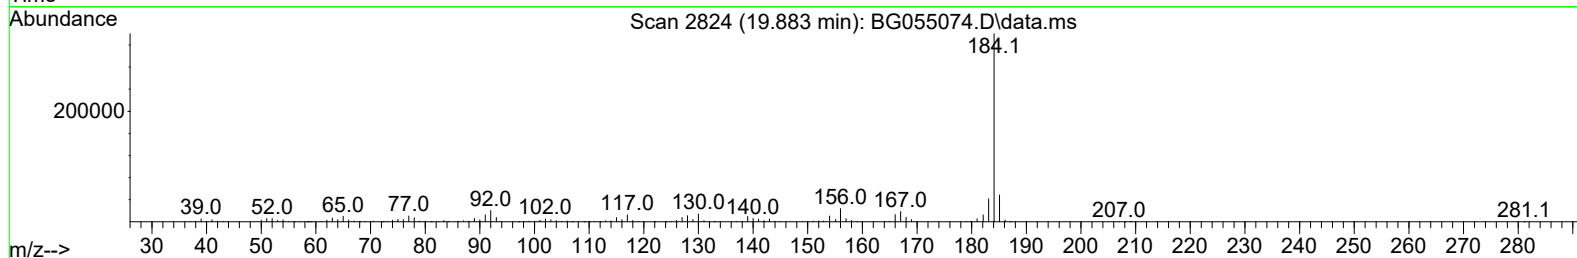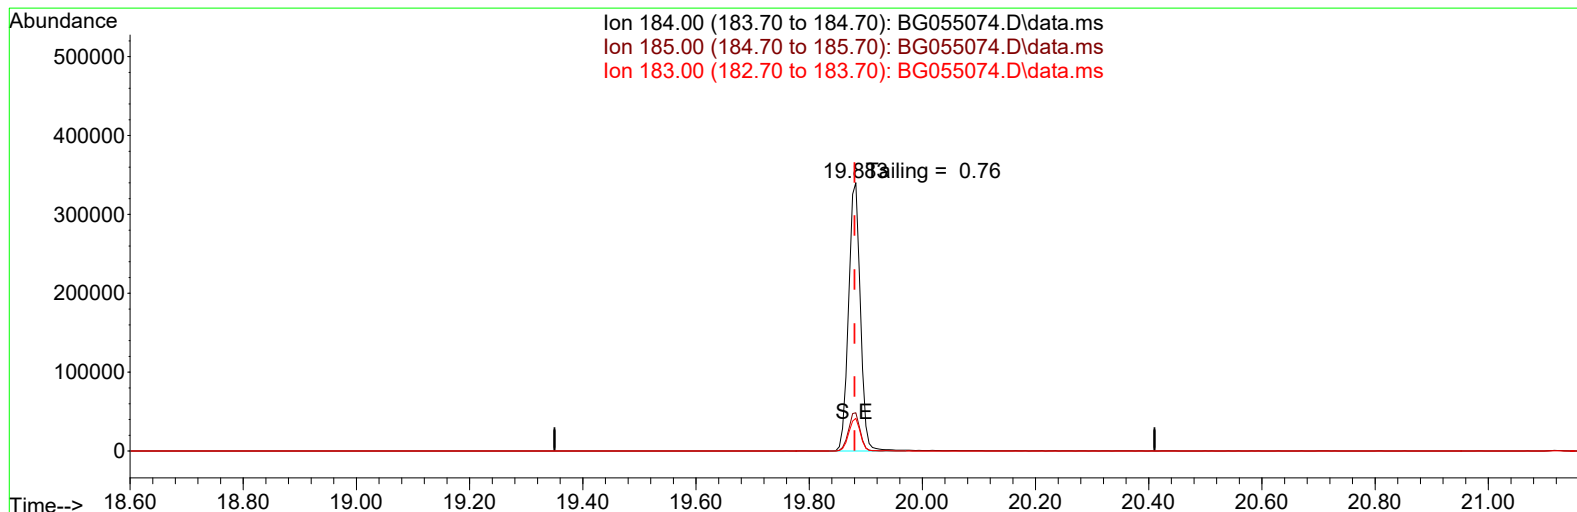

TIC: BG055074.D\data.ms

(77) Benzidine

19.883min (+ 0.003) 24859.54 ng

response 495923

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.27
183.00	11.70	12.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/5/2022	BNA_G	BG055074.D
Compound Name	Response	Retention Time
DDT	201927	21.122
DDD	2374	20.664
DDE	0	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2374	204301	1.16

Instrument :
BNA_G
ClientSampleId :
DFTPP