

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
 Data File : BG059306.D
 Acq On : 5 Oct 2023 21:31
 Operator : MA/JU
 Sample : 04592-01 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EZYX9

Quant Time: Oct 05 22:42:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 04:33:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.235	152	39824	20.000	ng/ul	0.00
20) Naphthalene-d8	11.079	136	185020	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.869	164	108854	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.619	188	229566	20.000	ng/ul	0.00
79) Chrysene-d12	21.919	240	185292	20.000	ng/ul	0.00
88) Perylene-d12	25.409	264	221223	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.535	96	2334	2.212	ng/uL	0.01
4) Pyridine-d5	3.970	84	27574	8.956	ng/ul	0.00
7) Phenol-d5	7.366	99	26605	6.674	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.554	67	69839	27.425	ng/ul	0.00
11) 2-Chlorophenol-d4	7.759	132	68767	25.663	ng/ul	0.01
15) 4-Methylphenol-d8	8.929	113	46972	15.244	ng/ul	0.00
21) Nitrobenzene-d5	9.434	128	48519	37.162	ng/ul	0.00
24) 2-Nitrophenol-d4	10.157	143	50613	39.489	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.680	165	86732	32.941	ng/ul	0.00
31) 4-Chloroaniline-d4	11.226	131	116137	27.262	ng/ul	0.00
46) Dimethylphthalate-d6	14.264	166	287426	36.521	ng/ul	0.00
49) Acenaphthylene-d8	14.575	160	359397	36.382	ng/ul	0.00
54) 4-Nitrophenol-d4	15.069	143	8255	6.007	ng/ul	0.01
60) Fluorene-d10	15.856	176	275876	36.830	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.973	200	22721	19.255	ng/ul	0.01
73) Anthracene-d10	17.718	188	406946	38.904	ng/ul	0.00
81) Pyrene-d10	19.992	212	412225	39.727	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.169	264	406679	38.255	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	14.311	163	9753	1.210	ng/ul#	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
Data File : BG059306.D
Acq On : 5 Oct 2023 21:31
Operator : MA/JU
Sample : 04592-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EZYX9

Quant Time: Oct 05 22:42:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 28 04:33:25 2023
Response via : Initial Calibration

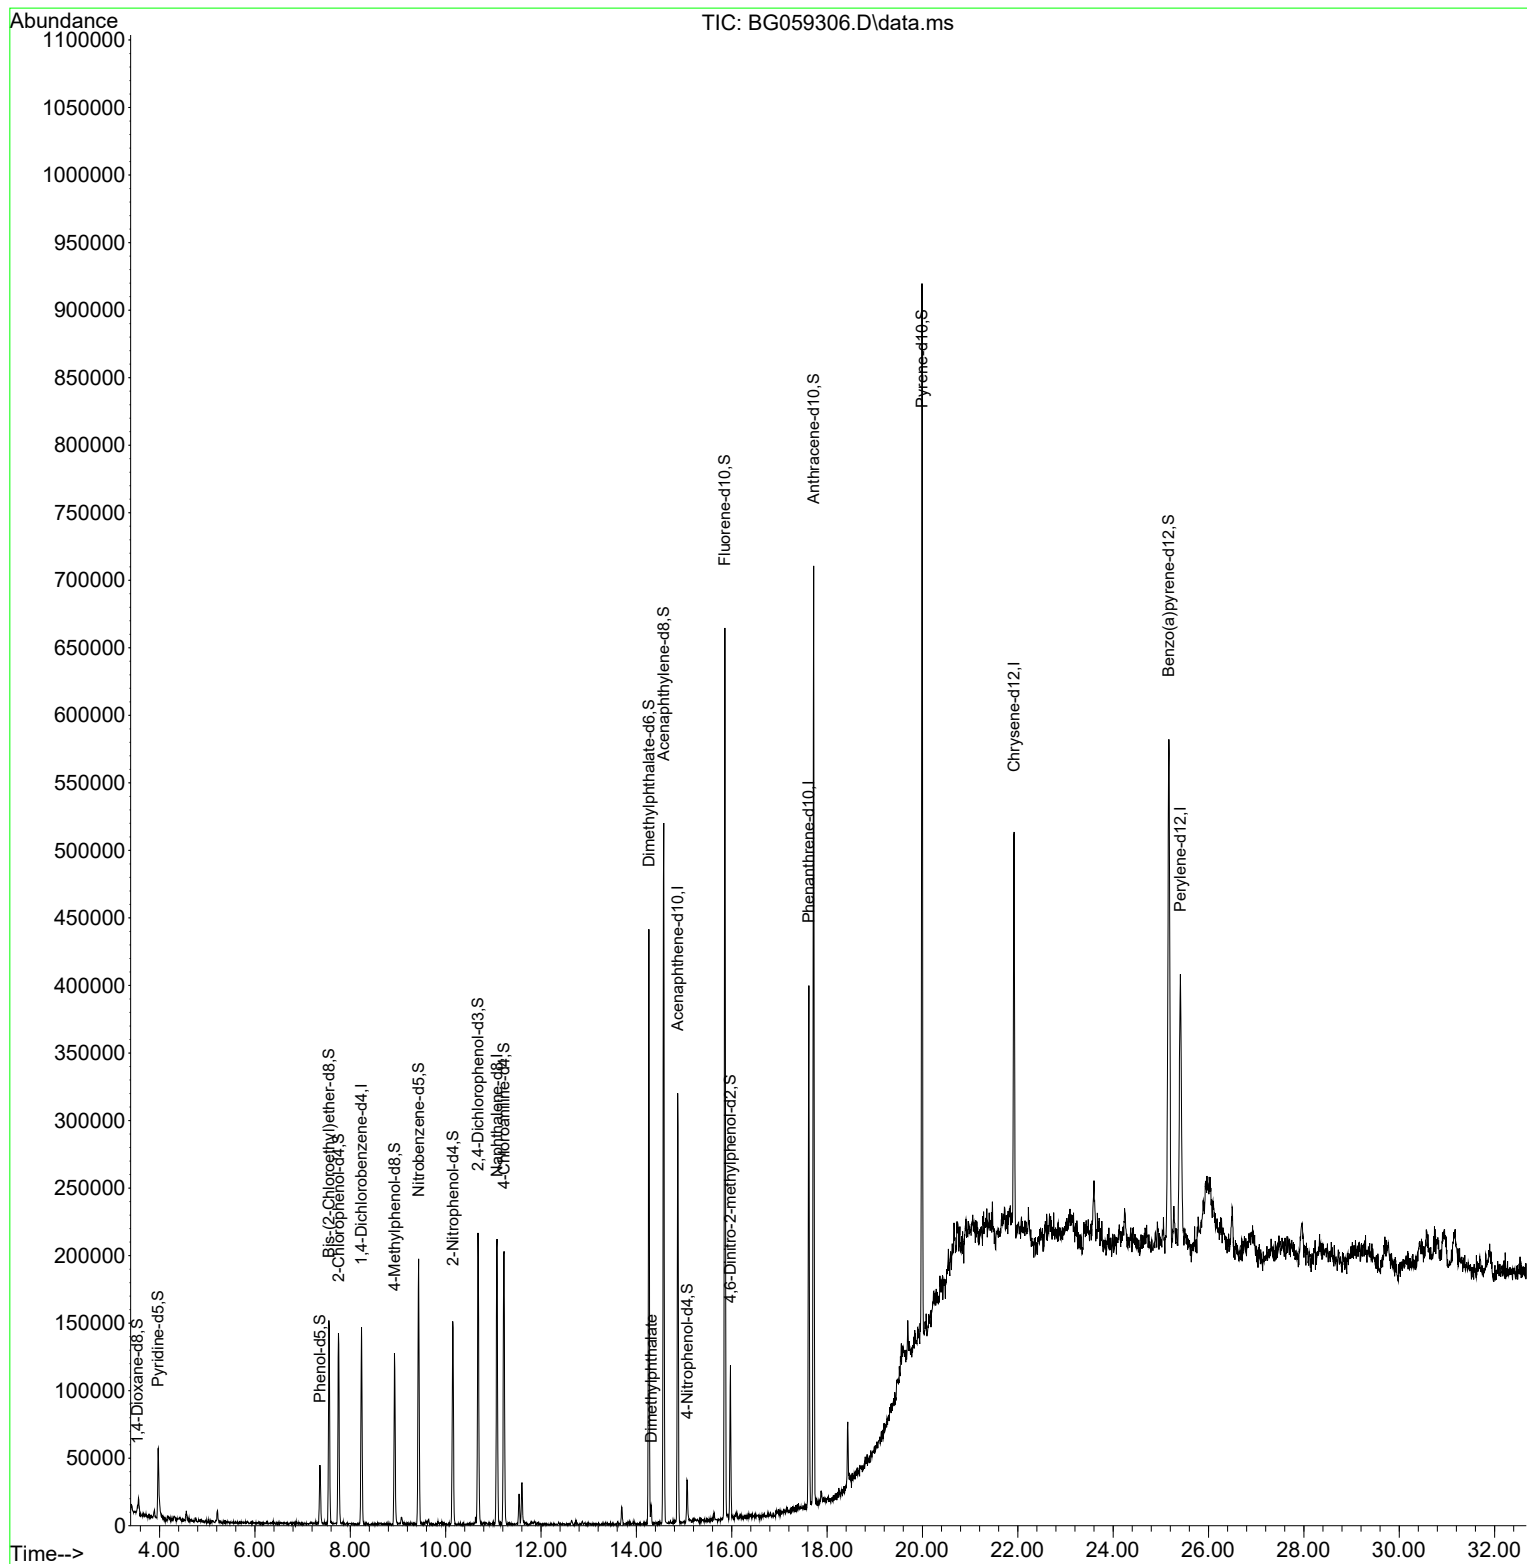

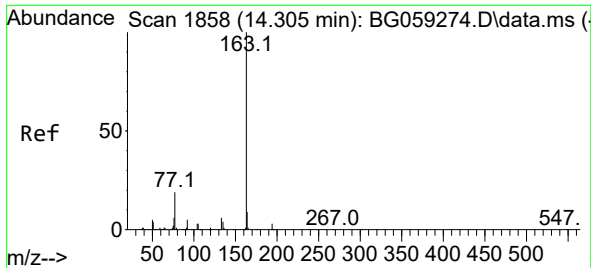

#47

Dimethylphthalate

Concen: 1.210 ng/ul

RT: 14.311 min Scan# 1859

Delta R.T. -0.002 min

Lab File: BG059306.D


Acq: 5 Oct 2023 21:31

Instrument :

BNA_G

ClientSampleId :

EZYX9

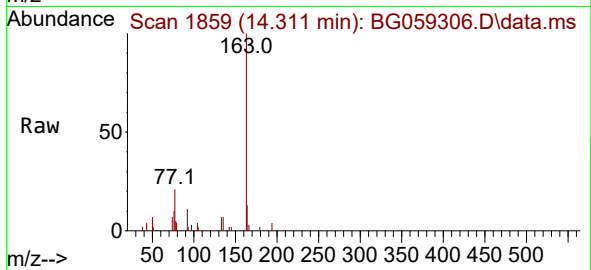

Tgt Ion:163 Resp: 9753

Ion Ratio Lower Upper

163 100

194 4.0 2.6 4.0

164 12.7 7.9 11.9#

