

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028078.D
 Acq On : 06 Oct 2023 10:57
 Operator : MA/JU
 Sample : PB155952BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 07 00:30:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	5801	0.400	ng/ul	0.00
4) Naphthalene-d8	10.746	136	18163	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.578	164	9783	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	19093	0.400	ng/ul	0.00
17) Chrysene-d12	21.533	240	16965	0.400	ng/ul	# 0.01
23) Perylene-d12	24.000	264	19495	0.400	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	46695	6.409	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.335	152	8613	0.294	ng/ul	0.00
18) Fluoranthene-d10	19.366	212	16573	0.308	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.577	166	2836	0.072	ng/ul#	16
20) Pyrene	19.738	202	2901	0.043	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028078.D
Acq On : 06 Oct 2023 10:57
Operator : MA/JU
Sample : PB155952BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :


Quant Time: Oct 07 00:30:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration

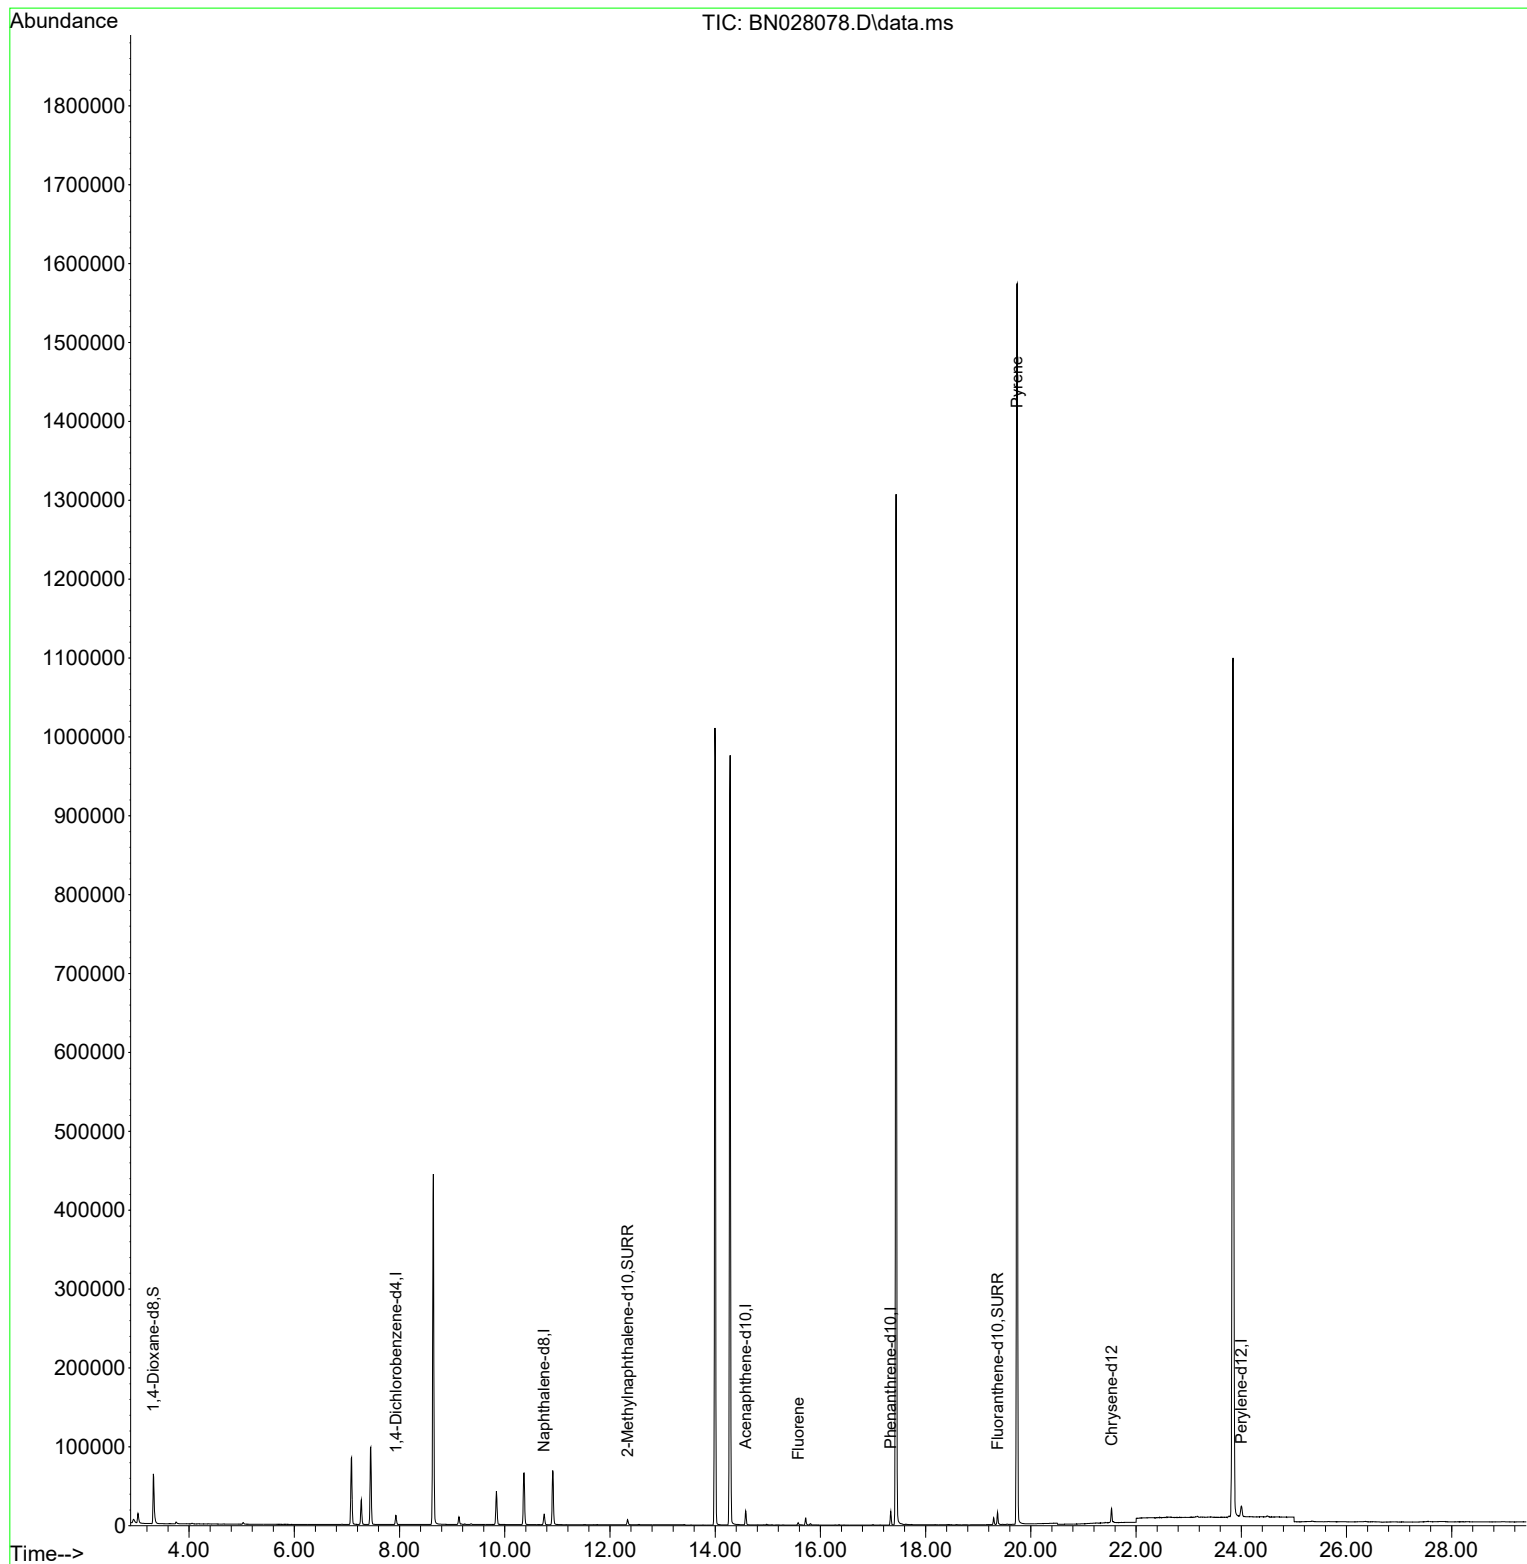



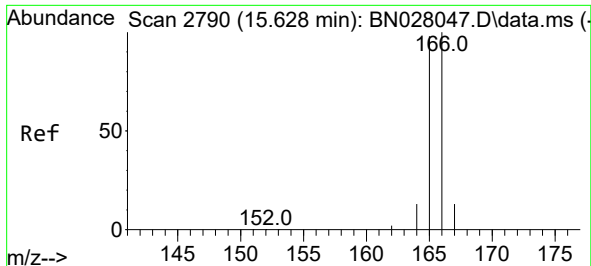


#12
Fluorene
Concen: 0.072 ng/ul
RT: 15.577 min Scan# 21
Delta R.T. -0.056 min
Lab File: BN028078.D
Acq: 06 Oct 2023 10:57

Instrument :
BNA_G
ClientSampleId :

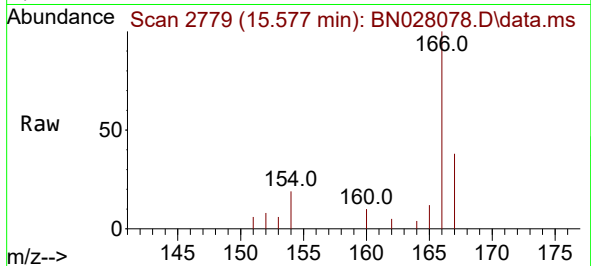

Tgt Ion:166 Resp: 2836
Ion Ratio Lower Upper
166 100
165 11.5 78.5 117.7#
167 37.7 11.2 16.8#

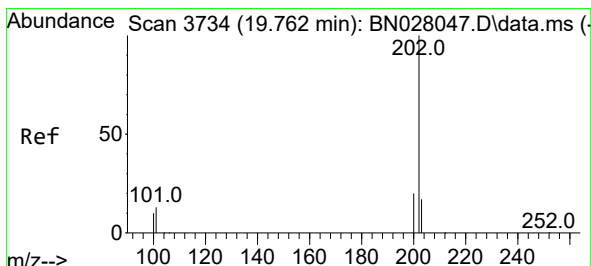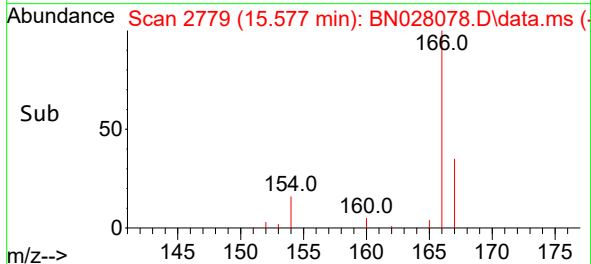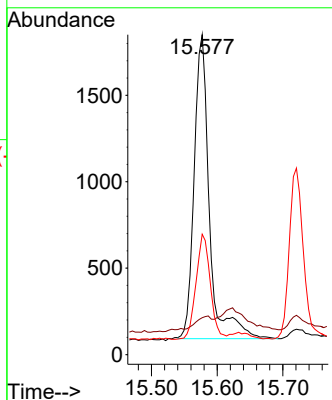

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.738 min Scan# 3729
Delta R.T. -0.019 min
Lab File: BN028078.D
Acq: 06 Oct 2023 10:57

Tgt Ion:202 Resp: 2901
Ion Ratio Lower Upper
202 100
101 140.7 11.2 16.8#
100 957.8 9.1 13.7#

