

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP100423\  
 Data File : BP017563.D  
 Acq On : 05 Oct 2023 13:40  
 Operator : MA/JU  
 Sample : 04679-04  
 Misc :  
 ALS Vial : 37 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :

Quant Time: Oct 06 01:59:16 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP100423.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Oct 04 16:33:47 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min)     |
|-------------------------------|--------|------|----------|--------|-------|--------------|
| Internal Standards            |        |      |          |        |       |              |
| 1) 1,4-Dichlorobenzene-d4     | 7.940  | 152  | 109726   | 20.000 | ng/ul | 0.00         |
| 20) Naphthalene-d8            | 10.775 | 136  | 442308   | 20.000 | ng/ul | 0.00         |
| 38) Acenaphthene-d10          | 14.628 | 164  | 278527   | 20.000 | ng/ul | -0.01        |
| 64) Phenanthrene-d10          | 17.422 | 188  | 664169   | 20.000 | ng/ul | 0.00         |
| 79) Chrysene-d12              | 21.557 | 240  | 689349   | 20.000 | ng/ul | 0.00         |
| 88) Perylene-d12              | 24.139 | 264  | 773349   | 20.000 | ng/ul | 0.00         |
| System Monitoring Compounds   |        |      |          |        |       |              |
| 3) 1,4-Dioxane-d8             | 3.287  | 96   | 11258    | 4.102  | ng/uL | 0.00         |
| 4) Pyridine-d5                | 3.728  | 84   | 104039   | 14.482 | ng/ul | 0.00         |
| 7) Phenol-d5                  | 7.099  | 99   | 83838    | 9.081  | ng/ul | 0.00         |
| 9) Bis-(2-Chloroethyl)eth...  | 7.281  | 67   | 219351   | 38.938 | ng/ul | 0.00         |
| 11) 2-Chlorophenol-d4         | 7.457  | 132  | 222522   | 30.612 | ng/ul | 0.00         |
| 15) 4-Methylphenol-d8         | 8.657  | 113  | 176700   | 23.908 | ng/ul | -0.01        |
| 21) Nitrobenzene-d5           | 9.146  | 128  | 138621   | 40.737 | ng/ul | 0.00         |
| 24) 2-Nitrophenol-d4          | 9.863  | 143  | 151575   | 39.494 | ng/ul | 0.00         |
| 28) 2,4-Dichlorophenol-d3     | 10.393 | 165  | 276239   | 38.824 | ng/ul | 0.00         |
| 31) 4-Chloroaniline-d4        | 10.945 | 131  | 313765   | 30.956 | ng/ul | 0.00         |
| 46) Dimethylphthalate-d6      | 14.045 | 166  | 969277   | 44.614 | ng/ul | 0.00         |
| 49) Acenaphthylene-d8         | 14.328 | 160  | 1022586  | 42.684 | ng/ul | 0.00         |
| 54) 4-Nitrophenol-d4          | 14.881 | 143  | 25258    | 6.639  | ng/ul | 0.00         |
| 60) Fluorene-d10              | 15.633 | 176  | 823351   | 44.679 | ng/ul | 0.00         |
| 65) 4,6-Dinitro-2-methylph... | 15.775 | 200  | 142160   | 34.333 | ng/ul | 0.00         |
| 73) Anthracene-d10            | 17.522 | 188  | 1349413  | 43.892 | ng/ul | 0.00         |
| 81) Pyrene-d10                | 19.774 | 212  | 1775534  | 46.353 | ng/ul | 0.00         |
| 92) Benzo(a)pyrene-d12        | 23.968 | 264  | 1778998  | 45.583 | ng/ul | 0.00         |
| Target Compounds              |        |      |          |        |       |              |
| 34) Caprolactam               | 11.810 | 113  | 5002     | 2.333  | ng/ul | Qvalue<br>97 |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP100423\  
Data File : BP017563.D  
Acq On : 05 Oct 2023 13:40  
Operator : MA/JU  
Sample : 04679-04  
Misc :  
ALS Vial : 37 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :

Quant Time: Oct 06 01:59:16 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP100423.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Oct 04 16:33:47 2023  
Response via : Initial Calibration

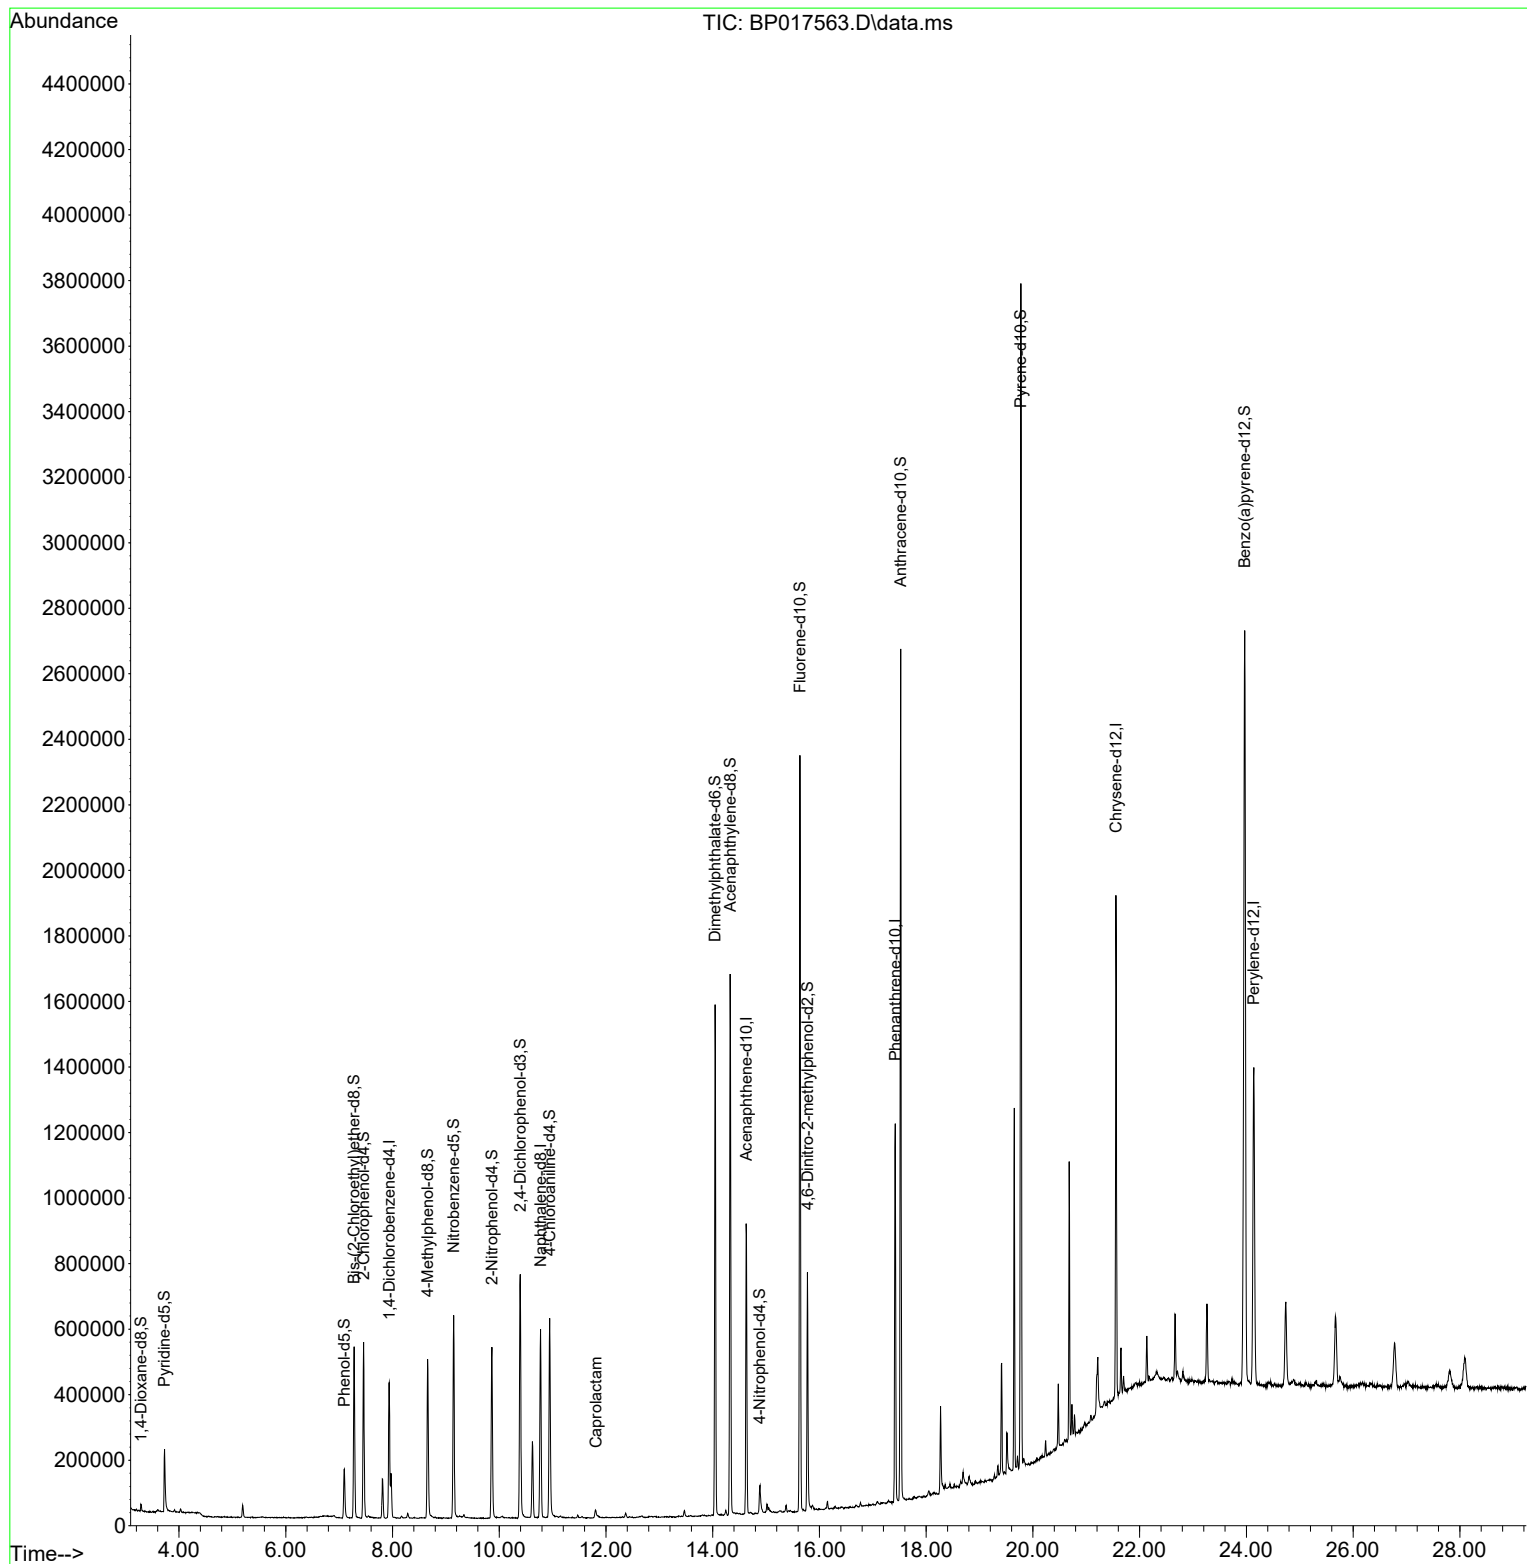

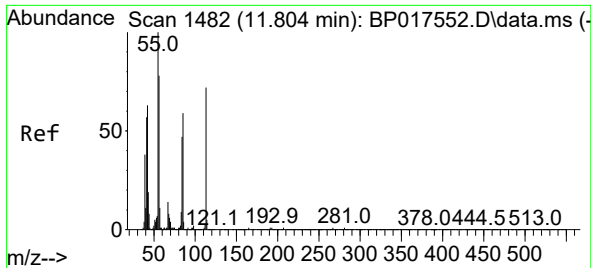

#34  
Caprolactam  
Concen: 2.333 ng/ul  
RT: 11.810 min Scan# 14  
Delta R.T. -0.006 min  
Lab File: BP017563.D  
Acq: 05 Oct 2023 13:40

Instrument :  
BNA\_G  
ClientSampleId :

Tgt Ion:113 Resp: 5002  
Ion Ratio Lower Upper  
113 100  
55 157.6 124.6 187.0  
56 114.0 94.7 142.1

