

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
 Data File : BG059313.D
 Acq On : 6 Oct 2023 2:19
 Operator : MA/JU
 Sample : 04469-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EZYL7

Quant Time: Oct 06 04:12:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 28 04:33:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.236	152	60912	20.000	ng/ul	0.00
20) Naphthalene-d8	11.074	136	262019	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.869	164	154387	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.613	188	346453	20.000	ng/ul	0.00
79) Chrysene-d12	21.920	240	298164	20.000	ng/ul	0.00
88) Perylene-d12	25.404	264	354956	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.535	96	4713	2.920	ng/uL	0.01
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.360	99	101197	16.597	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.554	67	58584	15.041	ng/ul	0.00
11) 2-Chlorophenol-d4	7.754	132	76142	18.578	ng/ul	0.00
15) 4-Methylphenol-d8	8.929	113	64814	13.752	ng/ul	0.00
21) Nitrobenzene-d5	9.434	128	37463	20.262	ng/ul	0.00
24) 2-Nitrophenol-d4	10.145	143	43592	24.016	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.680	165	73504	19.713	ng/ul	0.00
31) 4-Chloroaniline-d4	11.221	131	80066	13.272	ng/ul	0.00
46) Dimethylphthalate-d6	14.258	166	224974	20.155	ng/ul	0.00
49) Acenaphthylene-d8	14.570	160	270996	19.342	ng/ul	0.00
54) 4-Nitrophenol-d4	15.063	143	34892	17.901	ng/ul	0.00
60) Fluorene-d10	15.856	176	214726	20.212	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.968	200	16722	9.390	ng/ul	0.00
73) Anthracene-d10	17.713	188	342209	21.678	ng/ul	0.00
81) Pyrene-d10	19.993	212	433939	25.988	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.157	264	413486	24.241	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	9.076	105	22783	3.121	ng/ul#	94
86) Bis(2-ethylhexyl)phtha...	21.726	149	40659	3.485	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
Data File : BG059313.D
Acq On : 6 Oct 2023 2:19
Operator : MA/JU
Sample : 04469-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EZY7

Quant Time: Oct 06 04:12:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 28 04:33:25 2023
Response via : Initial Calibration




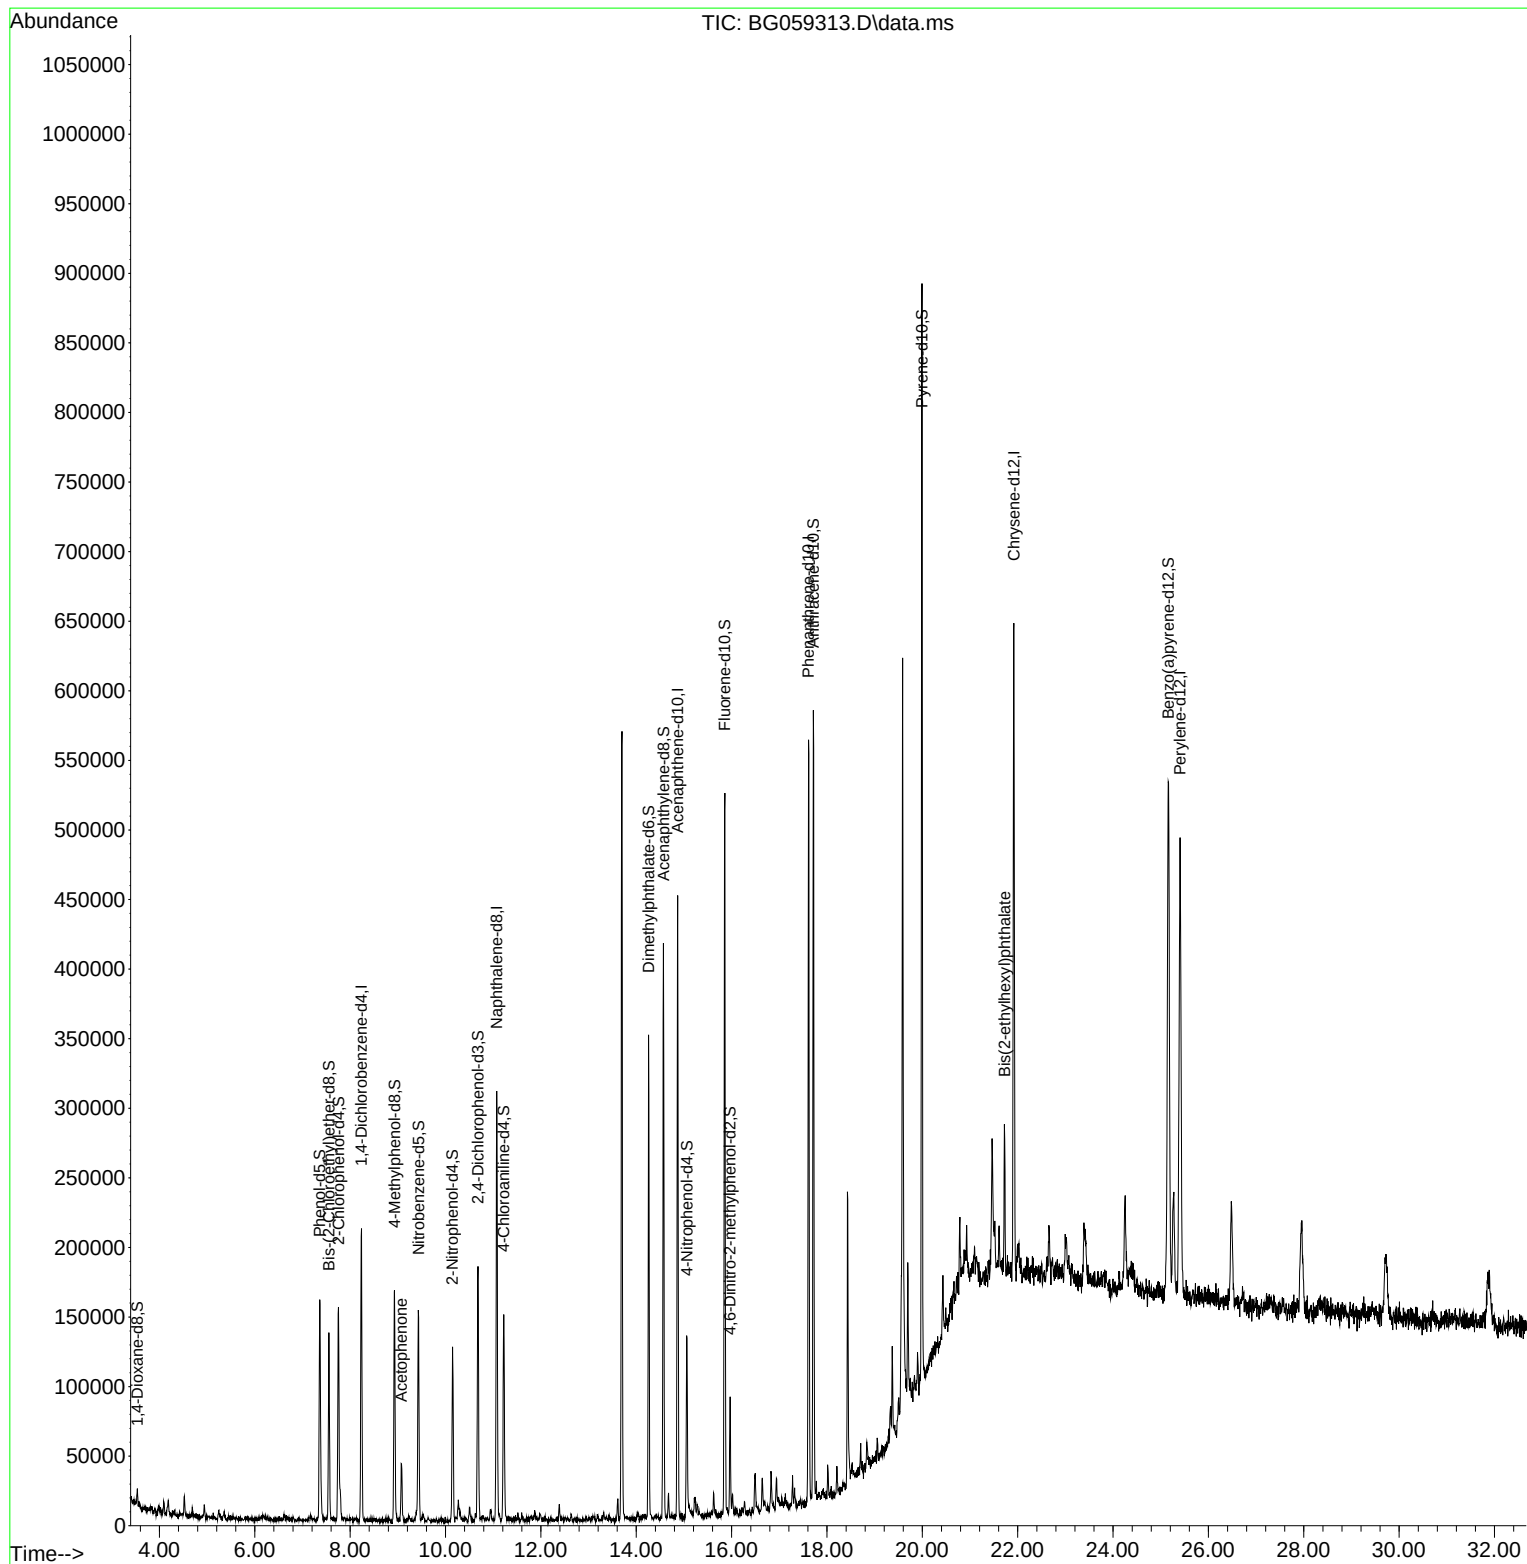


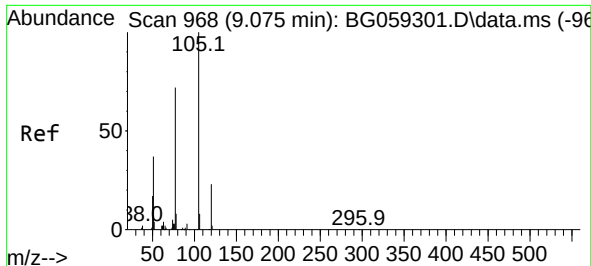

#16
Acetophenone
Concen: 3.121 ng/ul
RT: 9.076 min Scan# 90
Delta R.T. -0.001 min
Lab File: BG059313.D
Acq: 6 Oct 2023 2:19

Instrument :
BNA_G
ClientSampleId :
EZY7

Tgt Ion:105 Resp: 22783
Ion Ratio Lower Upper
105 100
77 74.2 58.8 88.2
51 31.5 32.6 48.8#

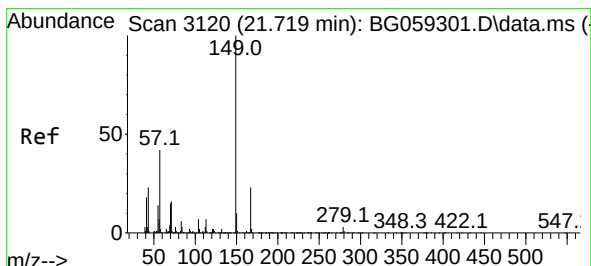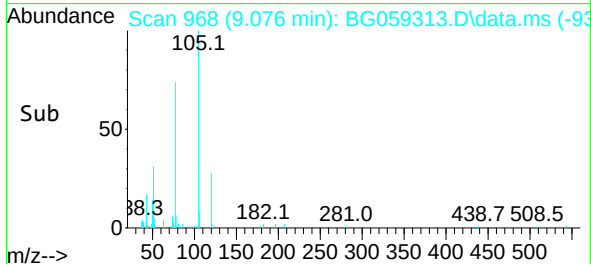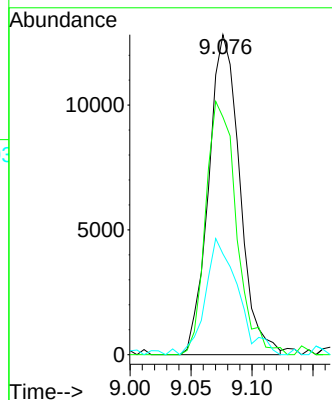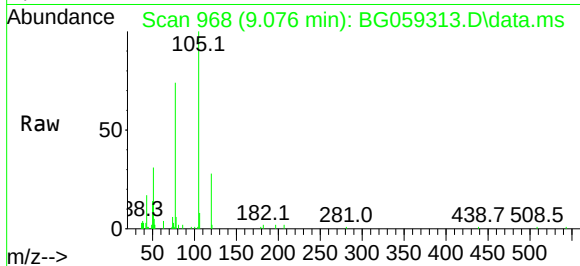

#86
Bis(2-ethylhexyl)phthalate
Concen: 3.485 ng/ul
RT: 21.726 min Scan# 3121
Delta R.T. -0.013 min
Lab File: BG059313.D
Acq: 6 Oct 2023 2:19

Tgt Ion:149 Resp: 40659
Ion Ratio Lower Upper
149 100
167 22.0 19.1 28.7
279 3.4 2.9 4.3

