

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
 Data File : BG059289.D
 Acq On : 5 Oct 2023 9:54
 Operator : MA/JU
 Sample : PB155951BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK951

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059289.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.530	19	24	29	rBB3	12243	19143	1.62%	0.155%
2	3.959	92	97	110	rBV	168945	288721	24.42%	2.342%
3	4.294	151	154	162	rVB2	12513	20191	1.71%	0.164%
4	4.722	224	227	229	rBV2	1499	2096	0.18%	0.017%
5	5.040	279	281	284	rBV2	1723	1631	0.14%	0.013%
6	5.081	284	288	290	rBV2	1726	1921	0.16%	0.016%
7	5.463	350	353	357	rVB2	1333	1635	0.14%	0.013%
8	5.698	391	393	395	rBV	2751	2505	0.21%	0.020%
9	6.338	500	502	505	rVB	1574	1599	0.14%	0.013%
10	6.385	505	510	511	rBV2	1741	1699	0.14%	0.014%
11	6.420	514	516	518	rBV	1744	1723	0.15%	0.014%
12	6.914	597	600	602	rBV2	1568	1817	0.15%	0.015%
13	7.355	668	675	687	rBV	188808	323796	27.38%	2.626%
14	7.549	698	708	718	rBV	144367	248562	21.02%	2.016%
15	7.742	735	741	751	rBV	173846	305118	25.80%	2.475%
16	8.224	816	823	832	rBV	126441	223723	18.92%	1.815%
17	8.923	935	942	951	rBV	227862	393424	33.27%	3.191%
18	9.423	1020	1027	1034	rBV	177993	313183	26.49%	2.540%
19	10.146	1142	1150	1157	rBV	141247	254968	21.56%	2.068%
20	10.674	1231	1240	1249	rBV	207872	392272	33.17%	3.182%
21	10.804	1258	1262	1265	rVB	1488	1843	0.16%	0.015%
22	11.068	1299	1307	1321	rVB	201293	362139	30.63%	2.937%
23	11.215	1321	1332	1340	rBV	241674	426440	36.06%	3.459%
24	11.526	1380	1385	1388	rBV	1358	1630	0.14%	0.013%
25	12.184	1492	1497	1500	rBV	1273	1874	0.16%	0.015%
26	12.631	1569	1573	1578	rVB	4361	5619	0.48%	0.046%
27	13.683	1750	1752	1754	rBV	4540	5327	0.45%	0.043%
28	13.935	1793	1795	1800	rVB	1180	1765	0.15%	0.014%
29	14.258	1841	1850	1858	rBV	442620	599531	50.70%	4.863%
30	14.564	1895	1902	1910	rBV	479915	760603	64.32%	6.170%
31	14.864	1946	1953	1960	rBV	338790	506052	42.80%	4.105%
32	15.052	1978	1985	1997	rBV	174991	286446	24.22%	2.323%
33	15.234	2012	2016	2018	rBV	2026	1709	0.14%	0.014%
34	15.422	2044	2048	2049	rBV	1728	1945	0.16%	0.016%
35	15.851	2114	2121	2127	rBV	615470	918197	77.65%	7.448%
36	15.956	2134	2139	2146	rBV	151355	228079	19.29%	1.850%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
 Data File : BG059289.D
 Acq On : 5 Oct 2023 9:54
 Operator : MA/JU
 Sample : PB155951BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK951

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

37	16.086	2157	2161	2165	rVB2	2613	4208	0.36%	0.034%
38	16.162	2173	2174	2178	rVB2	1685	1679	0.14%	0.014%
39	16.215	2178	2183	2186	rBV	1257	1830	0.15%	0.015%
40	16.468	2220	2226	2227	rVB	1602	1884	0.16%	0.015%
41	17.290	2362	2366	2369	rVB	1591	2133	0.18%	0.017%
42	17.408	2381	2386	2394	rVB2	2450	3025	0.26%	0.025%
43	17.613	2414	2421	2427	rBV	394964	599661	50.71%	4.864%
44	17.713	2430	2438	2445	rBV2	650243	1005107	85.00%	8.153%
45	17.995	2481	2486	2488	rBV	1482	1744	0.15%	0.014%
46	18.383	2551	2552	2556	rVB	1546	1773	0.15%	0.014%
47	18.536	2575	2578	2580	rBV3	1409	1626	0.14%	0.013%
48	18.706	2602	2607	2609	rBV3	1805	2190	0.19%	0.018%
49	18.953	2647	2649	2651	rBV2	2159	2070	0.18%	0.017%
50	18.994	2654	2656	2658	rBV3	2581	1620	0.14%	0.013%
51	19.247	2697	2699	2702	rBV3	1896	2145	0.18%	0.017%
52	19.358	2716	2718	2719	rBV	2986	1903	0.16%	0.015%
53	19.546	2743	2750	2756	rVB6	9269	15897	1.34%	0.129%
54	19.617	2760	2762	2767	rVB4	6307	7000	0.59%	0.057%
55	19.834	2797	2799	2804	rVB3	2412	3254	0.28%	0.026%
56	19.875	2804	2806	2809	rVB3	3089	3042	0.26%	0.025%
57	19.987	2818	2825	2834	rBV2	818476	1151929	97.42%	9.344%
58	20.187	2856	2859	2862	rBV3	1746	3015	0.25%	0.024%
59	20.240	2866	2868	2870	rBV2	2078	2055	0.17%	0.017%
60	20.428	2894	2900	2901	rBV3	2711	4912	0.42%	0.040%
61	20.498	2910	2912	2914	rBV2	2324	2164	0.18%	0.018%
62	20.533	2916	2918	2921	rVV3	2173	2375	0.20%	0.019%
63	20.563	2921	2923	2926	rBV4	3492	2392	0.20%	0.019%
64	20.786	2959	2961	2962	rBV2	2949	2292	0.19%	0.019%
65	20.821	2965	2967	2970	rVB3	3326	2594	0.22%	0.021%
66	21.274	3042	3044	3049	rBV5	3197	2232	0.19%	0.018%
67	21.614	3101	3102	3104	rBV2	3681	2231	0.19%	0.018%
68	21.908	3145	3152	3162	rBV2	380900	656939	55.56%	5.329%
69	22.502	3251	3253	3254	rBV2	4135	2320	0.20%	0.019%
70	23.495	3420	3422	3424	rBV2	4159	2675	0.23%	0.022%
71	24.029	3511	3513	3514	rBV2	4030	2431	0.21%	0.020%
72	25.146	3692	3703	3714	rBV4	395911	1182458	100.00%	9.591%
73	25.386	3734	3744	3756	rVB3	235197	703964	59.53%	5.710%
74	25.792	3811	3813	3814	rVB2	4695	1902	0.16%	0.015%
75	26.379	3911	3913	3915	rVB3	4789	2508	0.21%	0.020%
76	27.255	4060	4062	4064	rBV3	3994	3057	0.26%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
Data File : BG059289.D
Acq On : 5 Oct 2023 9:54
Operator : MA/JU
Sample : PB155951BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK951

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Title : SVOA CALIBRATION

77	27.402	4085	4087	4089	rBV3	3994	3318	0.28%	0.027%
78	28.806	4324	4326	4329	rBV4	4018	3666	0.31%	0.030%
79	28.894	4340	4341	4344	rBV3	4315	3740	0.32%	0.030%
80	29.035	4363	4365	4366	rVB2	4588	2378	0.20%	0.019%
81	30.686	4642	4646	4647	rBV3	4375	3709	0.31%	0.030%
82	30.927	4685	4687	4688	rVB	5126	2366	0.20%	0.019%




Sum of corrected areas: 12328339

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
Data File : BG059289.D
Acq On : 5 Oct 2023 9:54
Operator : MA/JU
Sample : PB155951BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK951

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

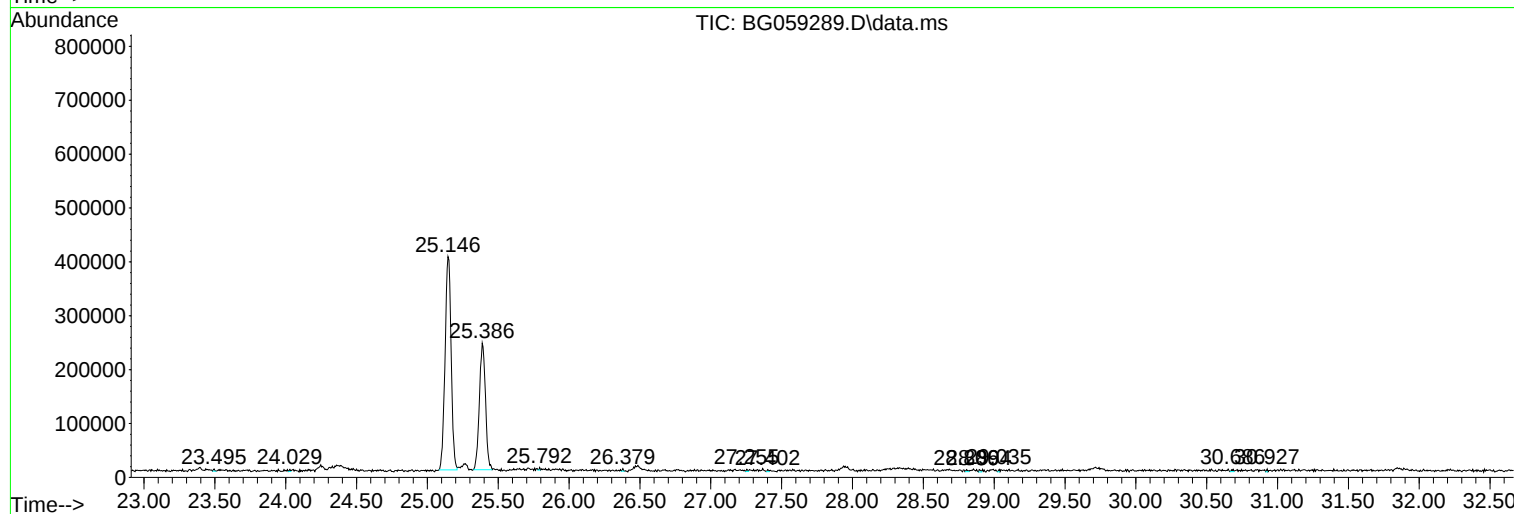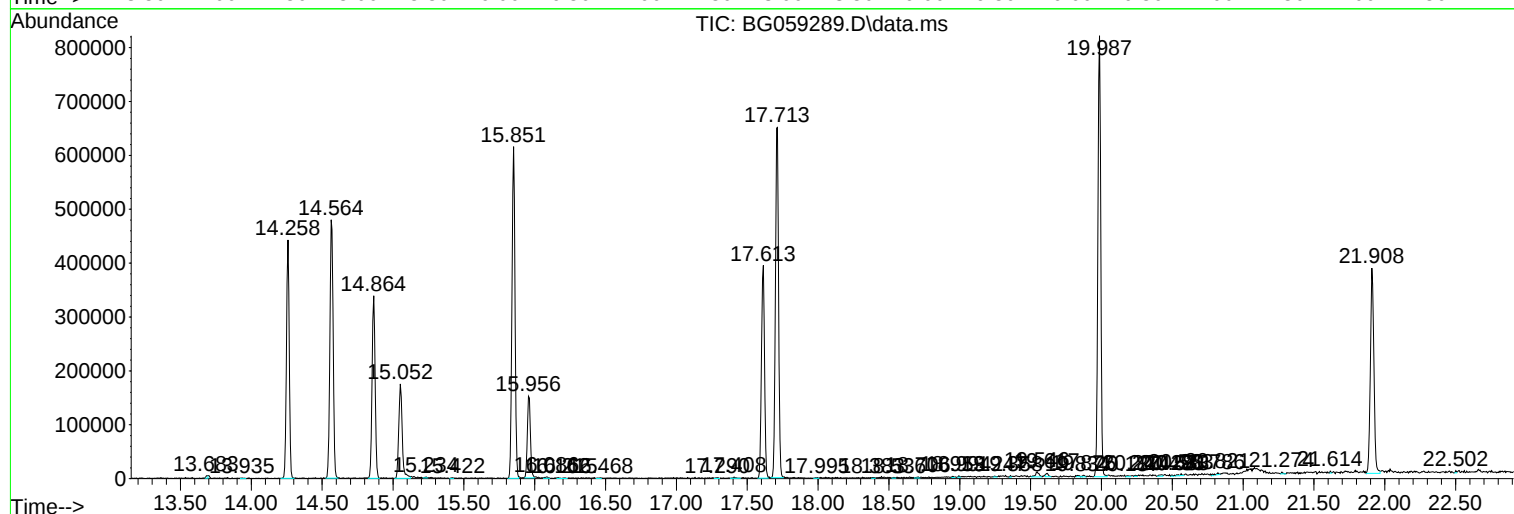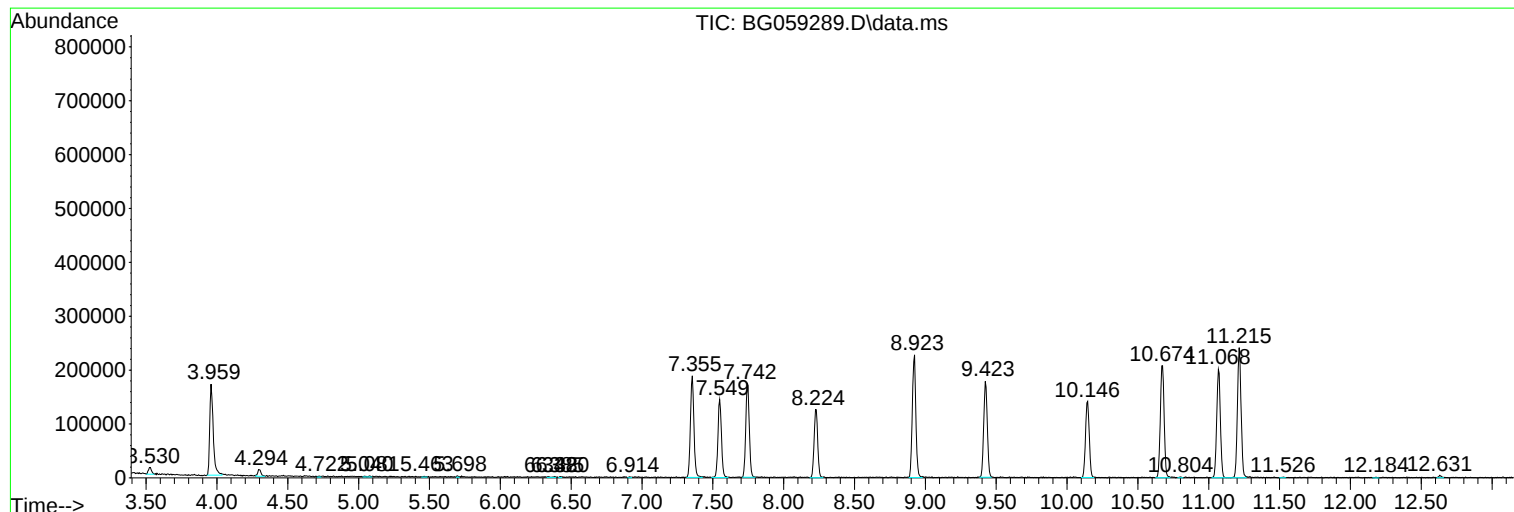

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
Data File : BG059289.D
Acq On : 5 Oct 2023 9:54
Operator : MA/JU
Sample : PB155951BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK951

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
Data File : BG059289.D
Acq On : 5 Oct 2023 9:54
Operator : MA/JU
Sample : PB155951BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK951

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc