

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
 Data File : BG059325.D
 Acq On : 6 Oct 2023 11:14
 Operator : MA/JU
 Sample : 04592-05 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EZYY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.529	21	24	29	rVB5	8378	13354	0.76%	0.076%
2	3.888	81	85	91	rVB3	14426	23087	1.31%	0.131%
3	3.970	94	99	109	rBV	89936	158901	8.99%	0.899%
4	4.111	120	123	125	rBV4	3580	4580	0.26%	0.026%
5	4.158	128	131	132	rBV2	6059	5848	0.33%	0.033%
6	4.299	152	155	159	rBV2	6306	7452	0.42%	0.042%
7	4.563	197	200	205	rVB	9855	14218	0.80%	0.080%
8	4.645	210	214	216	rBV3	3008	3606	0.20%	0.020%
9	4.869	247	252	254	rBV2	2384	4375	0.25%	0.025%
10	5.063	283	285	288	rVB3	4985	4500	0.25%	0.025%
11	5.104	288	292	295	rBV3	4007	7009	0.40%	0.040%
12	5.133	295	297	301	rVB4	2789	3467	0.20%	0.020%
13	5.721	393	397	400	rBV4	2744	4533	0.26%	0.026%
14	5.797	405	410	411	rBV3	3531	4207	0.24%	0.024%
15	7.049	621	623	629	rVB4	3155	3972	0.22%	0.022%
16	7.160	635	642	647	rBV6	6643	14990	0.85%	0.085%
17	7.360	669	676	687	rVB	69726	131583	7.44%	0.745%
18	7.477	694	696	700	rVB3	2464	3546	0.20%	0.020%
19	7.554	702	709	717	rVB	233625	392500	22.21%	2.221%
20	7.748	736	742	753	rBV	237086	417370	23.61%	2.362%
21	7.824	753	755	758	rVV3	5250	5800	0.33%	0.033%
22	7.848	758	759	762	rVB2	5251	4427	0.25%	0.025%
23	8.094	796	801	803	rBV	2865	4259	0.24%	0.024%
24	8.229	818	824	836	rVB	208587	371257	21.01%	2.101%
25	8.564	876	881	882	rBV3	3239	3779	0.21%	0.021%
26	8.829	924	926	931	rBV2	2688	4598	0.26%	0.026%
27	8.923	936	942	951	rVV	190952	326066	18.45%	1.845%
28	9.005	954	956	960	rVB	3546	3879	0.22%	0.022%
29	9.076	963	968	975	rVB4	10566	20690	1.17%	0.117%
30	9.146	977	980	983	rBV3	2384	3913	0.22%	0.022%
31	9.328	1009	1011	1014	rVB3	4625	5682	0.32%	0.032%
32	9.428	1018	1028	1039	rBV	284805	516704	29.23%	2.924%
33	9.534	1045	1046	1051	rVB2	2715	3319	0.19%	0.019%
34	9.581	1051	1054	1059	rBV2	4251	5719	0.32%	0.032%
35	9.904	1105	1109	1115	rVB5	4002	7705	0.44%	0.044%
36	10.027	1128	1130	1133	rBV5	3683	4499	0.25%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
 Data File : BG059325.D
 Acq On : 6 Oct 2023 11:14
 Operator : MA/JU
 Sample : 04592-05 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EZYY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

37	10.145	1140	1150	1161	rBV	239221	439738	24.88%	2.488%
38	10.251	1164	1168	1170	rVB	4219	5042	0.29%	0.029%
39	10.280	1170	1173	1175	rBV	2673	3462	0.20%	0.020%
40	10.304	1175	1177	1178	rBV2	5134	3525	0.20%	0.020%

41	10.433	1195	1199	1203	rVB5	4671	6066	0.34%	0.034%
42	10.515	1208	1213	1219	rBV5	12878	21362	1.21%	0.121%
43	10.627	1227	1232	1234	rBV2	10931	14735	0.83%	0.083%
44	10.674	1234	1240	1248	rVB	324331	586629	33.19%	3.320%
45	10.821	1264	1265	1270	rVB4	3950	3463	0.20%	0.020%

46	11.073	1299	1308	1315	rBV	306591	551681	31.21%	3.122%
47	11.220	1324	1333	1340	rBV	338000	615760	34.84%	3.484%
48	11.537	1381	1387	1392	rBV2	35389	58197	3.29%	0.329%
49	11.596	1392	1397	1409	rVB2	46362	80972	4.58%	0.458%
50	11.743	1420	1422	1427	rVB4	2711	3282	0.19%	0.019%

51	11.802	1430	1432	1434	rVB2	3570	3425	0.19%	0.019%
52	11.872	1441	1444	1448	rVB3	4750	7834	0.44%	0.044%
53	11.925	1448	1453	1455	rBV2	2916	5403	0.31%	0.031%
54	12.366	1525	1528	1530	rBV3	4236	4519	0.26%	0.026%
55	12.513	1547	1553	1555	rBV3	2225	3909	0.22%	0.022%

56	12.636	1571	1574	1578	rVB2	6435	7392	0.42%	0.042%
57	12.765	1592	1596	1598	rBV3	3154	4452	0.25%	0.025%
58	12.859	1608	1612	1613	rBV2	3711	4194	0.24%	0.024%
59	12.877	1613	1615	1617	rVB2	3936	3124	0.18%	0.018%
60	13.582	1731	1735	1736	rBV	3271	3544	0.20%	0.020%

61	13.694	1748	1754	1758	rVB2	21233	32992	1.87%	0.187%
62	13.799	1767	1772	1774	rBV3	5561	7468	0.42%	0.042%
63	13.982	1799	1803	1804	rBV	2217	3196	0.18%	0.018%
64	14.258	1843	1850	1857	rBV	601673	854766	48.36%	4.837%
65	14.569	1895	1903	1911	rBV2	731967	1148199	64.96%	6.497%

66	14.722	1925	1929	1933	rBV2	7320	8807	0.50%	0.050%
67	14.798	1940	1942	1946	rVB3	3720	3959	0.22%	0.022%
68	14.863	1946	1953	1960	rBV	463404	721390	40.82%	4.082%
69	15.057	1981	1986	1993	rBV3	45304	86517	4.90%	0.490%
70	15.210	2008	2012	2018	rBV5	11023	17710	1.00%	0.100%

71	15.339	2030	2034	2041	rVB4	3336	6978	0.39%	0.039%
72	15.468	2052	2056	2057	rVV	4272	3824	0.22%	0.022%
73	15.509	2060	2063	2064	rBV2	3060	3169	0.18%	0.018%
74	15.621	2077	2082	2087	rBV2	10491	19843	1.12%	0.112%
75	15.850	2114	2121	2129	rBV	917477	1411357	79.85%	7.986%

76	15.962	2134	2140	2147	rBV	253123	387905	21.95%	2.195%
----	--------	------	------	------	-----	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
 Data File : BG059325.D
 Acq On : 6 Oct 2023 11:14
 Operator : MA/JU
 Sample : 04592-05 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EZYY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
 Title : SVOA CALIBRATION

77	16.620	2249	2252	2253	rBV	3560	3188	0.18%	0.018%
78	16.720	2267	2269	2272	rVB3	3679	4085	0.23%	0.023%
79	16.749	2272	2274	2276	rBV	3505	3871	0.22%	0.022%
80	17.119	2334	2337	2338	rBV	4039	3232	0.18%	0.018%
81	17.278	2360	2364	2365	rBV2	5202	4601	0.26%	0.026%
82	17.613	2414	2421	2429	rBV	555750	861550	48.75%	4.875%
83	17.713	2432	2438	2445	rVV2	1030972	1551160	87.76%	8.778%
84	18.124	2506	2508	2510	rVB2	5932	5093	0.29%	0.029%
85	18.282	2533	2535	2538	rBV2	3241	3494	0.20%	0.020%
86	18.365	2547	2549	2552	rBV4	3972	4890	0.28%	0.028%
87	18.429	2556	2560	2567	rBV2	50975	75054	4.25%	0.425%
88	18.794	2619	2622	2624	rBV3	3952	4022	0.23%	0.023%
89	18.841	2628	2630	2632	rVB3	8723	5914	0.33%	0.033%
90	18.935	2644	2646	2650	rBV6	4106	5164	0.29%	0.029%
91	19.058	2666	2667	2670	rVB3	4732	3156	0.18%	0.018%
92	19.087	2670	2672	2674	rBV3	5526	5412	0.31%	0.031%
93	19.140	2680	2681	2683	rBV3	5191	3945	0.22%	0.022%
94	19.552	2747	2751	2754	rVB5	16966	24210	1.37%	0.137%
95	19.693	2770	2775	2782	rBV5	26457	48387	2.74%	0.274%
96	19.986	2819	2825	2835	rBV	1265951	1767422	100.00%	10.001%
97	20.245	2867	2869	2871	rBV2	7783	7779	0.44%	0.044%
98	21.913	3147	3153	3161	rVB2	536121	897856	50.80%	5.081%
99	25.157	3695	3705	3714	rVB	621610	1722133	97.44%	9.745%
100	25.398	3738	3746	3759	rVB2	335551	980987	55.50%	5.551%




Sum of corrected areas: 17671789

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
Data File : BG059325.D
Acq On : 6 Oct 2023 11:14
Operator : MA/JU
Sample : 04592-05 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EZY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

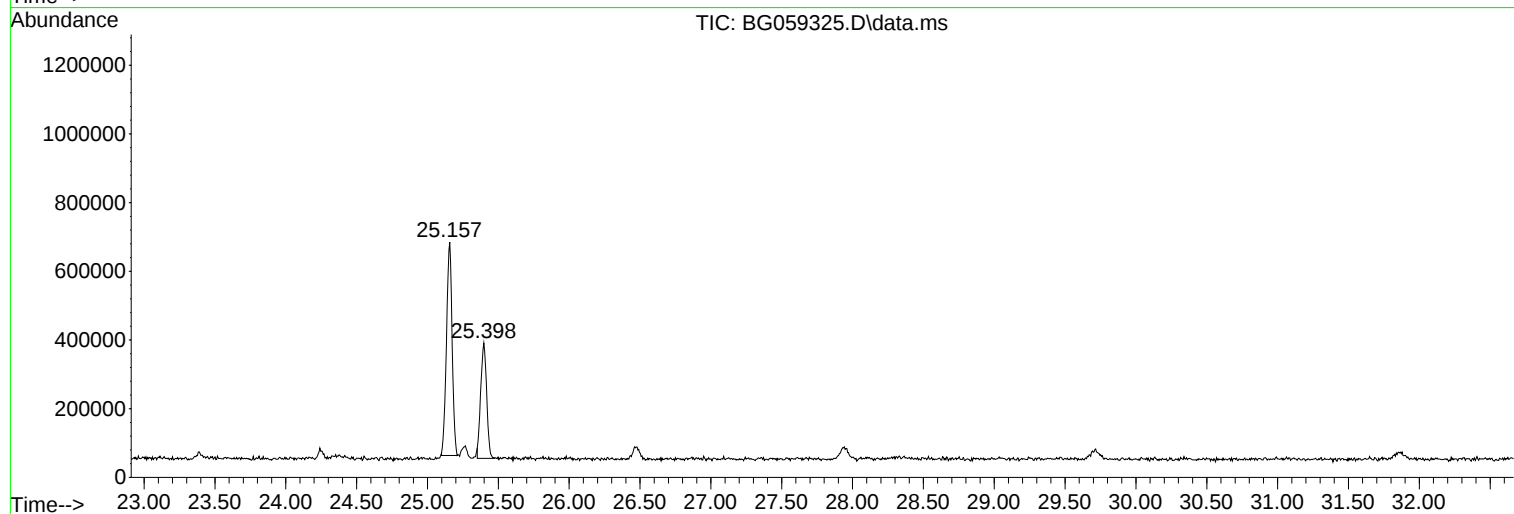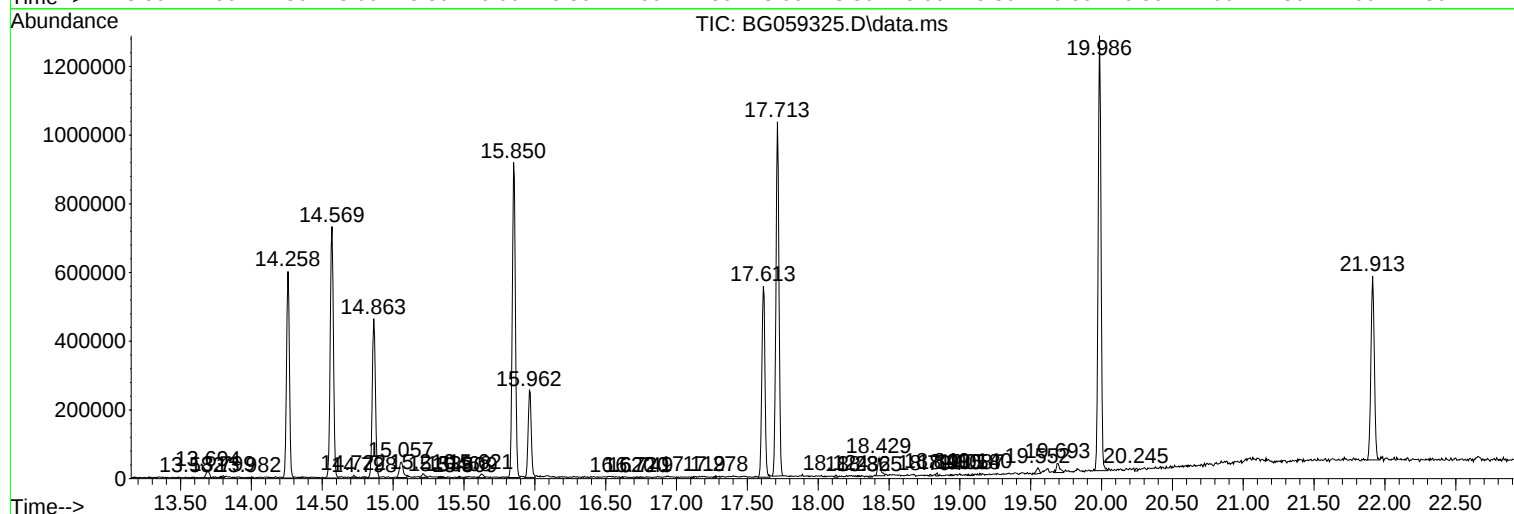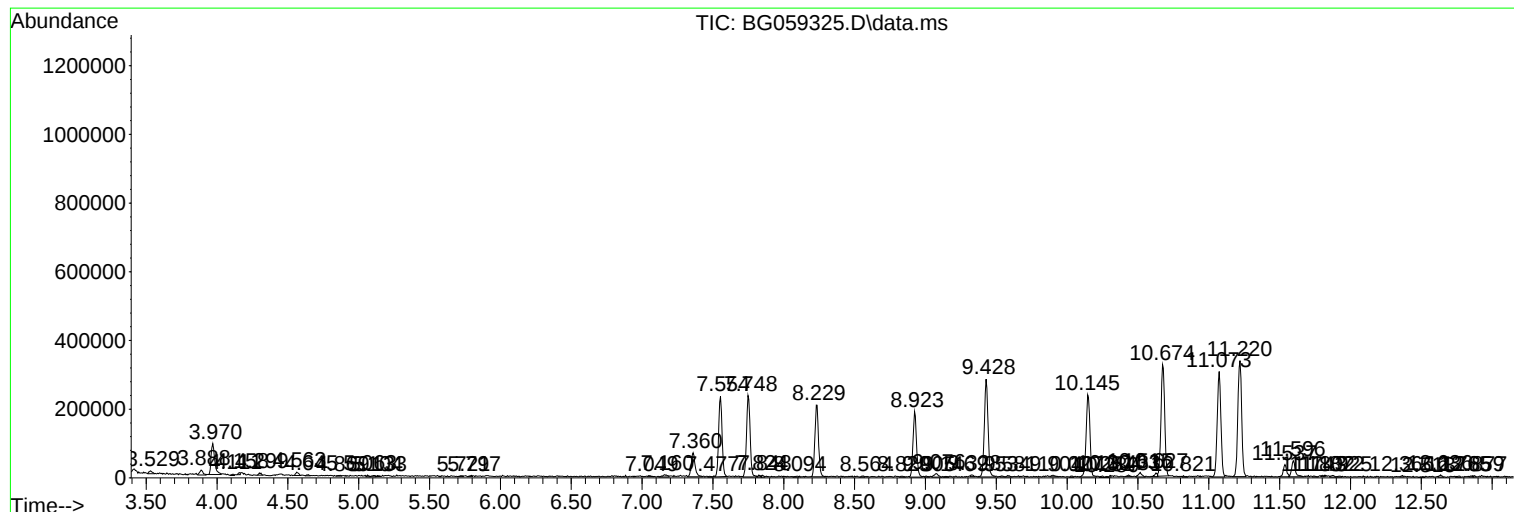

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
Data File : BG059325.D
Acq On : 6 Oct 2023 11:14
Operator : MA/JU
Sample : 04592-05 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EZY3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Methane, diethoxy- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.537	2.11 ng/ul	58197	Naphthalene-d8	11.073

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methane, diethoxy-	104	C5H12O2	000462-95-3	72
2			Dipropylene glycol (isomer 3)	134	C6H14O3	1000506-25-5	64
3			2-Propanol, 1,1'-[(1-methyl-1,2-...	192	C9H20O4	001638-16-0	64
4			1,4,7-Trimethyl-3,6-dioxaoctane-...	192	C9H20O4	1000423-63-2	64
5			2-Propanol, 1-(2-butoxy-1-methyl...	190	C10H22O3	029911-28-2	64

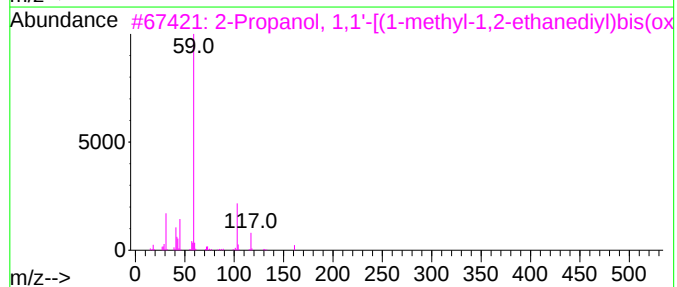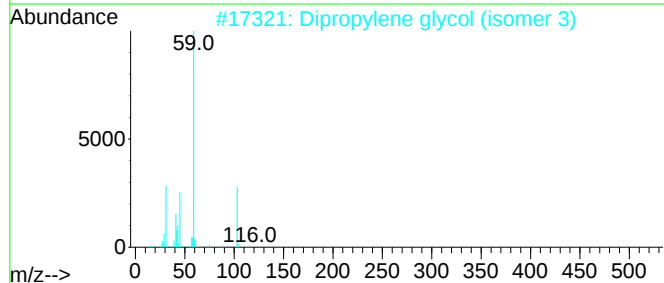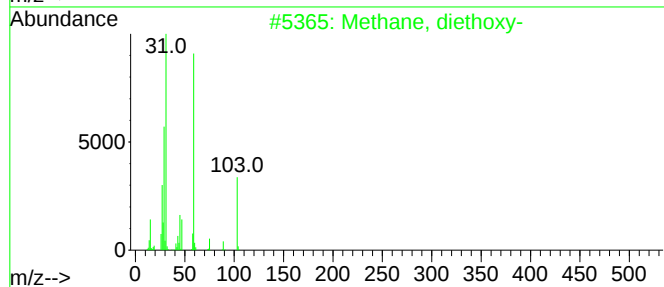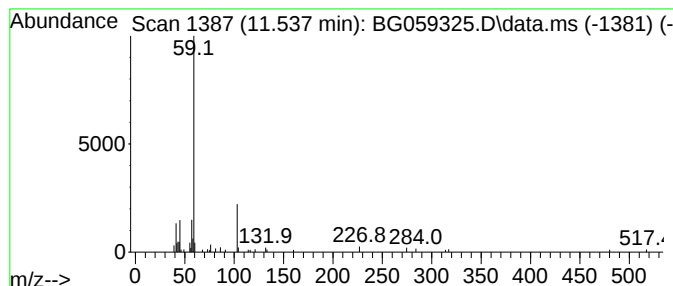

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
Data File : BG059325.D
Acq On : 6 Oct 2023 11:14
Operator : MA/JU
Sample : 04592-05 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EZY3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2,4-Diethyl-6-methyl-1,3,5-... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.596	2.94 ng/ul	80972	Naphthalene-d8	11.073

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2,4-Diethyl-6-methyl-1,3,5-trioxane	160	C8H16O3	117888-04-7	78
2		1-Propanol, 2-(2-hydroxypropoxy)-	134	C6H14O3	000106-62-7	72
3		1-Propanol, 2-(2-hydroxypropoxy)-	134	C6H14O3	000106-62-7	72
4		1-Propanol, 2-(2-hydroxypropoxy)-	134	C6H14O3	000106-62-7	72
5		Dipropylene glycol (isomer 2)	134	C6H14O3	1000506-25-4	72

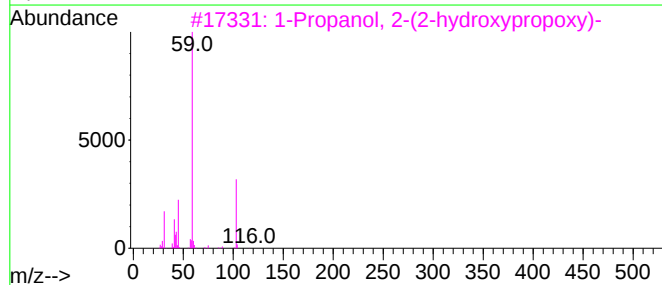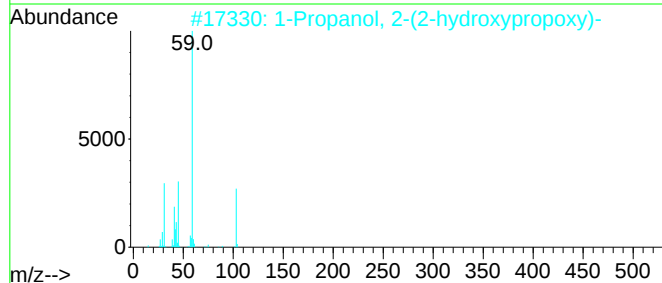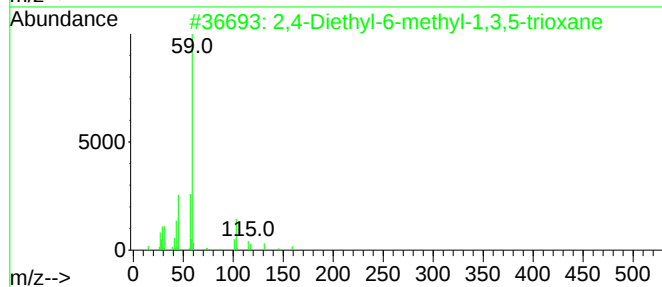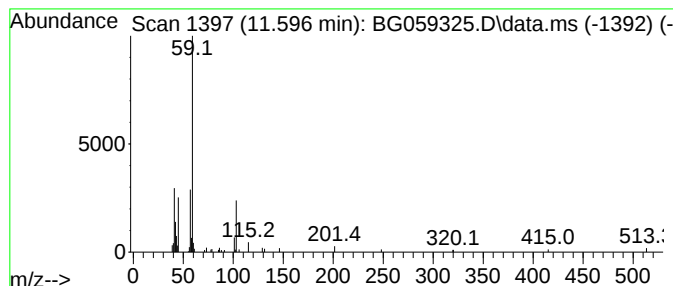

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100523\
Data File : BG059325.D
Acq On : 6 Oct 2023 11:14
Operator : MA/JU
Sample : 04592-05 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EZY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Methane, diethoxy-	11.537	2.1	ng/ul	58197	2	11.073	551681	20.0
2,4-Diethyl-6-m...	11.596	2.9	ng/ul	80972	2	11.073	551681	20.0