
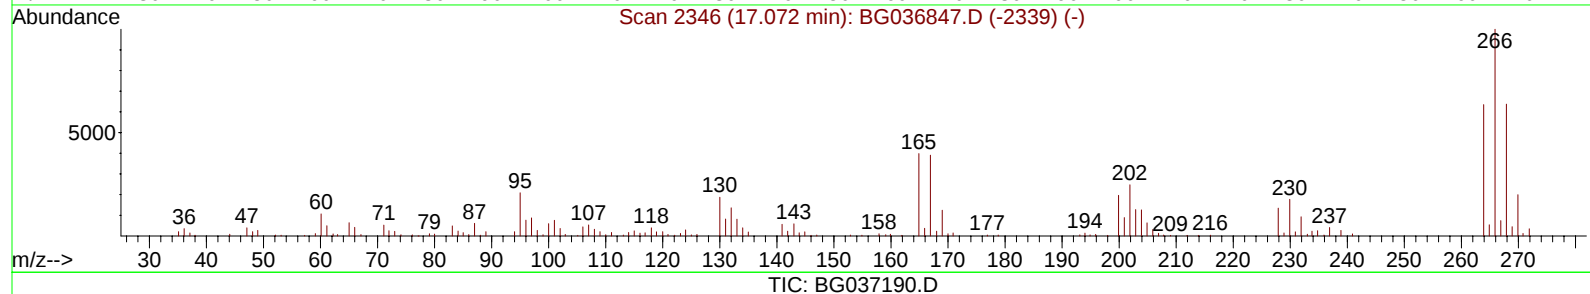
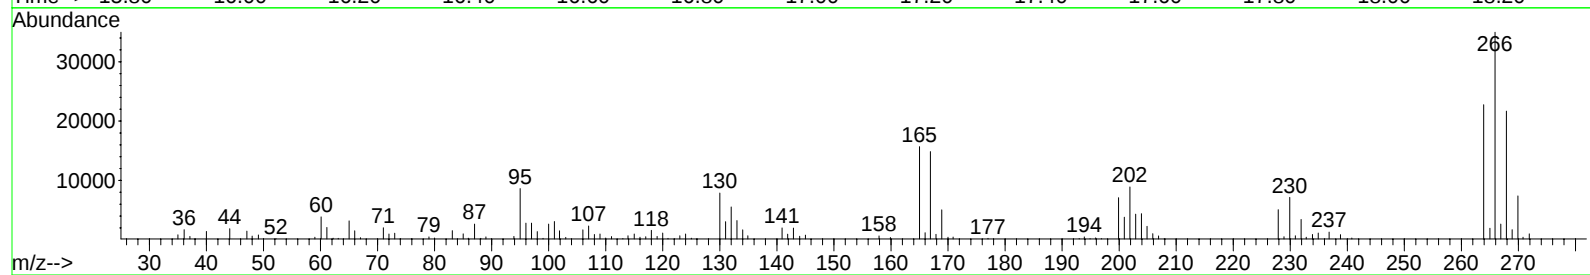


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG100618\
Data File : BG037190.D
Acq On : 5 Oct 2018 15:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 16:09:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

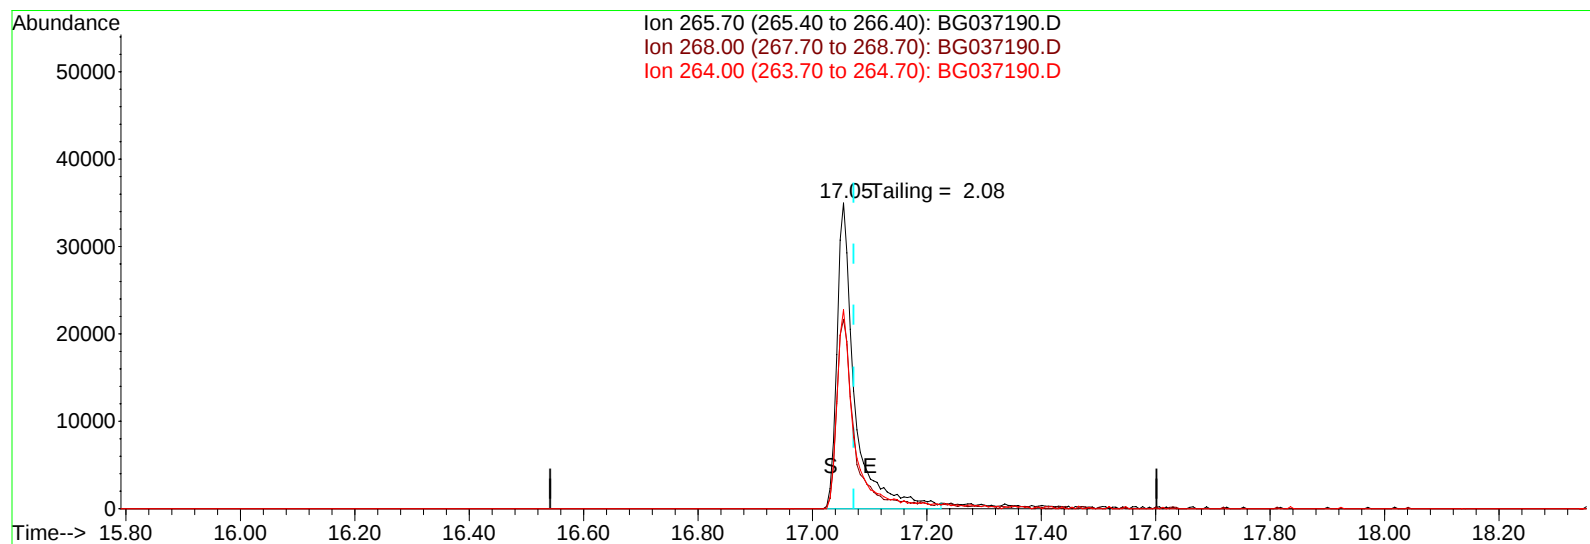

(69) Pentachlorophenol (C)




17.054min (-0.017) 33825.60ng

response 75595

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	61.93
264.00	61.10	65.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG100618\
Data File : BG037190.D
Acq On : 5 Oct 2018 15:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 16:09:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

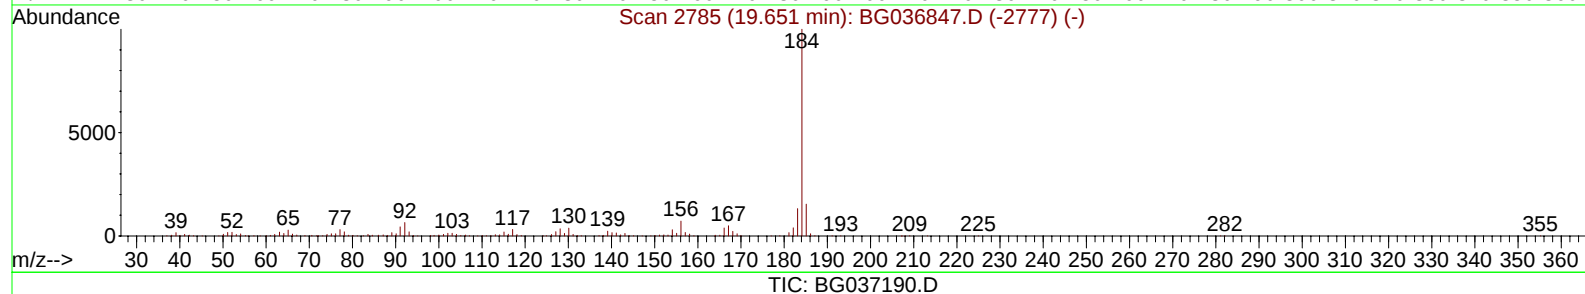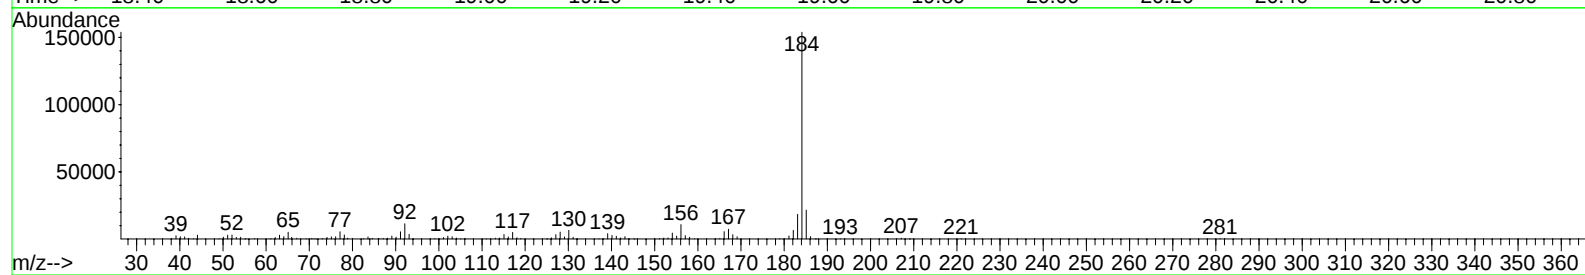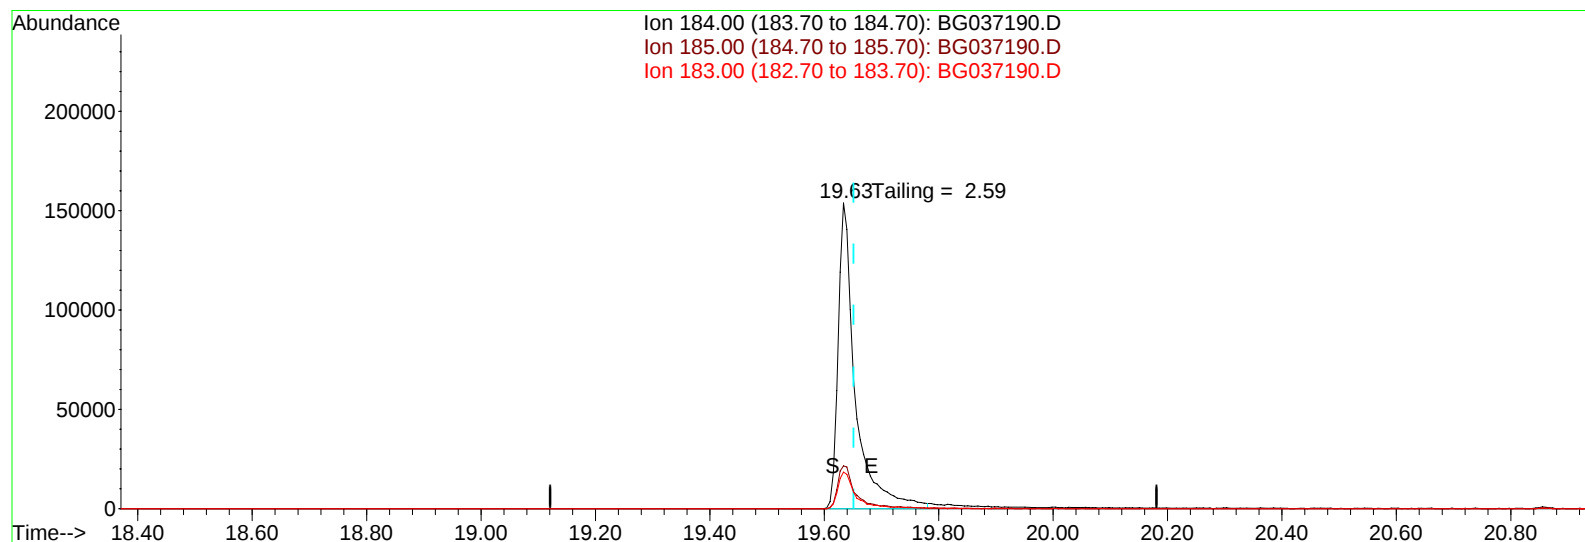

(76) Benzidine

19.634min (-0.017) 18961.98ng

response 325013

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.01
183.00	13.60	11.97
0.00	0.00	0.00