
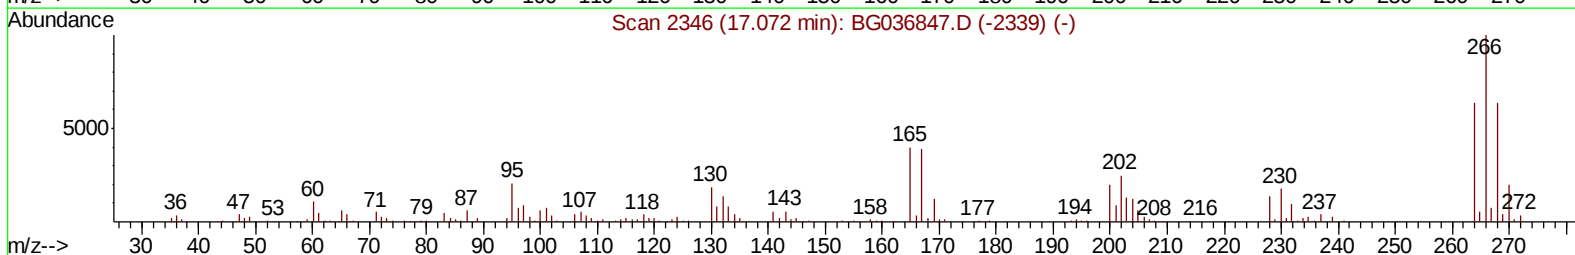
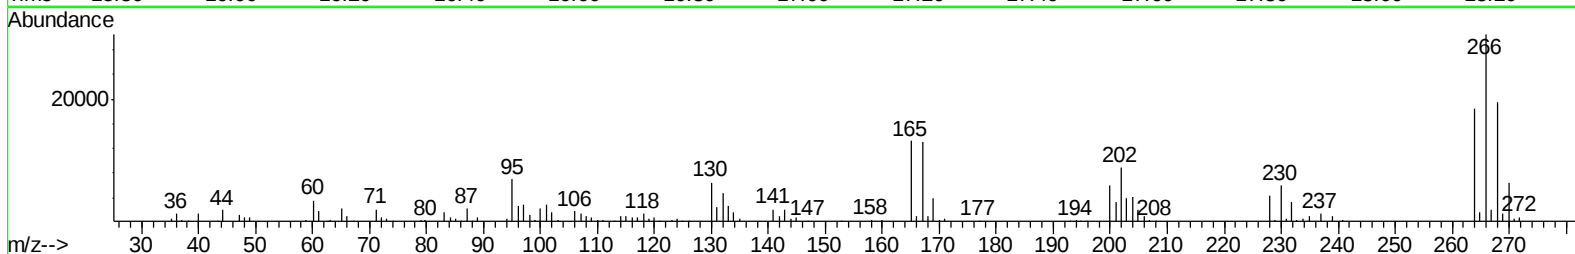


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG100618\
Data File : BG037208.D
Acq On : 6 Oct 2018 11:59
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 05:47:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

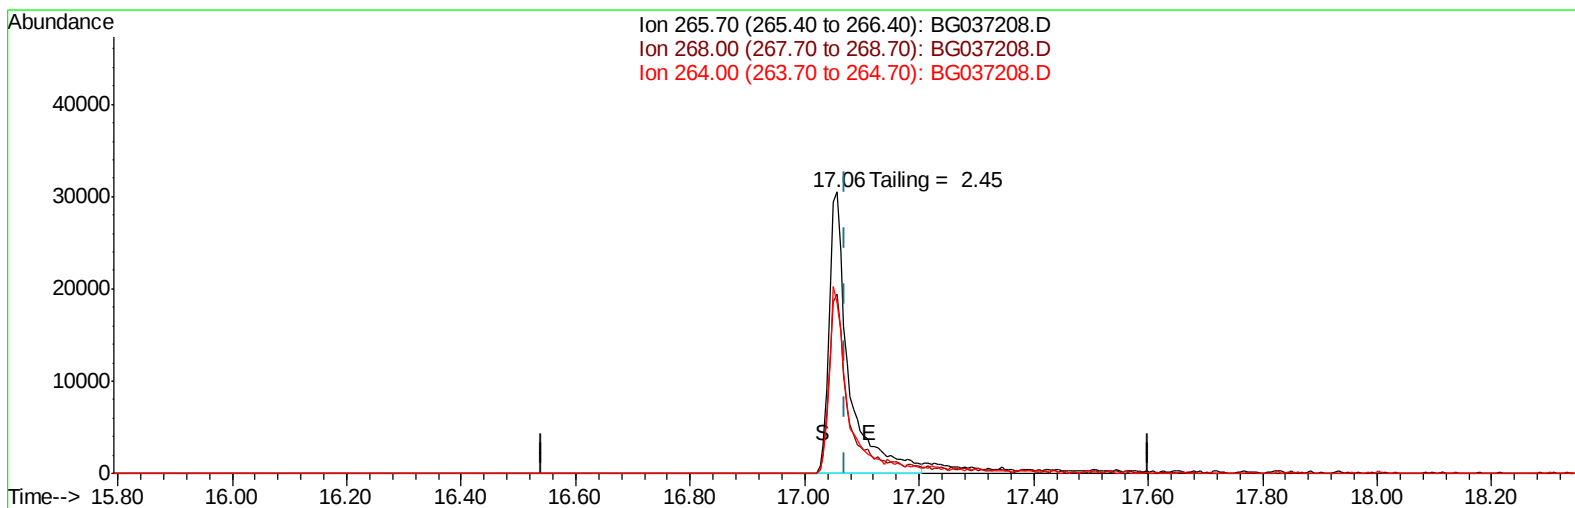

TIC: BG037208.D

(69) Pentachlorophenol (C)




17.056min (-0.015) 33432.26ng

response 73483

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	63.62
264.00	61.10	60.58
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG100618\
Data File : BG037208.D
Acq On : 6 Oct 2018 11:59
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 05:47:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

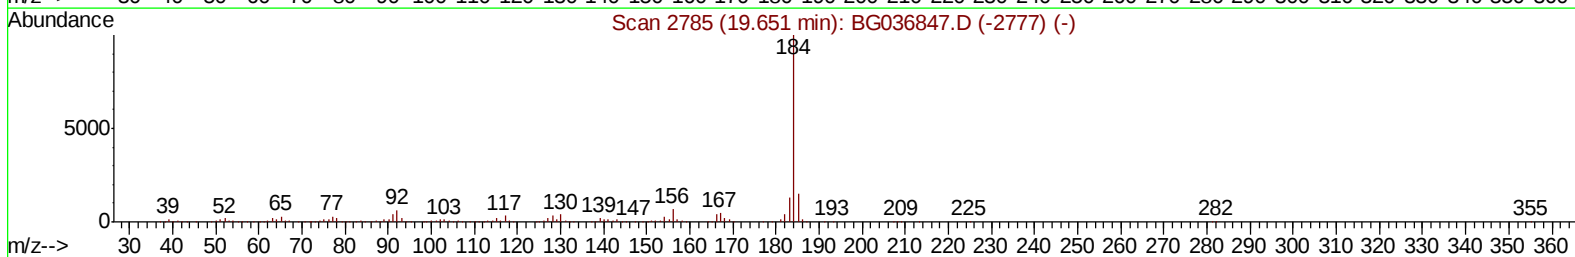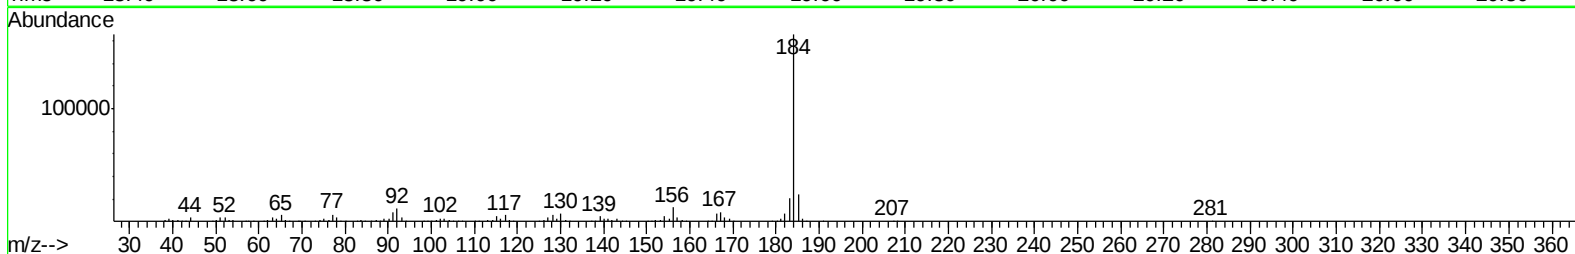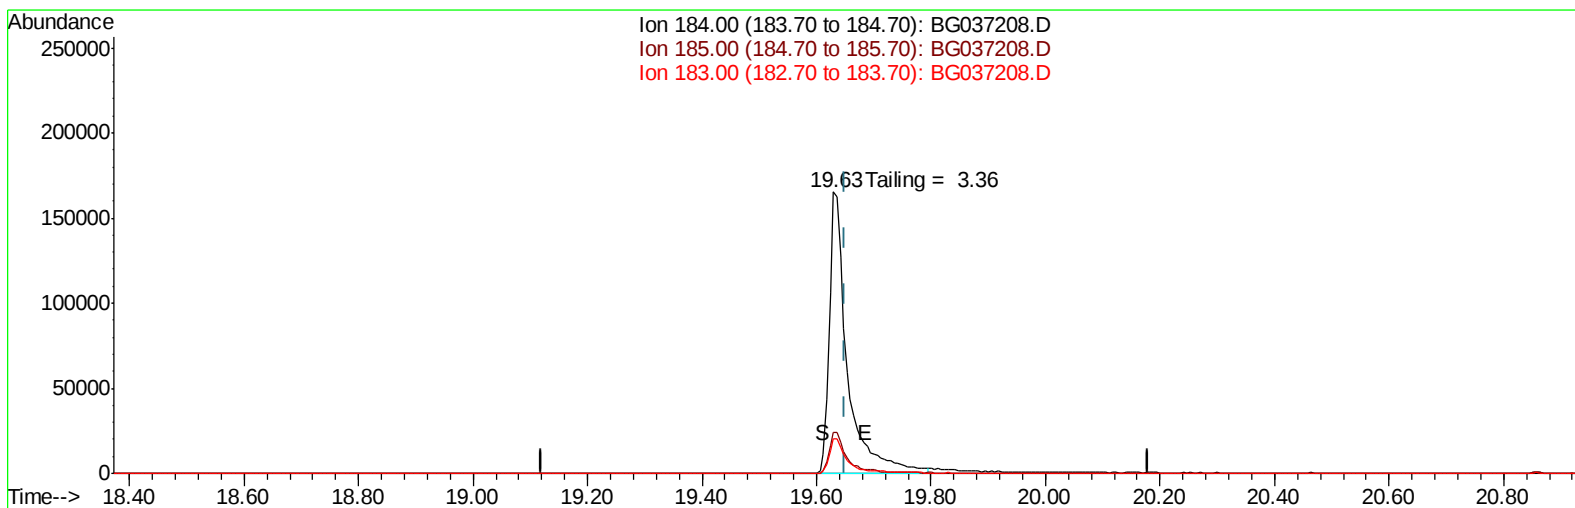

TIC: BG037208.D

(76) Benzidine

19.630min (-0.021) 27007.37ng

response 374739

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.37
183.00	13.60	12.49
0.00	0.00	0.00