


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100618\
 Data File : BG037190.D
 Acq On : 5 Oct 2018 15:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 24 10:41:23 2018

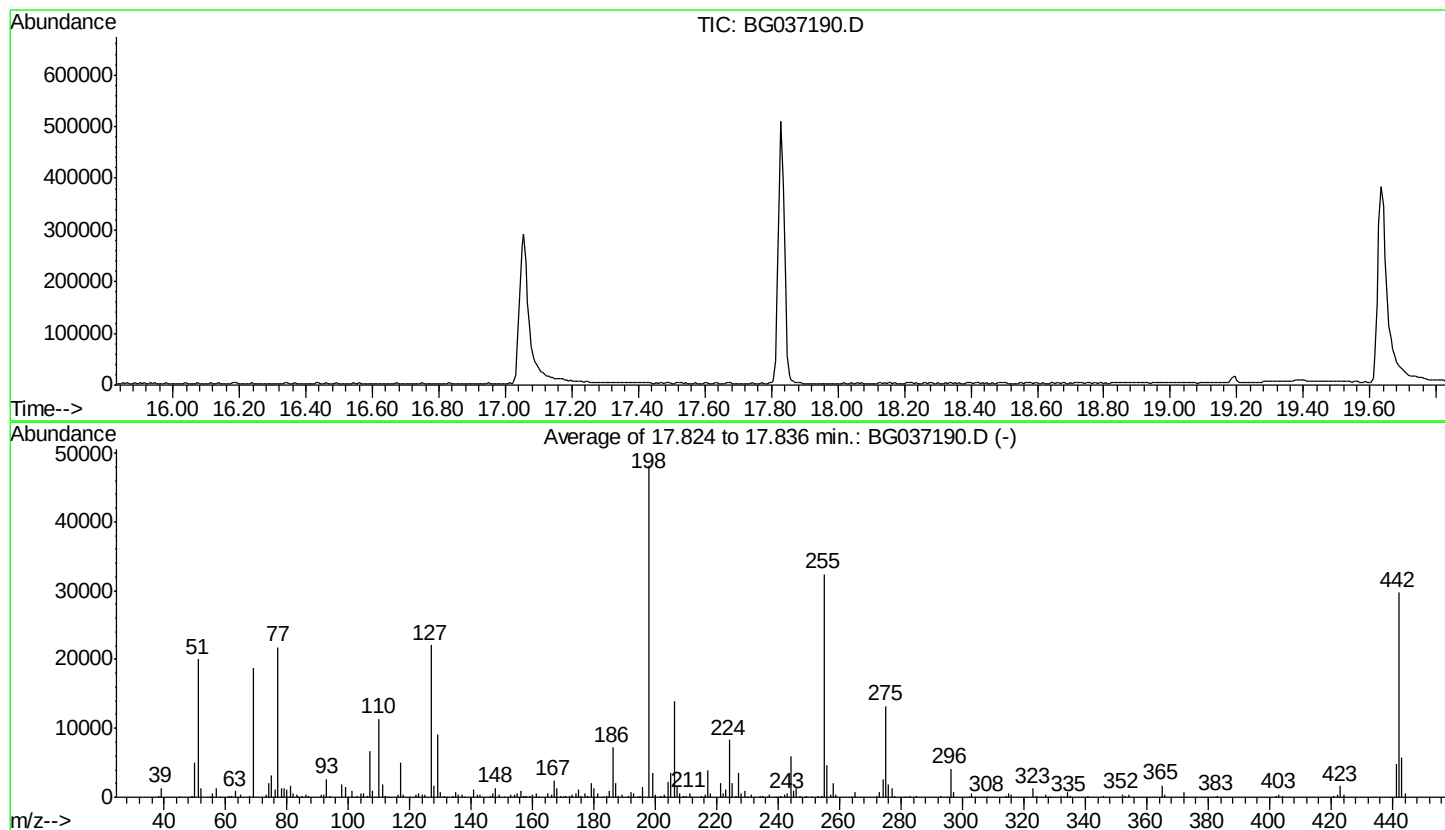

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	20004	PASS
68	69	0.00	2	0.8	155	PASS
69	198	0.00	100	39.0	18795	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.9	22098	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48149	PASS
199	198	5	9	7.4	3578	PASS
275	198	10	60	27.5	13251	PASS
365	198	1	100	3.6	1736	PASS
441	198	0.01	100	10.0	4826	PASS
442	198	50	100	61.7	29720	PASS
443	442	15	24	19.2	5721	PASS