


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG100618\
Data File : BG037208.D
Acq On : 6 Oct 2018 11:59
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 24 10:41:23 2018

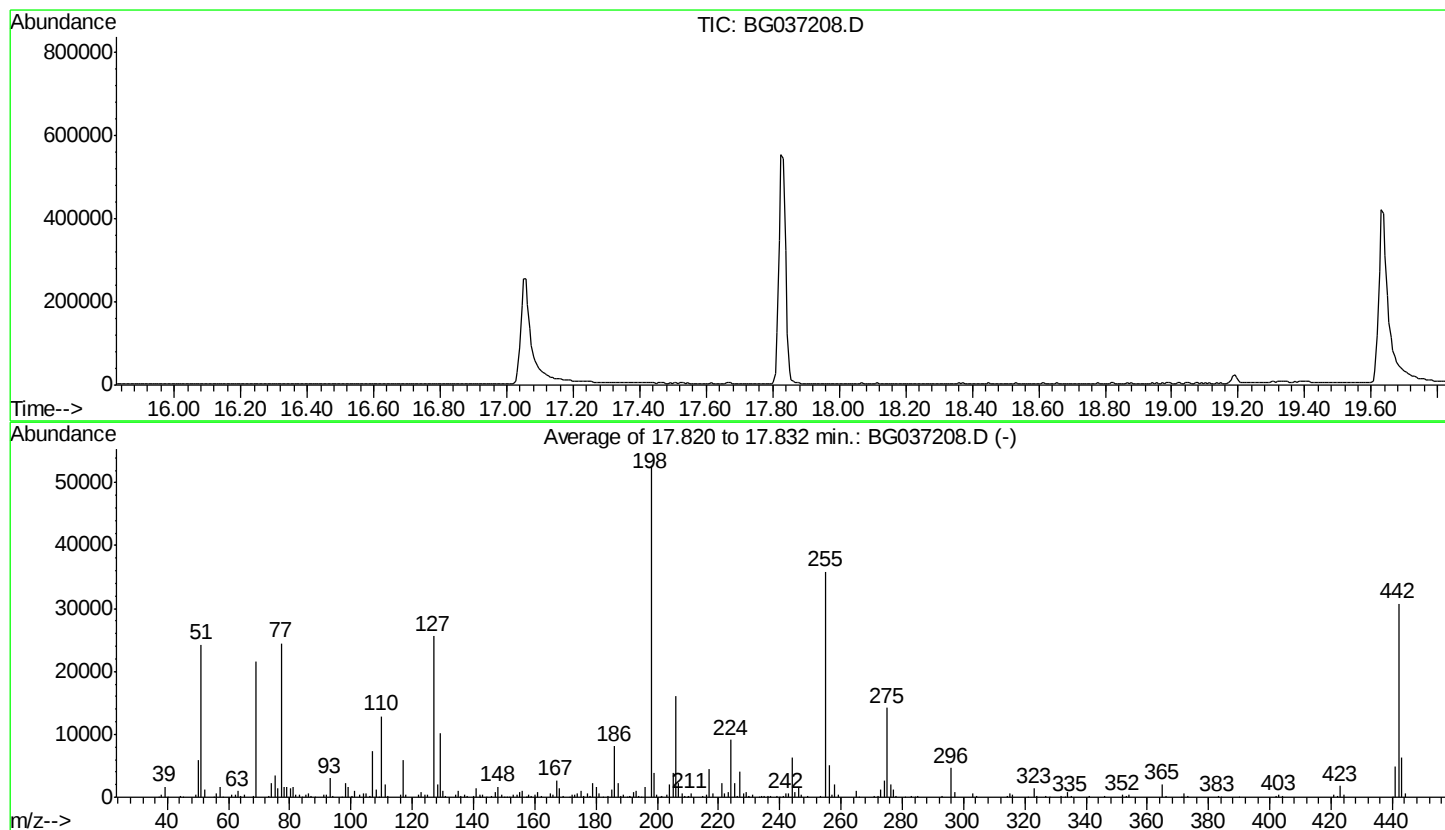

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	24258	PASS
68	69	0.00	2	0.7	150	PASS
69	198	0.00	100	41.1	21645	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	25565	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52725	PASS
199	198	5	9	7.4	3909	PASS
275	198	10	60	27.0	14226	PASS
365	198	1	100	3.7	1970	PASS
441	198	0.01	100	9.4	4972	PASS
442	198	50	100	58.4	30808	PASS
443	442	15	24	20.7	6374	PASS