


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100621\
 Data File : BG050461.D
 Acq On : 6 Oct 2021 10:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 06 15:51:01 2021

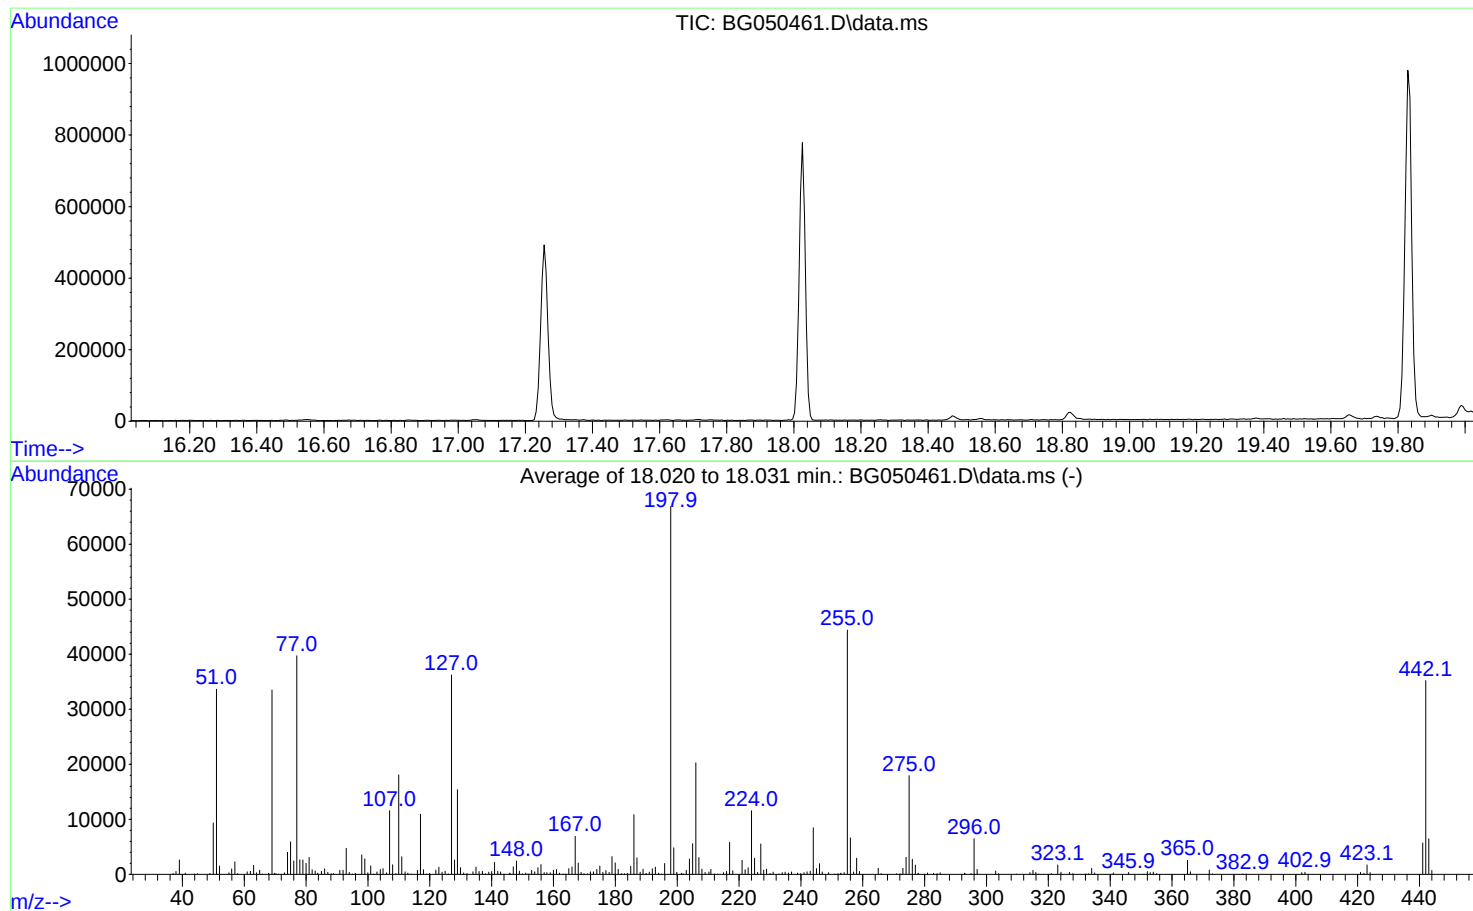




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.3	33653	PASS
68	69	0.00	2	0.6	206	PASS
69	198	0.00	100	50.1	33515	PASS
70	69	0.00	2	0.6	197	PASS
127	198	10	80	54.2	36240	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66851	PASS
199	198	5	9	7.2	4817	PASS
275	198	10	60	26.8	17943	PASS
365	198	1	100	3.8	2564	PASS
441	198	0.01	100	8.5	5711	PASS
442	442	50	100	100.0	35200	PASS
443	442	15	24	18.4	6468	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100621\
Data File : BG050461.D
Acq On : 6 Oct 2021 10:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 06 11:08:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 06 11:08:03 2021
Response via : Initial Calibration

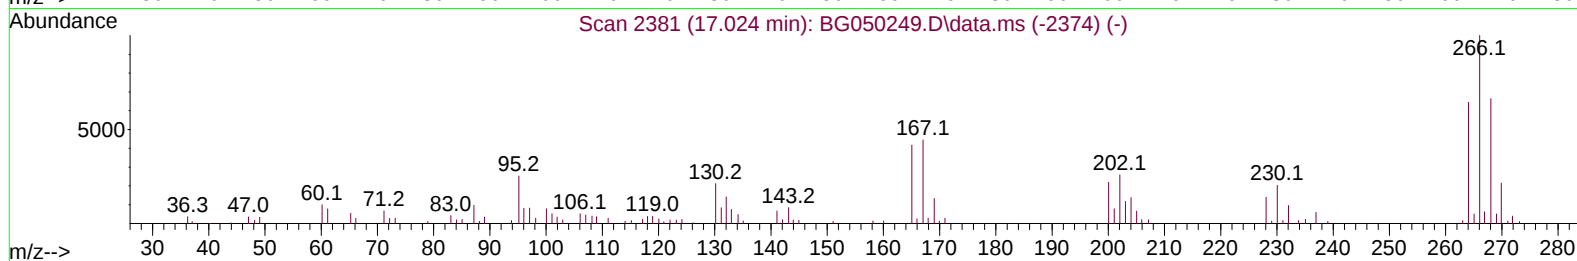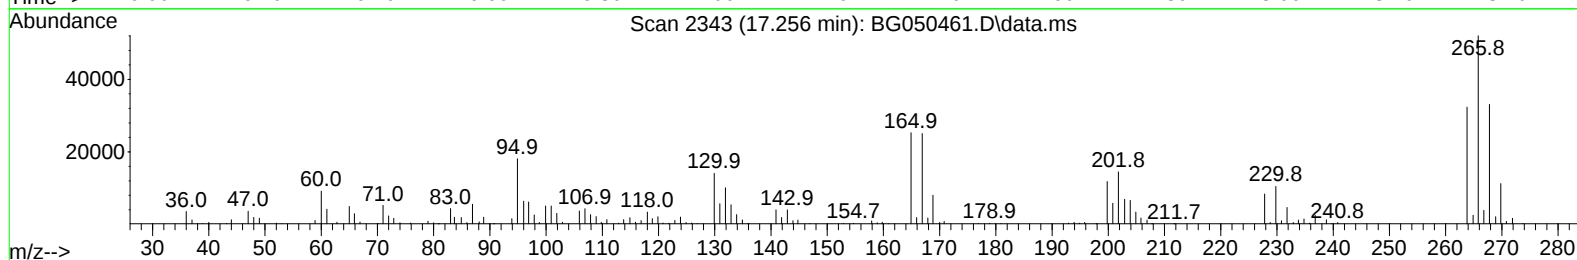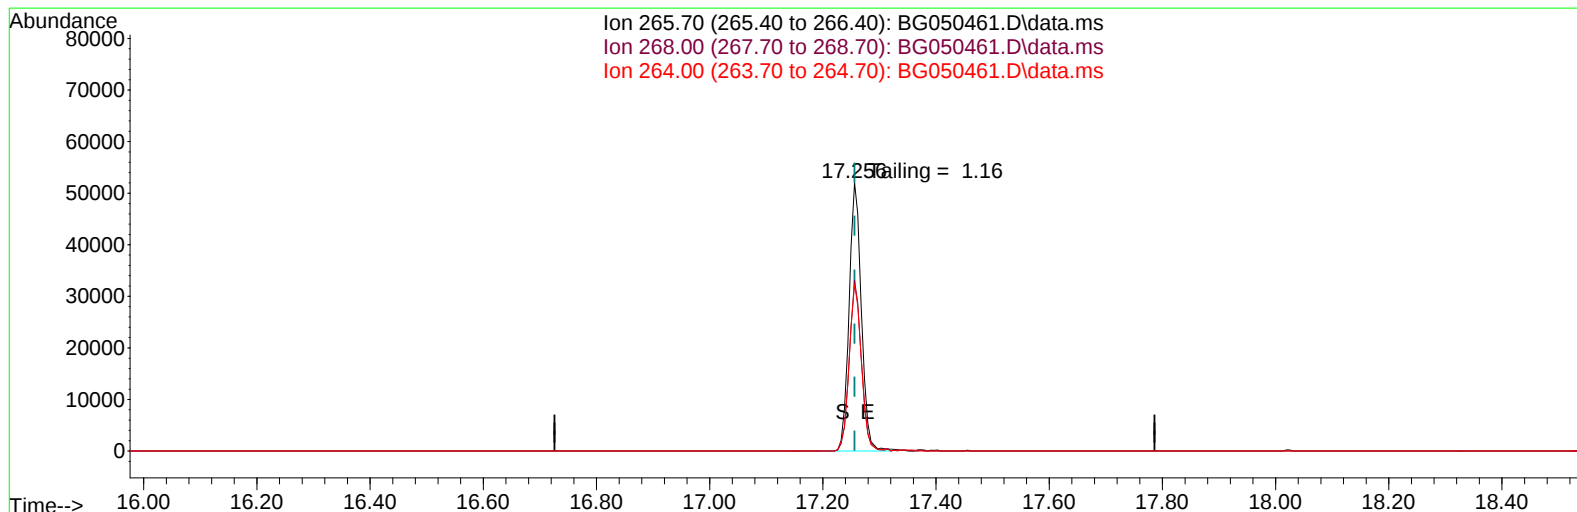

TIC: BG050461.D\data.ms

(70) Pentachlorophenol (C)

17.256min (0.000) 10283.12 ng


response 78356

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.62
264.00	61.30	62.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100621\
Data File : BG050461.D
Acq On : 6 Oct 2021 10:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 06 11:08:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 06 11:08:03 2021
Response via : Initial Calibration

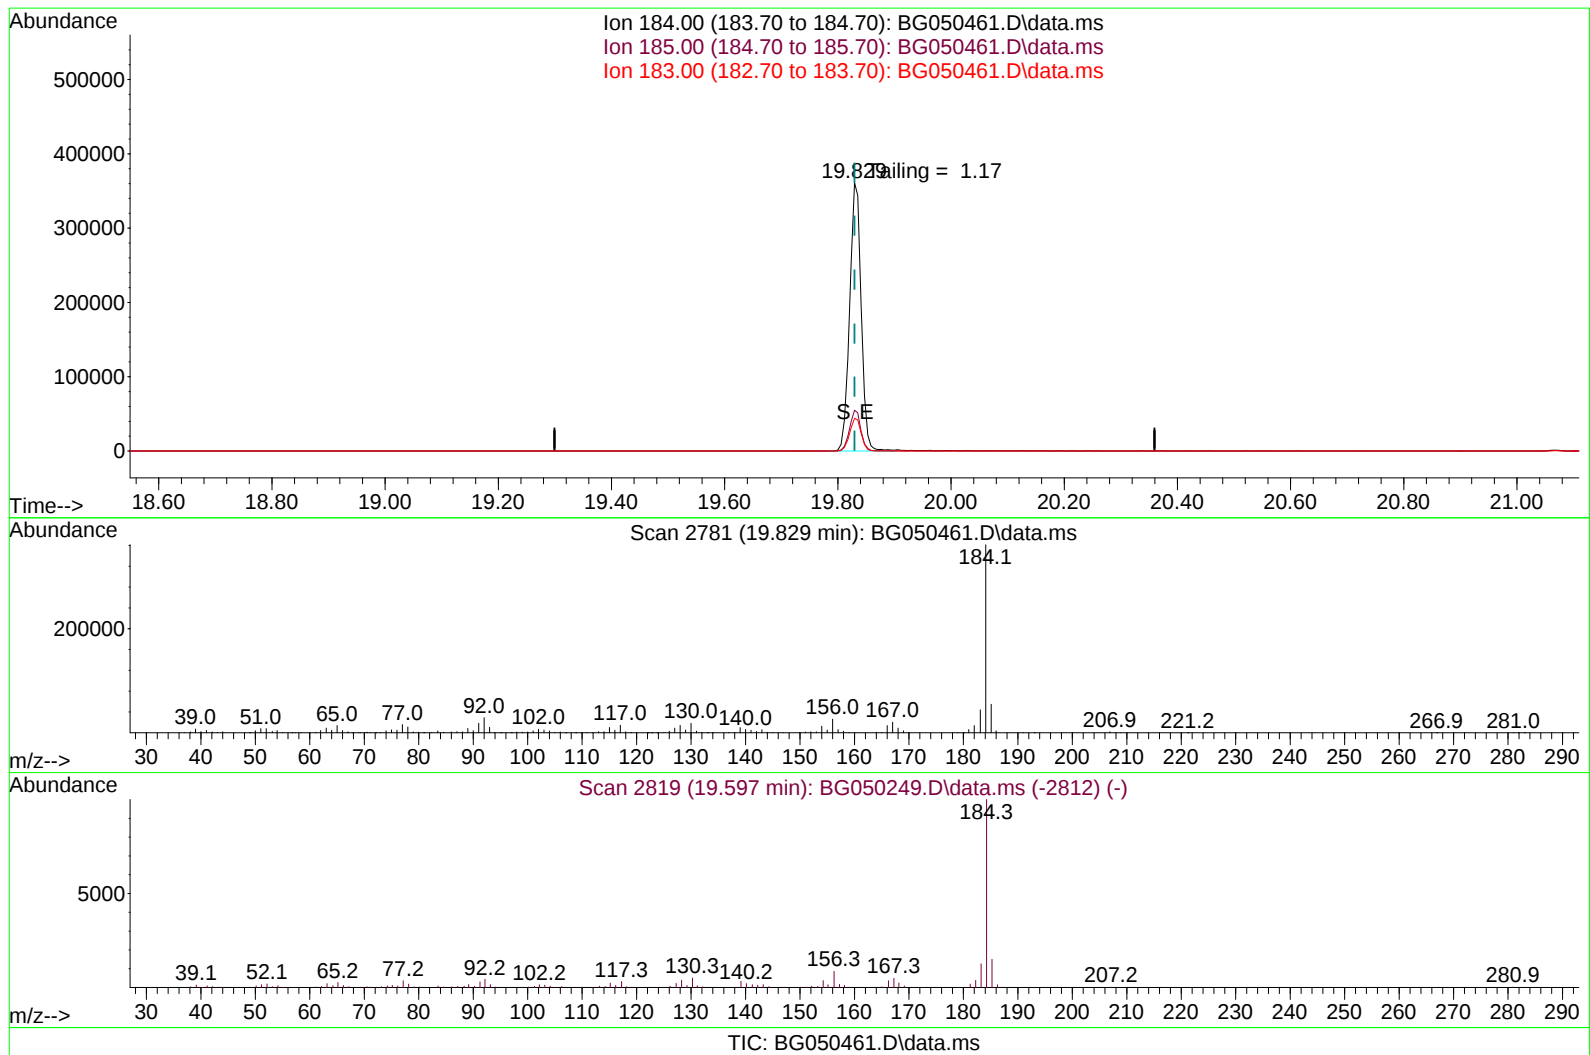

(77) Benzidine

19.829min (0.000) 1171.57 ng

response 510874

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.21
183.00	11.70	12.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/6/2021	BNA_G	BG050461.D
Compound Name	Response	Retention Time
DDT	252553	21.06
DDD	326	20.62
DDE	0	20.23
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
326	252879	0.13