
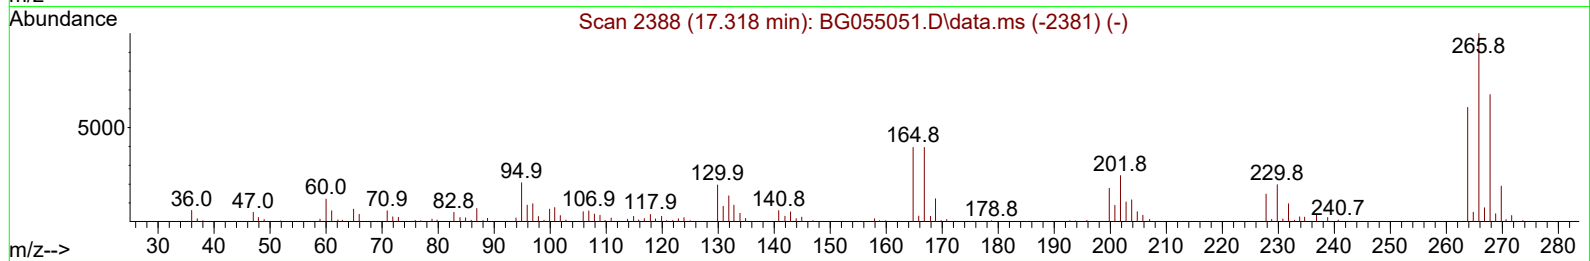
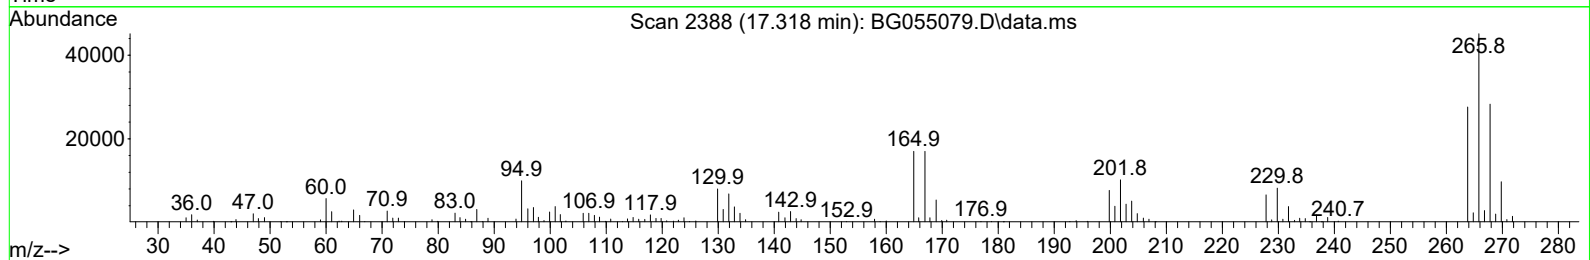


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100622\
Data File : BG055079.D
Acq On : 6 Oct 2022 10:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 05:35:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 07:12:22 2022
Response via : Initial Calibration

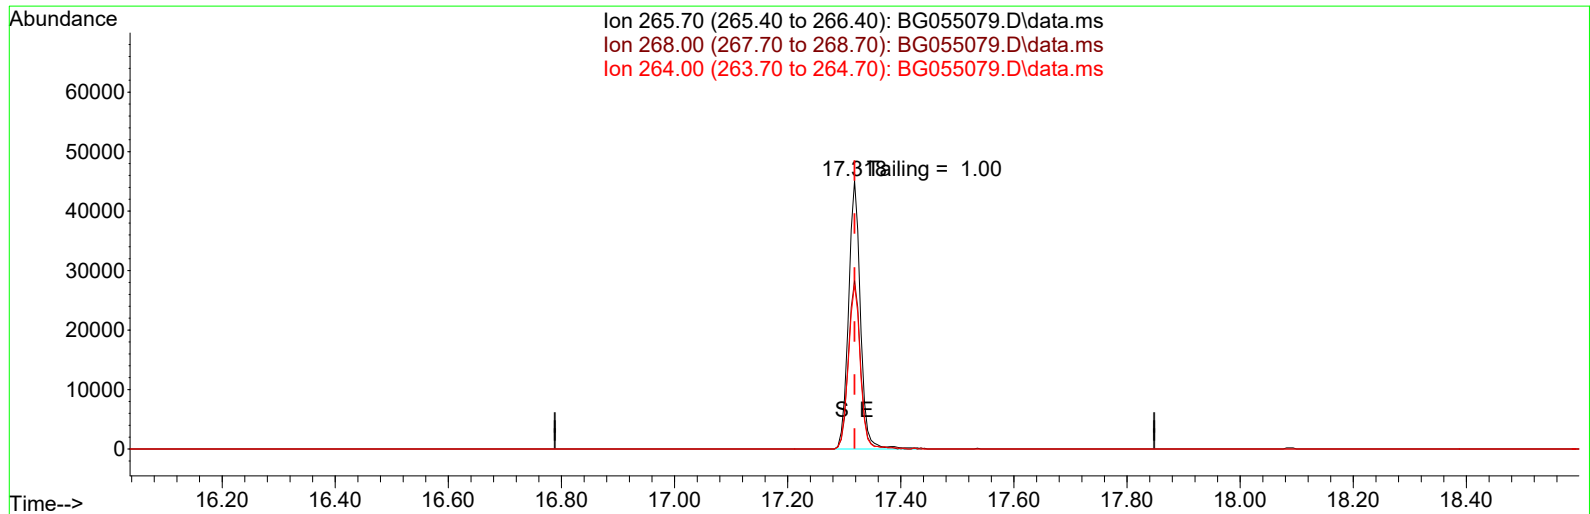

TIC: BG055079.D\data.ms

(70) Pentachlorophenol (C)




17.318min (+ 0.000) 30120.90 ng

response 65218

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	62.68
264.00	60.80	61.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100622\
Data File : BG055079.D
Acq On : 6 Oct 2022 10:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 05:35:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 07:12:22 2022
Response via : Initial Calibration

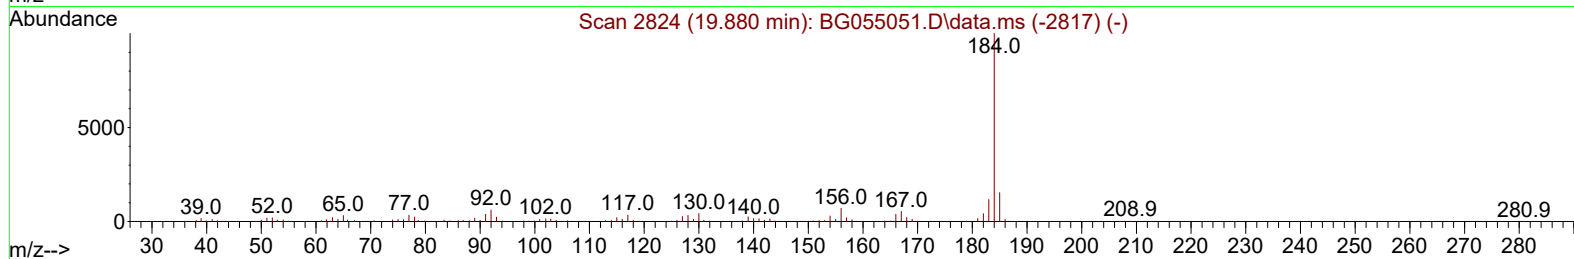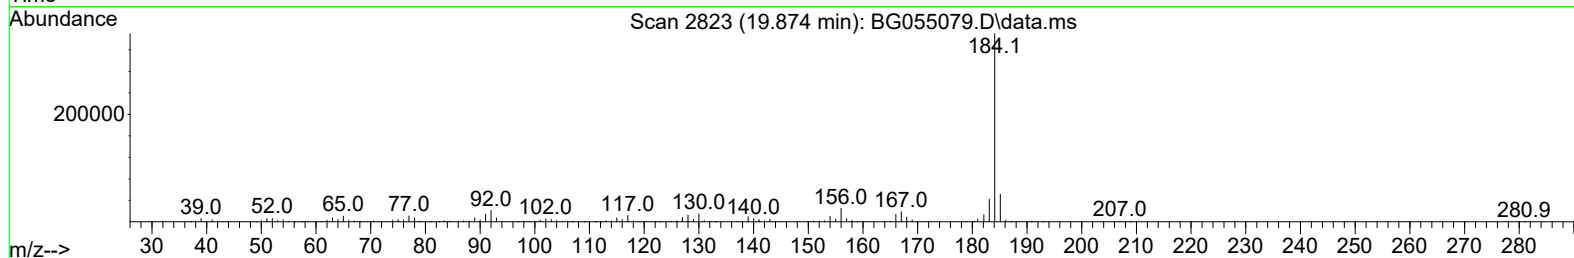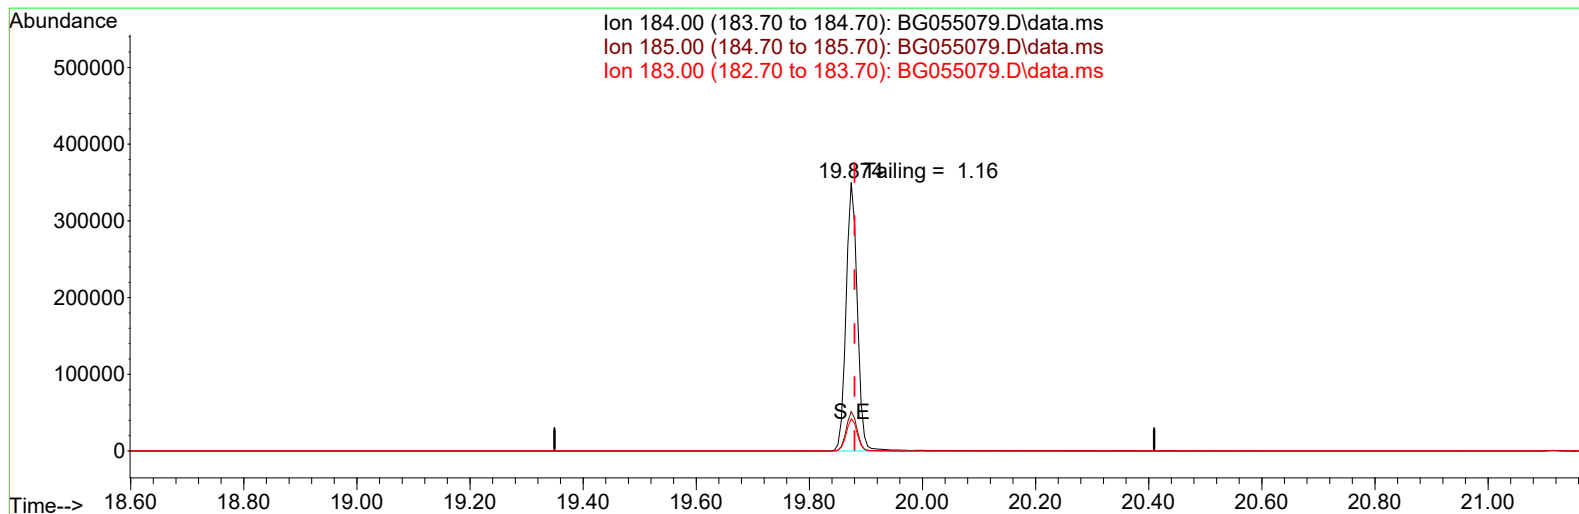

TIC: BG055079.D\data.ms

(77) Benzidine

19.874min (-0.006) 0.00 ng

response 484326

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.74
183.00	11.70	12.05
0.00	0.00	0.00