

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100622\
 Data File : BG055085.D
 Acq On : 6 Oct 2022 16:51
 Operator : CG/JU
 Sample : N5009-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 006-3

Quant Time: Oct 07 01:14:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 04 07:12:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.337	152	29381	20.000	ng	0.00
21) Naphthalene-d8	11.169	136	118012	20.000	ng	0.00
39) Acenaphthene-d10	14.941	164	81599	20.000	ng	0.00
64) Phenanthrene-d10	17.673	188	224923	20.000	ng	0.00
76) Chrysene-d12	21.968	240	243027	20.000	ng	0.00
86) Perylene-d12	25.417	264	256205	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.858	112	98827	74.711	ng	0.00
7) Phenol-d6	7.462	99	76923	38.812	ng	0.00
23) Nitrobenzene-d5	9.506	82	202948	102.760	ng	0.00
42) 2,4,6-Tribromophenol	16.416	330	181924	210.450	ng	0.00
45) 2-Fluorobiphenyl	13.572	172	465707	89.098	ng	0.00
79) Terphenyl-d14	20.253	244	1110242	92.336	ng	0.00
Target Compounds						
74) Di-n-butylphthalate	18.613	149	1528636	145.184	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100622\
Data File : BG055085.D
Acq On : 6 Oct 2022 16:51
Operator : CG/JU
Sample : N5009-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
006-3

Quant Time: Oct 07 01:14:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 07:12:22 2022
Response via : Initial Calibration




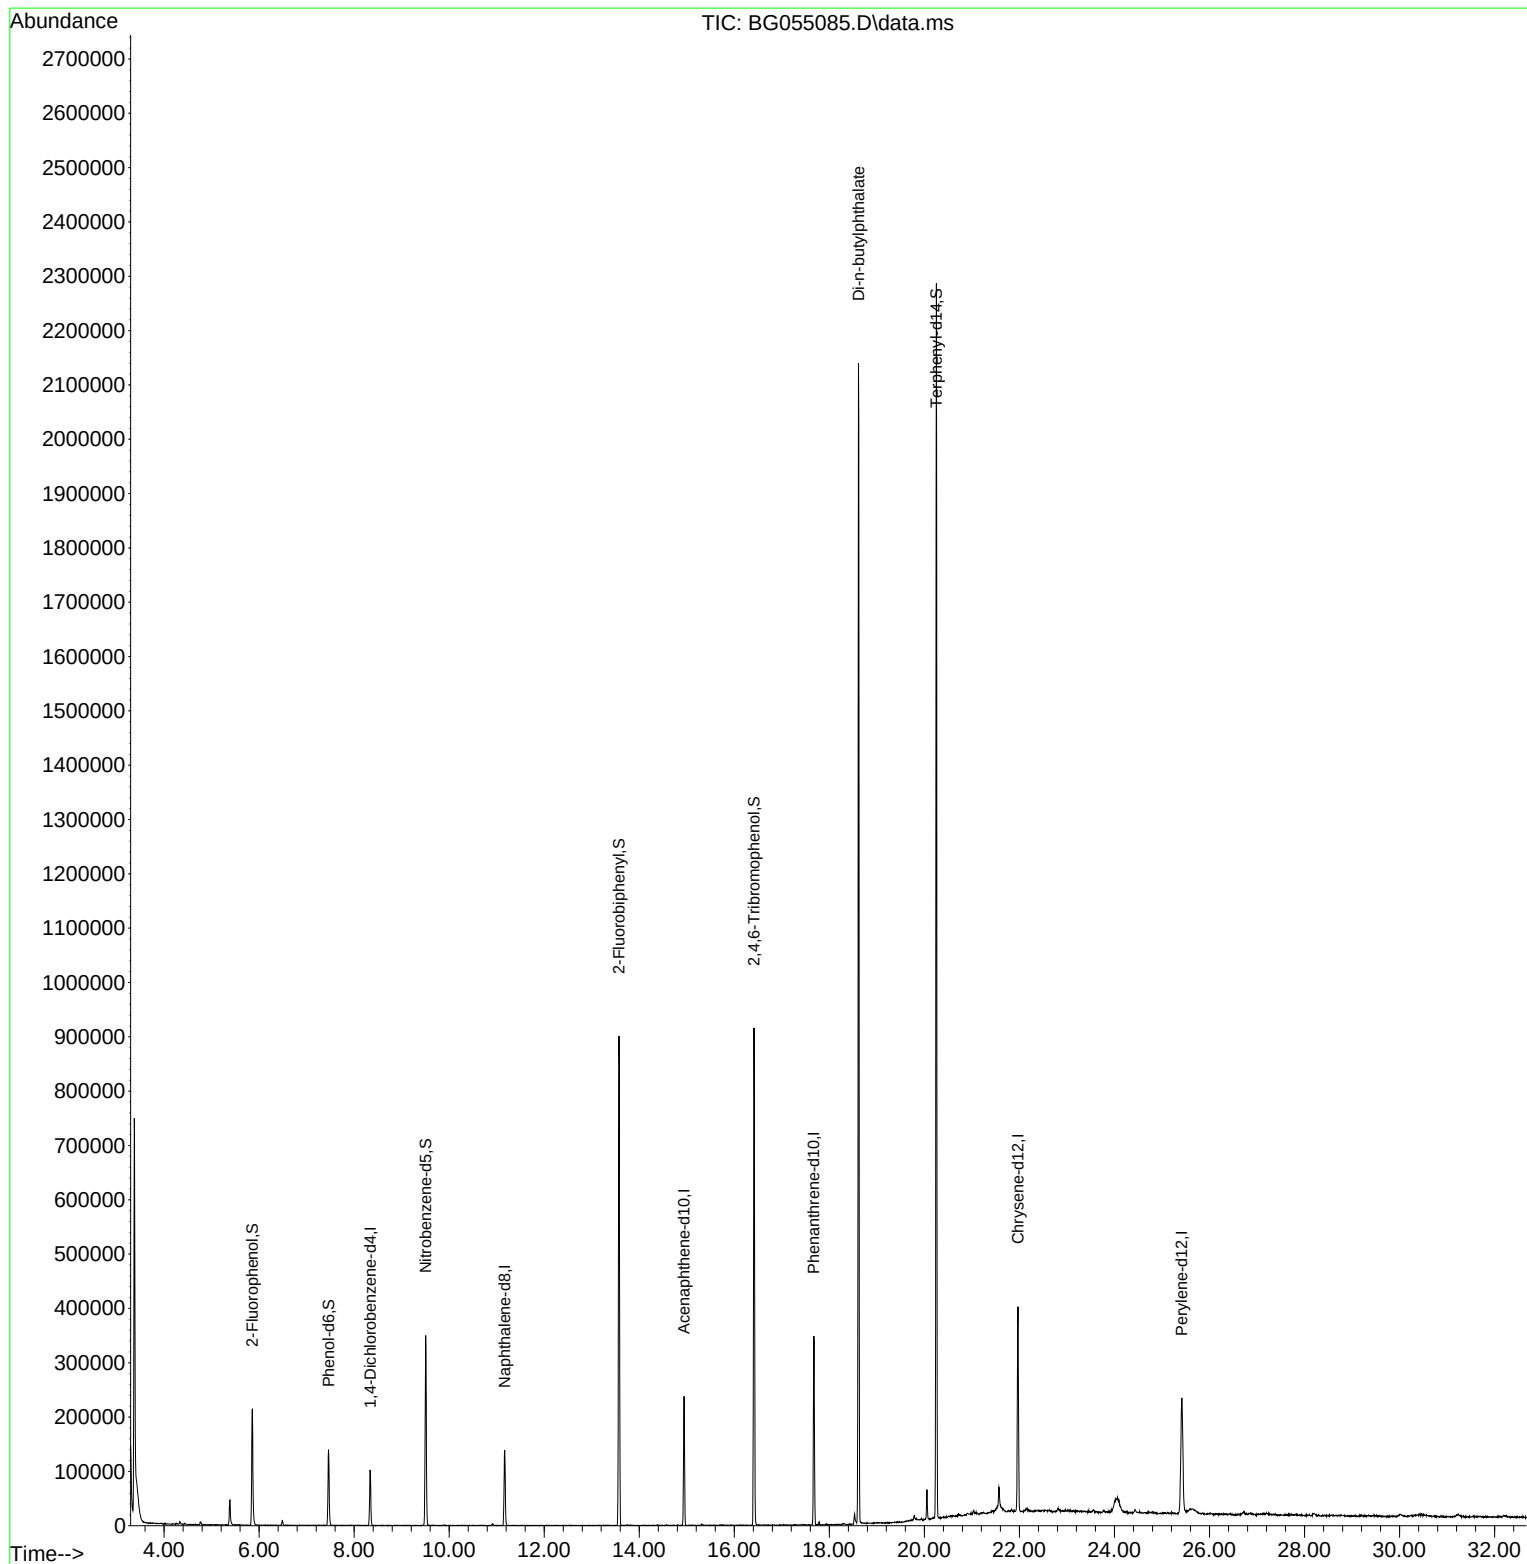


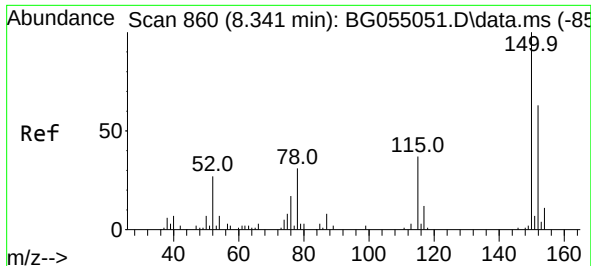

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.337 min Scan# 860
Delta R.T. -0.004 min
Lab File: BG055085.D
Acq: 6 Oct 2022 16:51




Instrument :
BNA_G
ClientSampleId :
006-3


Tgt Ion:152 Resp: 29381
Ion Ratio Lower Upper
152 100
150 159.3 128.0 192.0
115 58.9 47.7 71.5

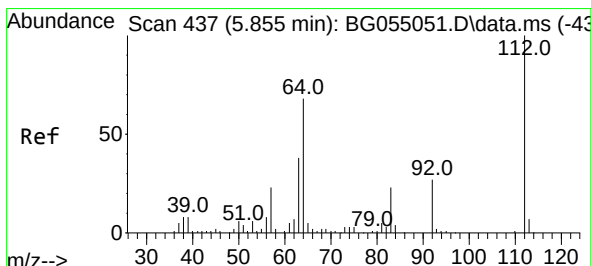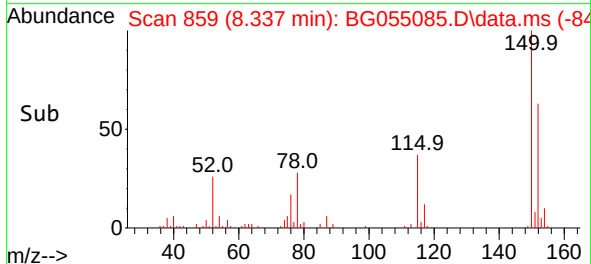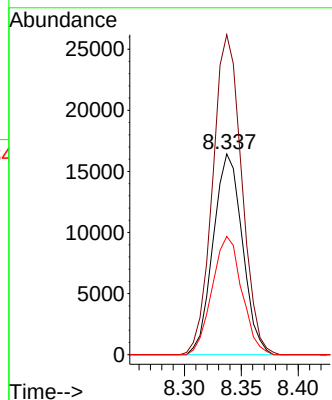

#5
2-Fluorophenol
Concen: 74.711 ng
RT: 5.858 min Scan# 437
Delta R.T. 0.003 min
Lab File: BG055085.D
Acq: 6 Oct 2022 16:51

Tgt Ion:112 Resp: 98827
Ion Ratio Lower Upper
112 100
64 63.5 54.5 81.7
63 35.9 30.5 45.7


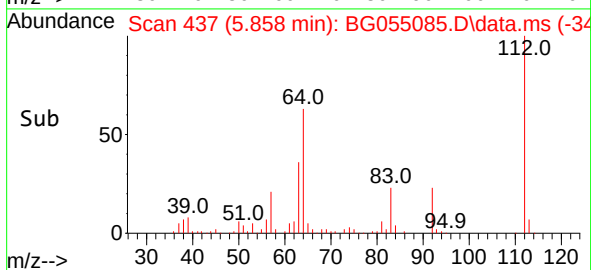
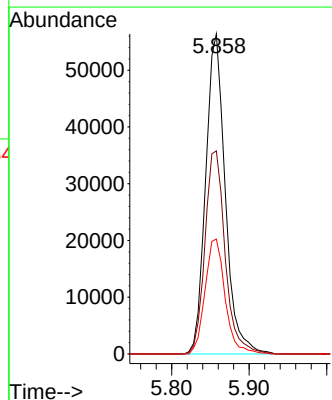
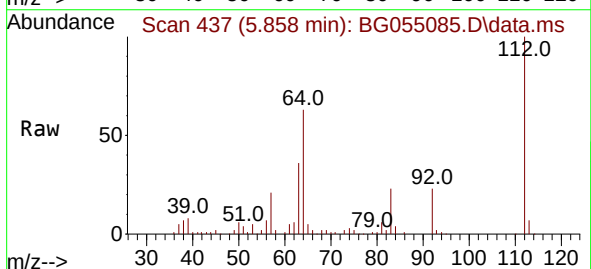




#7
Phenol-d6
Concen: 38.812 ng
RT: 7.462 min Scan# 711
Delta R.T. -0.003 min
Lab File: BG055085.D
Acq: 6 Oct 2022 16:51




Instrument :
BNA_G
ClientSampleId :
006-3


Tgt Ion: 99 Resp: 76923
Ion Ratio Lower Upper
99 100
42 22.6 18.6 28.0
71 37.0 31.2 46.8

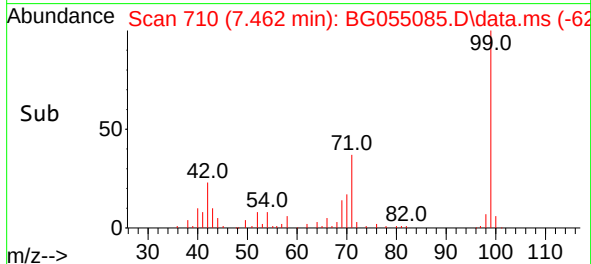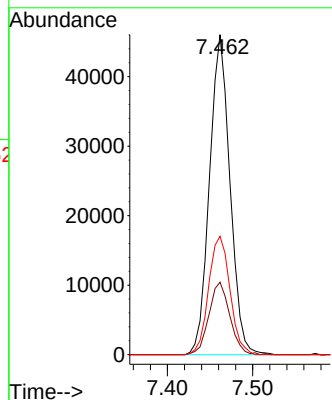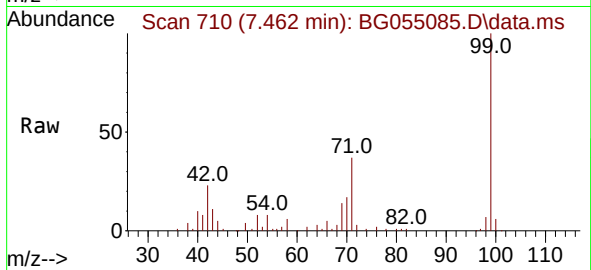

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.169 min Scan# 1341
Delta R.T. -0.004 min
Lab File: BG055085.D
Acq: 6 Oct 2022 16:51

Tgt Ion:136 Resp: 118012
Ion Ratio Lower Upper
136 100
137 11.0 8.7 13.1
54 8.8 8.2 12.4
68 6.3 4.9 7.3


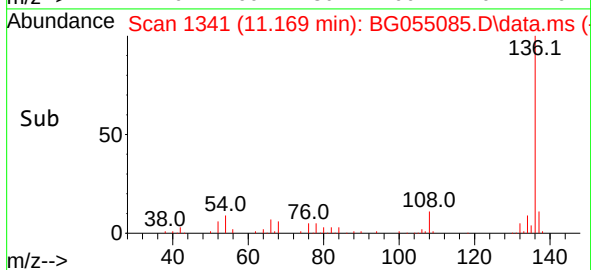
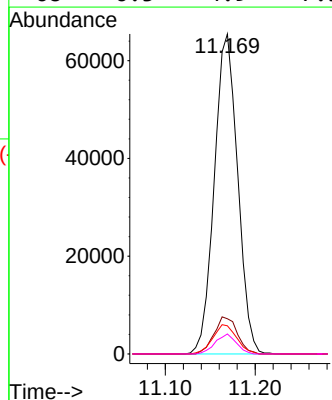
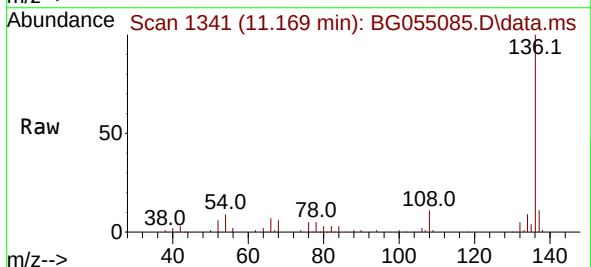


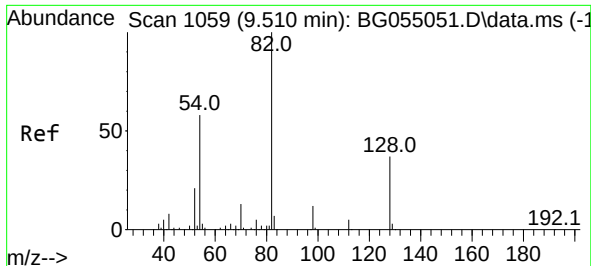

#23
Nitrobenzene-d5
Concen: 102.760 ng
RT: 9.506 min Scan# 1058
Delta R.T. -0.004 min
Lab File: BG055085.D
Acq: 6 Oct 2022 16:51




Instrument :
BNA_G
ClientSampleId :
006-3


Tgt Ion: 82 Resp: 202948
Ion Ratio Lower Upper
82 100
128 41.2 29.5 44.3
54 59.3 46.7 70.1

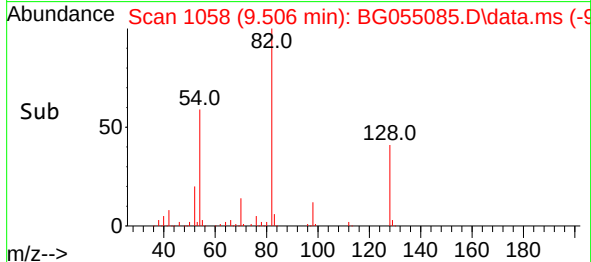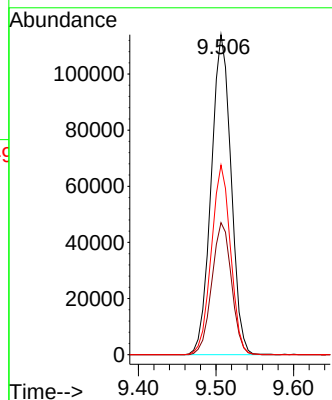

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.941 min Scan# 1983
Delta R.T. -0.009 min
Lab File: BG055085.D
Acq: 6 Oct 2022 16:51

Tgt Ion: 164 Resp: 81599
Ion Ratio Lower Upper
164 100
162 107.2 85.5 128.3
160 46.1 35.5 53.3


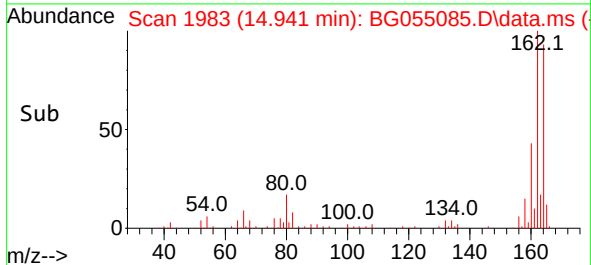
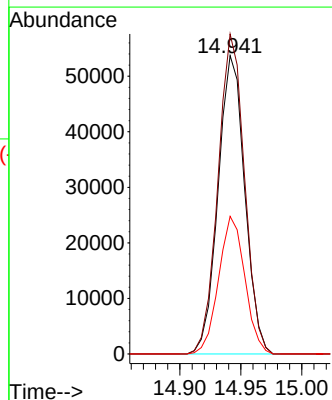
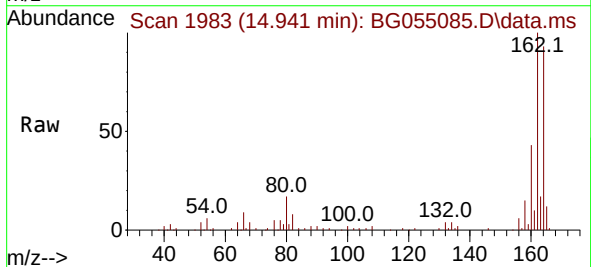


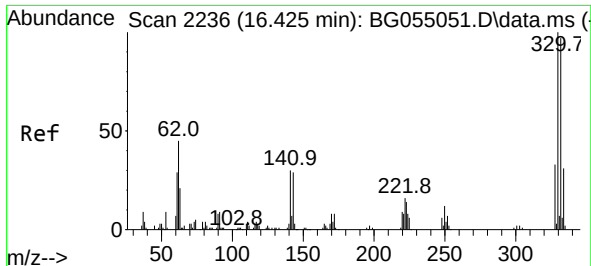

#42
2,4,6-Tribromophenol
Concen: 210.450 ng
RT: 16.416 min Scan# 21
Delta R.T. -0.009 min
Lab File: BG055085.D
Acq: 6 Oct 2022 16:51




Instrument :
BNA_G
ClientSampleId :
006-3


Tgt Ion:330 Resp: 181924
Ion Ratio Lower Upper
330 100
332 97.2 77.4 116.0
141 31.8 25.0 37.4

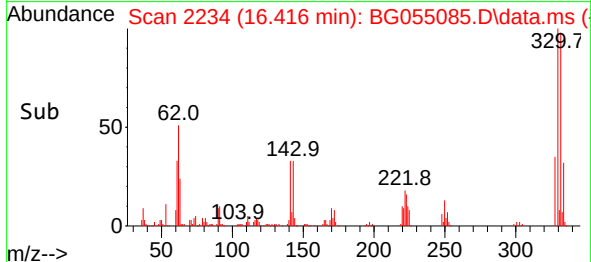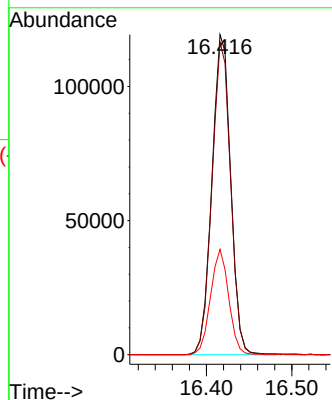

#45
2-Fluorobiphenyl
Concen: 89.098 ng
RT: 13.572 min Scan# 1750
Delta R.T. -0.010 min
Lab File: BG055085.D
Acq: 6 Oct 2022 16:51

Tgt Ion:172 Resp: 465707
Ion Ratio Lower Upper
172 100
171 37.1 30.1 45.1
170 24.4 20.0 30.0

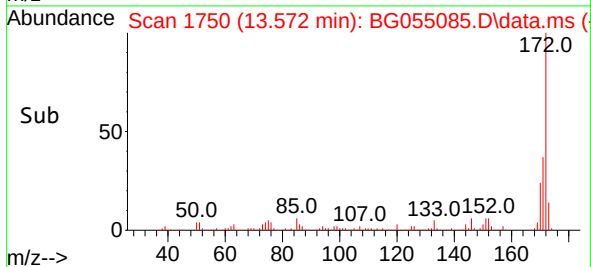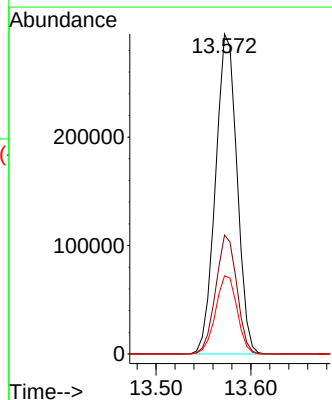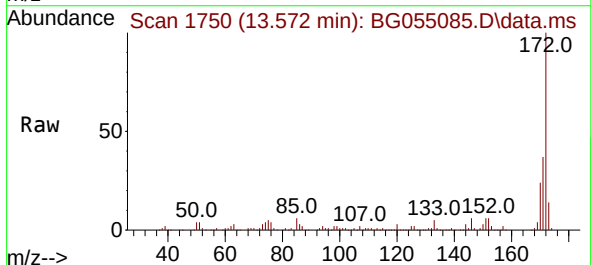



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.673 min Scan# 24

Delta R.T. -0.009 min

Lab File: BG055085.D

Acq: 6 Oct 2022 16:51

Instrument :

BNA_G

ClientSampleId :

006-3





Tgt Ion:188 Resp: 224923

Ion Ratio Lower Upper

188 100

94 7.3 6.2 9.2

80 8.4 7.2 10.8

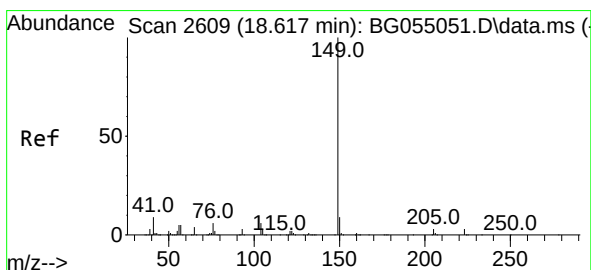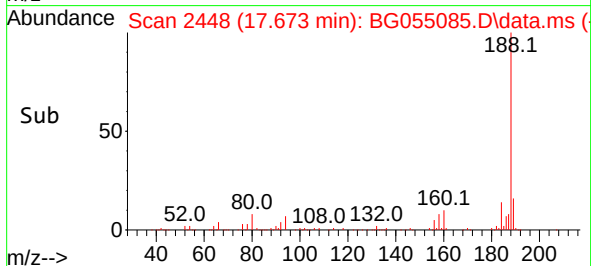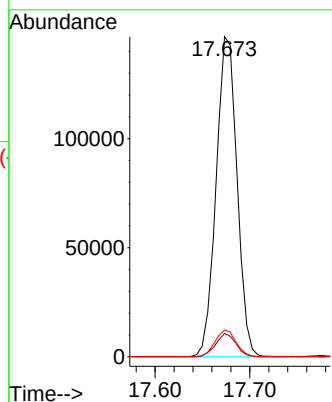

#74

Di-n-butylphthalate

Concen: 145.184 ng

RT: 18.613 min Scan# 2608

Delta R.T. -0.004 min

Lab File: BG055085.D

Acq: 6 Oct 2022 16:51




Tgt Ion:149 Resp: 1528636


Ion Ratio Lower Upper

149 100

150 10.4 7.5 11.3

104 6.7 4.8 7.2

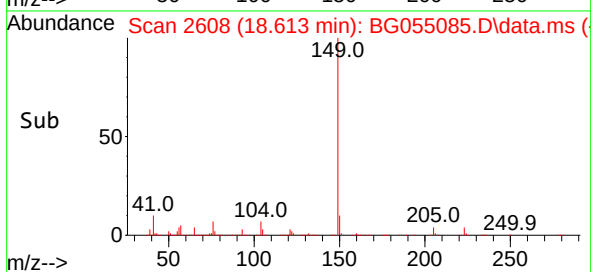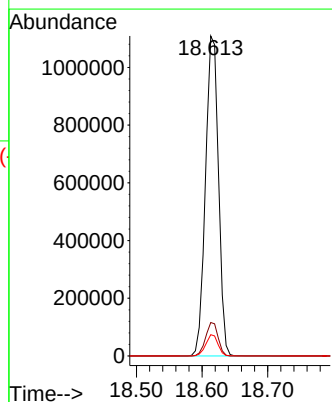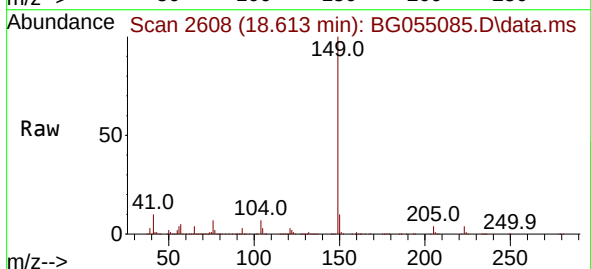



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.968 min Scan# 31

Delta R.T. -0.009 min

Lab File: BG055085.D

Acq: 6 Oct 2022 16:51

Instrument :

BNA_G

ClientSampleId :

006-3





Tgt Ion:240 Resp: 243027

Ion Ratio Lower Upper

240 100

120 7.4 6.2 9.4

236 26.2 20.6 30.8

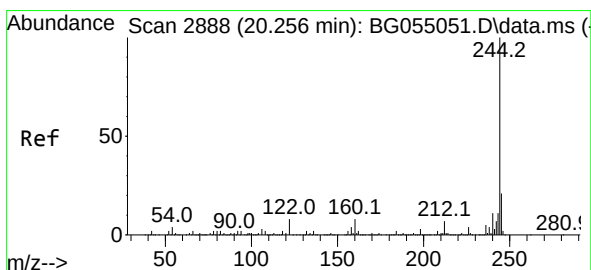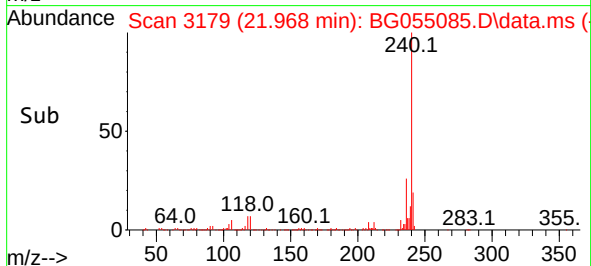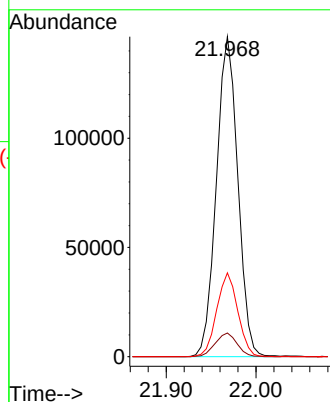

#79

Terphenyl-d14

Concen: 92.336 ng

RT: 20.253 min Scan# 2887

Delta R.T. -0.003 min

Lab File: BG055085.D

Acq: 6 Oct 2022 16:51




Tgt Ion:244 Resp: 1110242


Ion Ratio Lower Upper

244 100

212 7.6 6.0 9.0


122 8.1 6.6 10.0

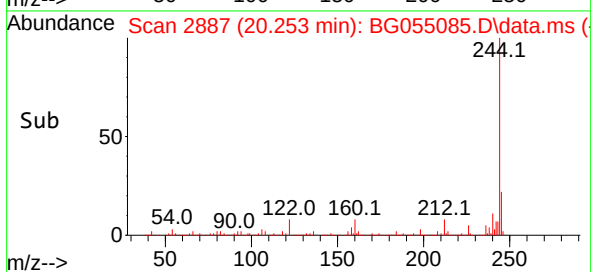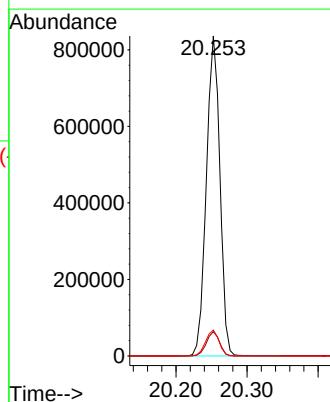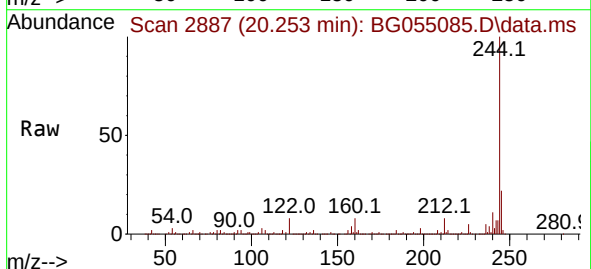



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.417 min Scan# 31
 Delta R.T. -0.015 min
 Lab File: BG055085.D
 Acq: 6 Oct 2022 16:51

Instrument :
 BNA_G
 ClientSampleId :
 006-3



Tgt Ion:264 Resp: 256205

Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.7	29.5
265	21.6	17.8	26.6

