


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100622\
 Data File : BG055079.D
 Acq On : 6 Oct 2022 10:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 04 07:12:22 2022

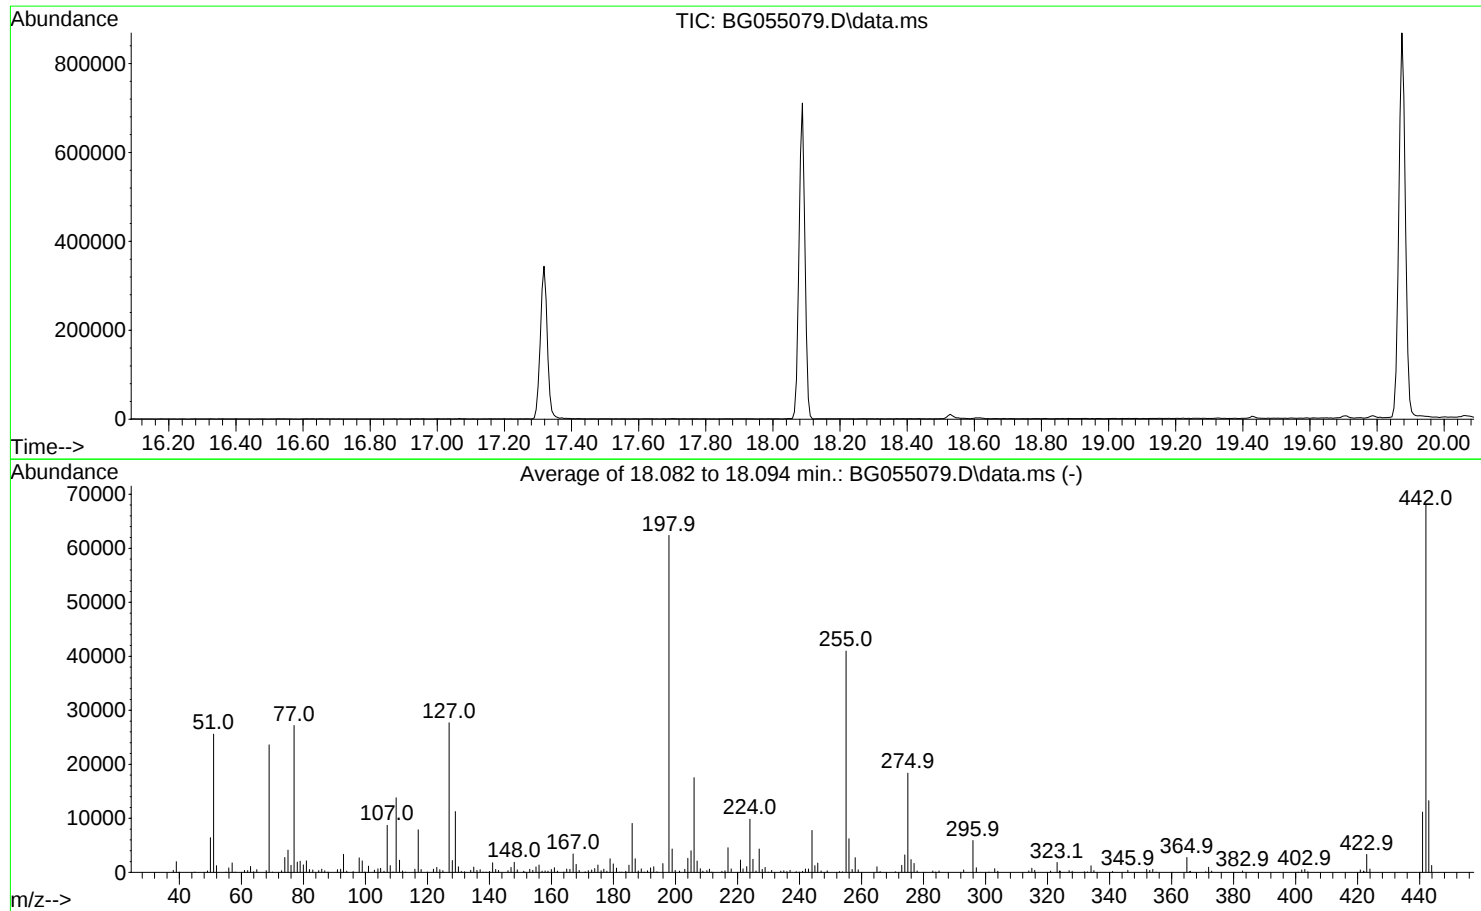




AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	25603	PASS
68	69	0.00	2	1.3	314	PASS
69	198	0.00	100	37.9	23620	PASS
70	69	0.00	2	0.2	53	PASS
127	198	10	80	44.4	27693	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62379	PASS
199	198	5	9	6.9	4325	PASS
275	198	10	60	29.4	18365	PASS
365	198	1	100	4.4	2764	PASS
441	198	0.01	100	17.9	11171	PASS
442	442	50	100	100.0	68104	PASS
443	442	15	24	19.5	13281	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100622\
 Data File : BG055079.D
 Acq On : 6 Oct 2022 10:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 07 05:35:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 04 07:12:22 2022
 Response via : Initial Calibration

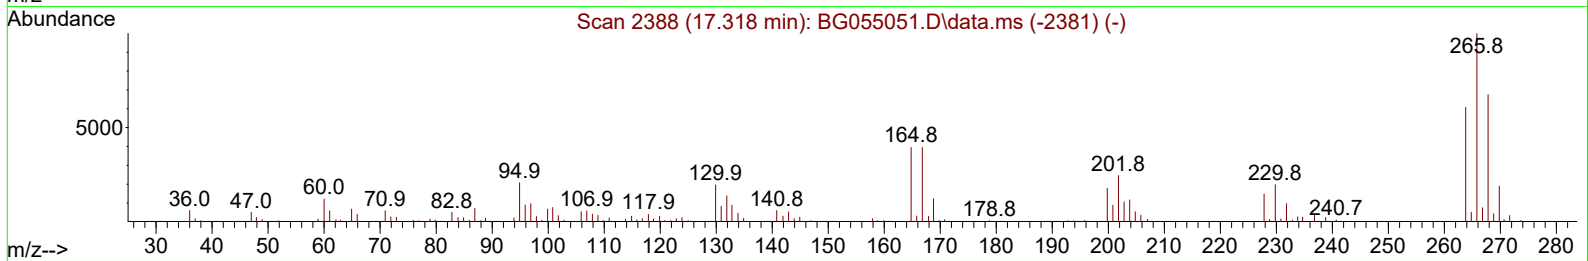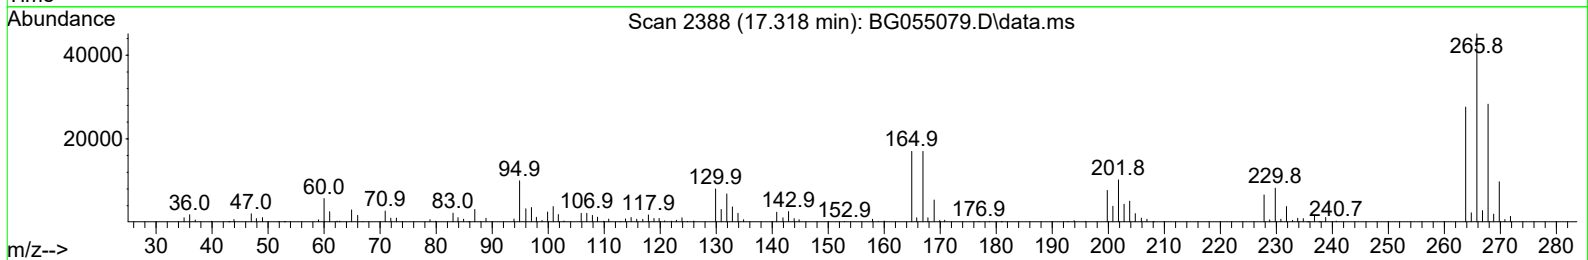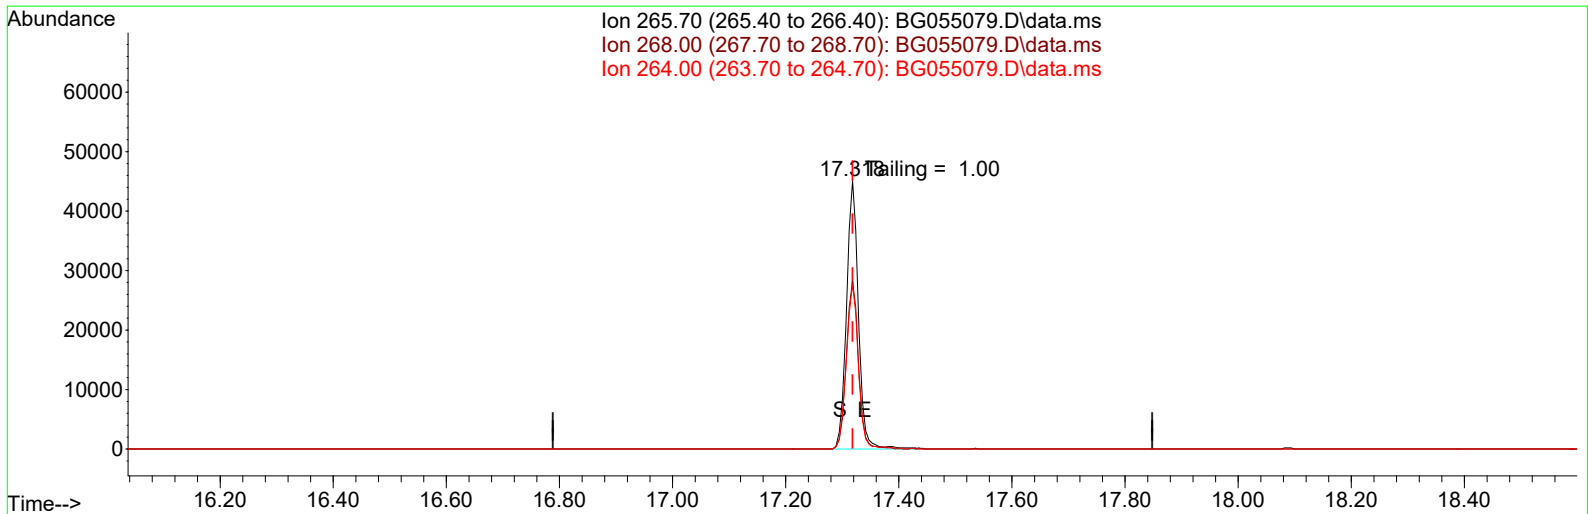

TIC: BG055079.D\data.ms

(70) Pentachlorophenol (C)

17.318min (+ 0.000) 30120.90 ng




response 65218

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	62.68
264.00	60.80	61.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100622\
 Data File : BG055079.D
 Acq On : 6 Oct 2022 10:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 07 05:35:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 04 07:12:22 2022
 Response via : Initial Calibration

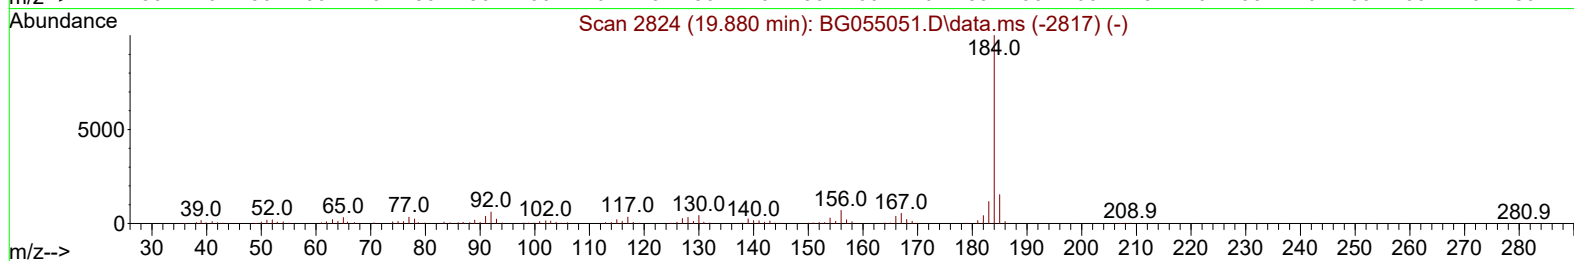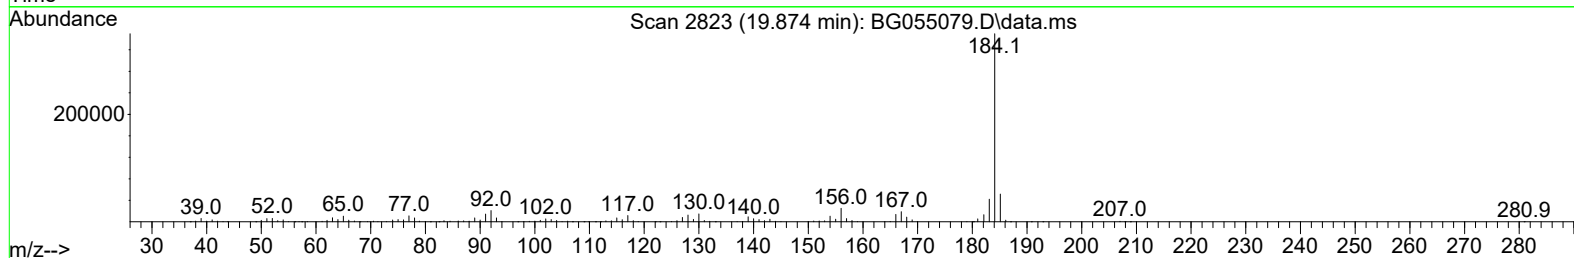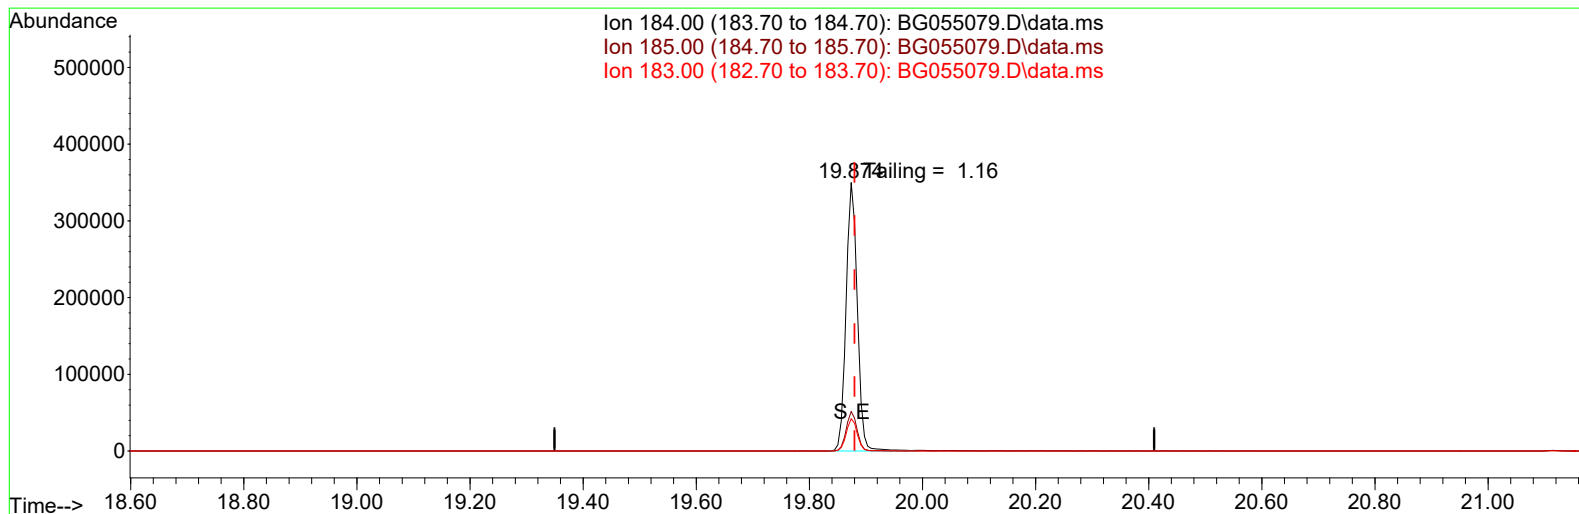

TIC: BG055079.D\data.ms

(77) Benzidine

19.874min (-0.006) 0.00 ng

response 484326

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.74
183.00	11.70	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/6/2022	BNA_G	<u>BG055079.D</u>
Compound Name	Response	Retention Time
DDT	179890	21.114
DDD	3724	20.655
DDE	61	20.162
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3785	183675	2.06

Instrument :
BNA_G
ClientSampleId :
DFTPP