


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG100719\
 Data File : BG043064.D
 Acq On : 7 Oct 2019 12:04
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 25 15:35:52 2019

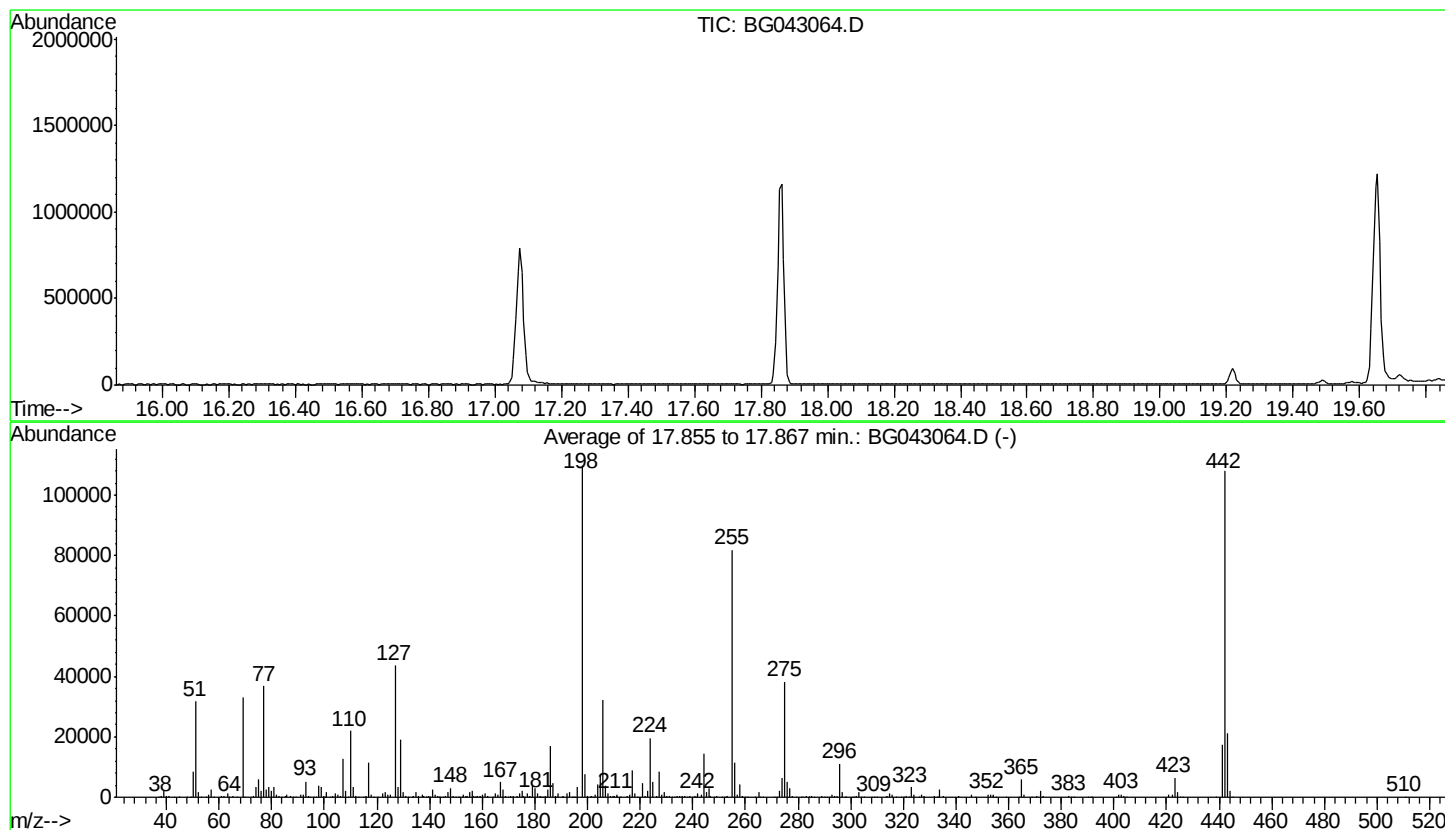

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	31756	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.1	33050	PASS
70	69	0.00	2	0.3	110	PASS
127	198	10	80	39.7	43592	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109773	PASS
199	198	5	9	6.8	7492	PASS
275	198	10	60	34.9	38282	PASS
365	198	1	100	5.3	5821	PASS
441	198	0.01	100	15.7	17279	PASS
442	198	50	100	98.4	108026	PASS
443	442	15	24	19.5	21074	PASS